
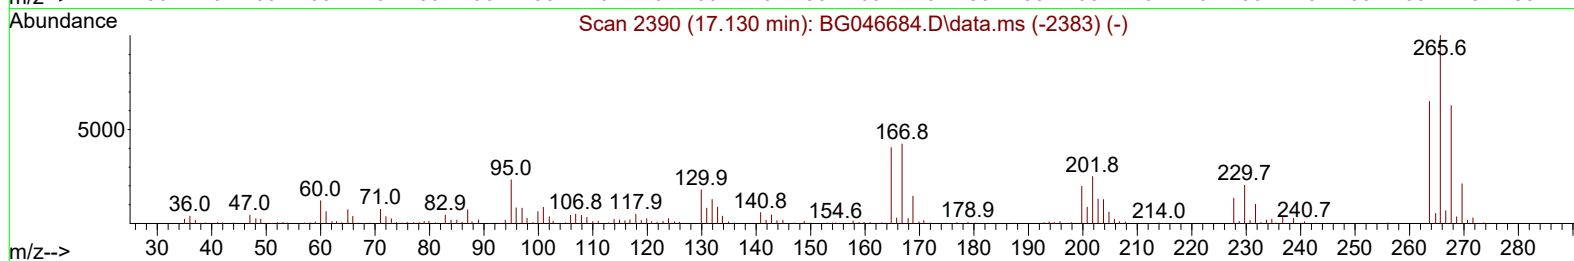
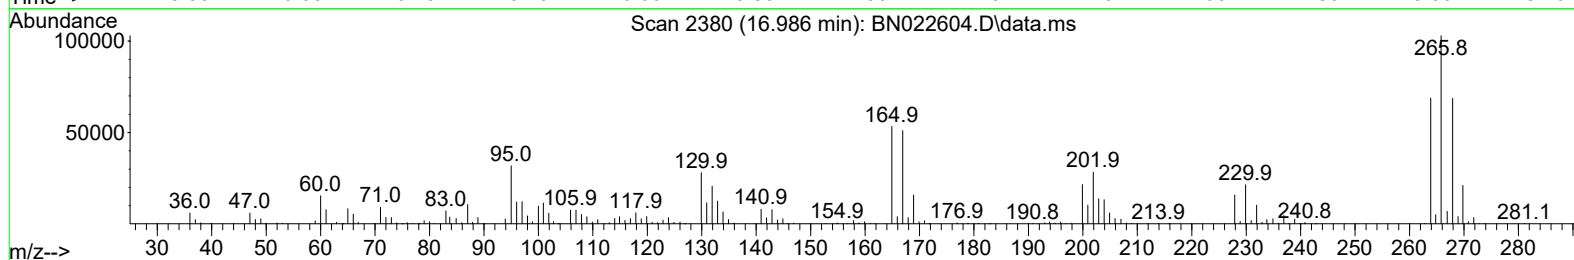


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\  
Data File : BN022604.D  
Acq On    : 11 Nov 2022  09:02  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Nov 12 05:31:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 12 05:31:08 2022
Response via : Initial Calibration

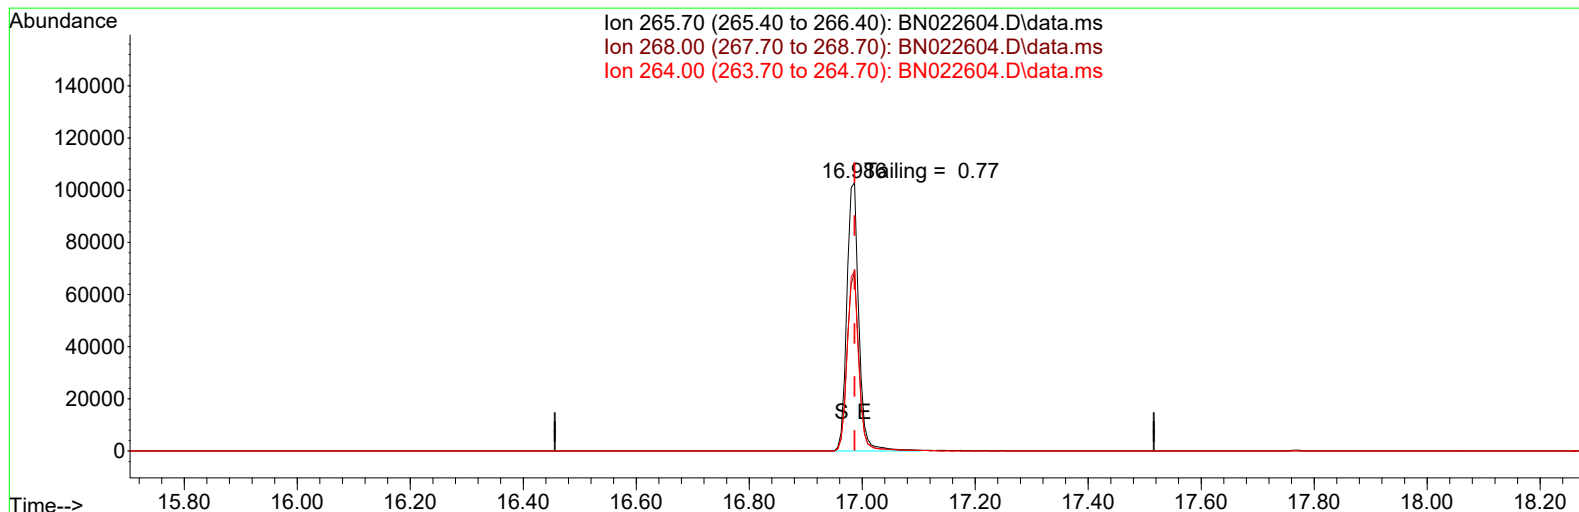

TIC: BN022604.D\data.ms

(70) Pentachlorophenol (C)

16.986min (0.000) 17431.59 ng

response **152257**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	62.20	66.81
--------	-------	-------

264.00	61.60	66.92
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
 Data File : BN022604.D
 Acq On : 11 Nov 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 12 05:31:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 12 05:31:08 2022
 Response via : Initial Calibration

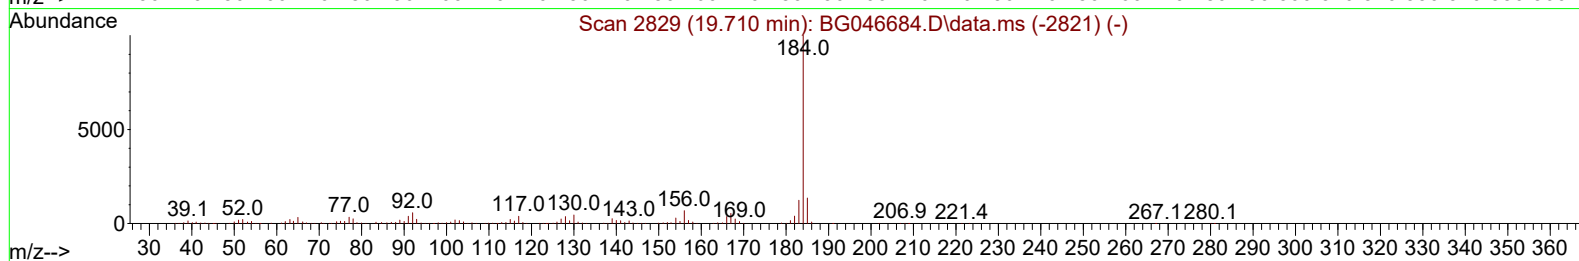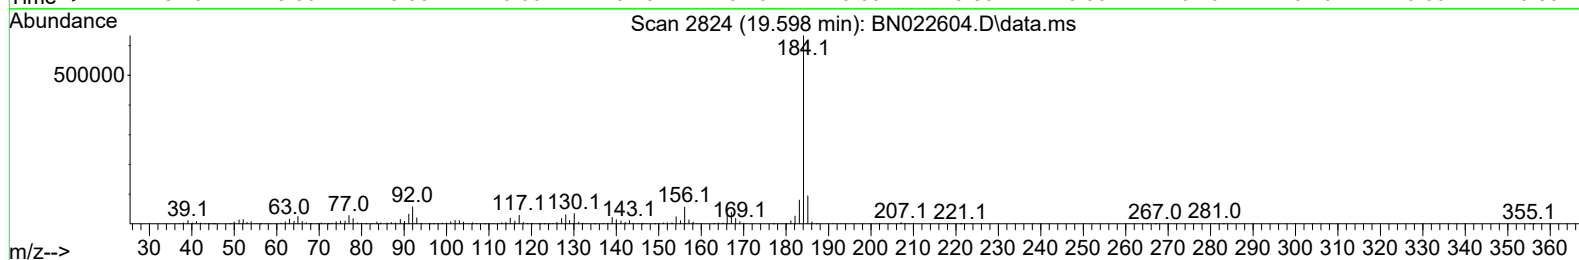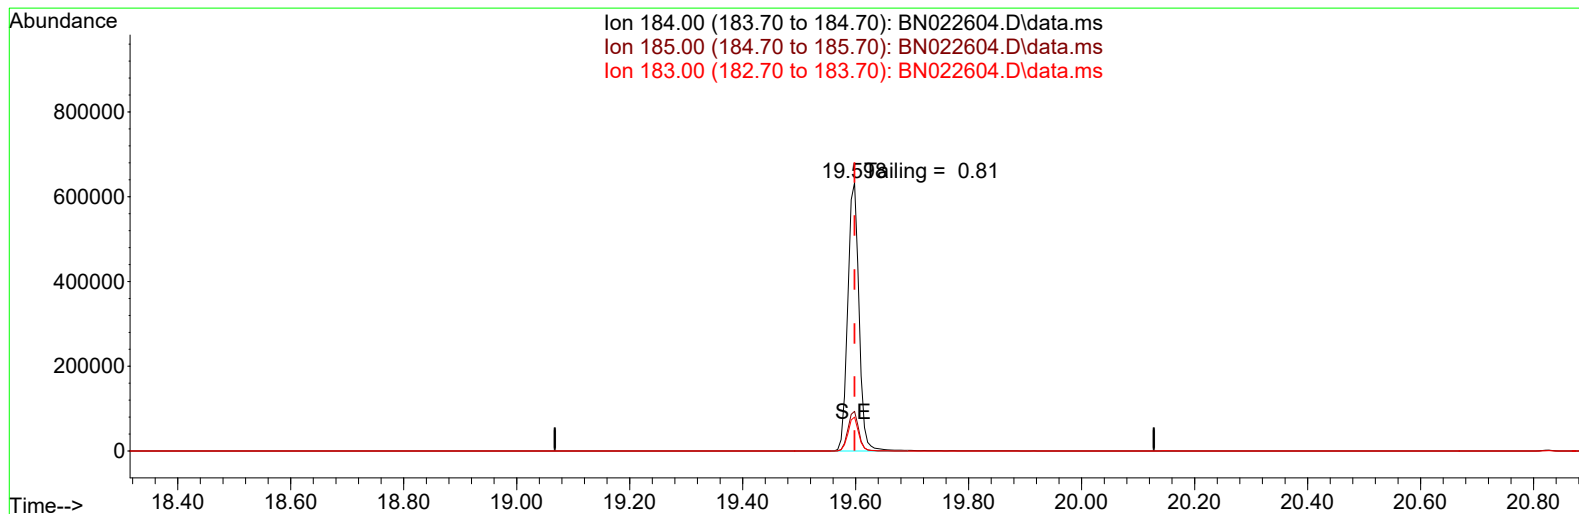

TIC: BN022604.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 879386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.79
183.00	13.20	12.65
0.00	0.00	0.00