


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
 Data File : BN022590.D
 Acq On : 10 Nov 2022 08:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 10 23:28:29 2022

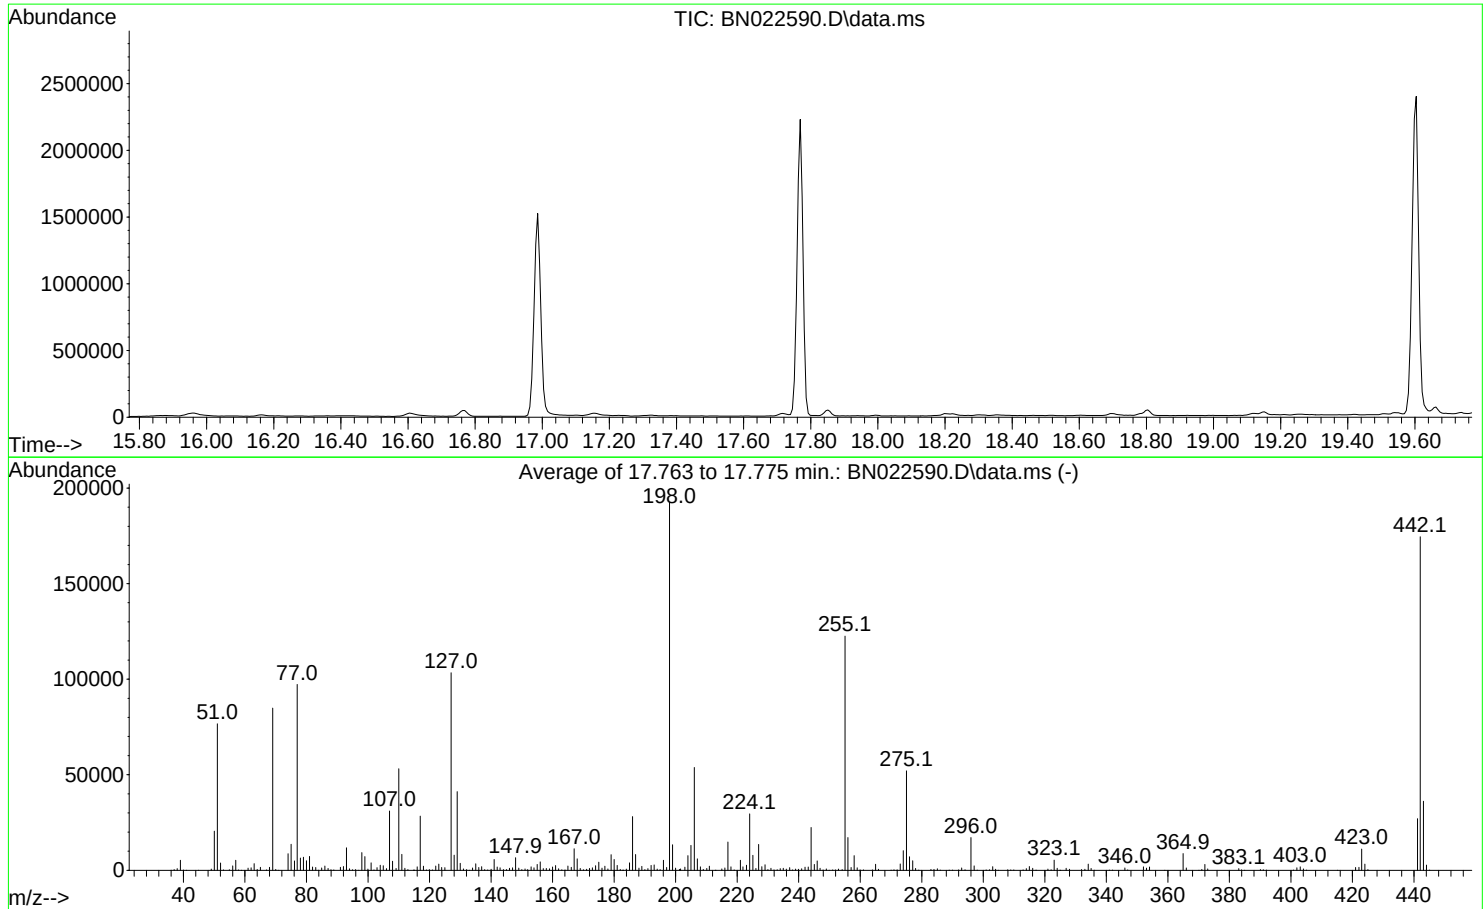




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	76621	PASS
68	69	0.00	2	1.9	1590	PASS
69	198	0.00	100	44.1	84851	PASS
70	69	0.00	2	0.6	476	PASS
127	198	10	80	53.7	103339	PASS
197	198	0.00	2	0.8	1454	PASS
198	198	100	100	100.0	192491	PASS
199	198	5	9	6.9	13352	PASS
275	198	10	60	27.0	52029	PASS
365	198	1	100	4.5	8724	PASS
441	198	0.01	100	14.0	27000	PASS
442	442	50	100	100.0	174523	PASS
443	442	15	24	20.7	36099	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
 Data File : BN022590.D
 Acq On : 10 Nov 2022 08:04
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 11 05:20:19 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 05:20:15 2022
 Response via : Initial Calibration

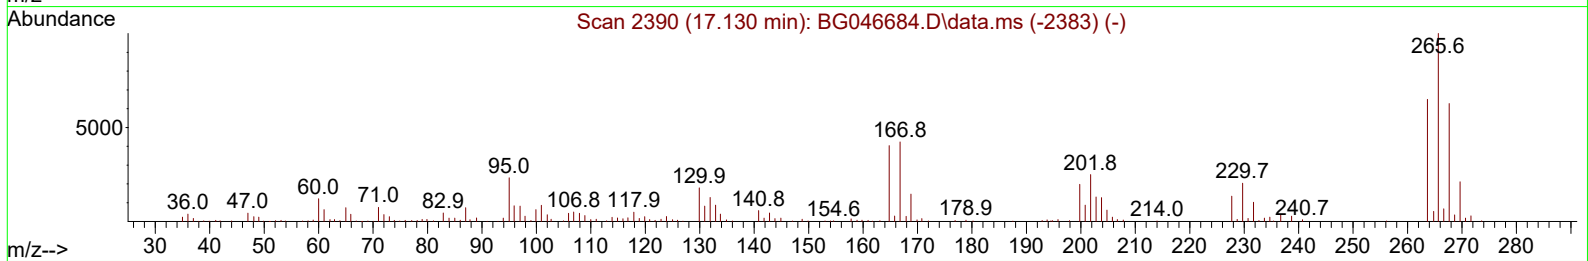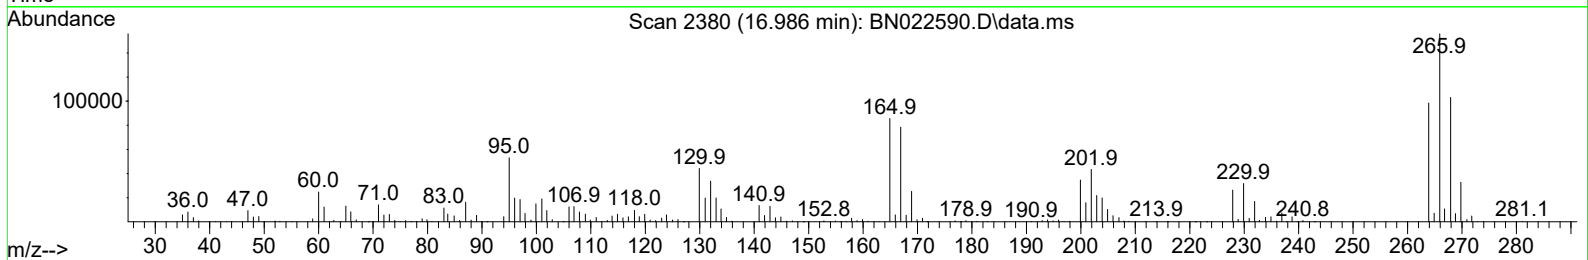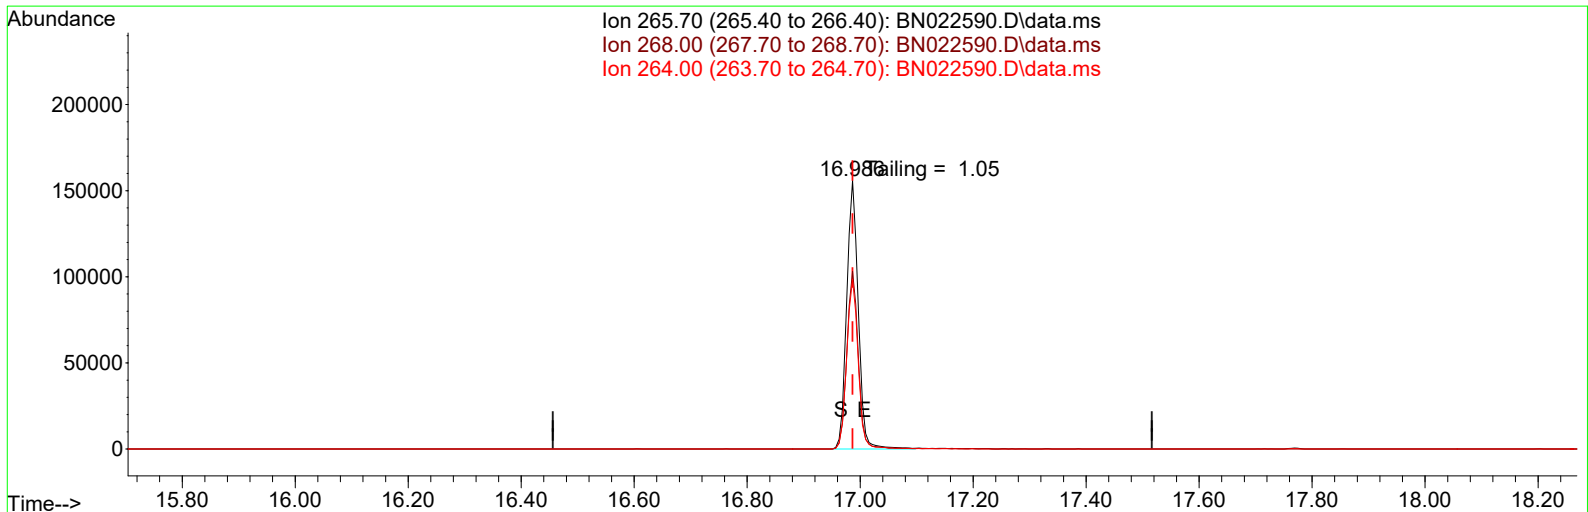

TIC: BN022590.D\data.ms

(70) Pentachlorophenol (C)

16.986min (0.000) 17653.78 ng




response 222222

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.18
264.00	61.60	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
Data File : BN022590.D
Acq On : 10 Nov 2022 08:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 11 05:20:19 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 05:20:15 2022
Response via : Initial Calibration

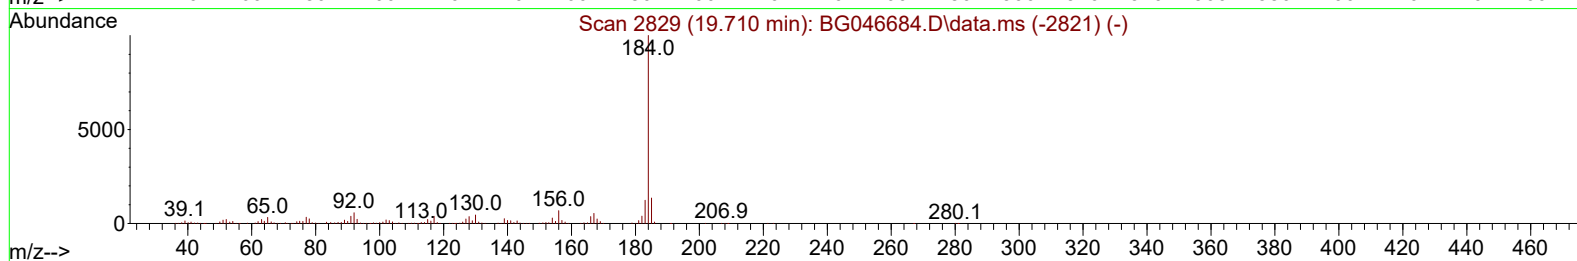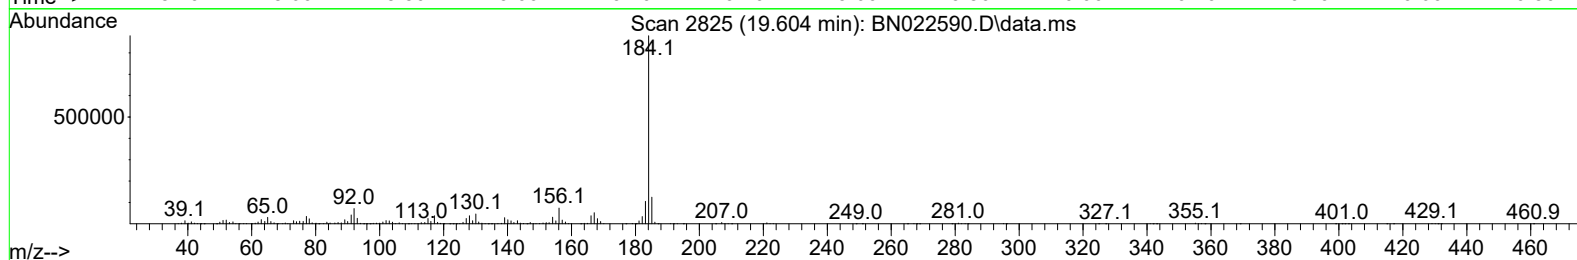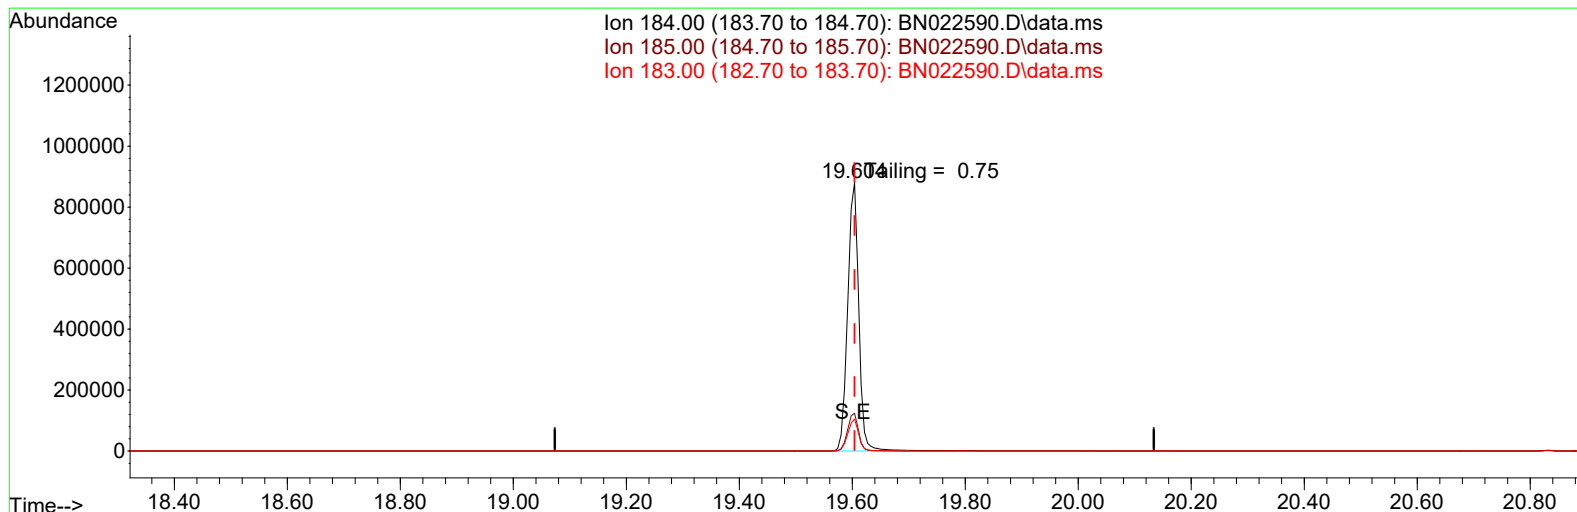

TIC: BN022590.D\data.ms

(77) Benzidine

19.604min (0.000) 0.00 ng

response 1201047

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2022	BNA_N	<u>BN022590.D</u>
Compound Name	Response	Retention Time
DDT	584529	20.833
DDD	32921	20.392
DDE	1018	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33939	618468	5.49

Instrument :
BNA_N
ClientSampleId :
DFTPP