


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
Data File : BN022604.D
Acq On : 11 Nov 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 10 23:28:29 2022

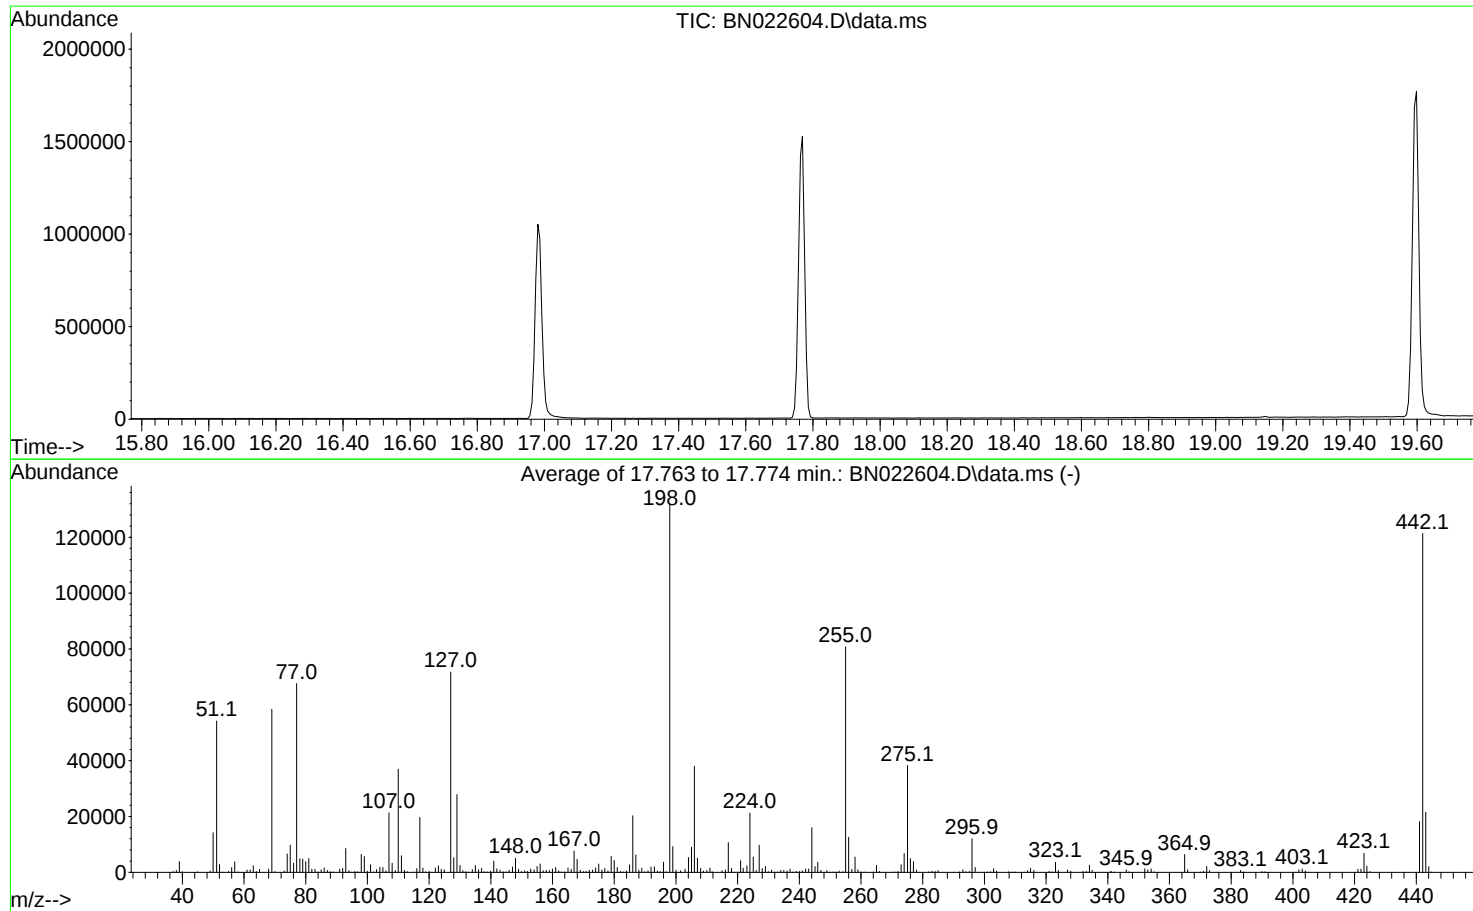




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	54179	PASS
68	69	0.00	2	1.9	1102	PASS
69	198	0.00	100	44.3	58381	PASS
70	69	0.00	2	0.5	285	PASS
127	198	10	80	54.4	71701	PASS
197	198	0.00	2	0.2	247	PASS
198	198	100	100	100.0	131760	PASS
199	198	5	9	7.0	9179	PASS
275	198	10	60	29.0	38253	PASS
365	198	1	100	4.8	6343	PASS
441	198	0.01	100	13.8	18140	PASS
442	442	50	100	100.0	121328	PASS
443	442	15	24	17.7	21501	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
 Data File : BN022604.D
 Acq On : 11 Nov 2022 09:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 12 05:31:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 12 05:31:08 2022
 Response via : Initial Calibration

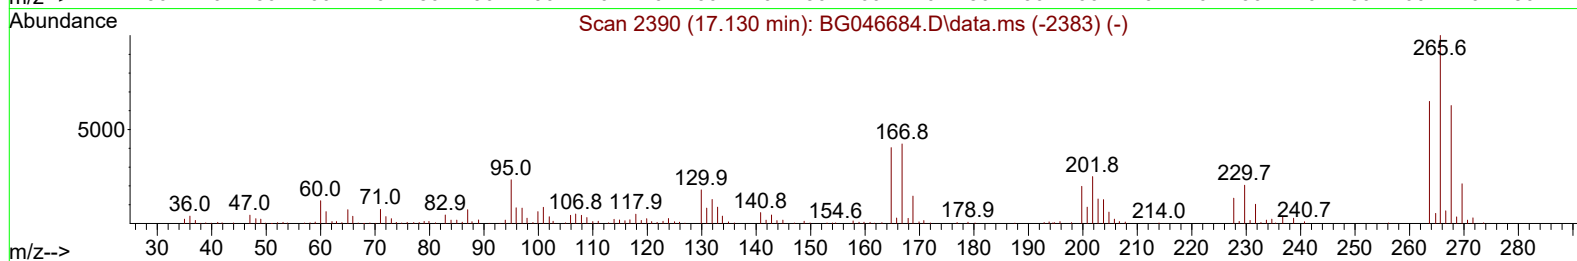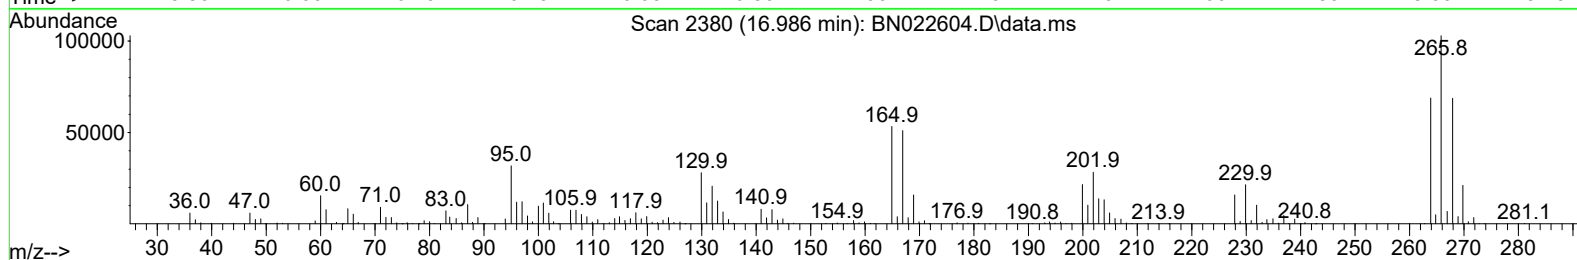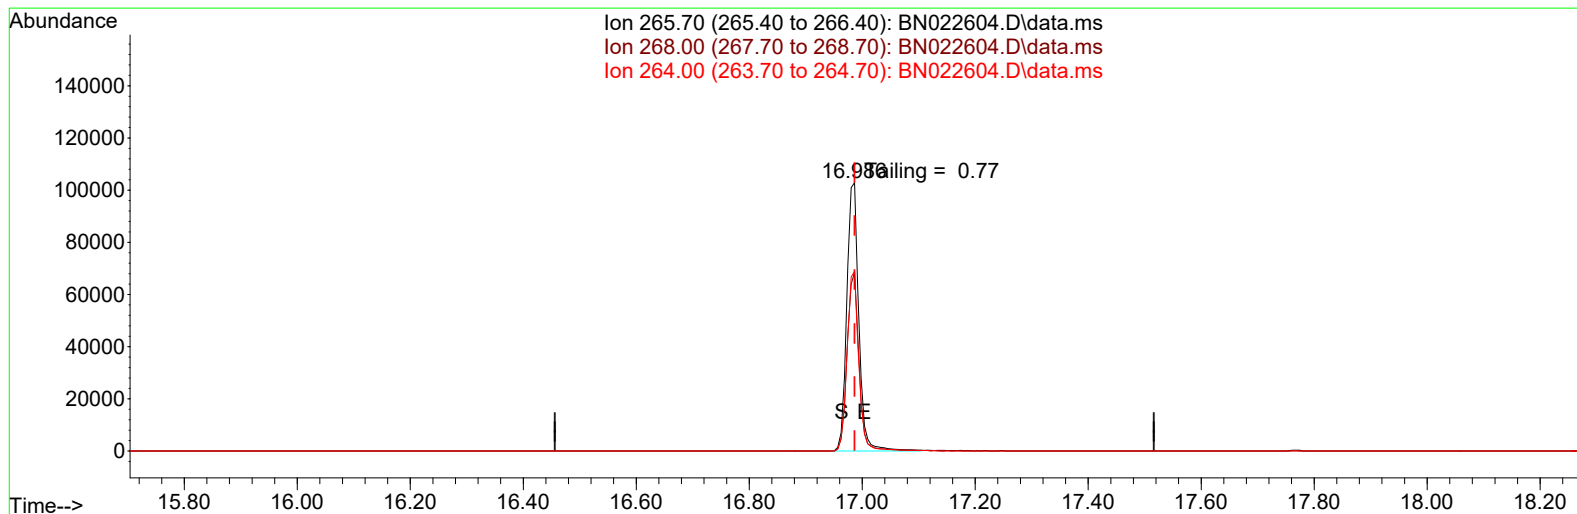

TIC: BN022604.D\data.ms

(70) Pentachlorophenol (C)

16.986min (0.000) 17431.59 ng




response 152257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.81
264.00	61.60	66.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111122\
Data File : BN022604.D
Acq On : 11 Nov 2022 09:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 12 05:31:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 12 05:31:08 2022
Response via : Initial Calibration

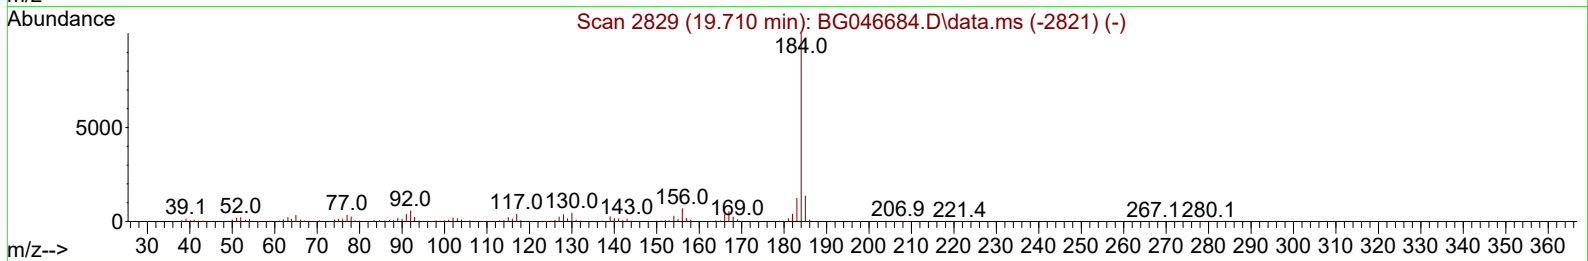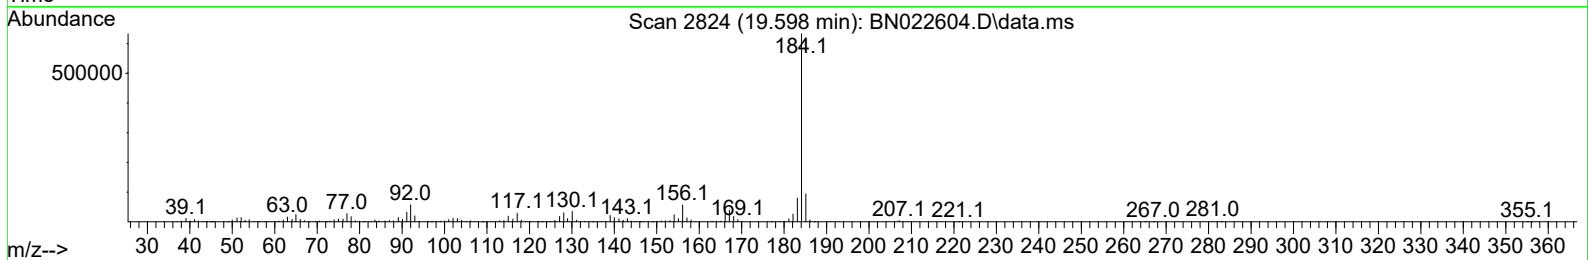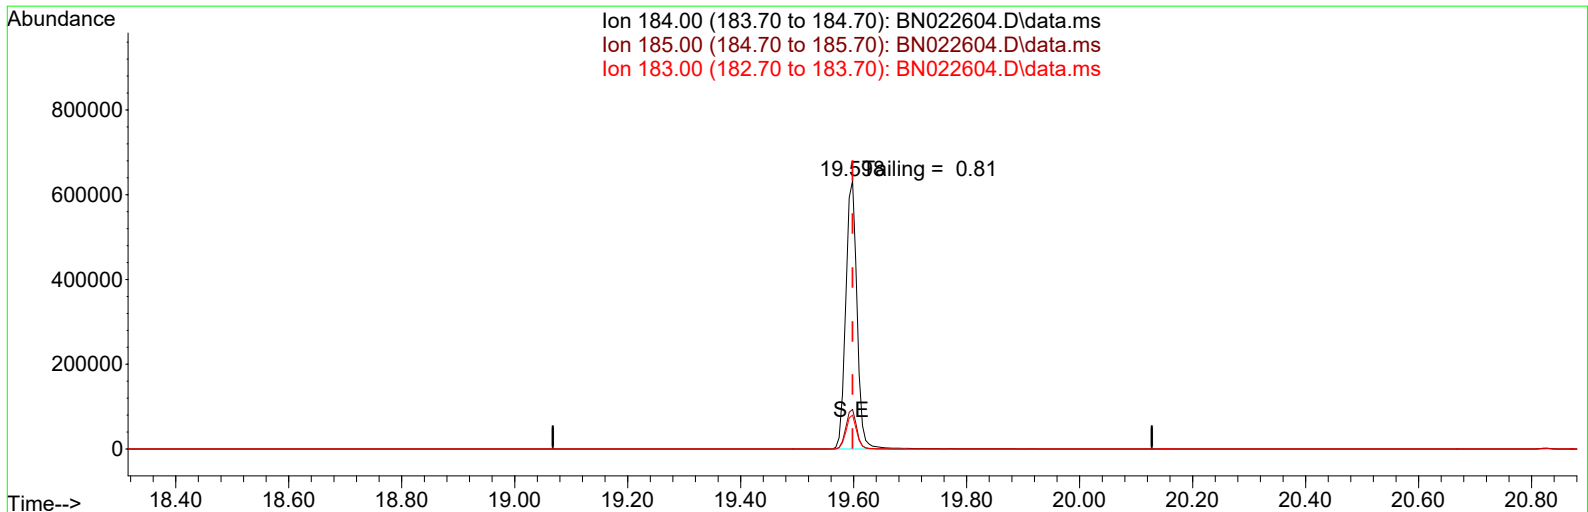

TIC: BN022604.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 879386

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.79
183.00	13.20	12.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/11/2022	BNA_N	<u>BN022604.D</u>
Compound Name	Response	Retention Time
DDT	413176	20.827
DDD	21924	20.386
DDE	1035	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22959	436135	5.26

Instrument :
BNA_N
ClientSampleId :
DFTPP