




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

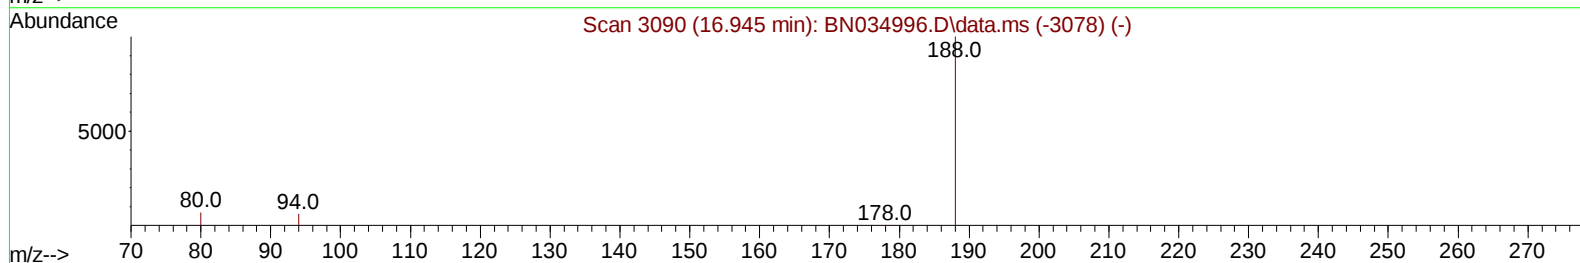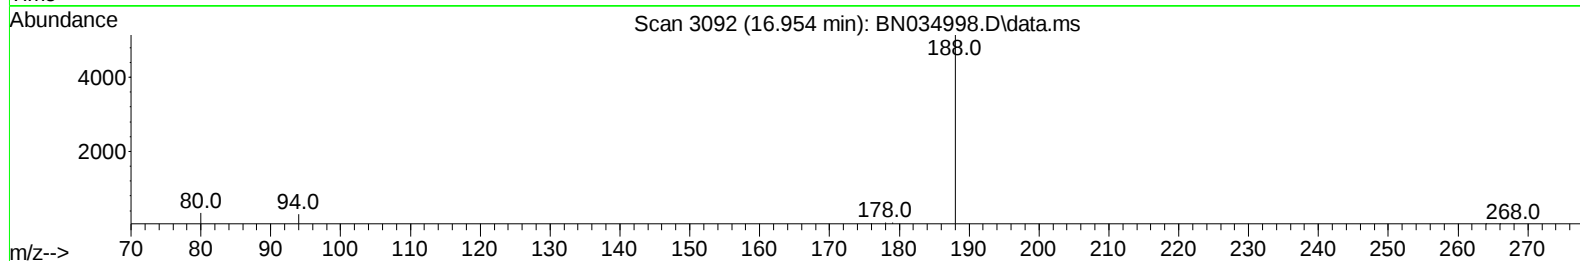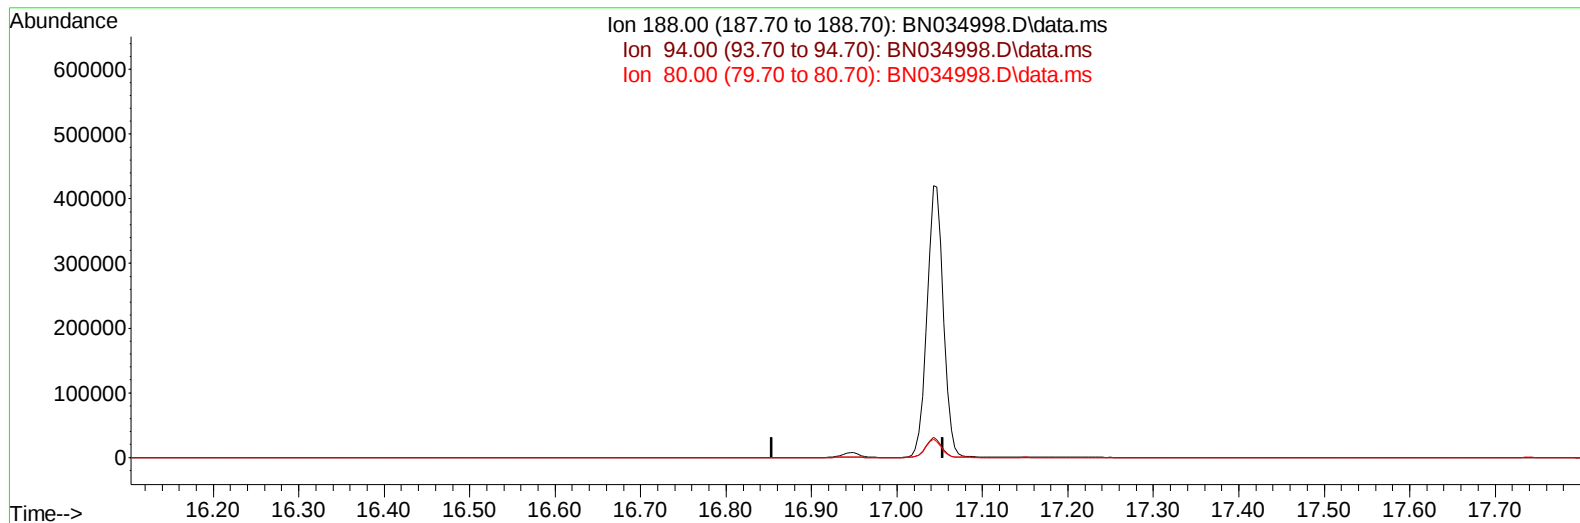

TIC: BN034998.D\data.ms

(13) Phenanthrene-d10 (I)

16.954min (-16.954) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.10	0.00#
80.00	7.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

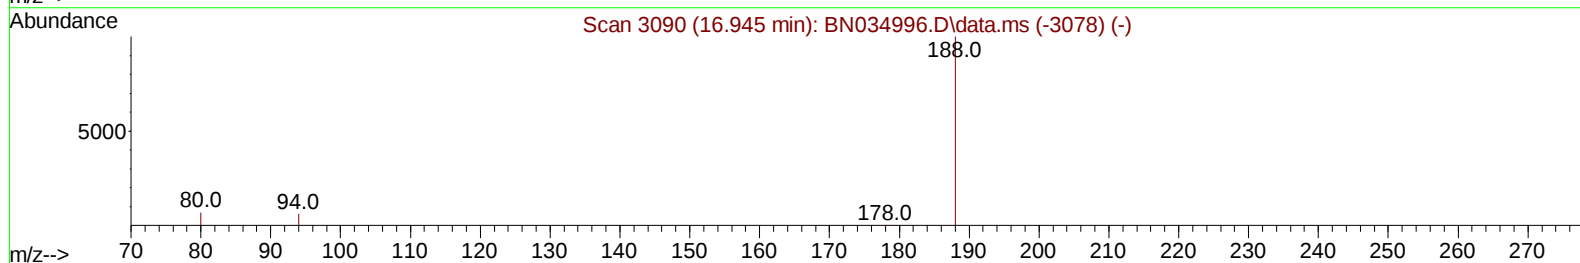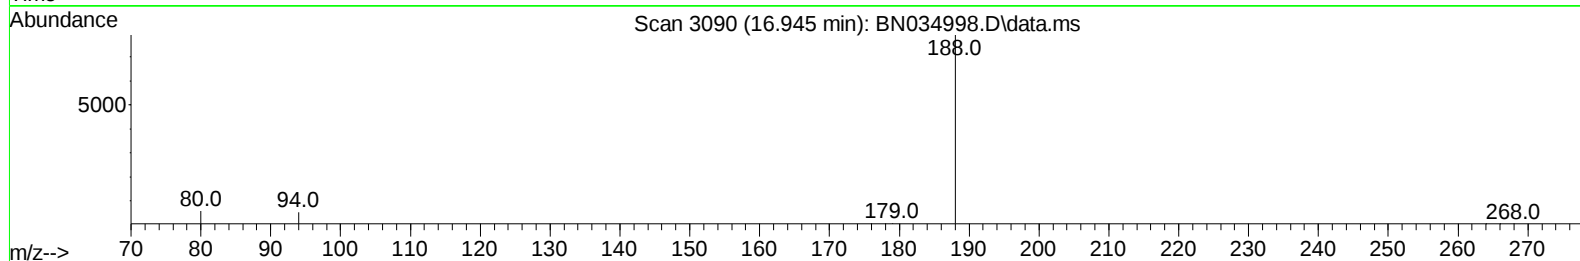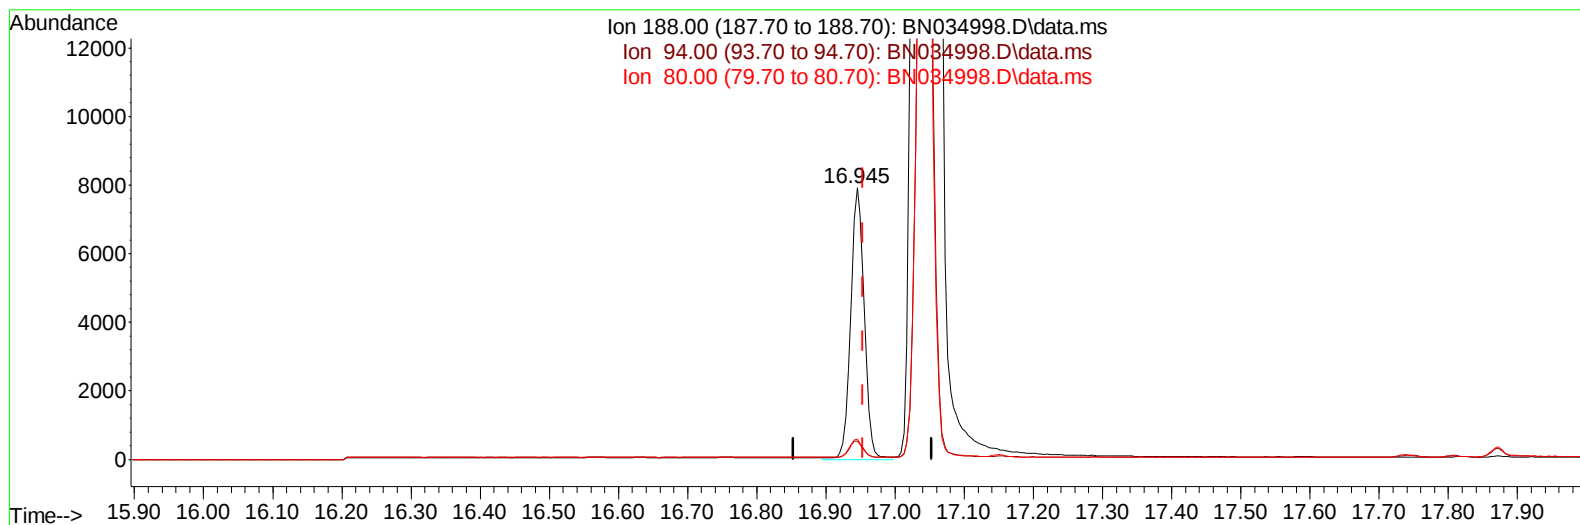

TIC: BN034998.D\data.ms

(13) Phenanthrene-d10 (I)

16.945min (-0.008) 0.40 ng/u1 m

response 10763

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.10	6.77
80.00	7.00	7.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

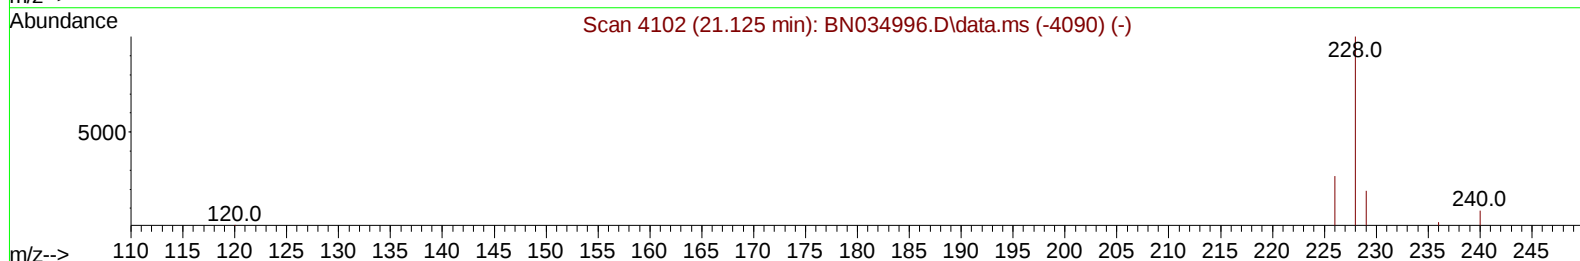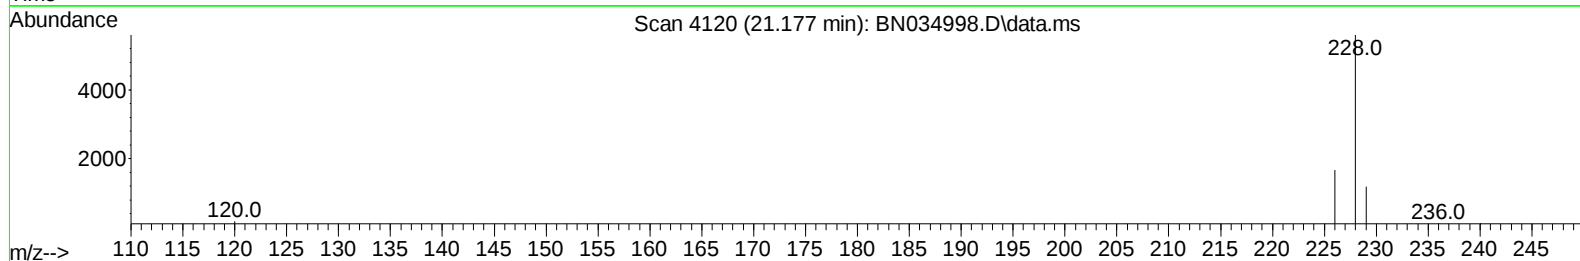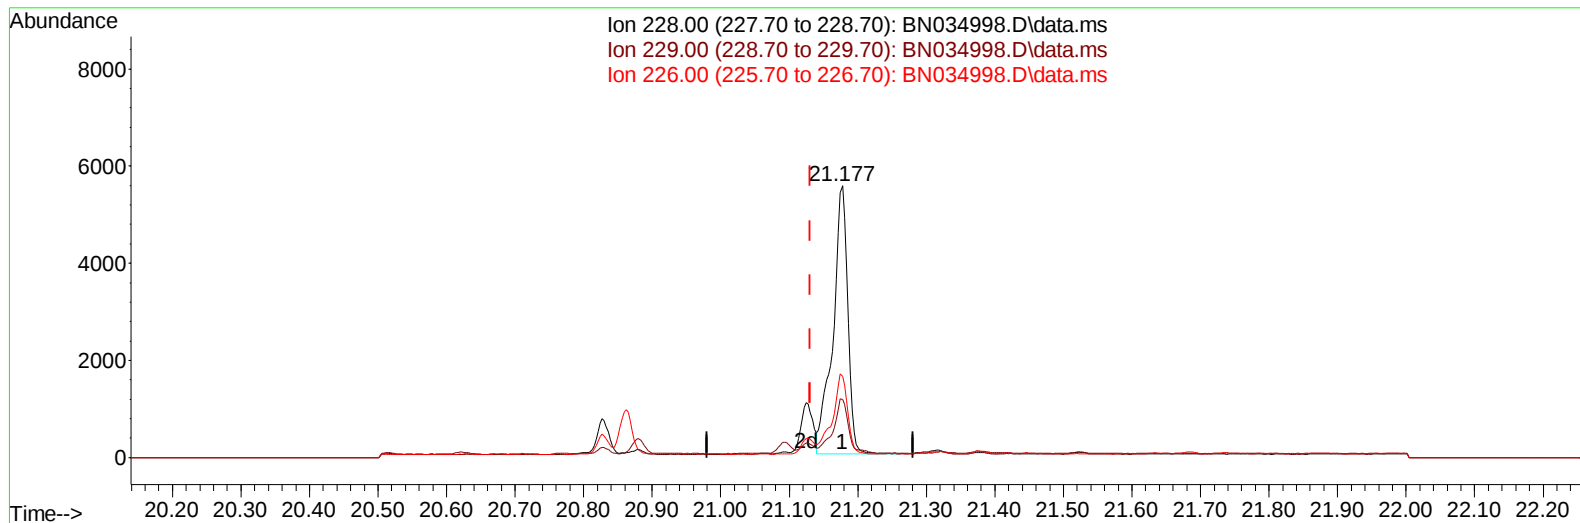

TIC: BN034998.D\data.ms

(21) Benzo(a)anthracene

21.177min (+ 0.047) 0.23 ng/u1

response 8259

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.80	21.28
226.00	27.70	29.92
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

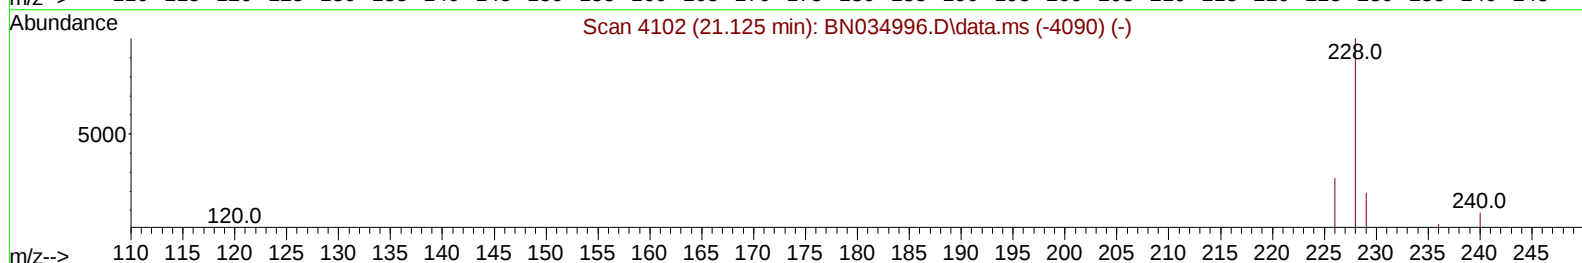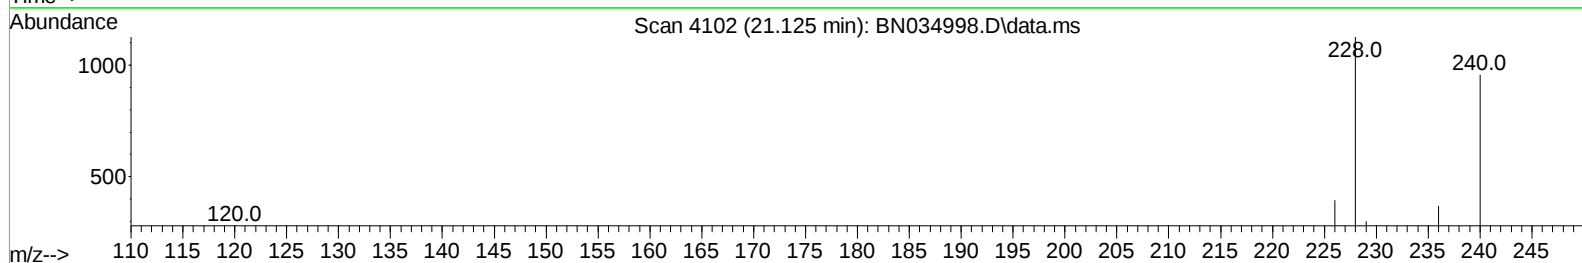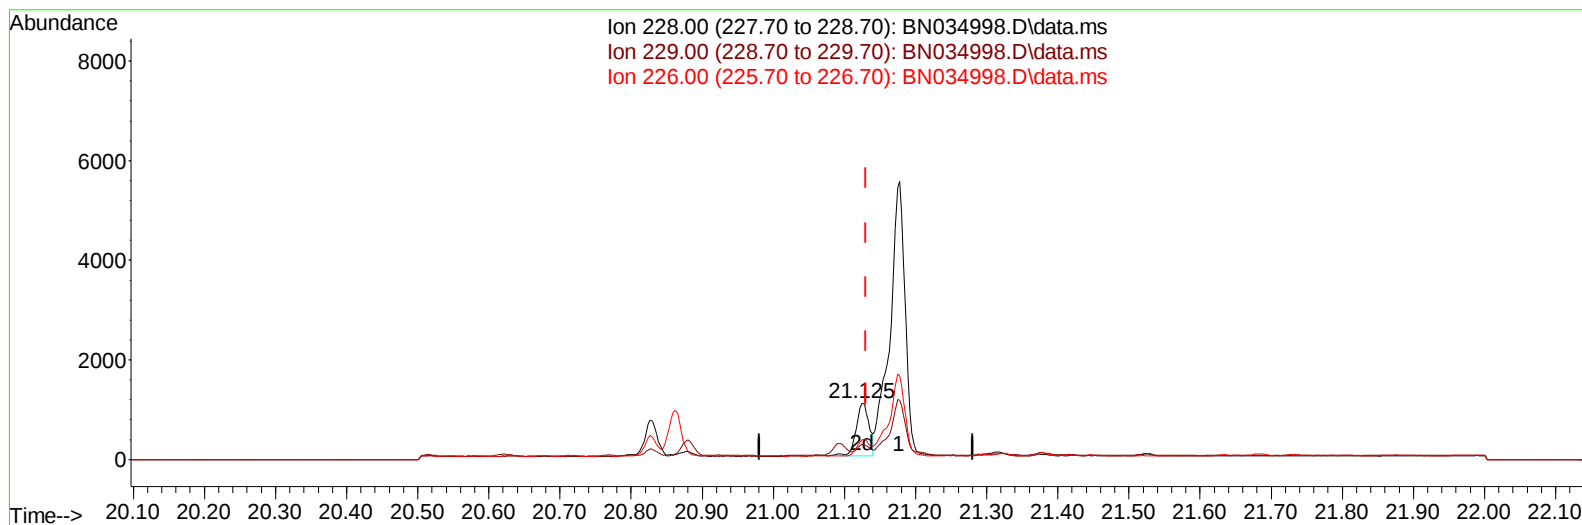

TIC: BN034998.D\data.ms

(21) Benzo(a)anthracene

21.125min (-0.006) 0.04 ng/u1 m

response 1293

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.80	26.62#
226.00	27.70	35.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

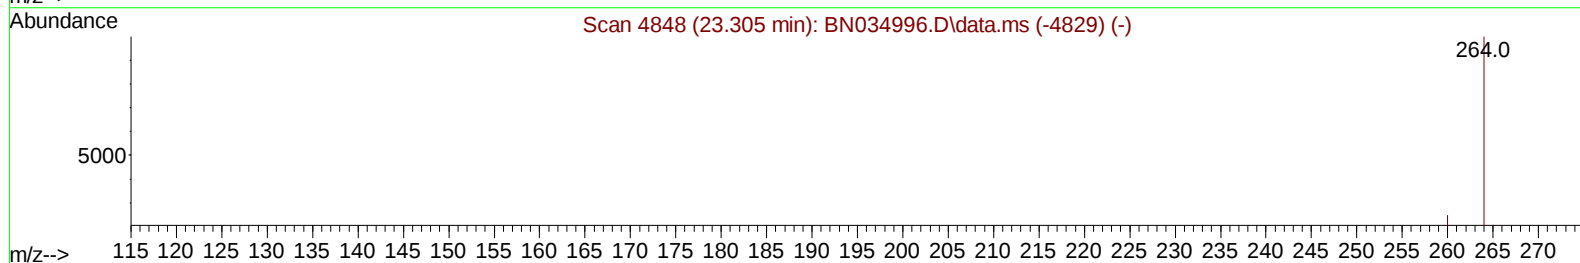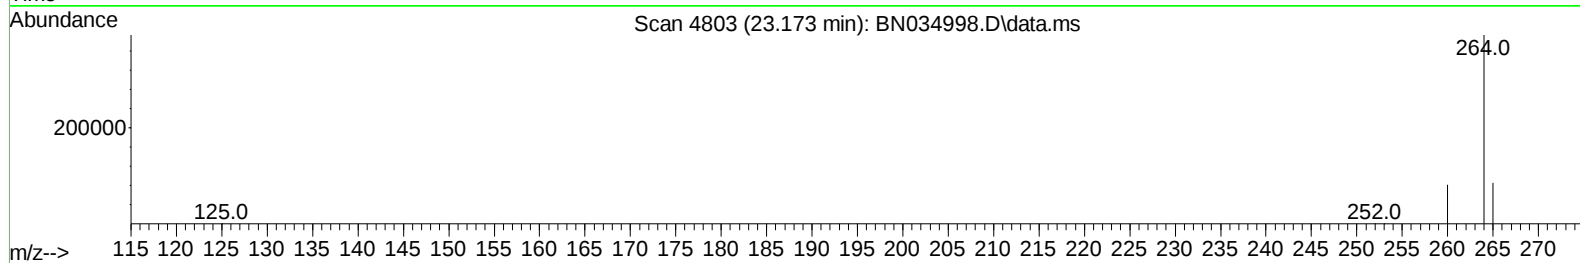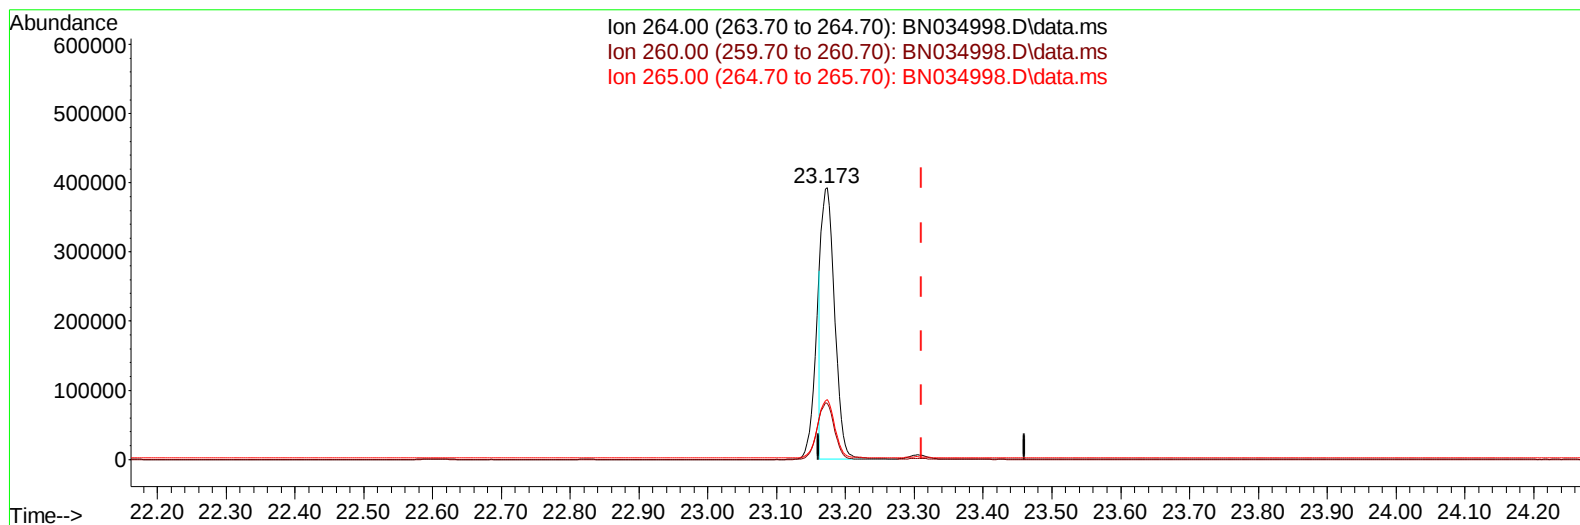

TIC: BN034998.D\data.ms

(23) Perylene-d12 (I)

23.173min (-0.137) 0.40 ng/u1

response 526879

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	20.73#
265.00	52.80	21.96#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

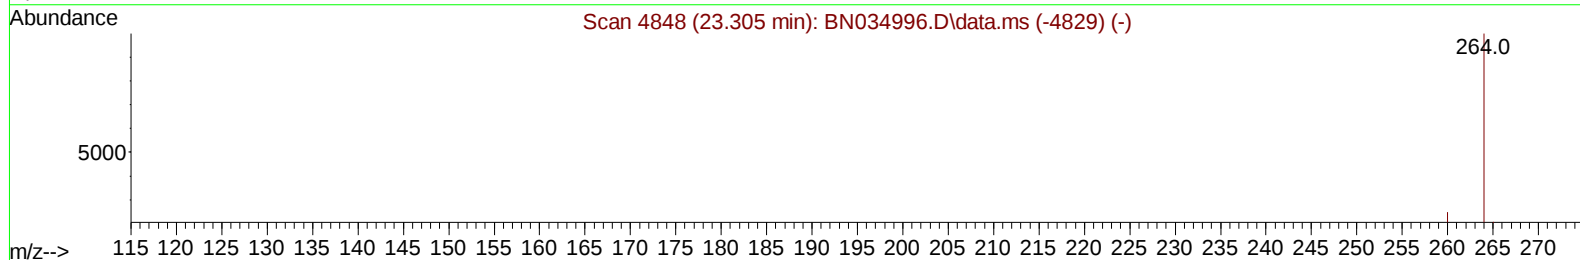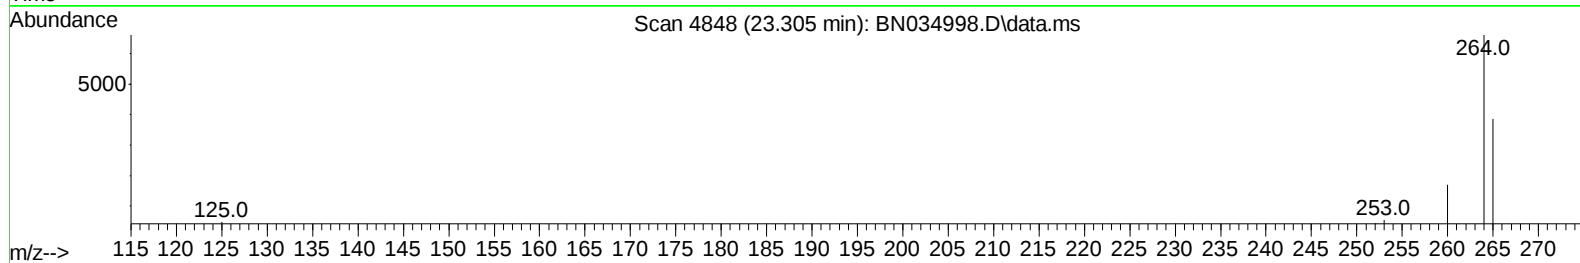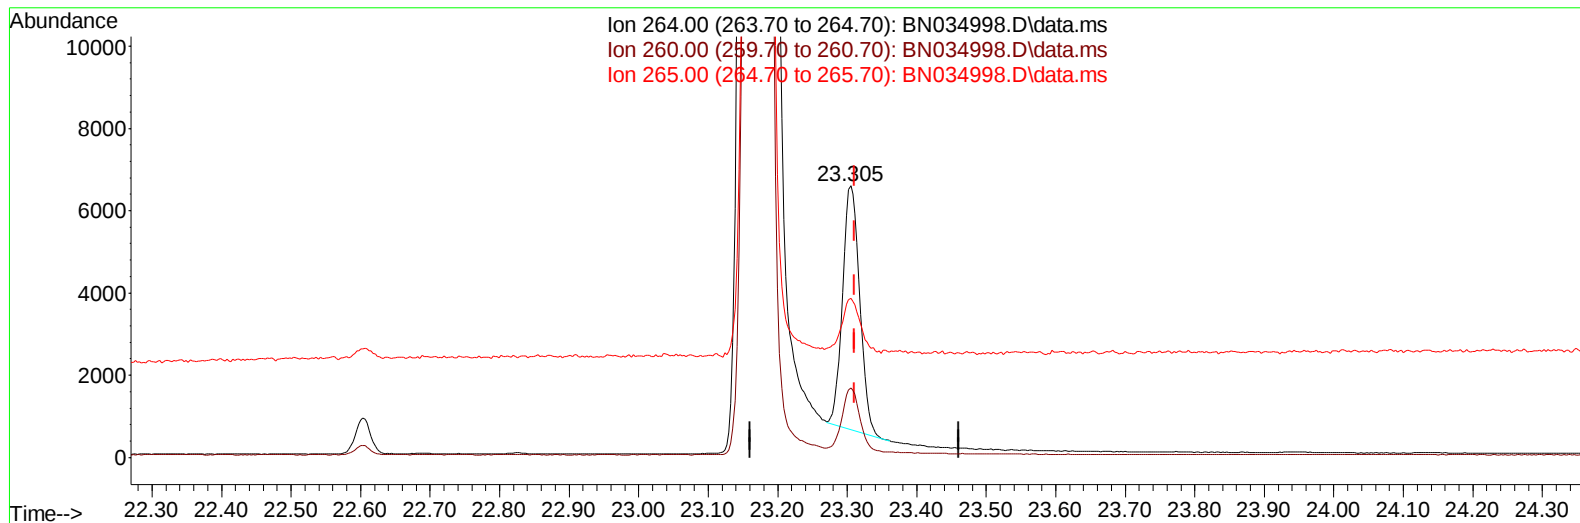

TIC: BN034998.D\data.ms

(23) Perylene-d12 (I)

23.305min (-0.006) 0.40 ng/ul m

response 10184

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	25.69
265.00	52.80	58.54
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0P17

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

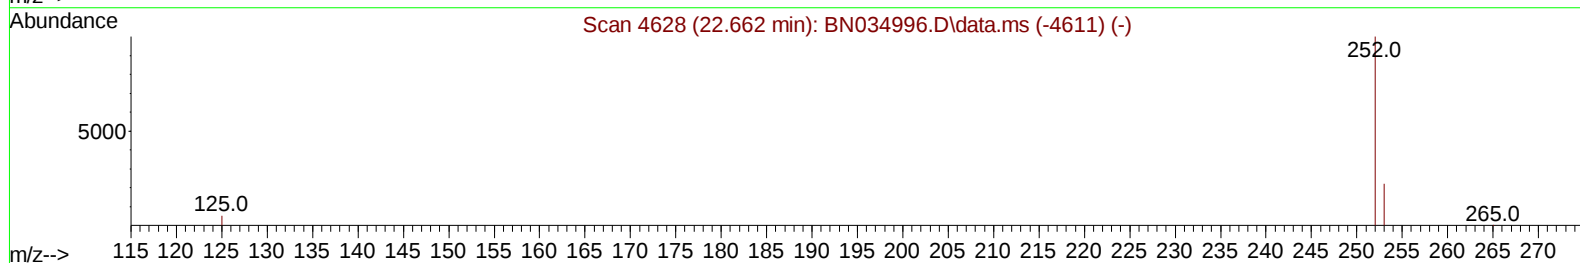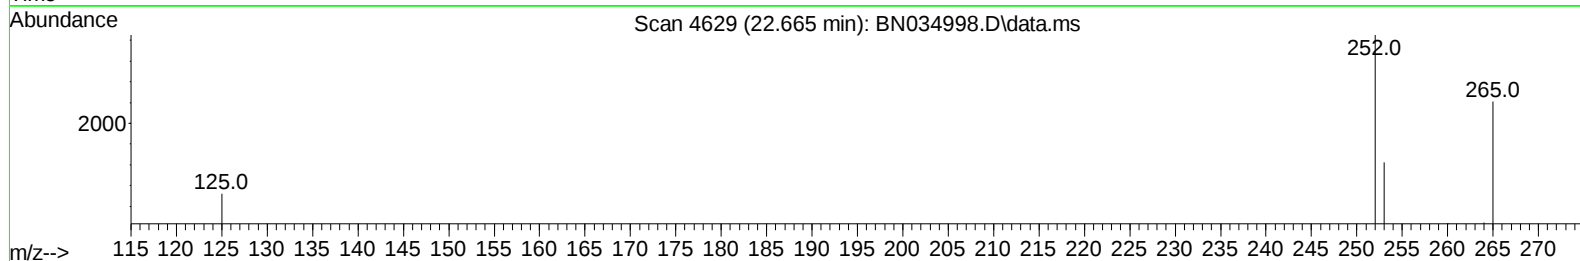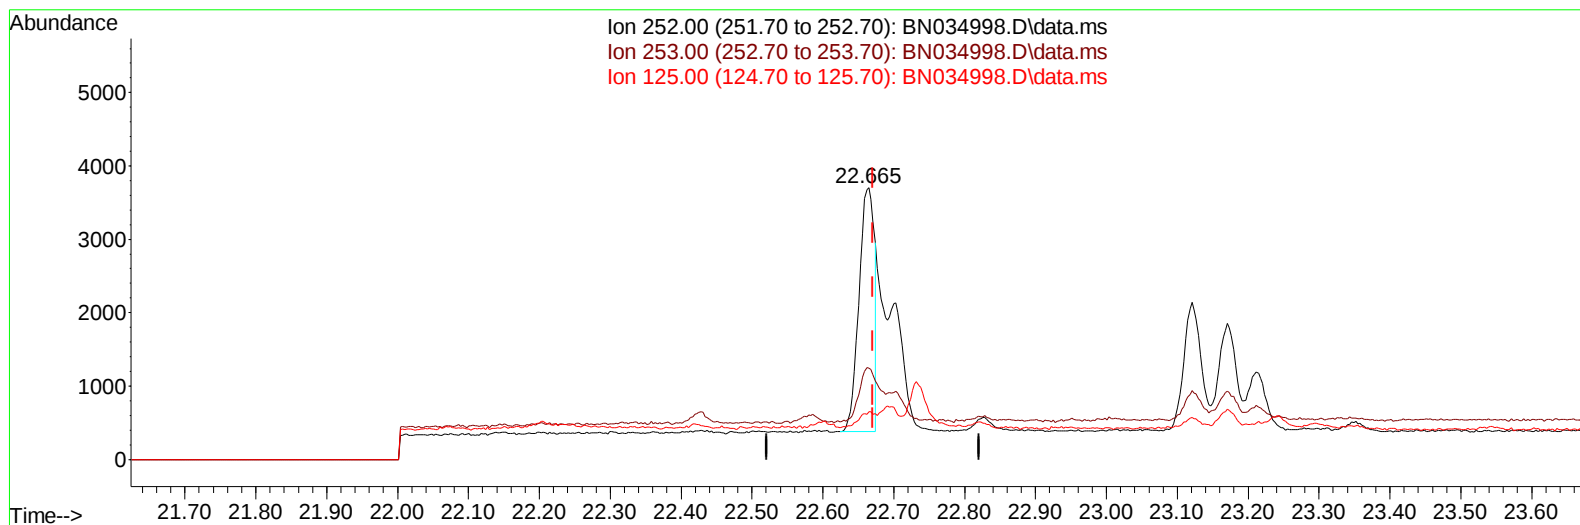

TIC: BN034998.D\data.ms

(24) Benzo(b)fluoranthene

22.665min (-0.006) 0.14 ng/u1

response 4948

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	33.68
125.00	7.00	17.54#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0P17

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

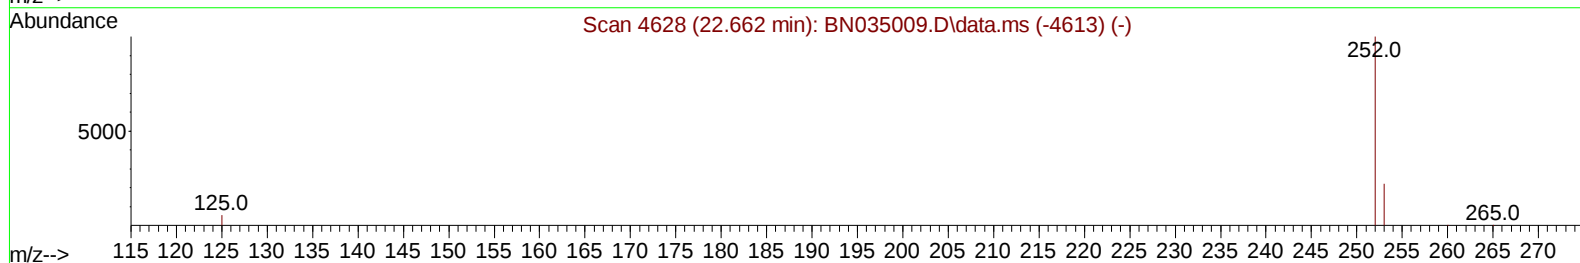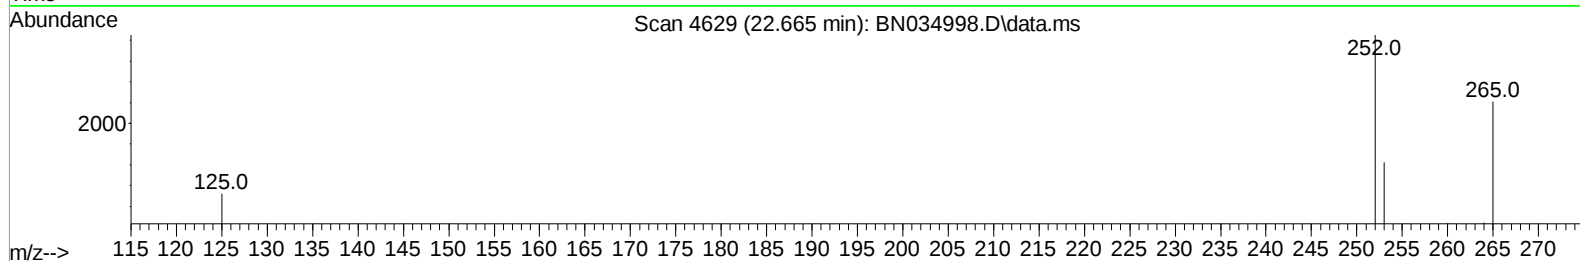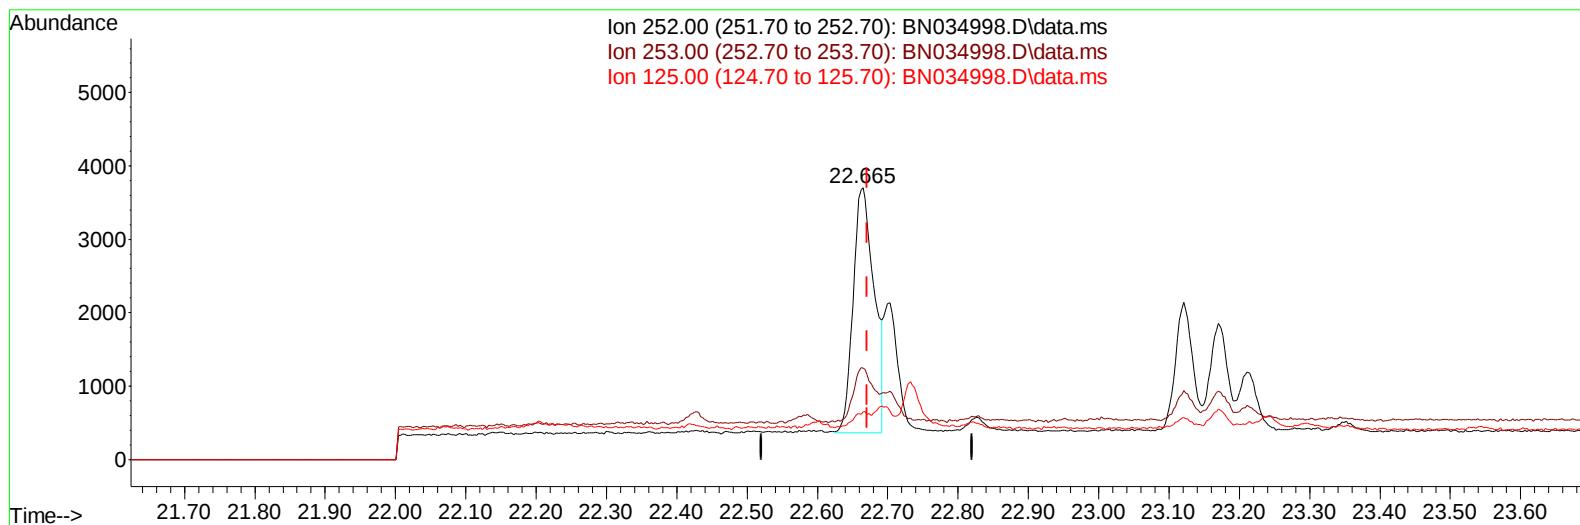

TIC: BN034998.D\data.ms

(24) Benzo(b)fluoranthene

22.665min (-0.006) 0.19 ng/u1 m

response 6901

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	33.68
125.00	7.00	17.54#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0P17

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

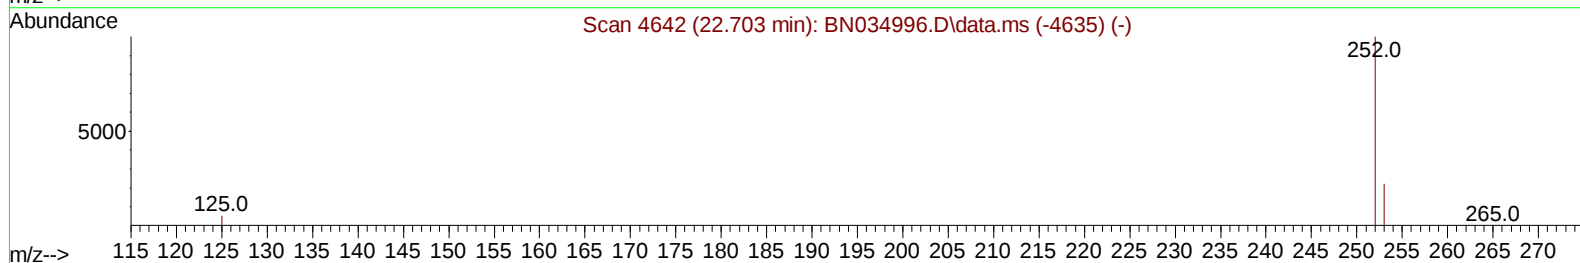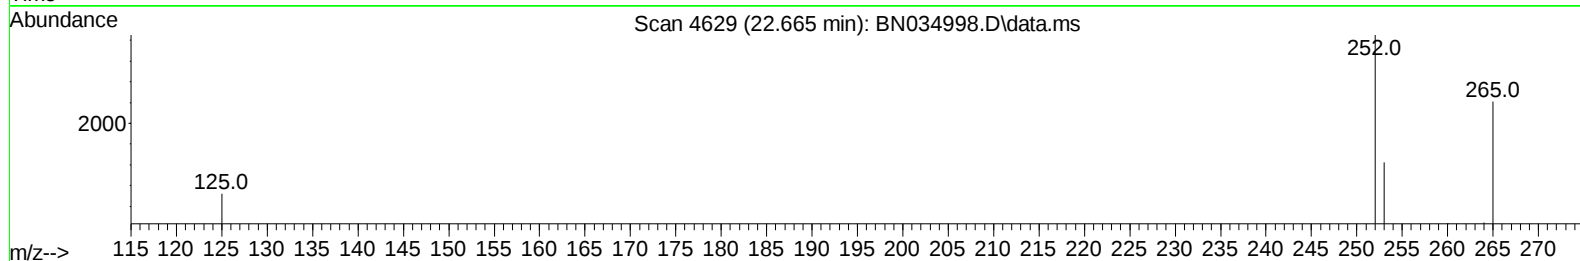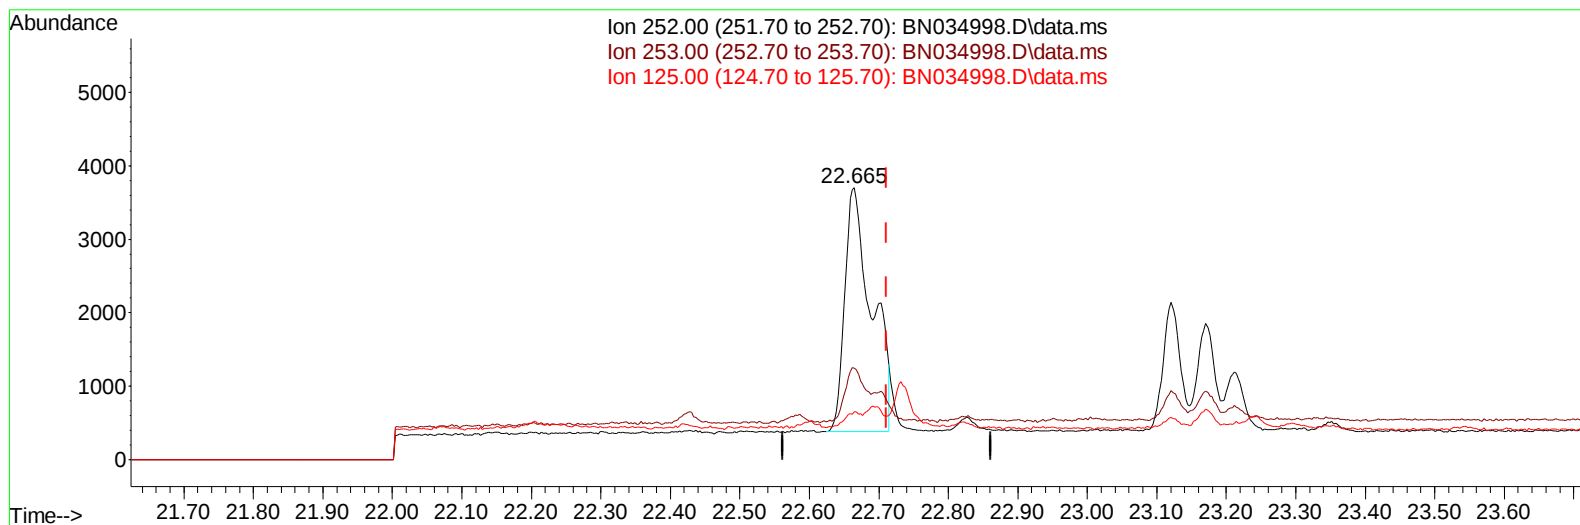

TIC: BN034998.D\data.ms

(25) Benzo(k)fluoranthene

22.665min (-0.047) 0.24 ng/u1

response 8926

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.30	33.68#
125.00	7.30	17.54#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

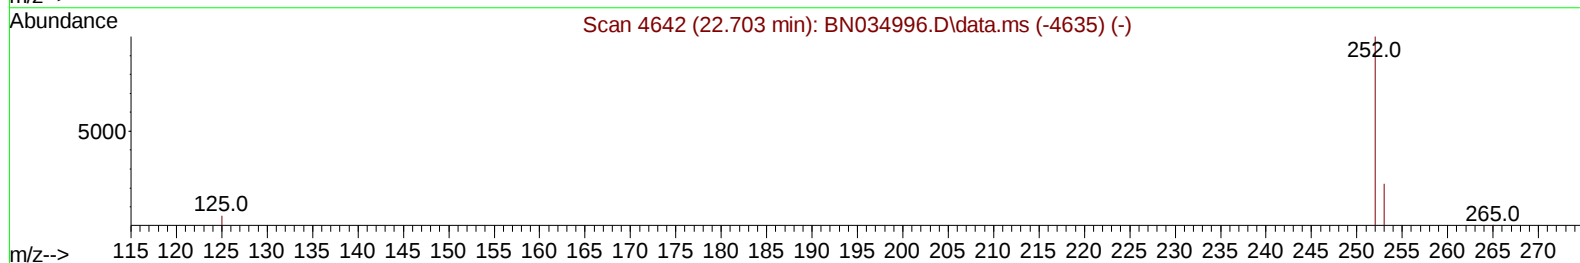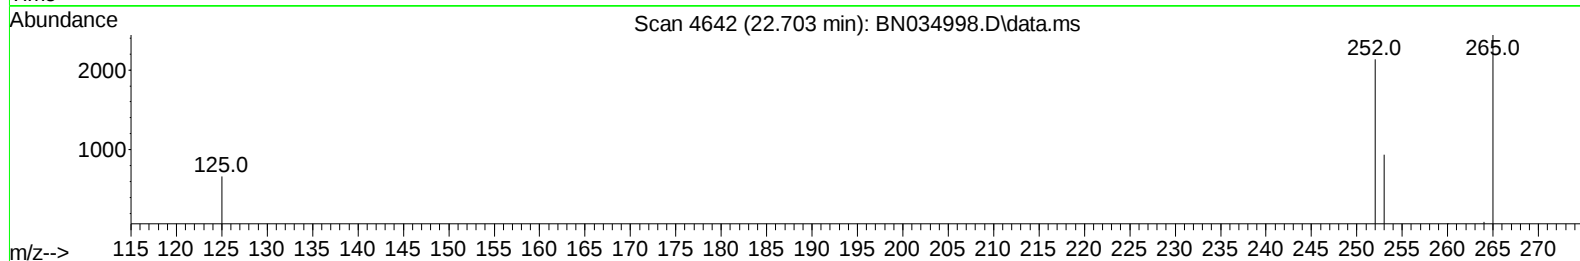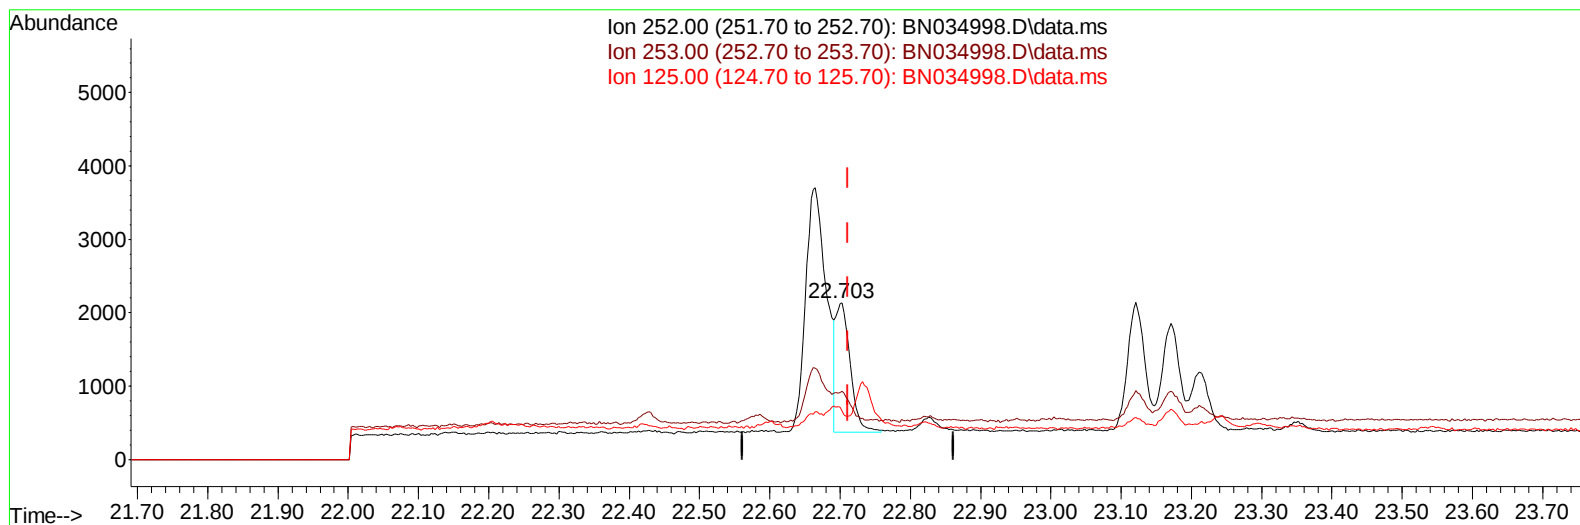

TIC: BN034998.D\data.ms

(25) Benzo(k)fluoranthene

22.703min (-0.009) 0.07 ng/u1 m

response 2512

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.30	43.71#
125.00	7.30	31.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

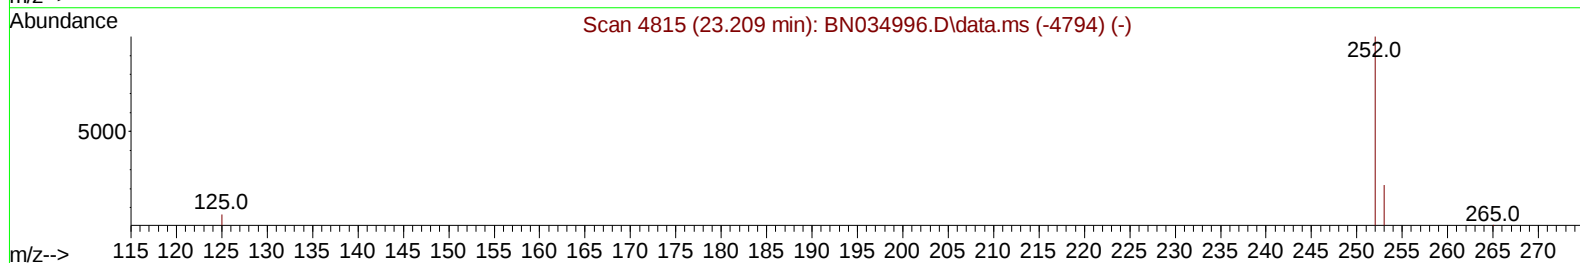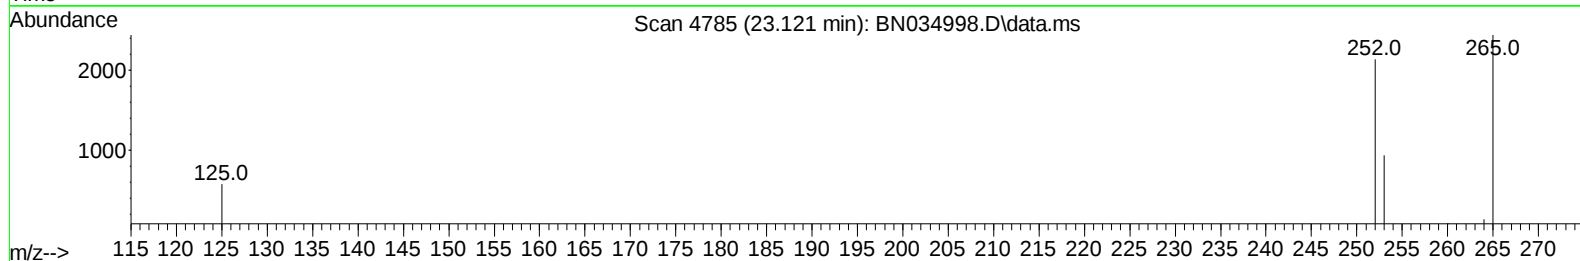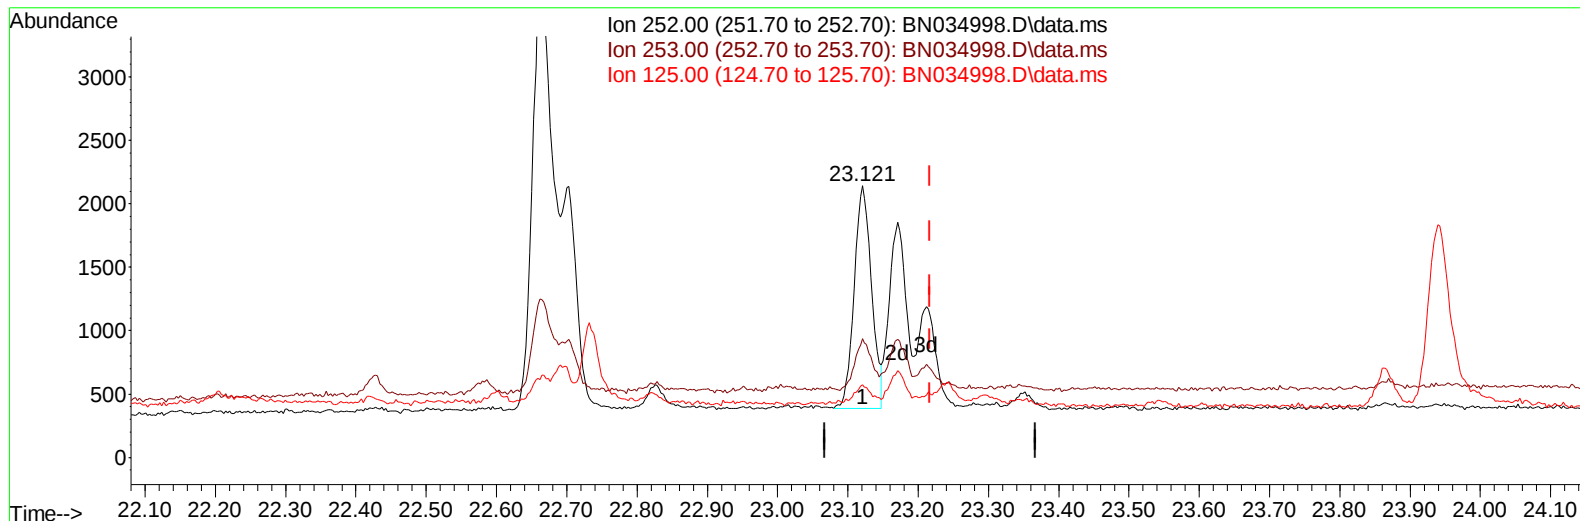

TIC: BN034998.D\data.ms

(26) Benzo(a)pyrene (C)

23.121min (-0.096) 0.09 ng/u1

response 3015

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	43.86#
125.00	7.90	26.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

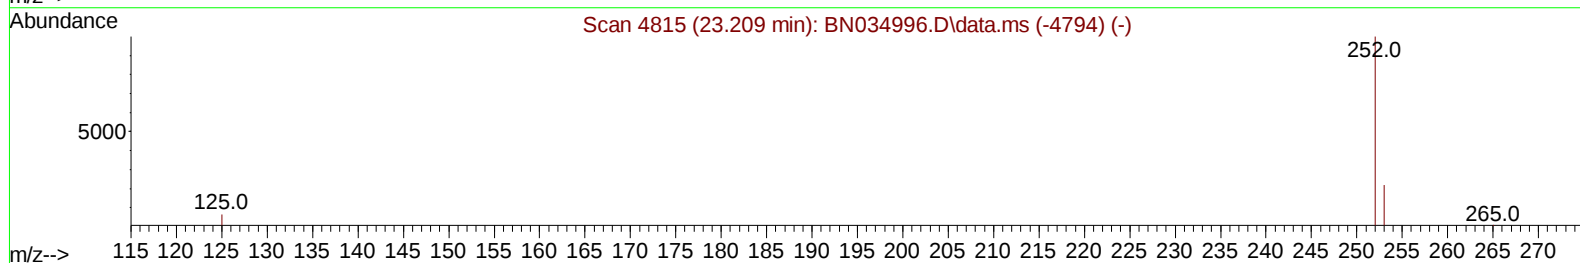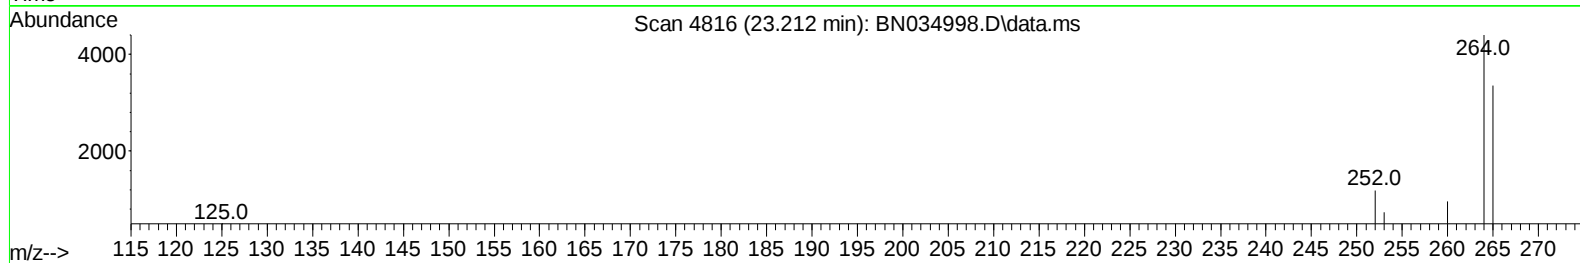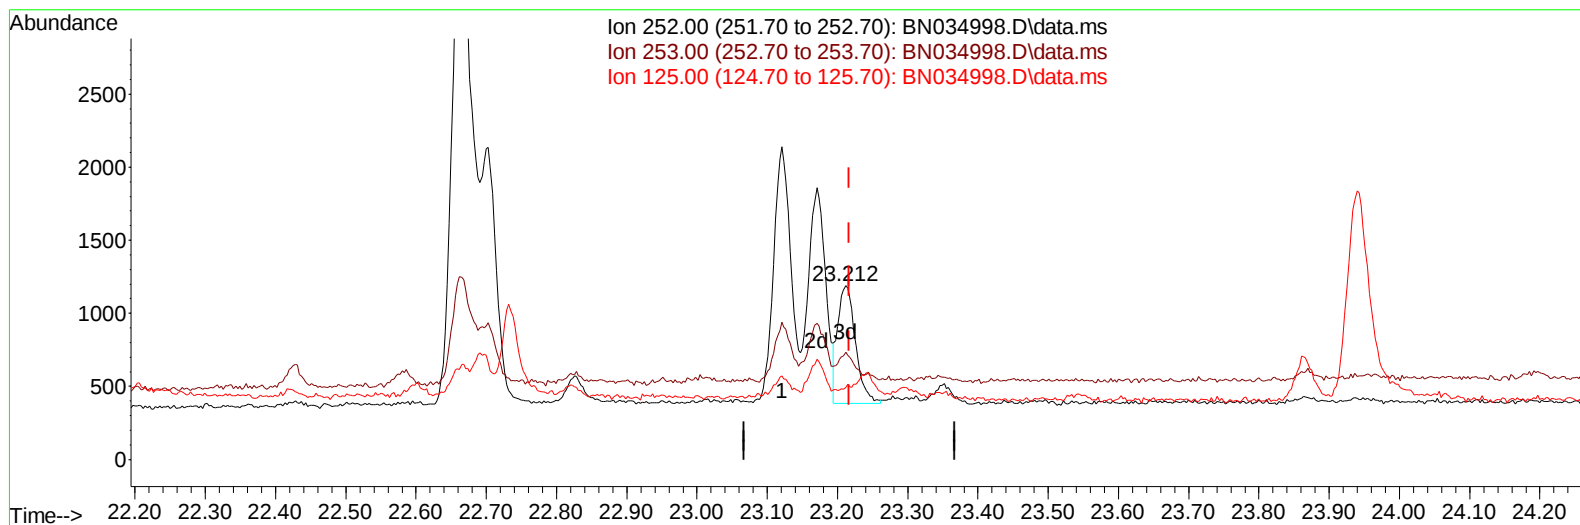

TIC: BN034998.D\data.ms

(26) Benzo(a)pyrene (C)

23.212min (-0.006) 0.04 ng/u1 m

response 1423

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	61.90#
125.00	7.90	41.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0P17

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

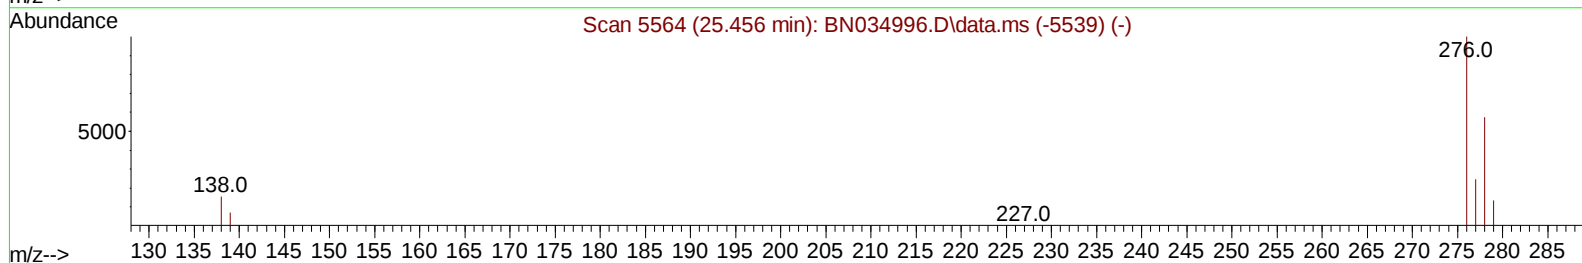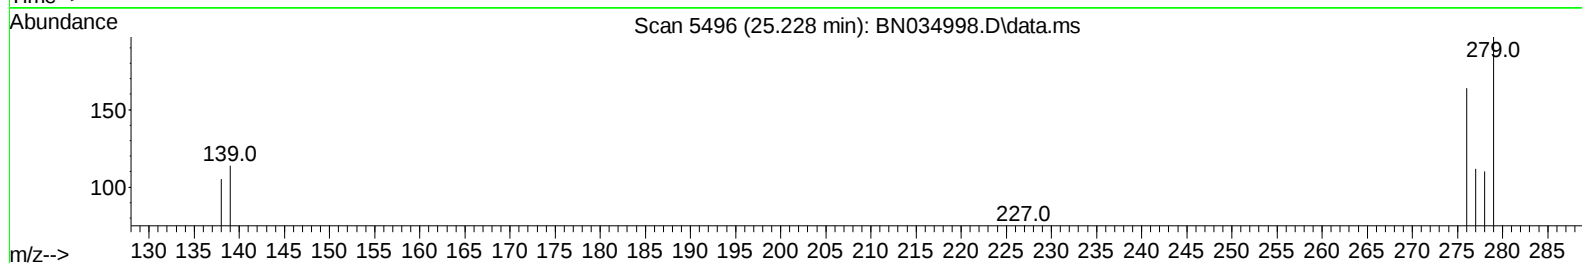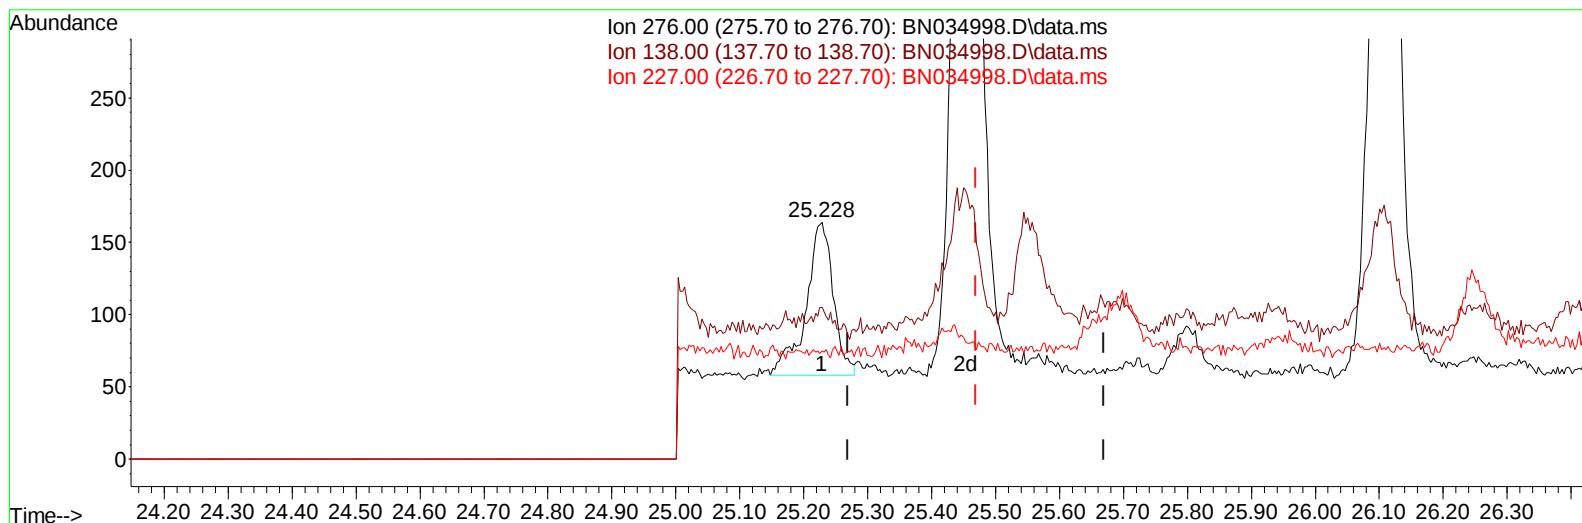

TIC: BN034998.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.228min (-0.241) 0.01 ng/u1

response 315

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	13.50	8.89#
227.00	0.30	0.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

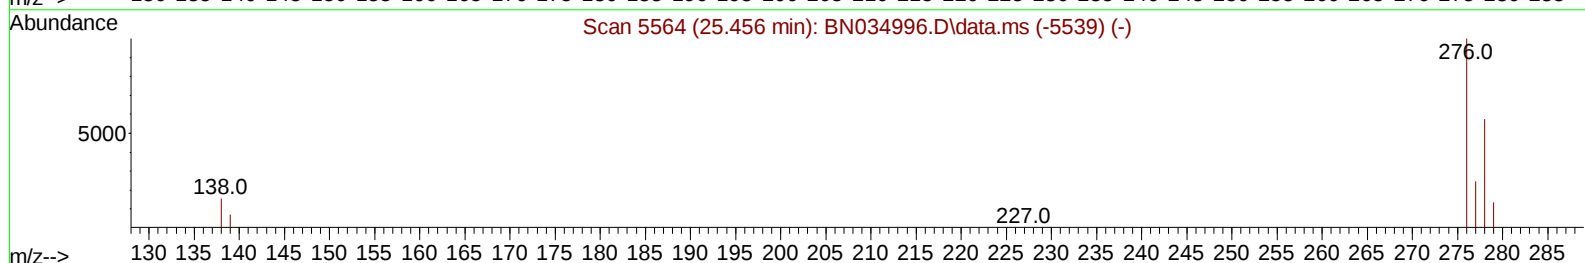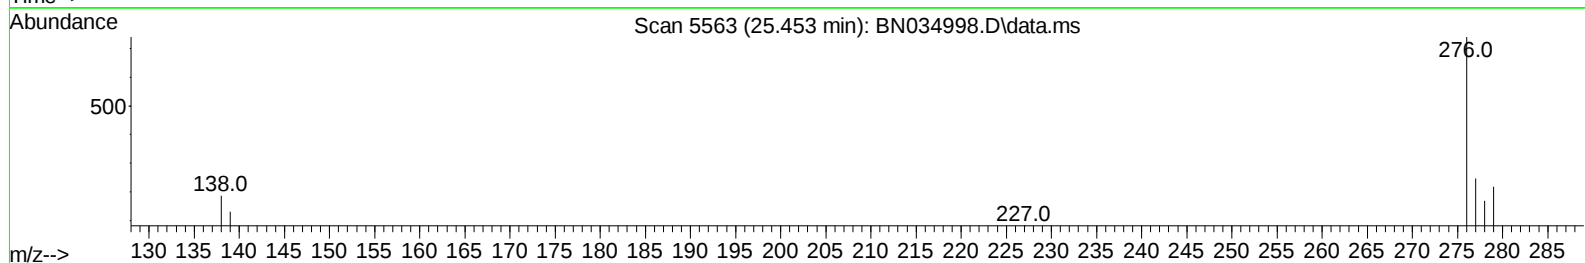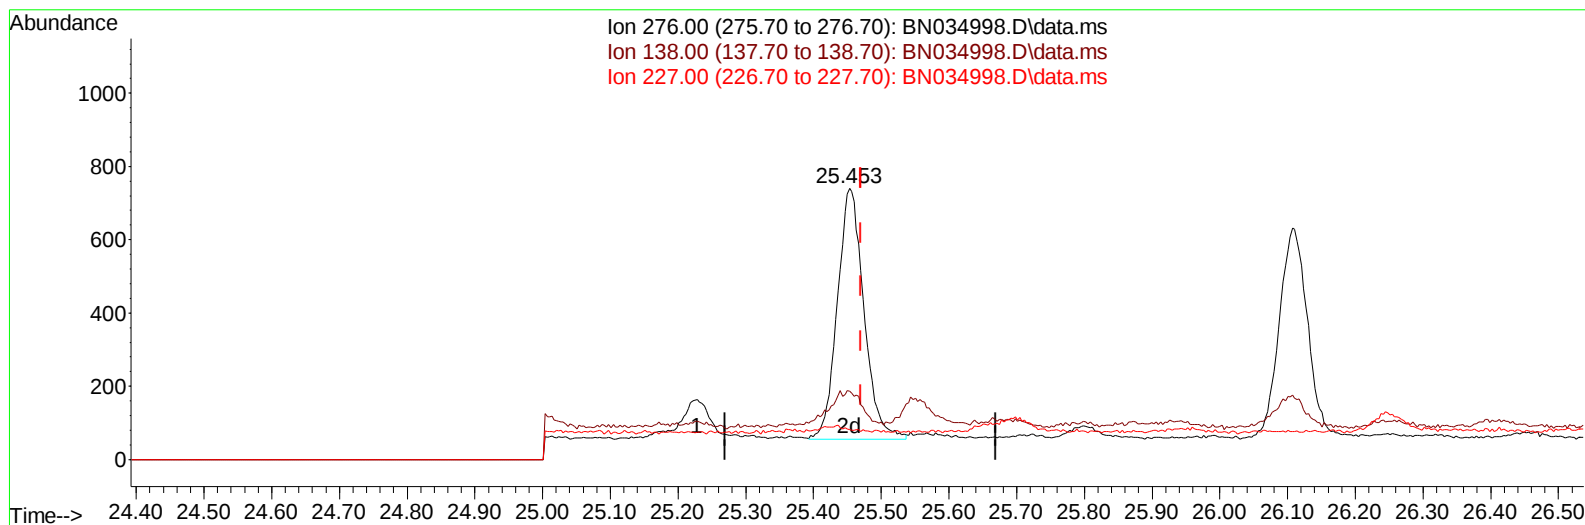

TIC: BN034998.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.453min (-0.017) 0.05 ng/u1 m

response 1862

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	13.50	1.50#
227.00	0.30	0.11#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0P17

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

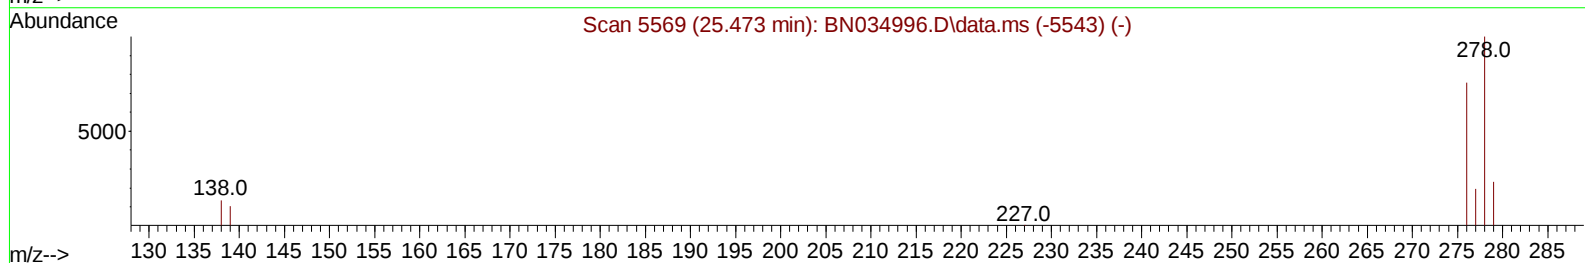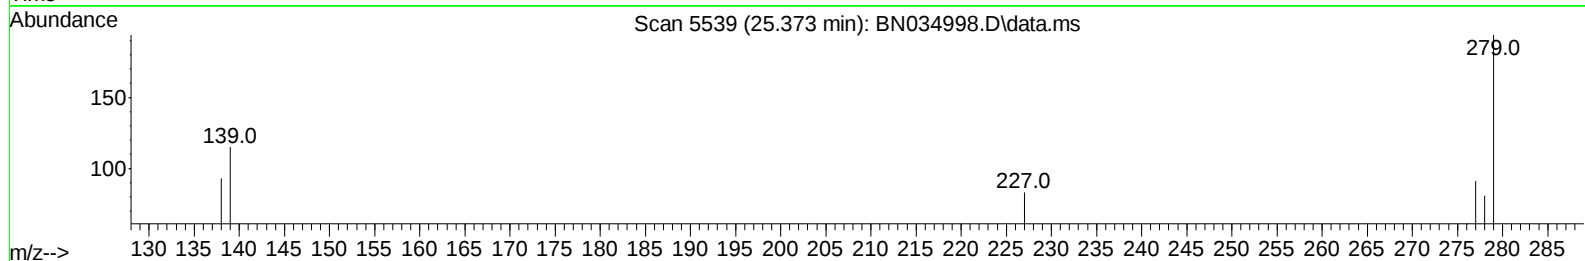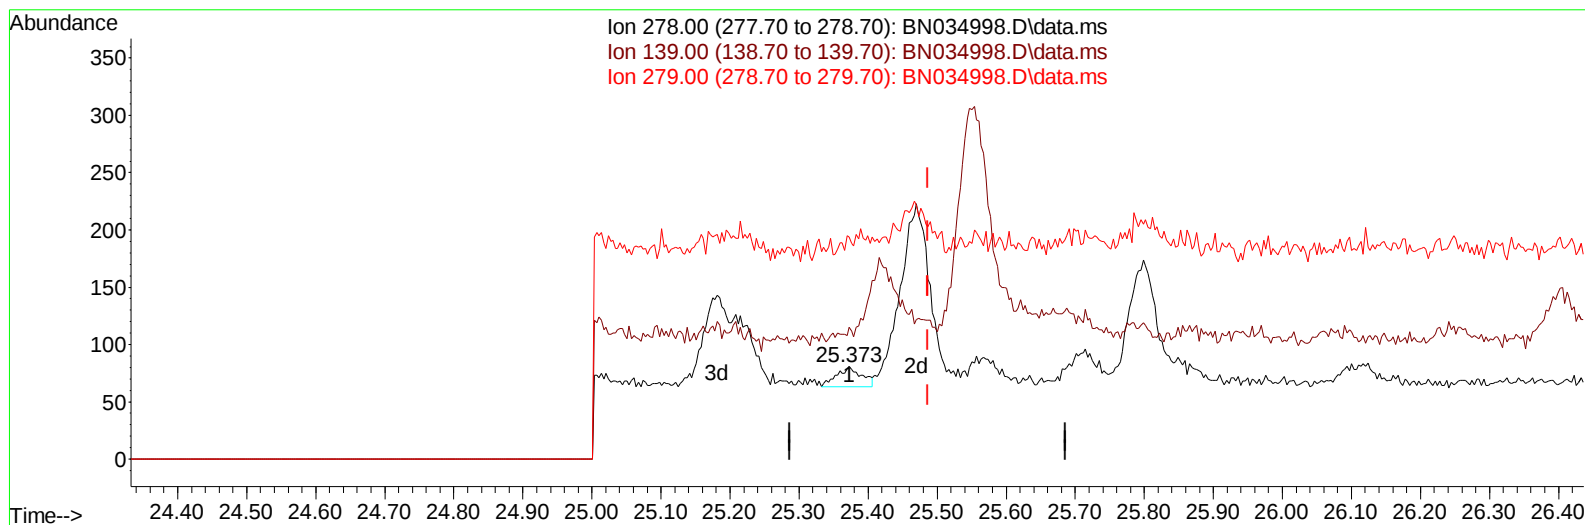

TIC: BN034998.D\data.ms

(28) Dibenzo(a,h)anthracene

25.373min (-0.114) 0.00 ng/u1

response 45

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	10.50	141.98#
279.00	26.90	239.51#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0P17

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

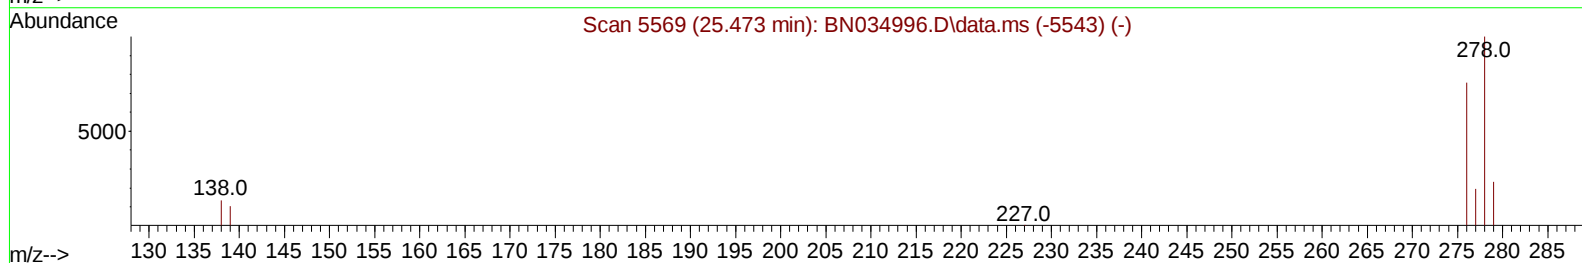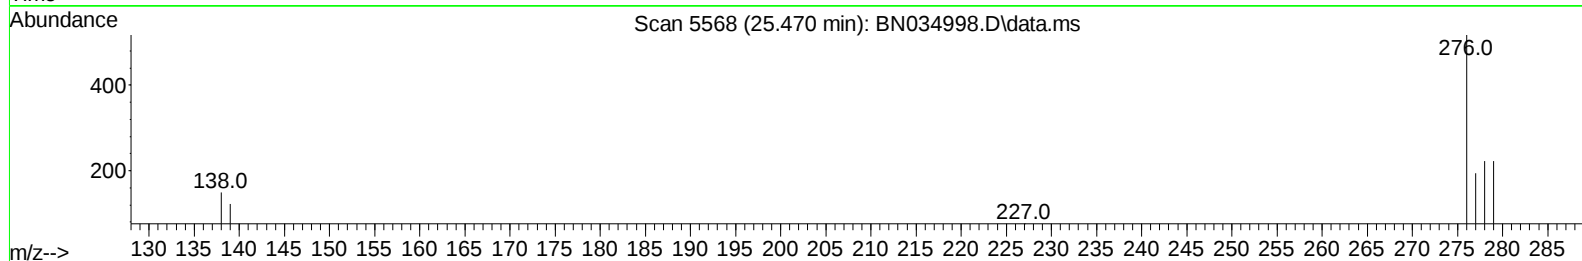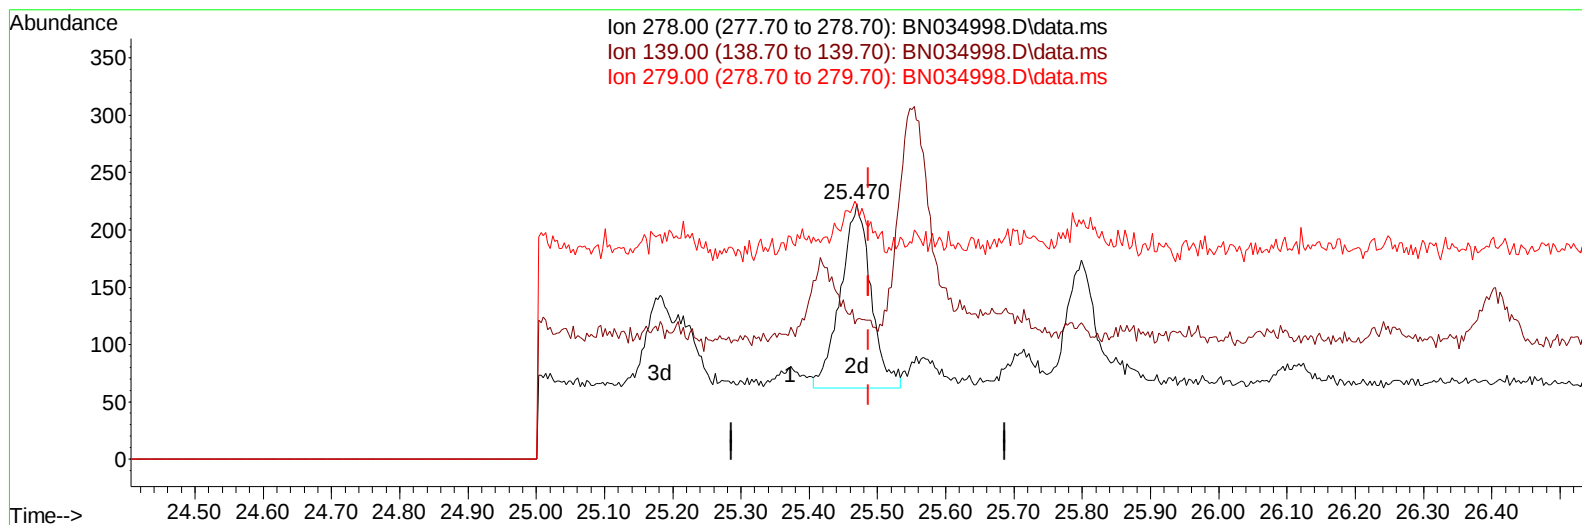

TIC: BN034998.D\data.ms

(28) Dibenzo(a,h)anthracene

25.470min (-0.017) 0.02 ng/u1 m

response 498

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	10.50	54.71#
279.00	26.90	99.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0P17

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

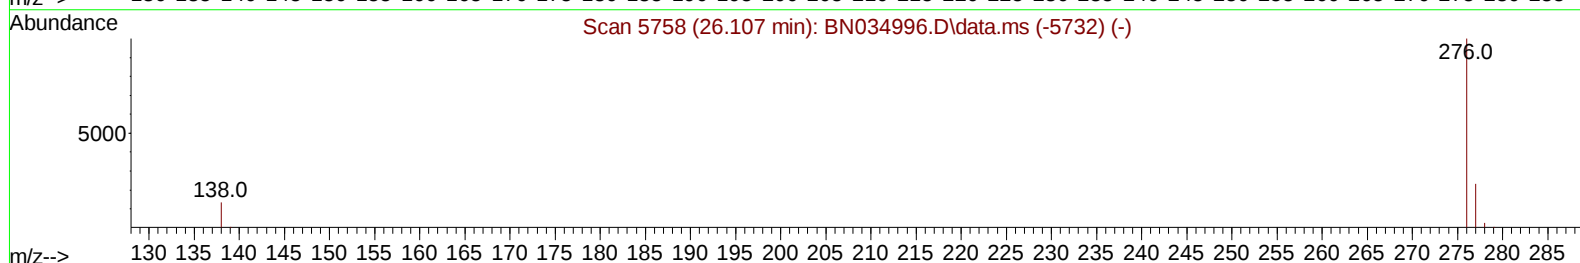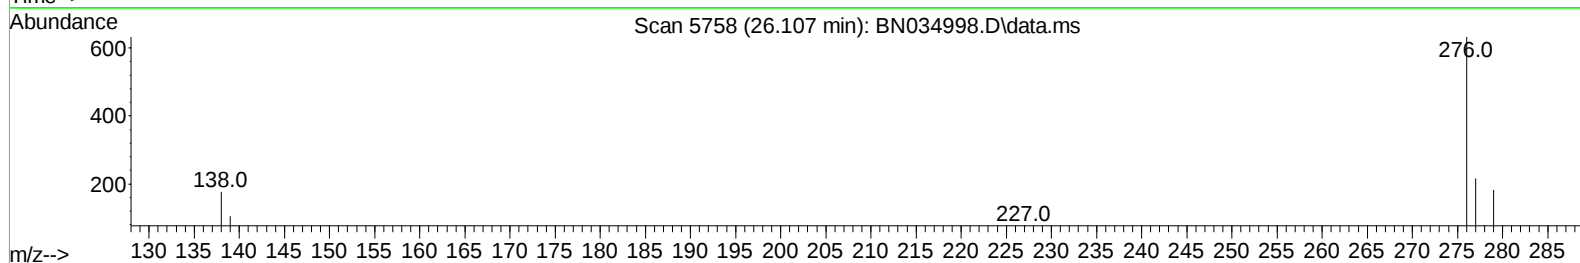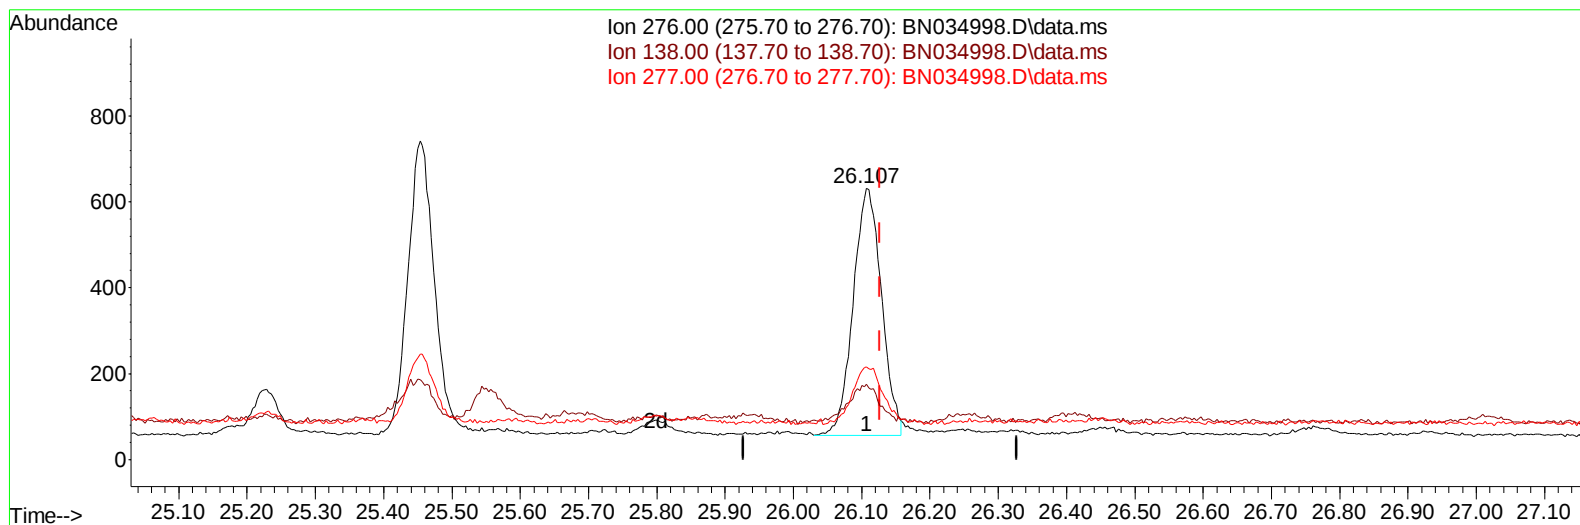

TIC: BN034998.D\data.ms

(29) Benzo(g,h,i)perylene

26.107min (-0.020) 0.06 ng/u1

response 1657

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.90	27.85#
277.00	25.20	34.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN034998.D
 Acq On : 11 Nov 2024 11:00
 Operator : RC/JU
 Sample : P4636-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0P17

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

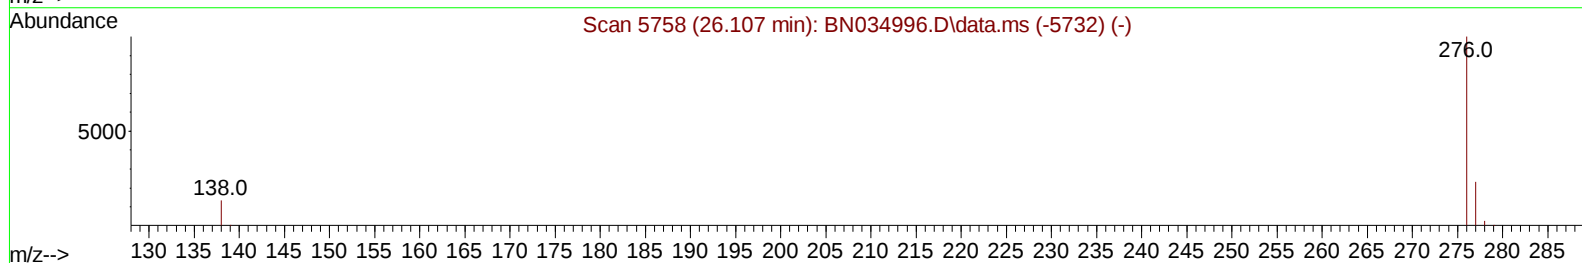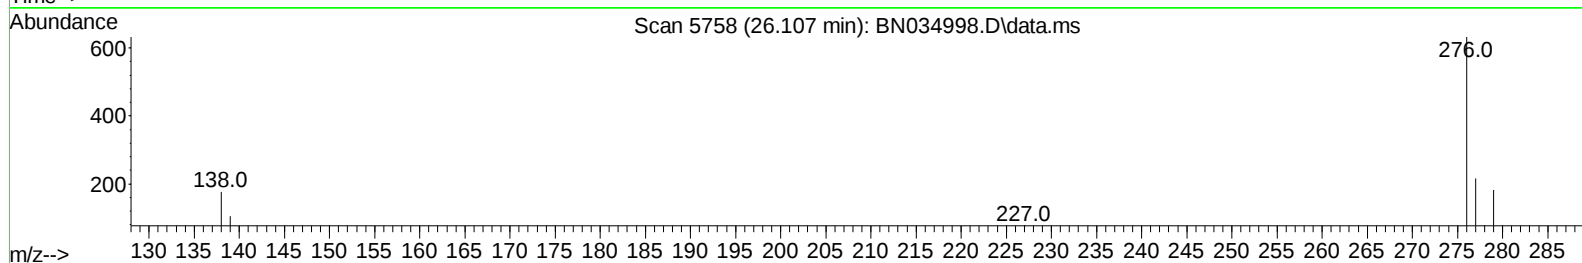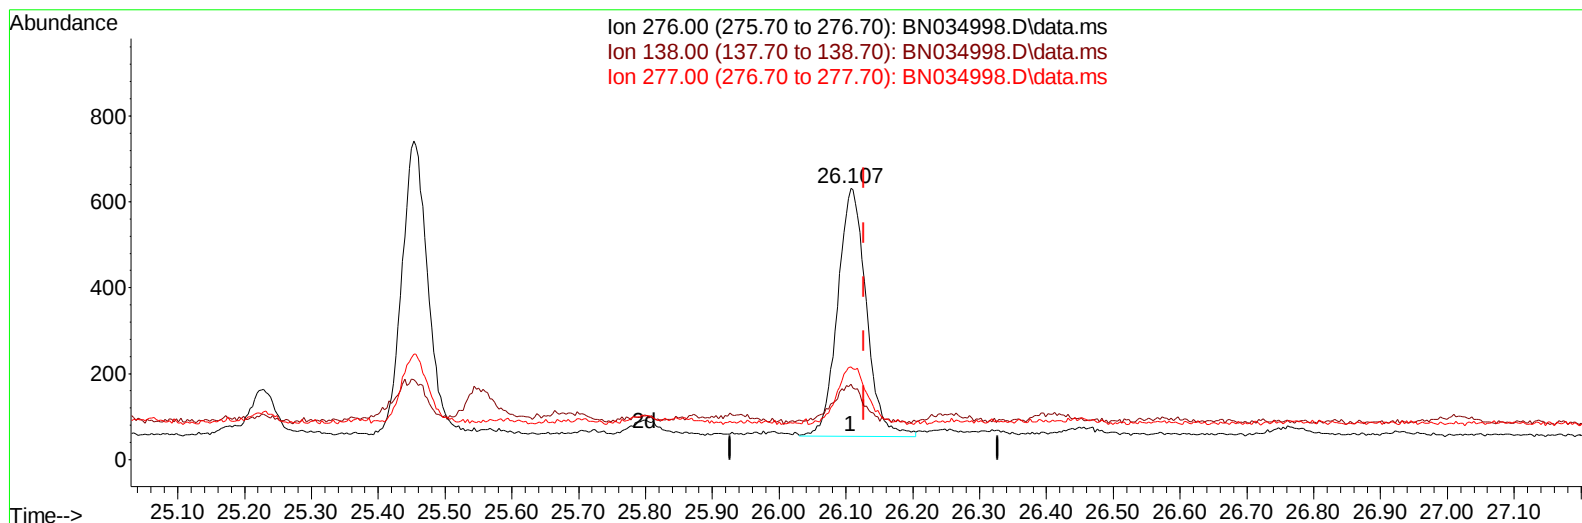

TIC: BN034998.D\data.ms

(29) Benzo(g,h,i)perylene

26.107min (-0.020) 0.06 ng/ul m

response 1713

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.90	27.85#
277.00	25.20	34.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN034998.D
 Acq On : 11 Nov 2024 11:00
 Operator : RC/JU
 Sample : P4636-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0P17

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 11 11:42:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.562	152		2659	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.328	136		6643	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.199	164		4667	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.945	188		10763m	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240		9992	0.400	ng/ul	# 0.00
23) Perylene-d12	23.305	264		10184m	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.149	96		9958	3.936	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152		2553	0.251	ng/ul	-0.01
18) Fluoranthene-d10	18.977	212		7119	0.277	ng/ul	0.00
Target Compounds							
							Qvalue
15) Phenanthrene	16.987	178		13672	0.475	ng/ul	99
16) Anthracene	17.080	178		564	0.021	ng/ul#	71
19) Fluoranthene	19.009	202		29488	0.883	ng/ul	97
20) Pyrene	19.372	202		20382	0.589	ng/ul#	96
21) Benzo(a)anthracene	21.125	228		1293m	0.036	ng/ul	
22) Chrysene	21.177	228		8283	0.224	ng/ul	98
24) Benzo(b)fluoranthene	22.665	252		6901m	0.193	ng/ul	
25) Benzo(k)fluoranthene	22.703	252		2512m	0.067	ng/ul	
26) Benzo(a)pyrene	23.212	252		1423m	0.044	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.453	276		1862m	0.048	ng/ul	
29) Benzo(g,h,i)perylene	26.107	276		1713m	0.057	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN034998.D
Acq On : 11 Nov 2024 11:00
Operator : RC/JU
Sample : P4636-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0PI7

Manual IntegrationsAPPROVED

Quant Time: Nov 11 11:42:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

