




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

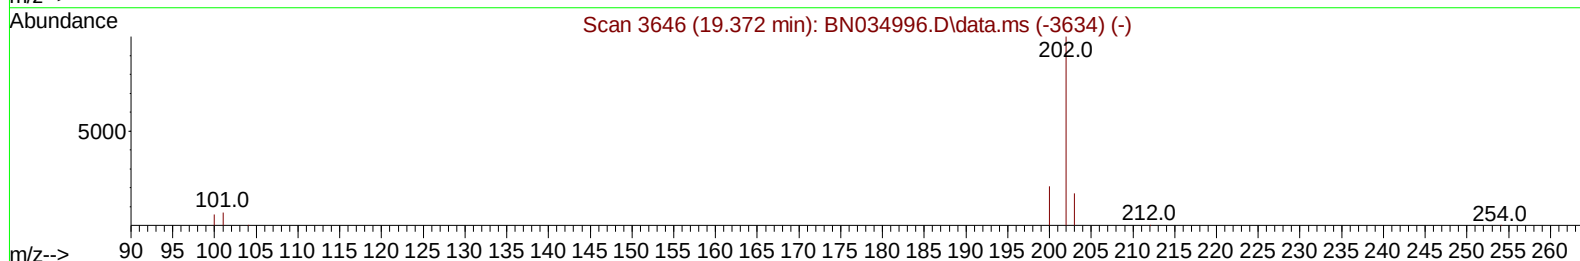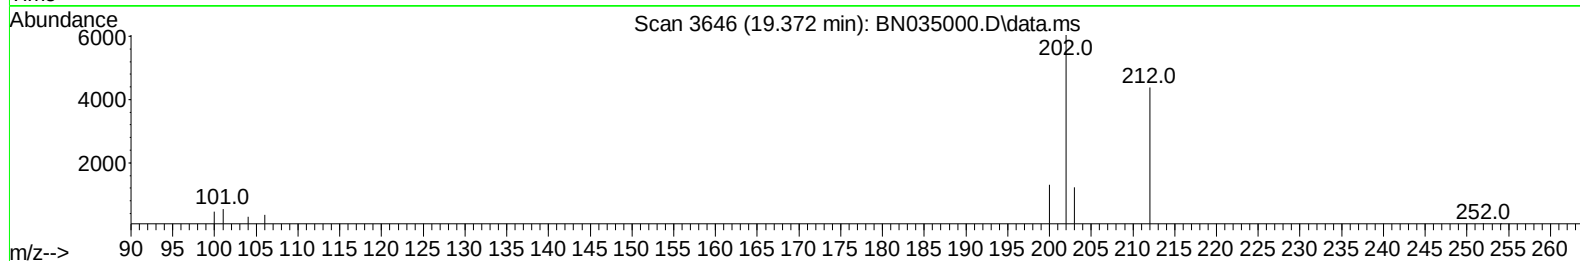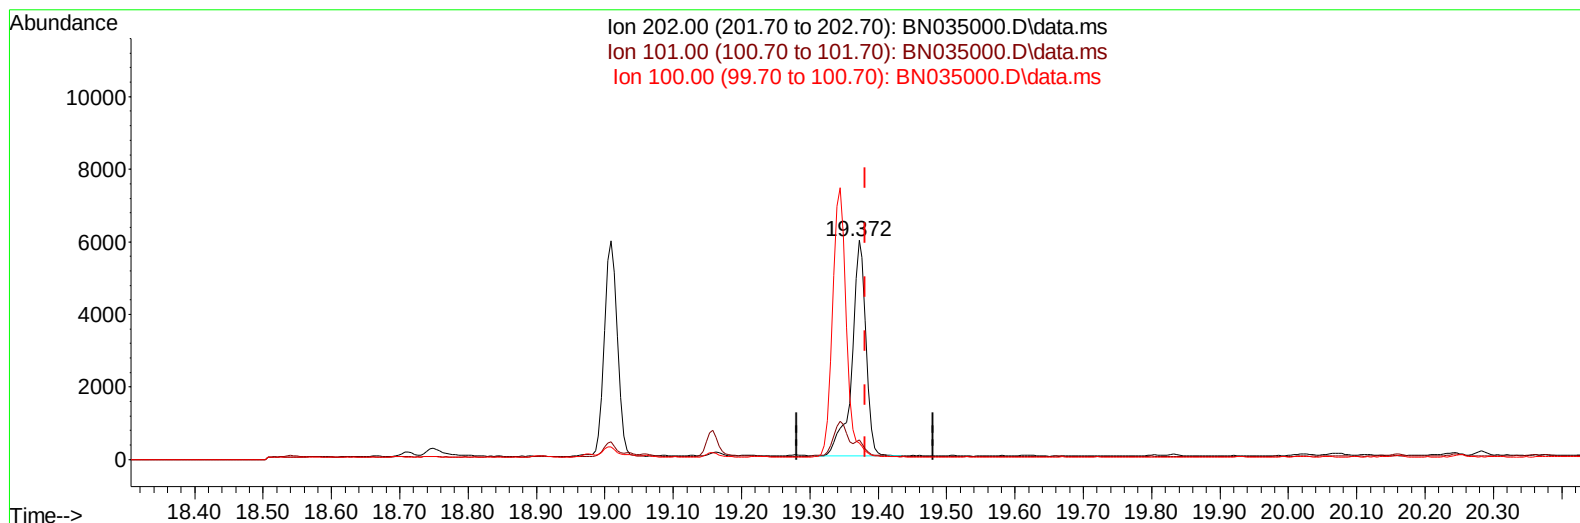

TIC: BN035000.D\data.ms

(20) Pyrene

19.372min (-0.009) 0.23 ng/u1

response 8734

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	6.20	9.01#
100.00	5.10	7.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

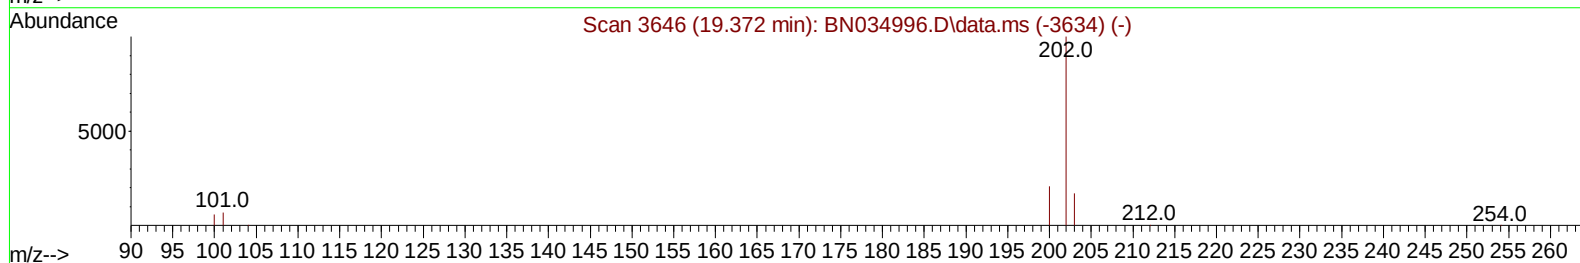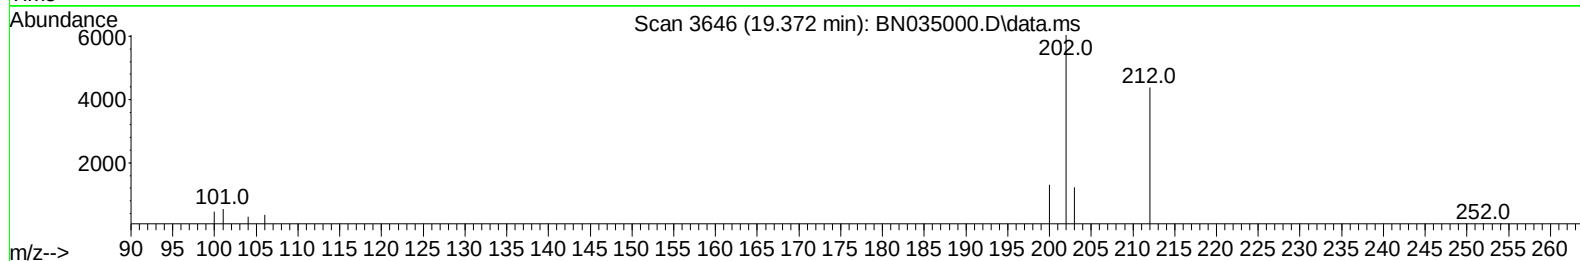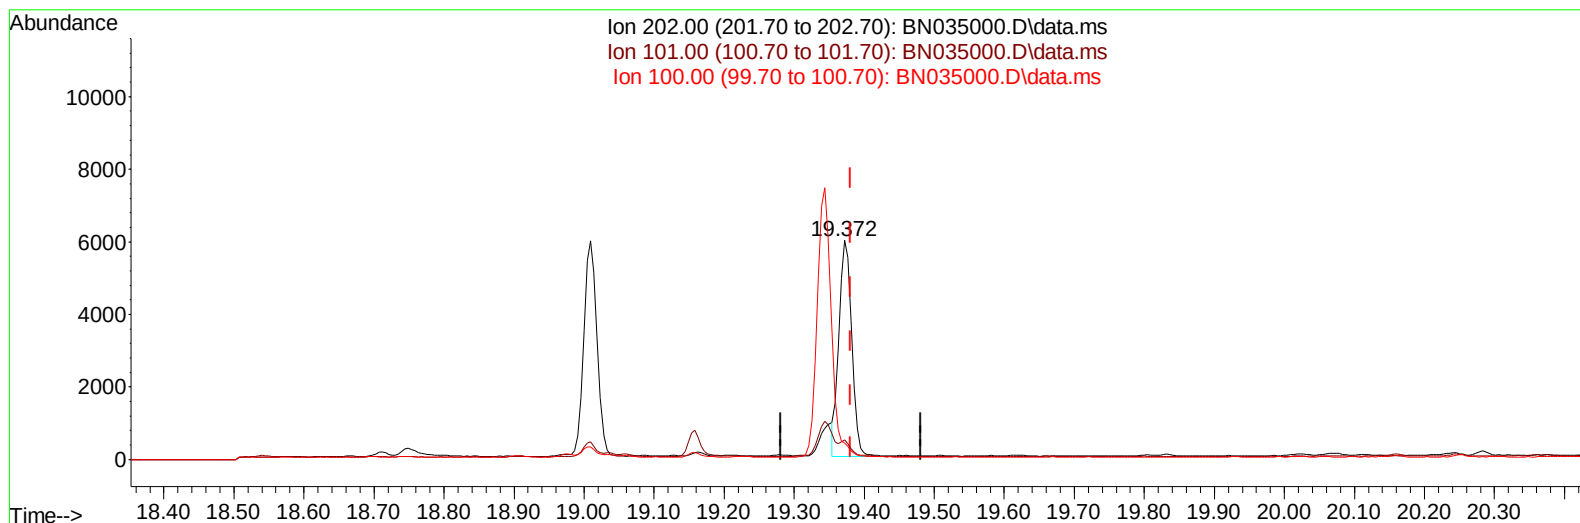

TIC: BN035000.D\data.ms

(20) Pyrene

19.372min (-0.009) 0.20 ng/ul m

response 7715

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	6.20	9.01#
100.00	5.10	7.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

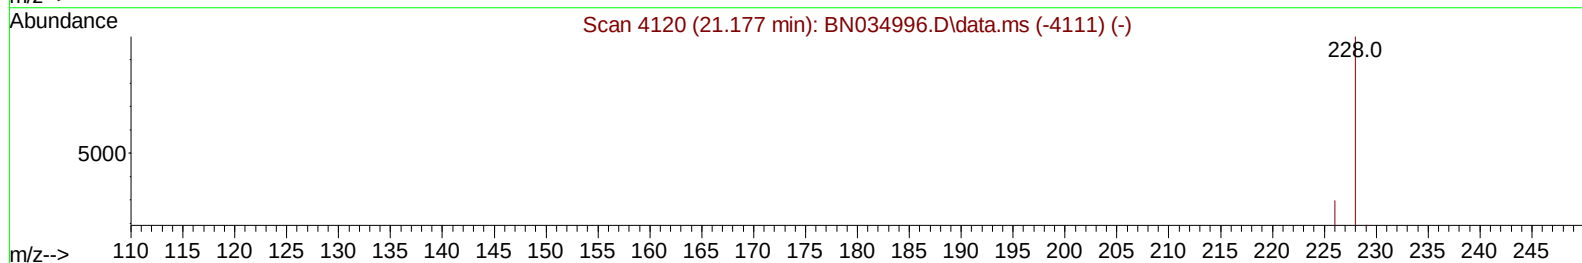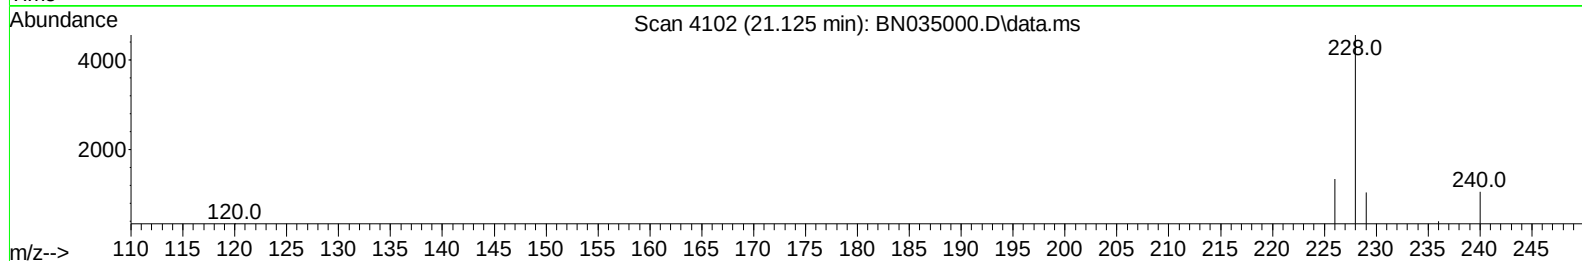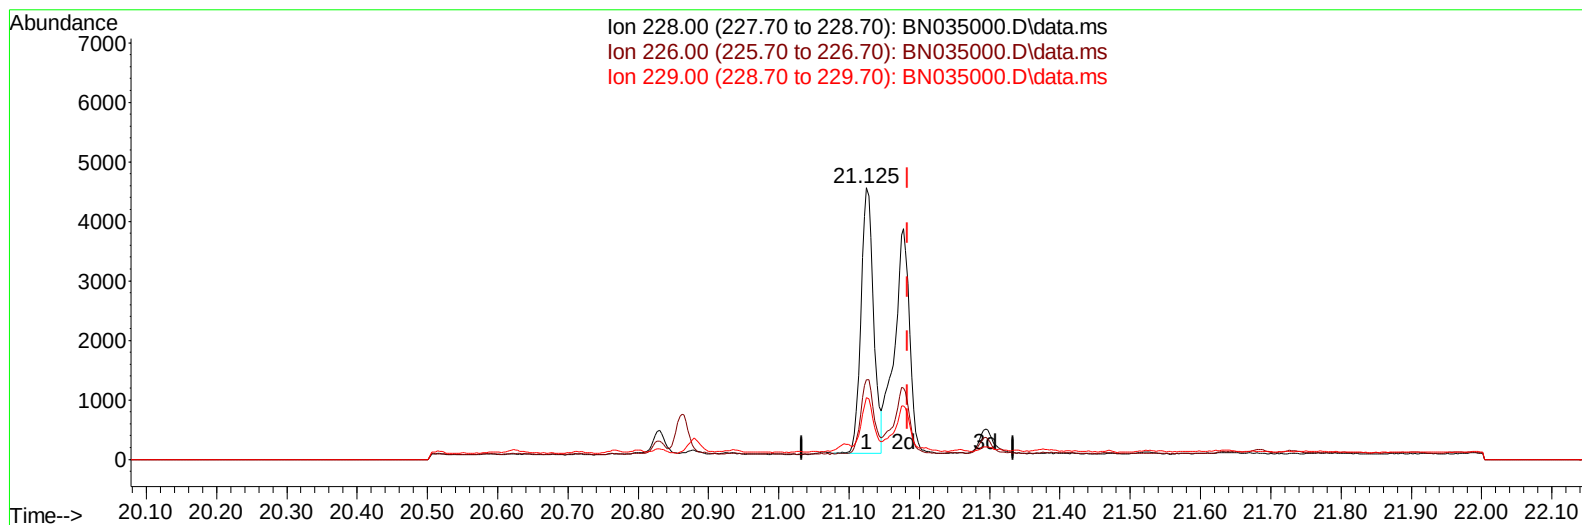

TIC: BN035000.D\data.ms

(22) Chrysene

21.125min (-0.058) 0.14 ng/u1

response 5536

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.30	29.36
229.00	19.30	22.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

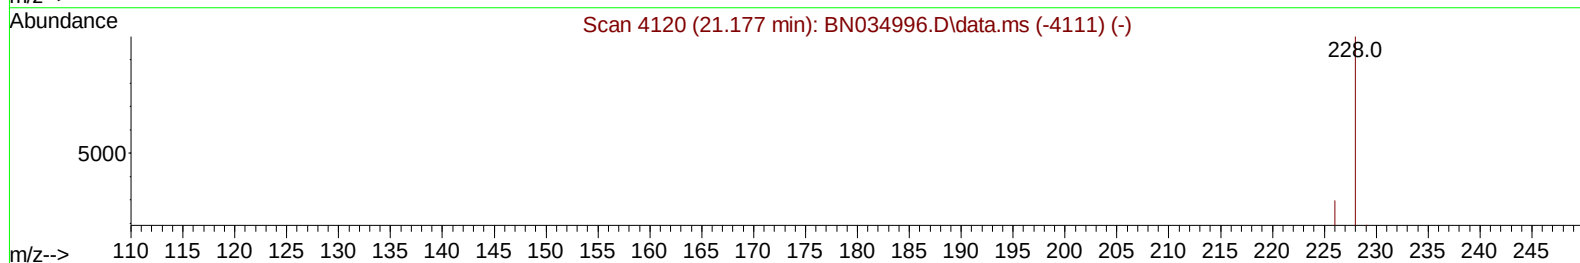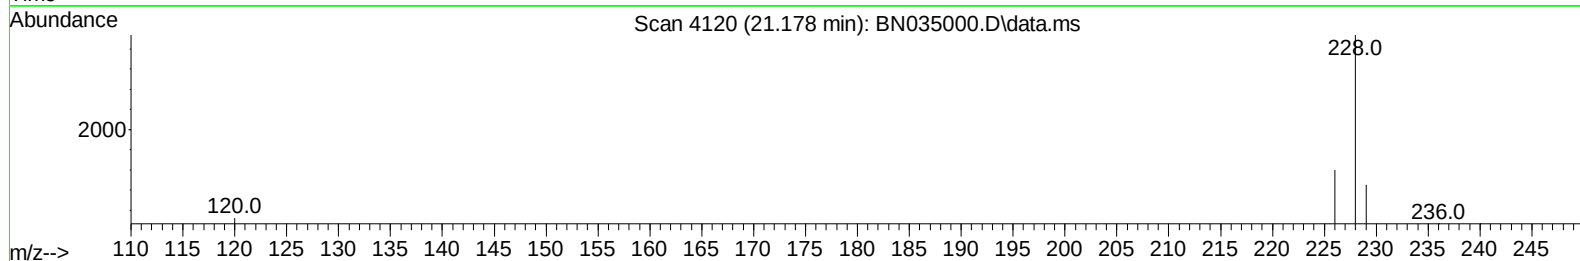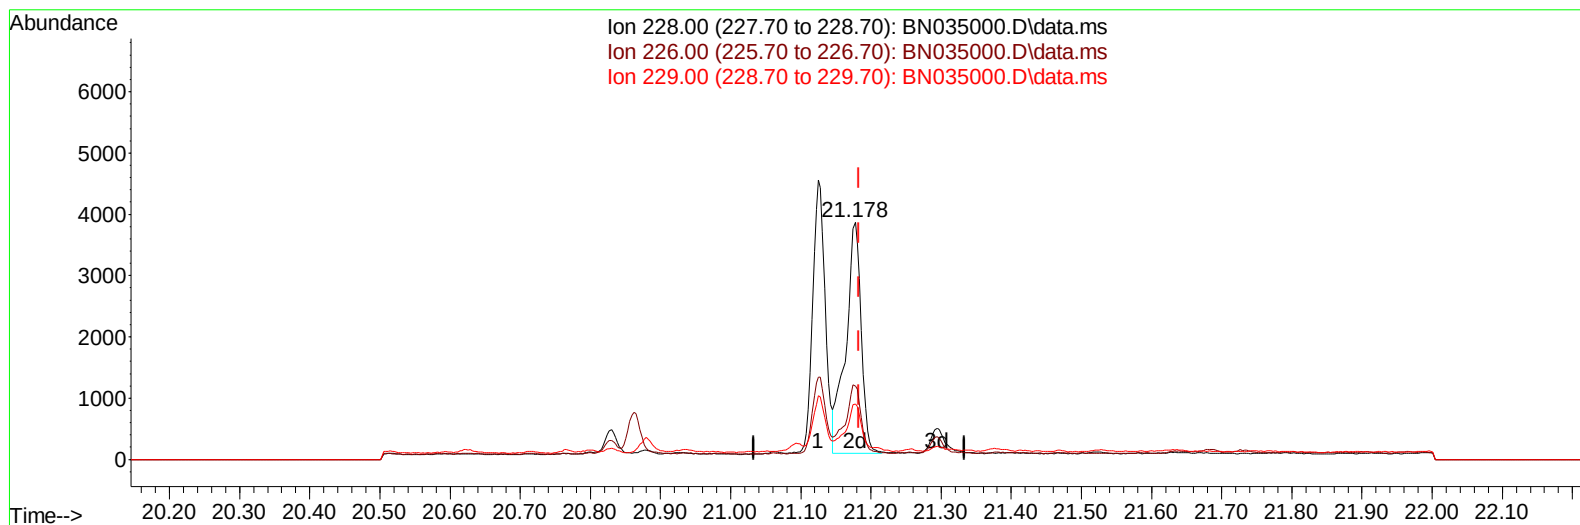

TIC: BN035000.D\data.ms

(22) Chrysene

21.178min (-0.006) 0.14 ng/ul m

response 5770

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	30.30	30.97
229.00	19.30	23.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

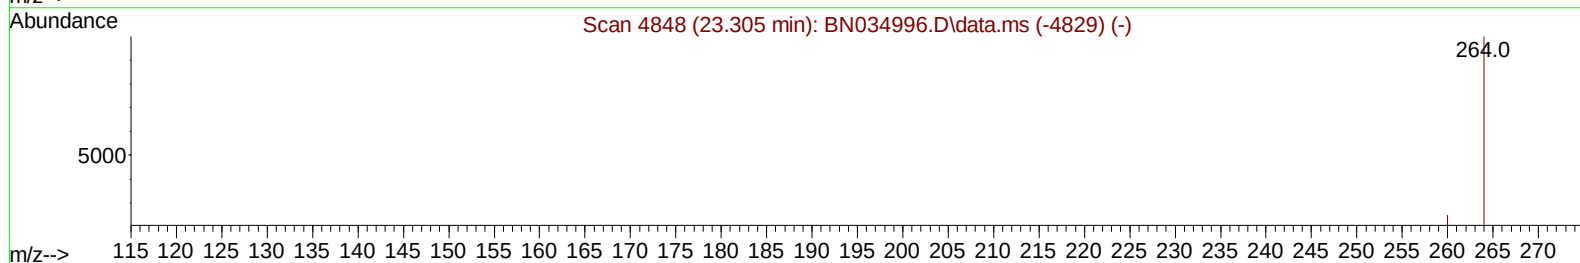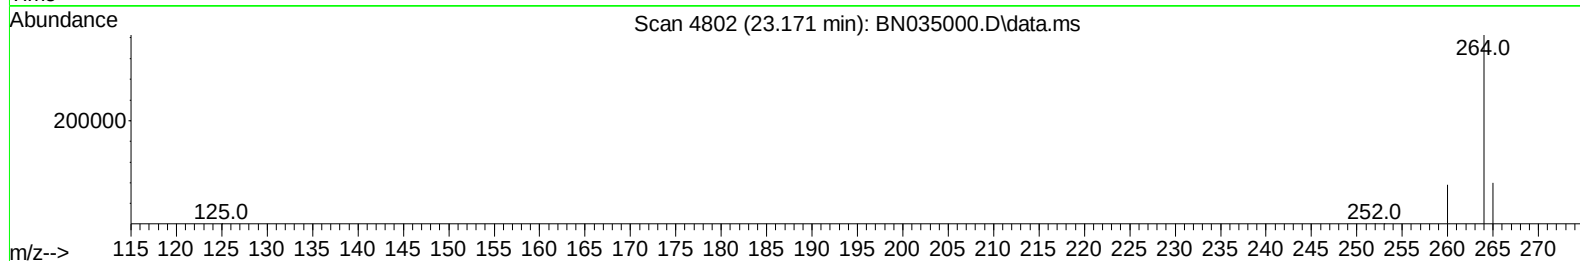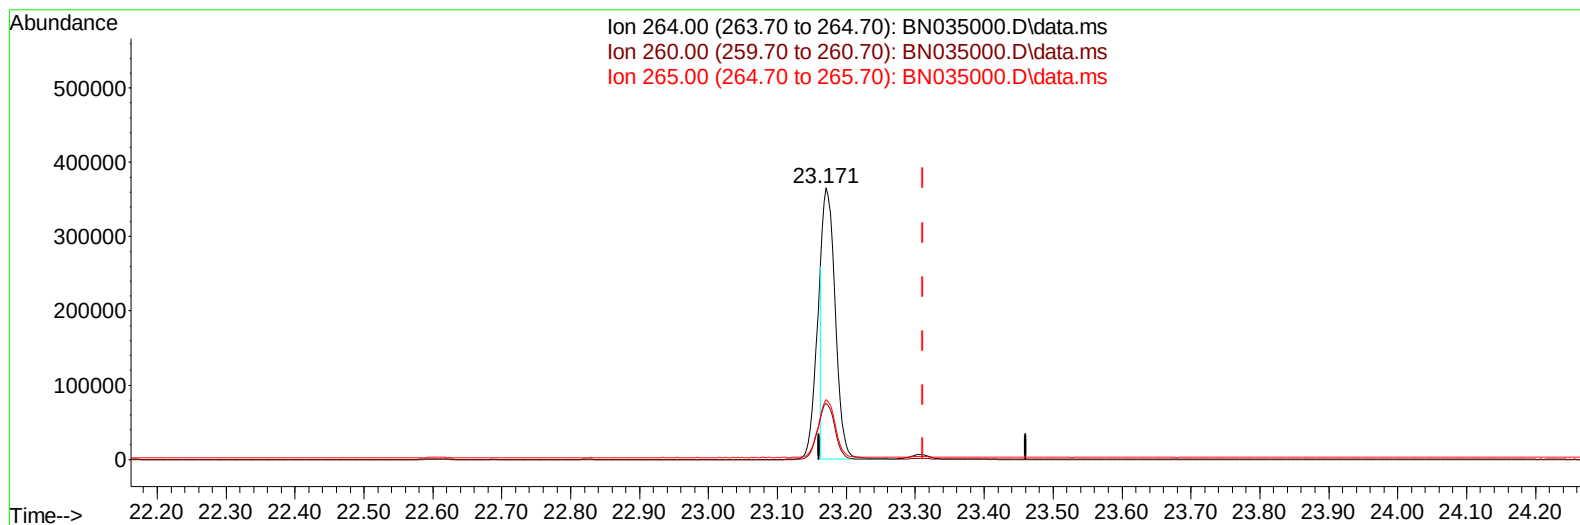

TIC: BN035000.D\data.ms

(23) Perylene-d12 (I)

23.171min (-0.140) 0.40 ng/u1

response 476722

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	20.68#
265.00	52.80	21.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

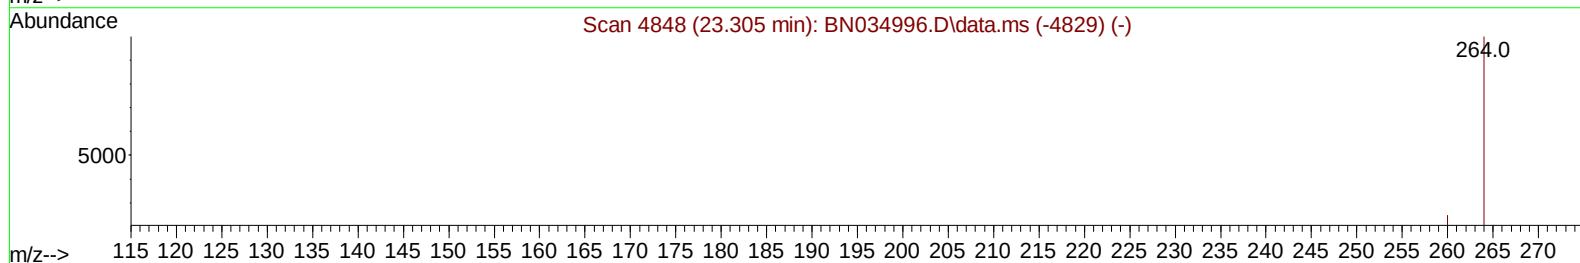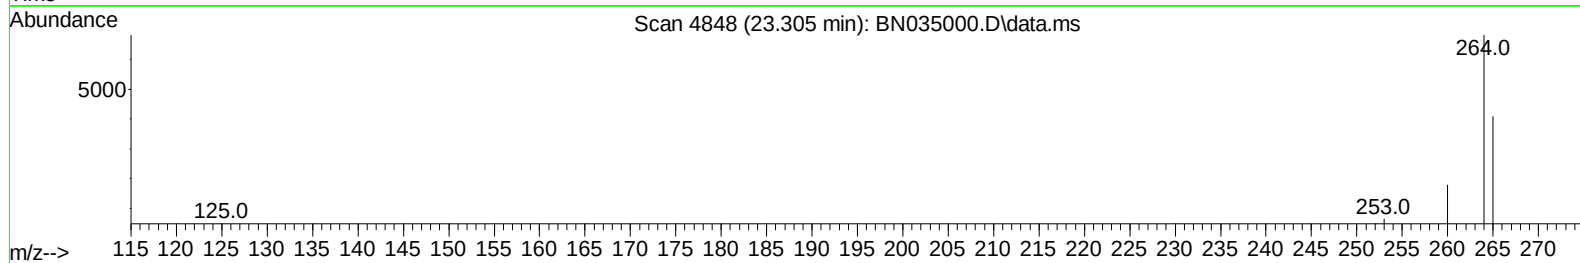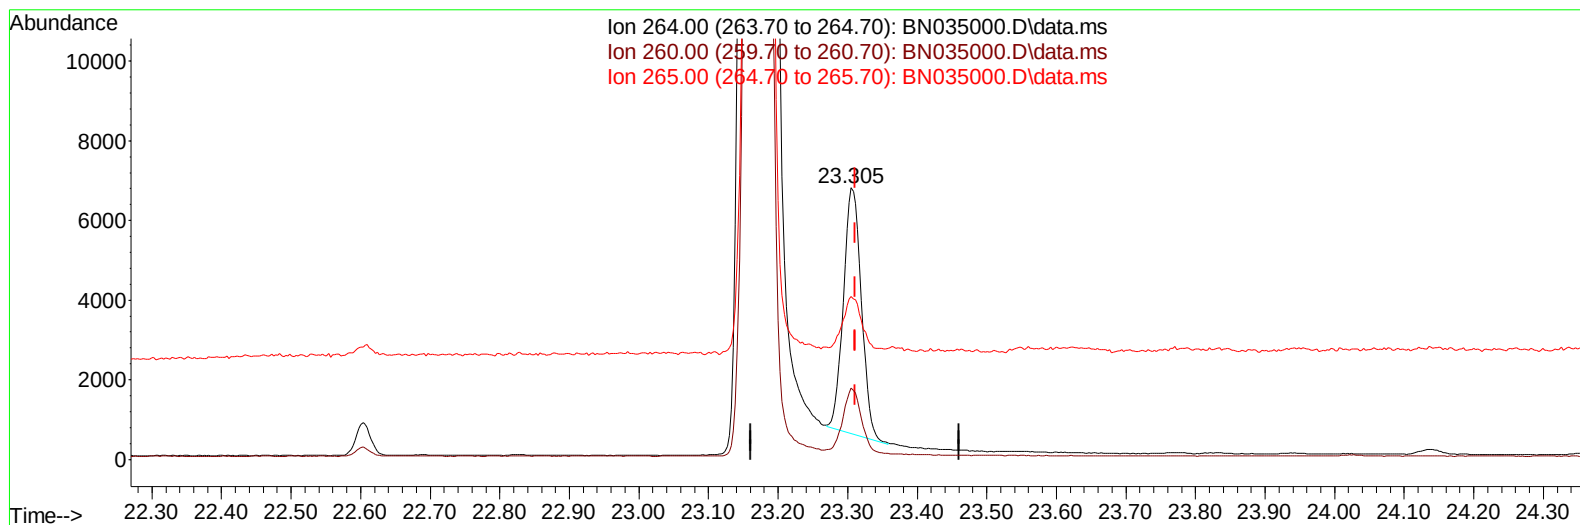

TIC: BN035000.D\data.ms

(23) Perylene-d12 (I)

23.305min (-0.006) 0.40 ng/ul m

response 11077

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	26.31
265.00	52.80	60.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

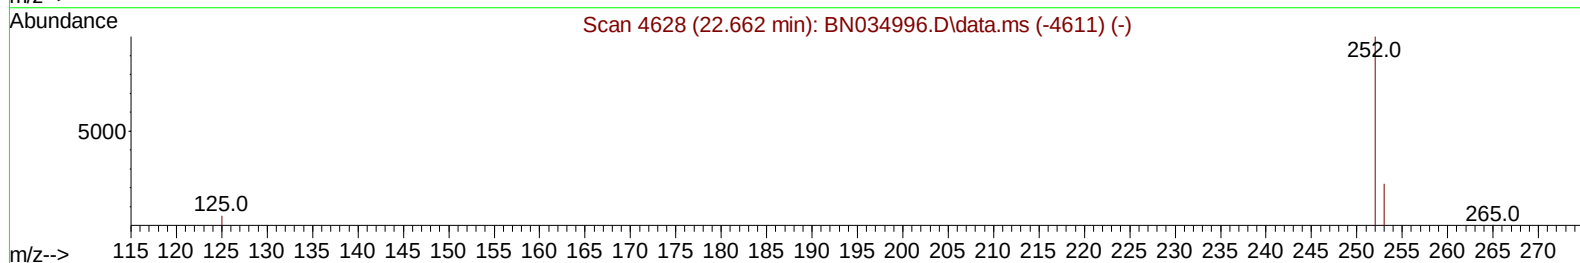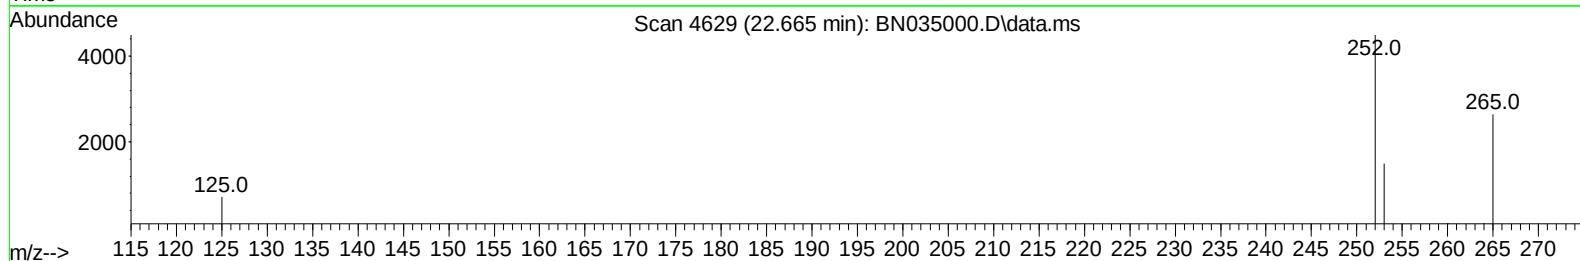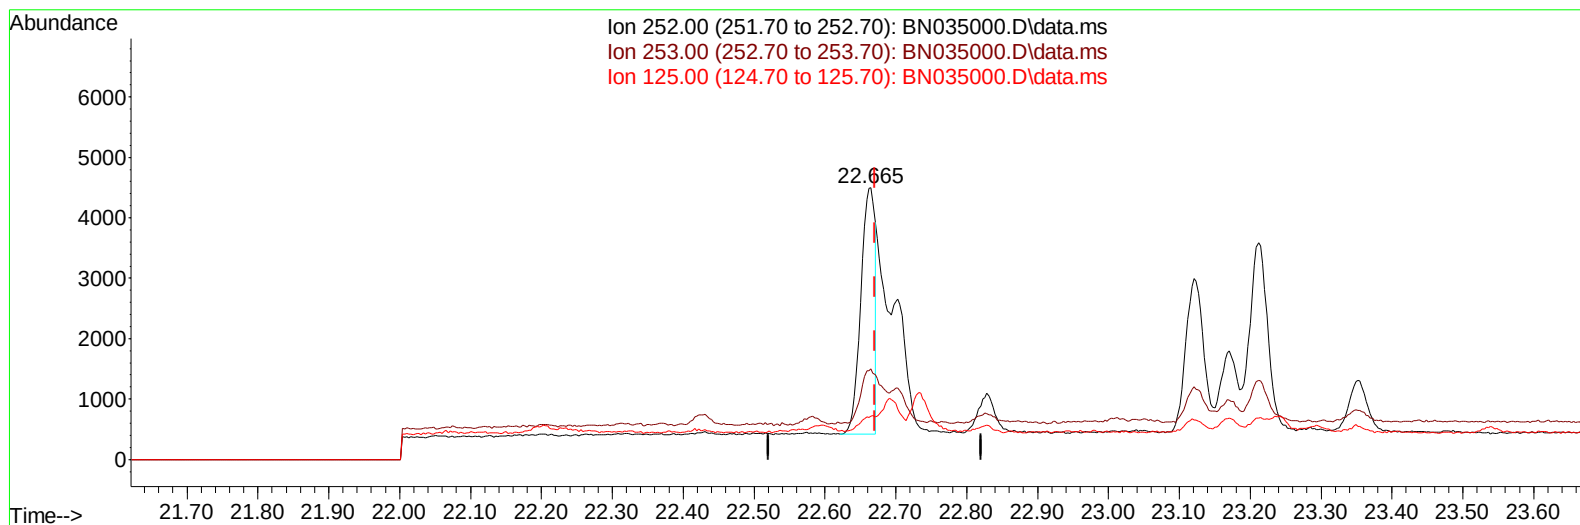

TIC: BN035000.D\data.ms

(24) Benzo(b)fluoranthene

22.665min (-0.006) 0.14 ng/u1

response 5561

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	33.36
125.00	7.00	15.87#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

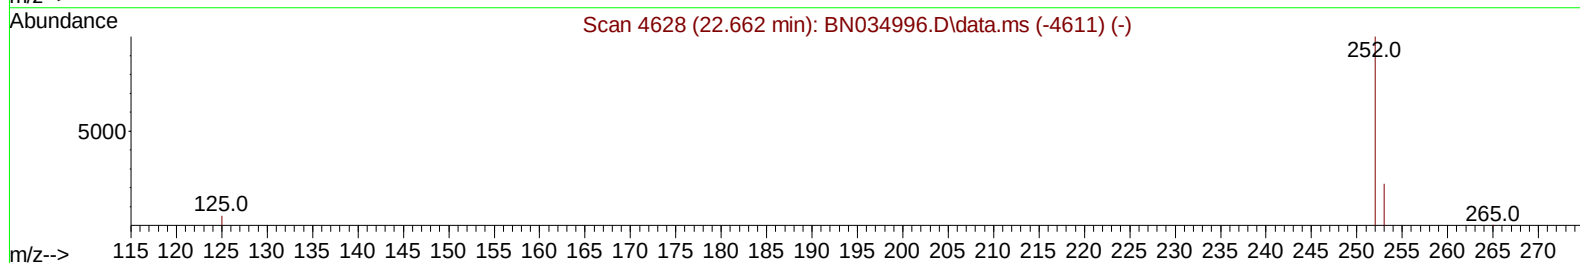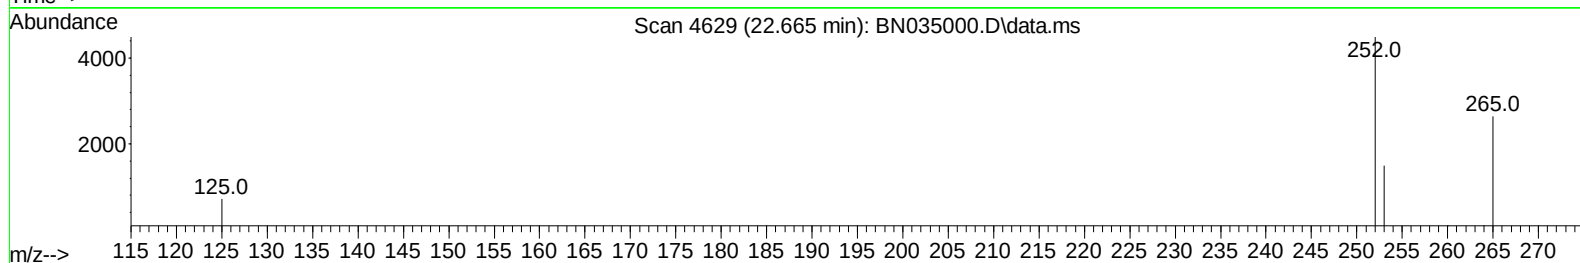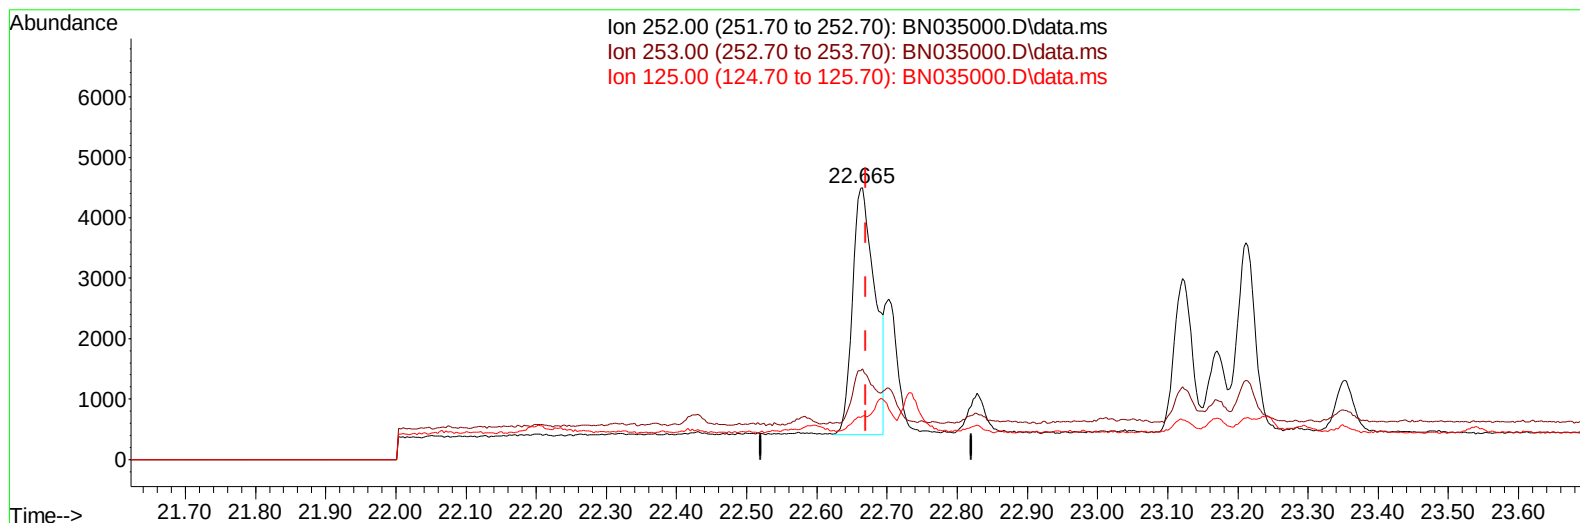

TIC: BN035000.D\data.ms

(24) Benzo(b)fluoranthene

22.665min (-0.006) 0.23 ng/ul m

response 9002

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.00	33.36
125.00	7.00	15.87#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

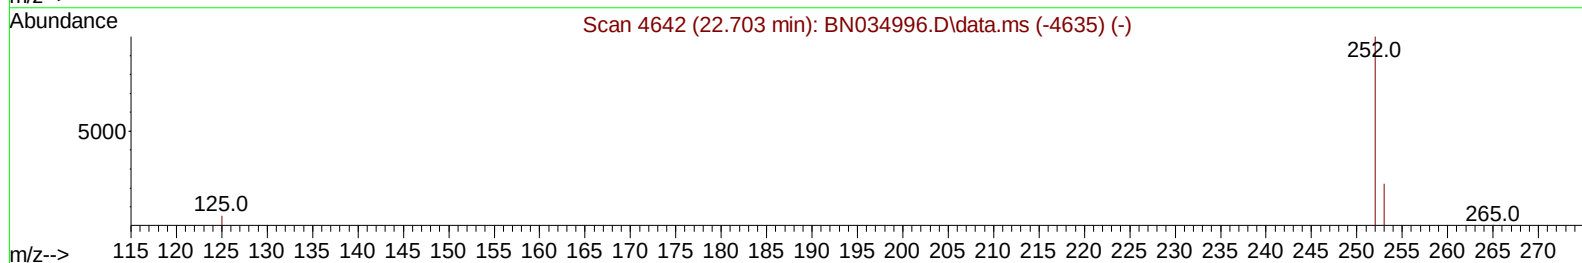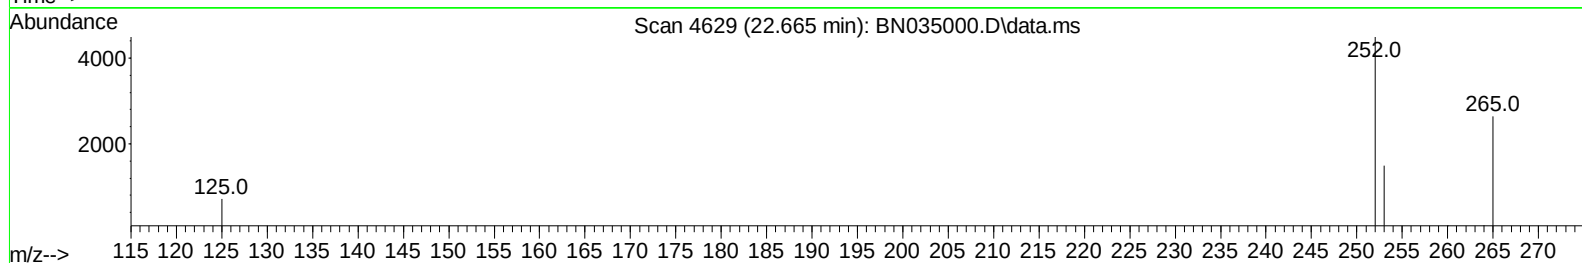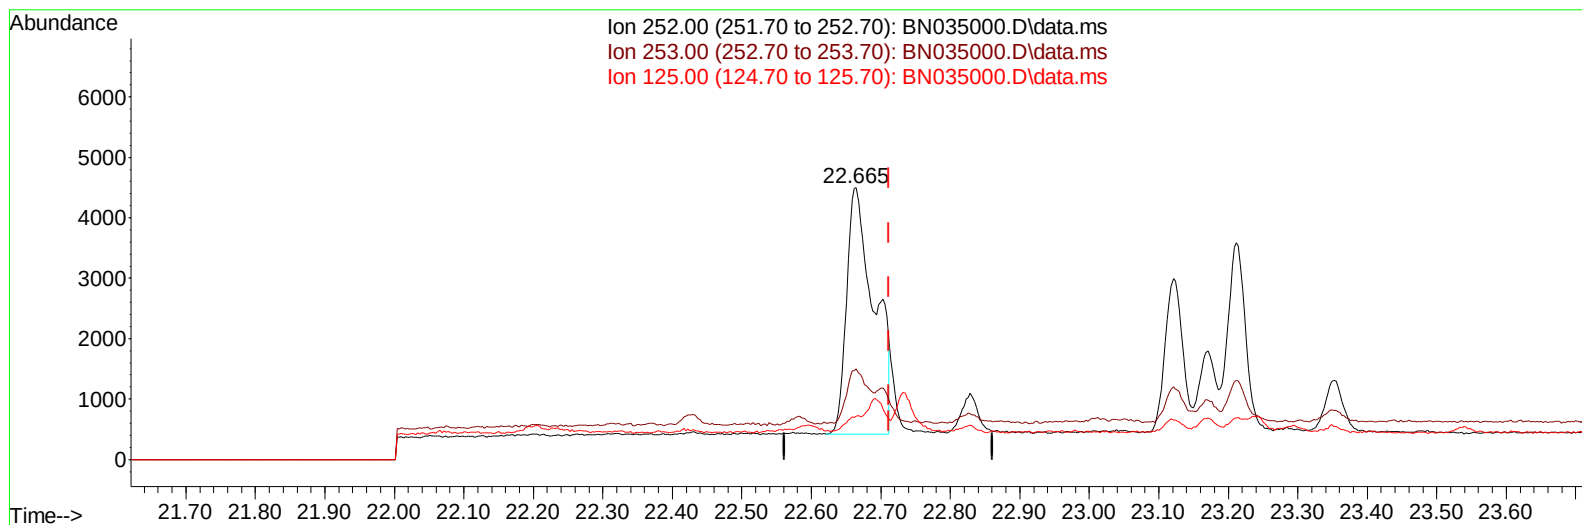

TIC: BN035000.D\data.ms

(25) Benzo(k)fluoranthene

22.665min (-0.047) 0.27 ng/u1

response 11101

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.30	33.36#
125.00	7.30	15.87#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

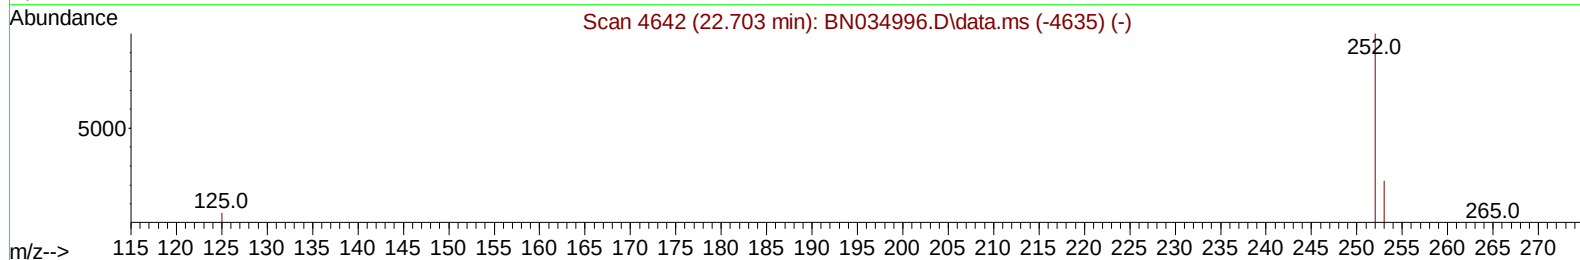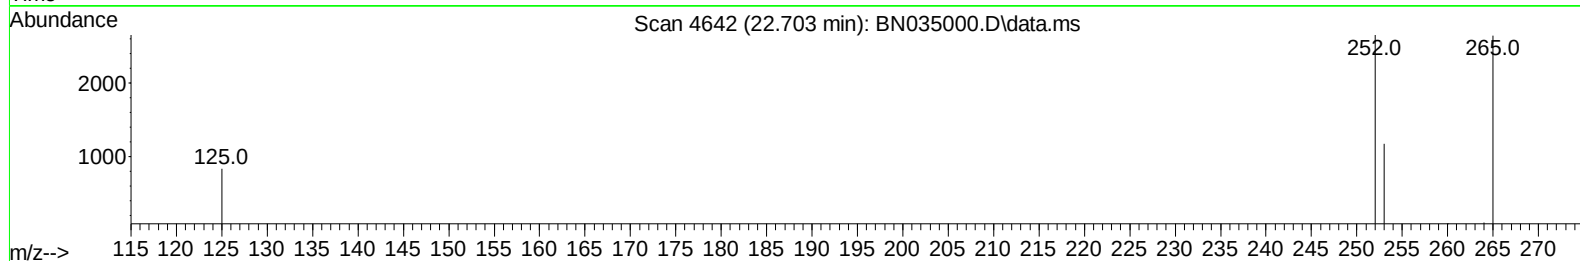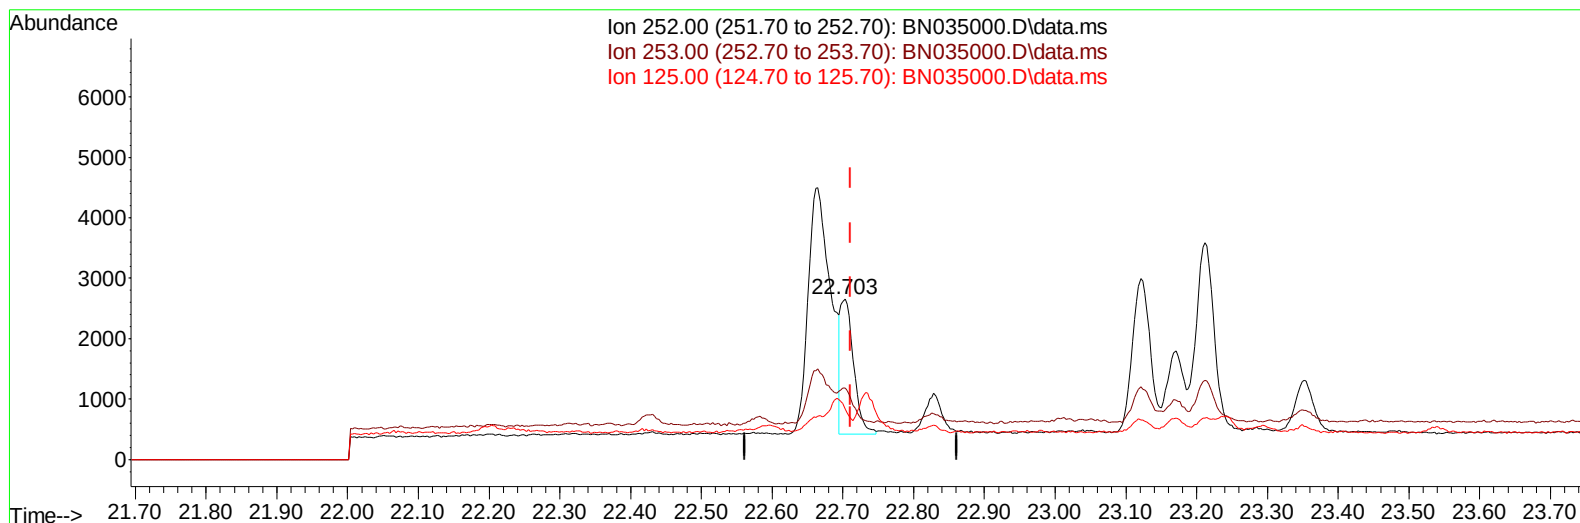

TIC: BN035000.D\data.ms

(25) Benzo(k)fluoranthene

22.703min (-0.009) 0.07 ng/ul m

response 2887

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.30	44.35#
125.00	7.30	31.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

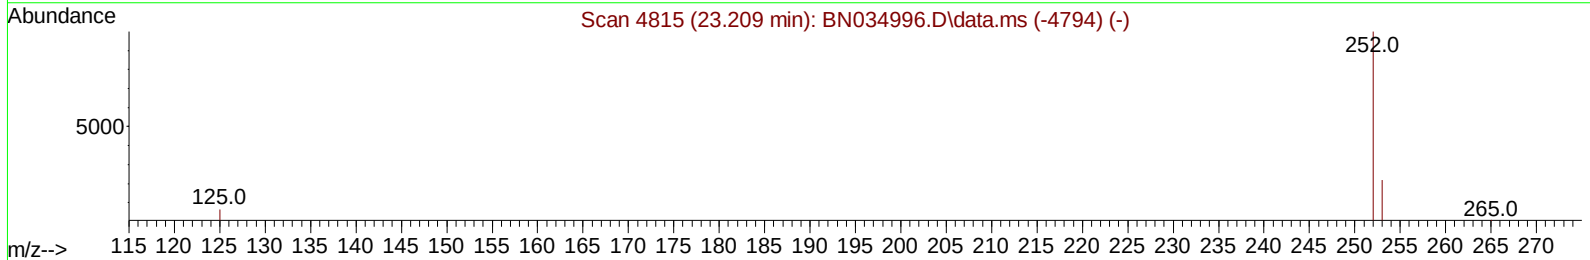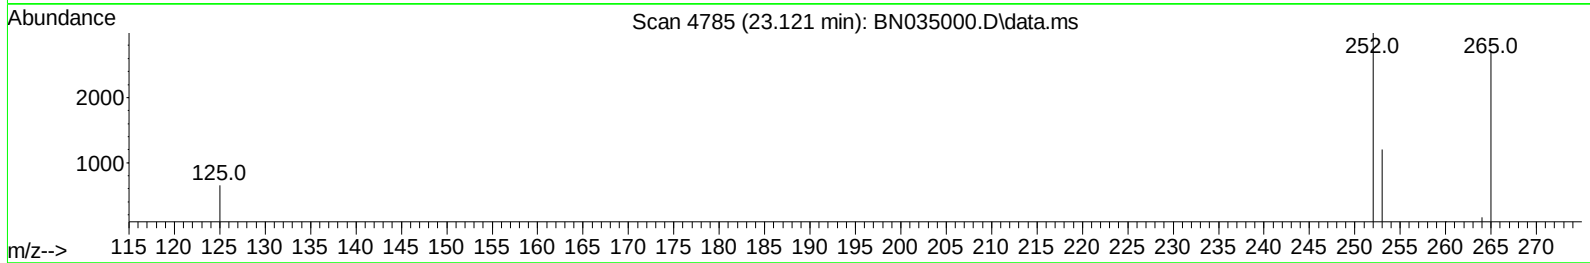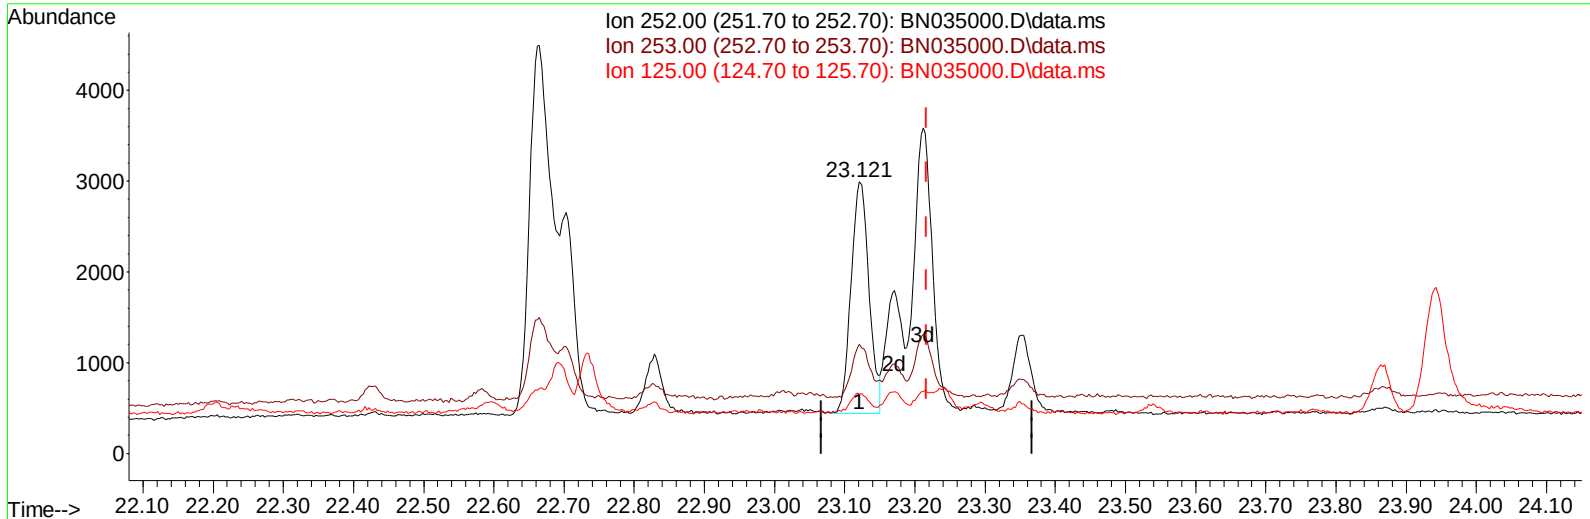

TIC: BN035000.D\data.ms

(26) Benzo(a)pyrene (C)

23.121min (-0.096) 0.13 ng/u1

response 4572

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	40.25#
125.00	7.90	21.90#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

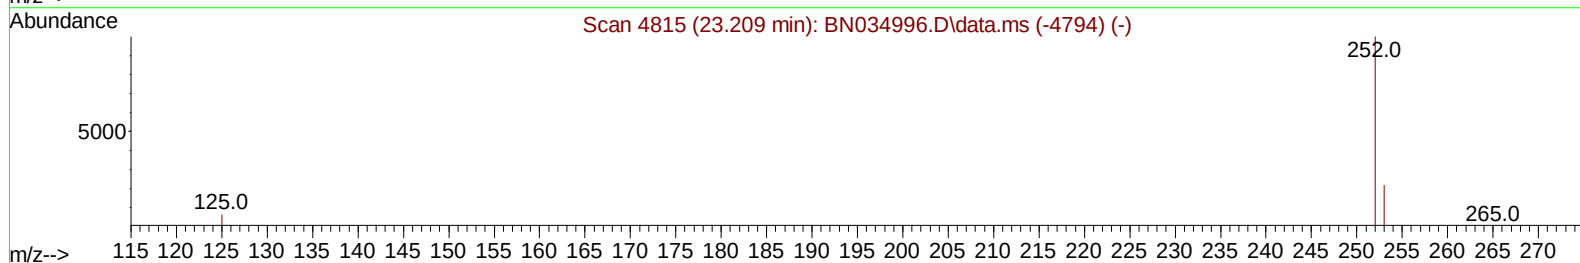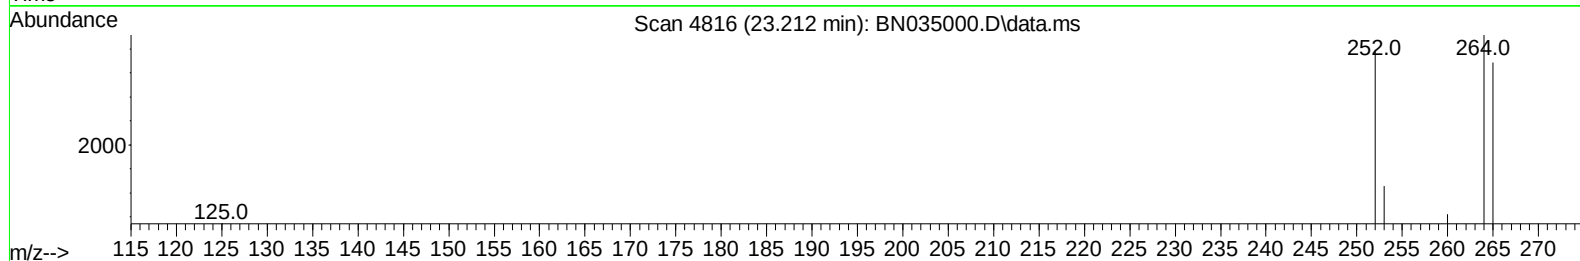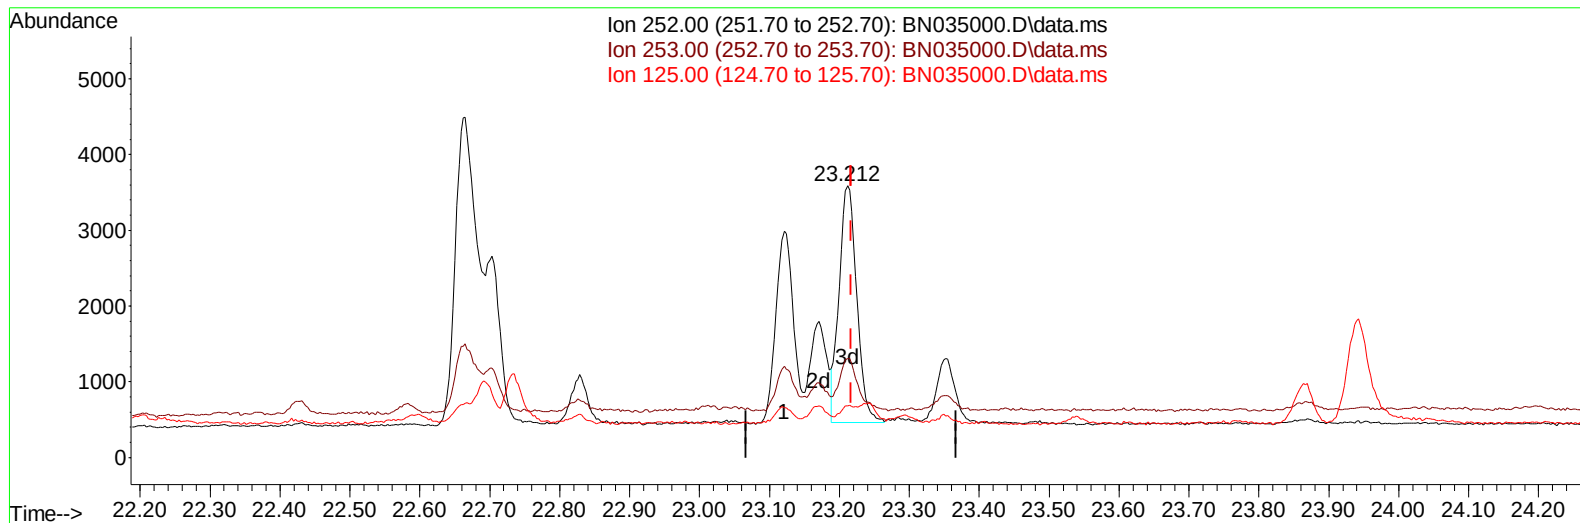

TIC: BN035000.D\data.ms

(26) Benzo(a)pyrene (C)

23.212min (-0.006) 0.16 ng/u1 m

response 5491

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.50	36.49#
125.00	7.90	19.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

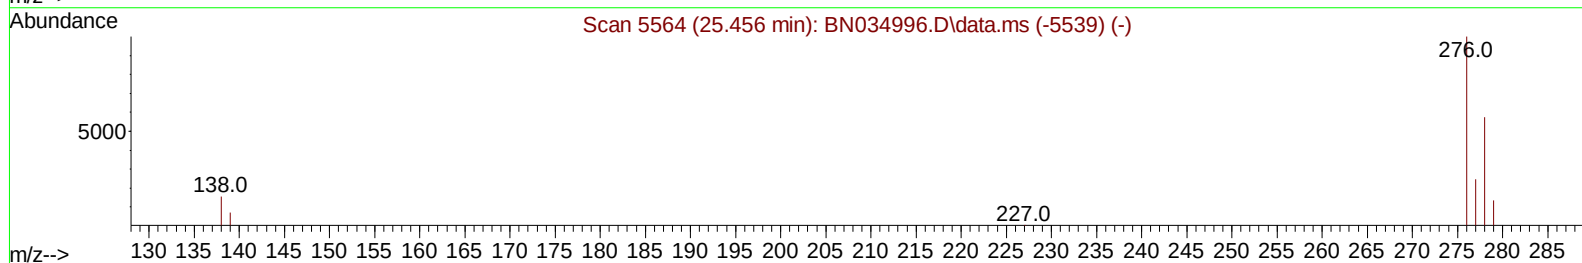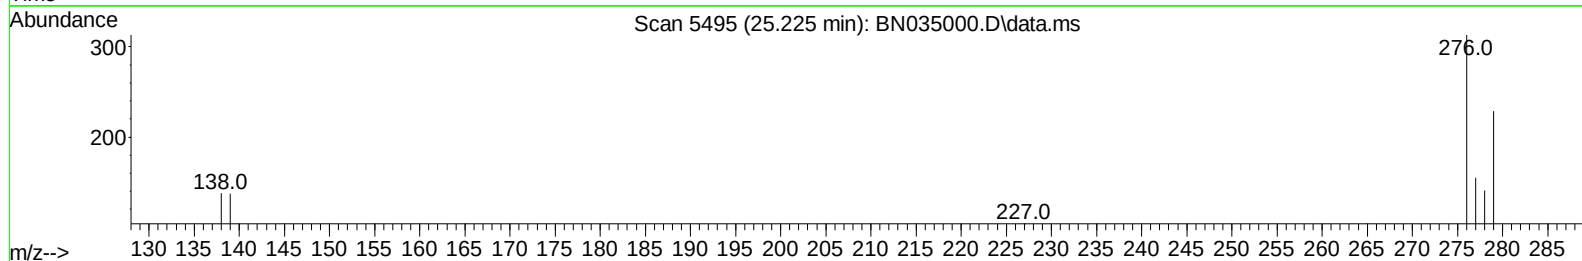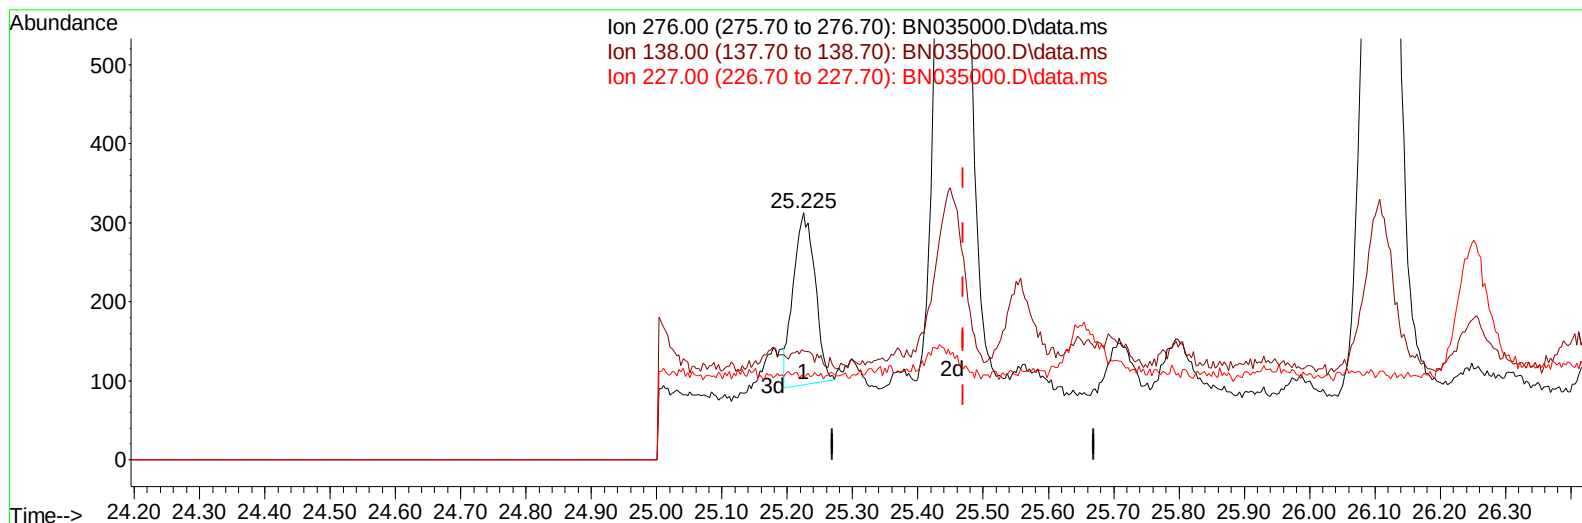

TIC: BN035000.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.225min (-0.245) 0.01 ng/u1

response 502

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	13.50	8.57#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

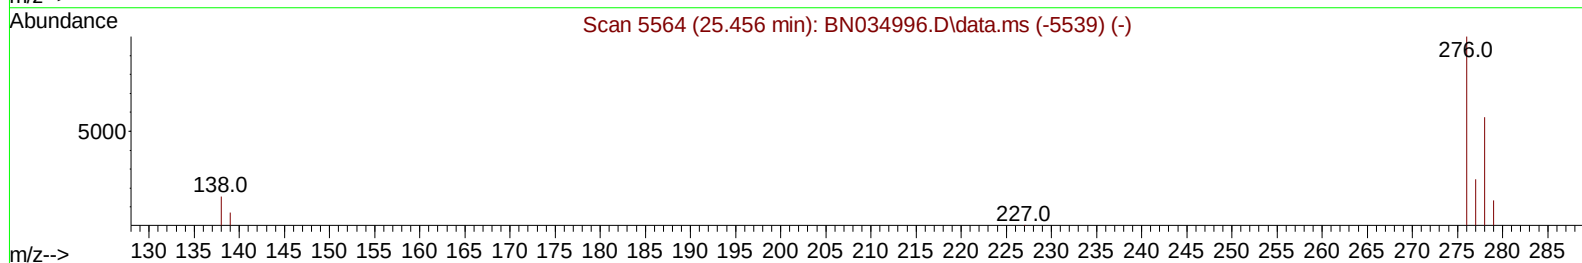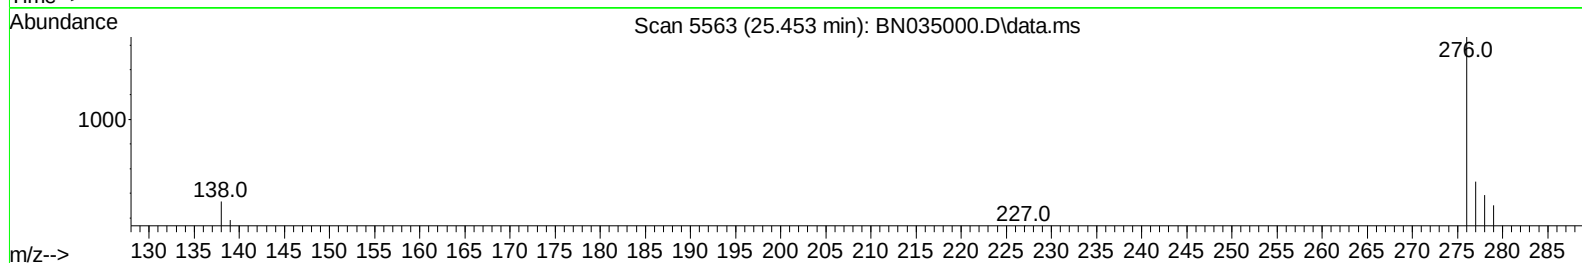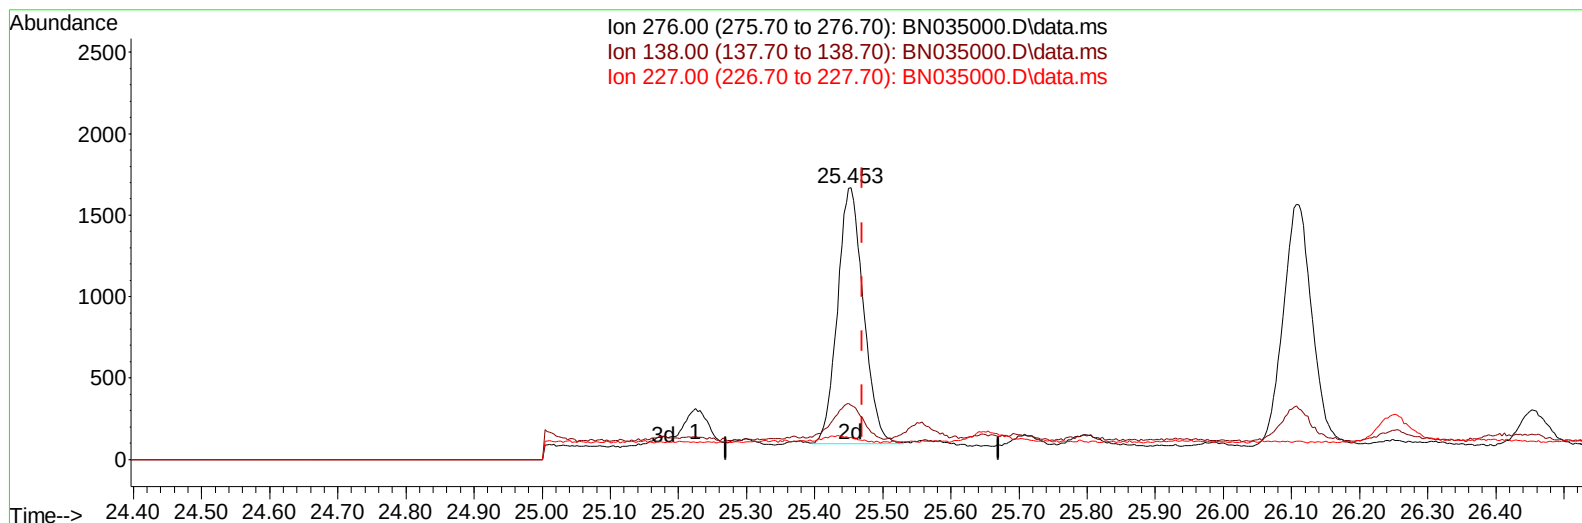

TIC: BN035000.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.453min (-0.017) 0.10 ng/ul m

response 4157

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	13.50	1.03#
227.00	0.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

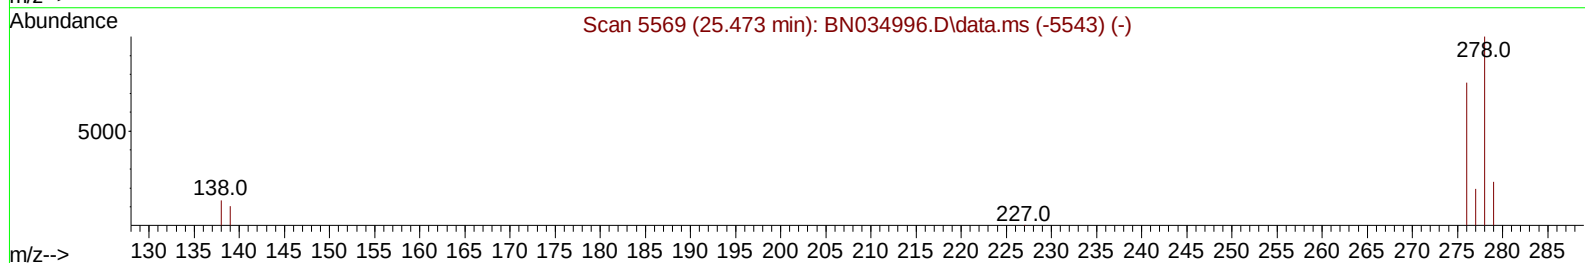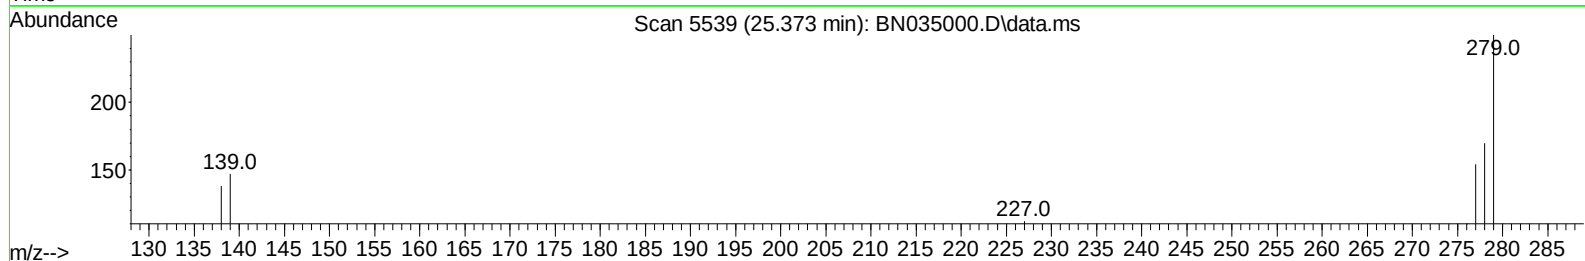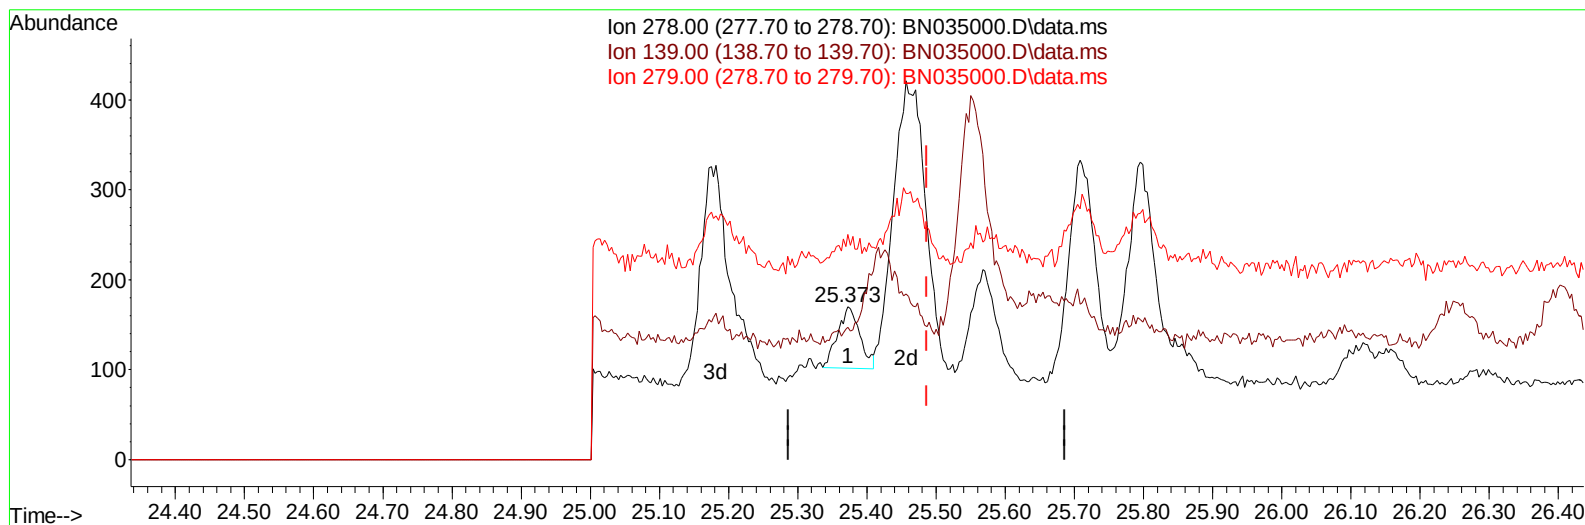

TIC: BN035000.D\data.ms

(28) Dibenzo(a,h)anthracene

25.373min (-0.114) 0.00 ng/u1

response 153

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	10.50	86.47#
279.00	26.90	147.06#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

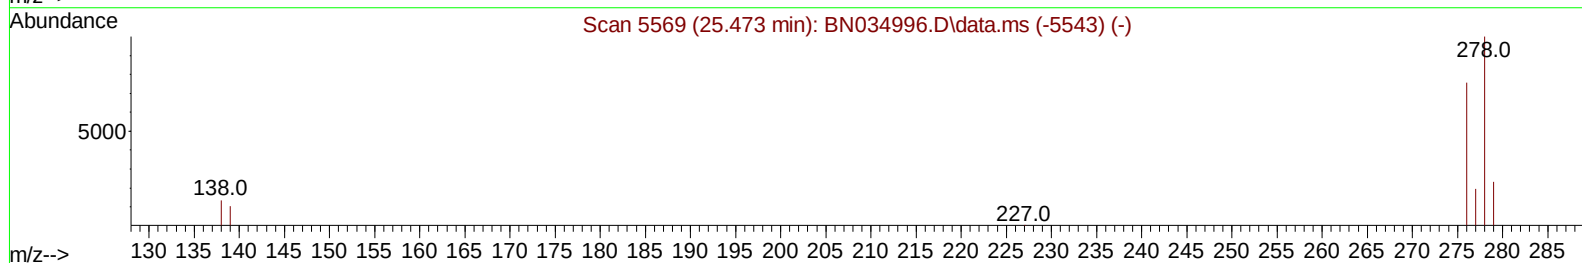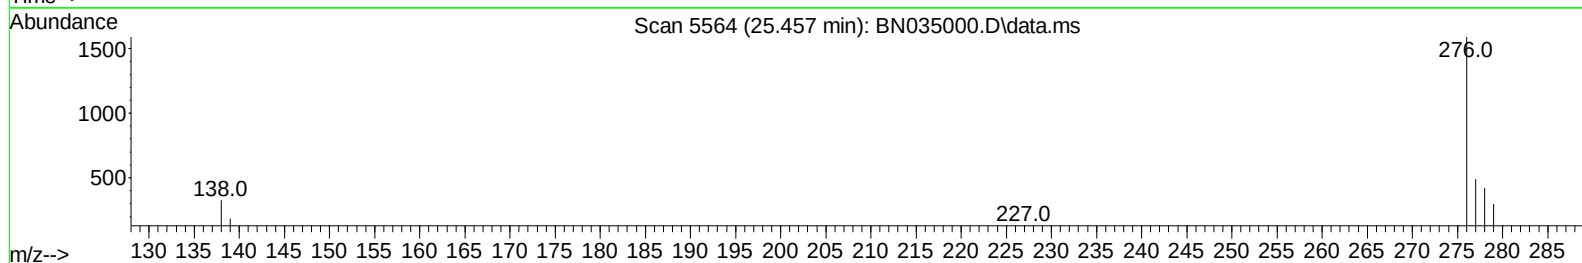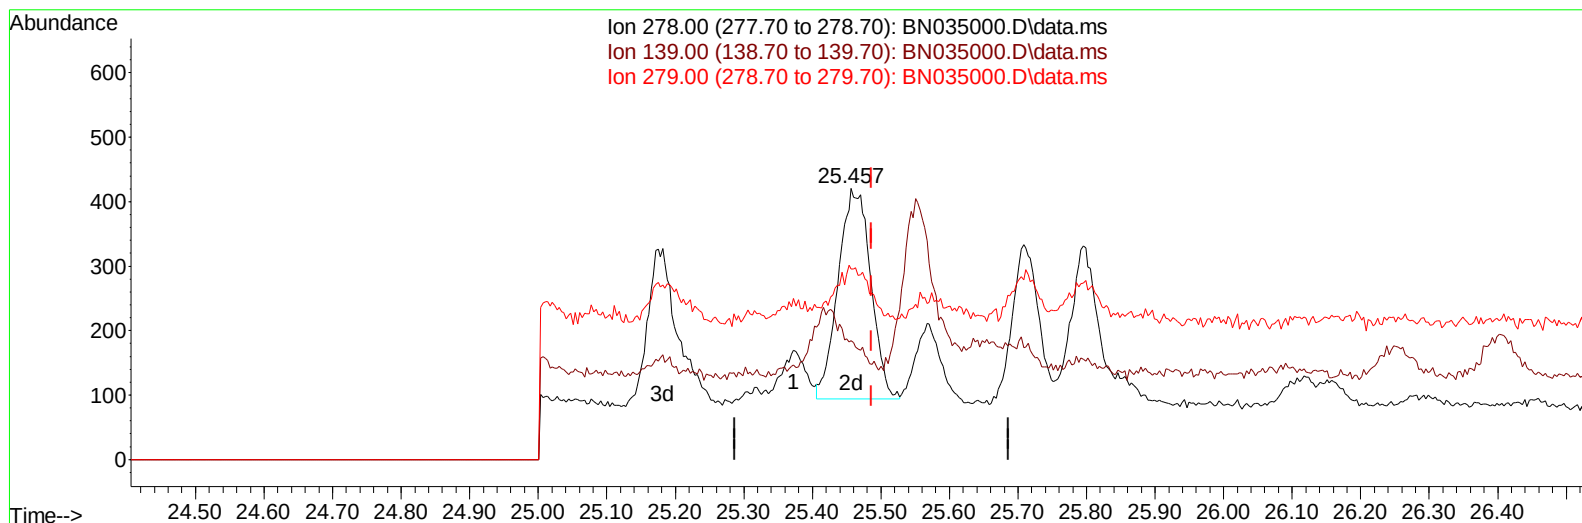

TIC: BN035000.D\data.ms

(28) Dibenzo(a,h)anthracene

25.457min (-0.030) 0.03 ng/ul m

response 1074

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	10.50	43.71#
279.00	26.90	70.31#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

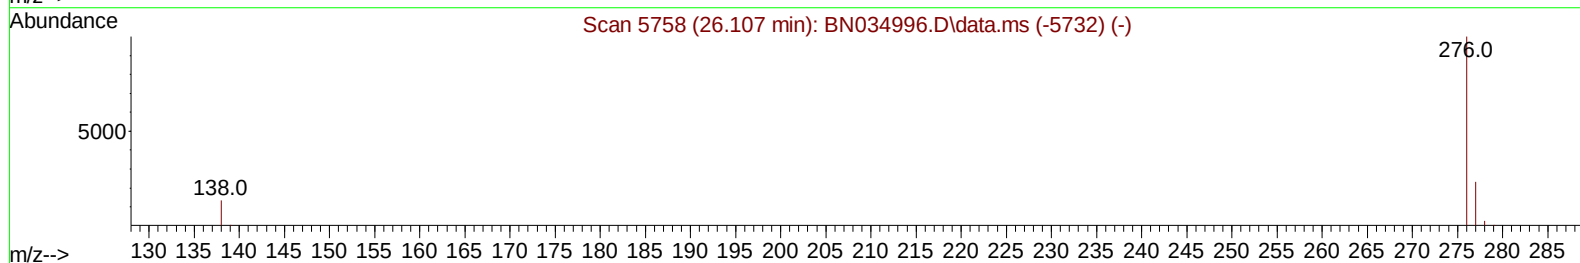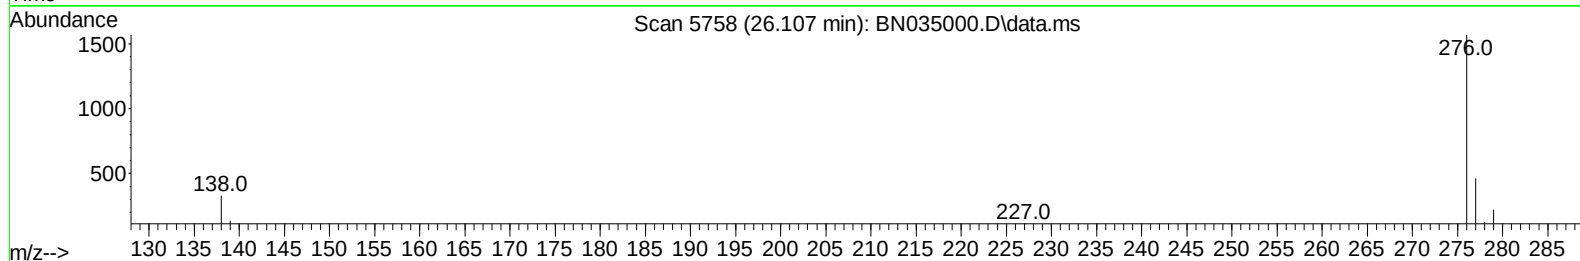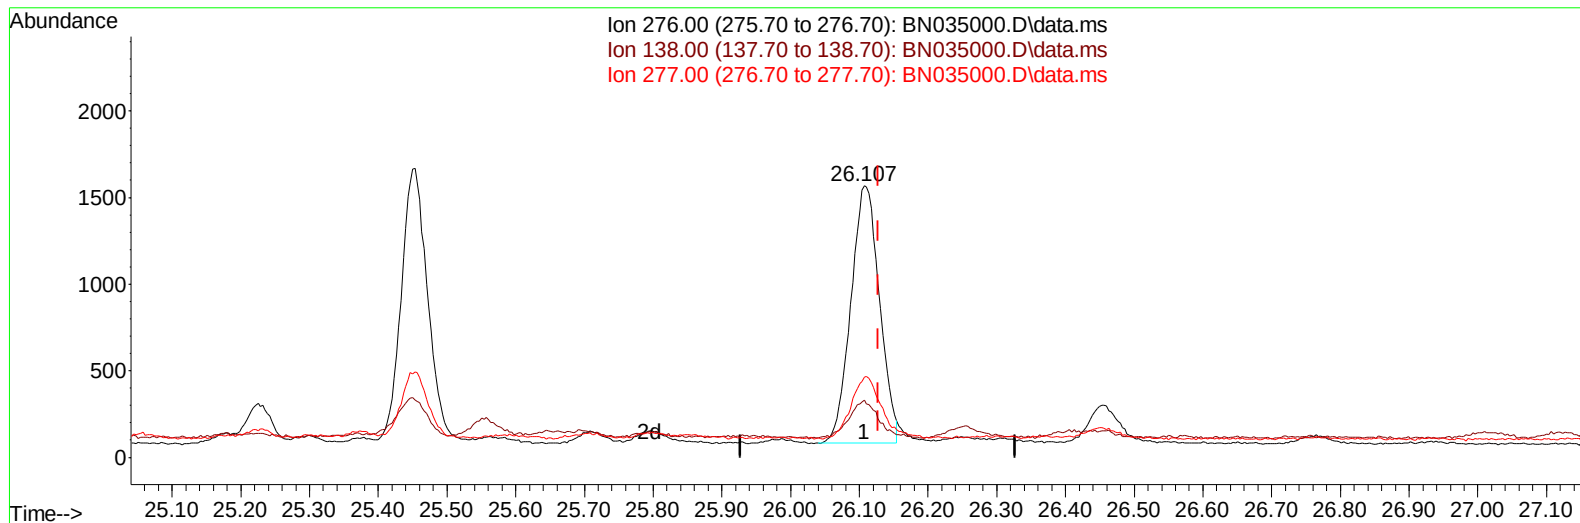

TIC: BN035000.D\data.ms

(29) Benzo(g,h,i)perylene

26.107min (-0.020) 0.13 ng/u1

response 4304

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.90	21.06#
277.00	25.20	29.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

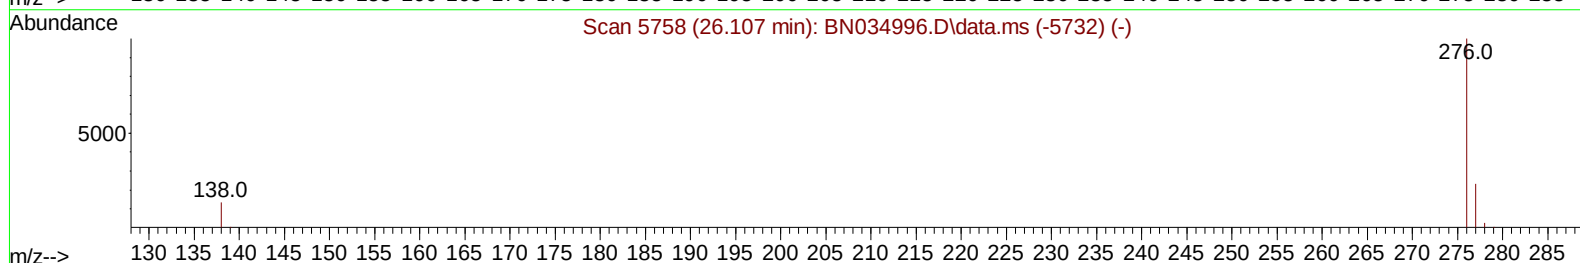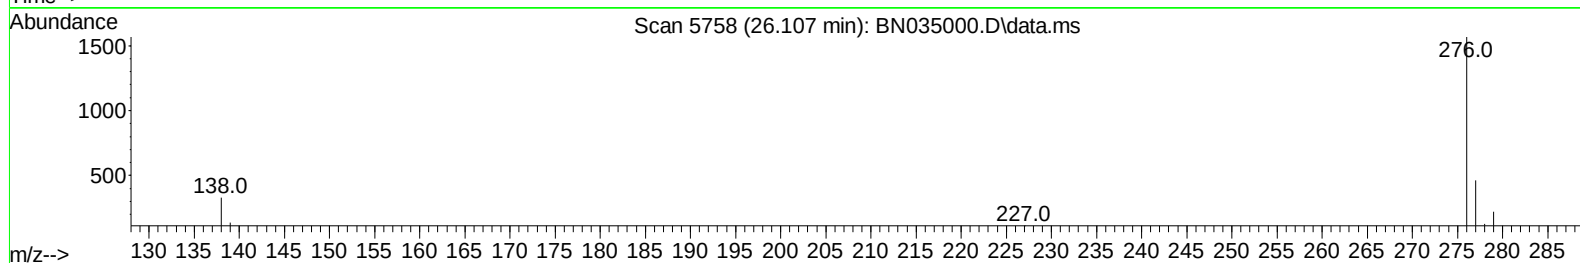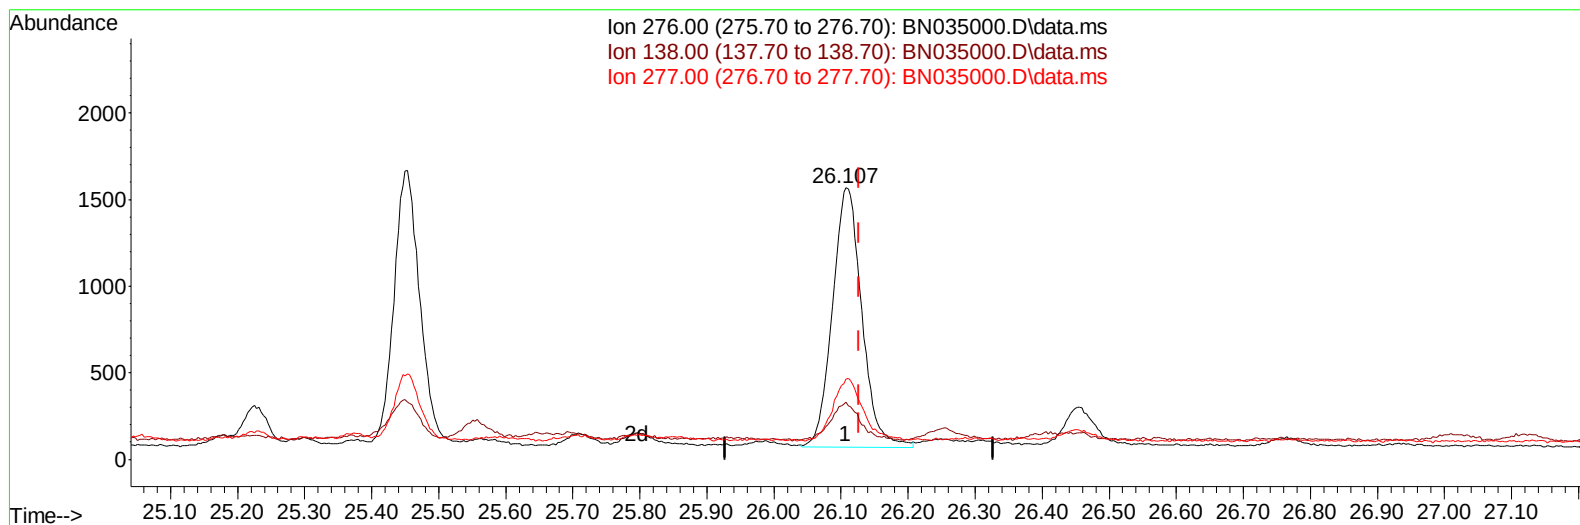

TIC: BN035000.D\data.ms

(29) Benzo(g,h,i)perylene

26.107min (-0.020) 0.14 ng/ul m

response 4538

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	12.90	21.06#
277.00	25.20	29.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035000.D
 Acq On : 11 Nov 2024 12:12
 Operator : RC/JU
 Sample : P4636-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CC0R1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 11 12:41:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.562	152	3378	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.328	136	8575	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.199	164	5691	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.945	188	11942	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240	10908	0.400	ng/ul	# 0.00
23) Perylene-d12	23.305	264	11077m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	10537	3.278	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152	2836	0.216	ng/ul	-0.01
18) Fluoranthene-d10	18.977	212	6756	0.241	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	16.988	178	1448	0.045	ng/ul#	90
16) Anthracene	17.076	178	642	0.021	ng/ul#	71
19) Fluoranthene	19.009	202	7922	0.217	ng/ul#	93
20) Pyrene	19.372	202	7715m	0.204	ng/ul	
21) Benzo(a)anthracene	21.125	228	5536	0.140	ng/ul	95
22) Chrysene	21.178	228	5770m	0.143	ng/ul	
24) Benzo(b)fluoranthene	22.665	252	9002m	0.231	ng/ul	
25) Benzo(k)fluoranthene	22.703	252	2887m	0.071	ng/ul	
26) Benzo(a)pyrene	23.212	252	5491m	0.158	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.453	276	4157m	0.098	ng/ul	
28) Dibenzo(a,h)anthracene	25.457	278	1074m	0.032	ng/ul	
29) Benzo(g,h,i)perylene	26.107	276	4538m	0.140	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035000.D
Acq On : 11 Nov 2024 12:12
Operator : RC/JU
Sample : P4636-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R1

Manual IntegrationsAPPROVED

Quant Time: Nov 11 12:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

