




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035021.D
Acq On : 12 Nov 2024 00:50
Operator : RC/JU
Sample : P4636-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R8

Manual IntegrationsAPPROVED

Quant Time: Nov 12 01:12:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

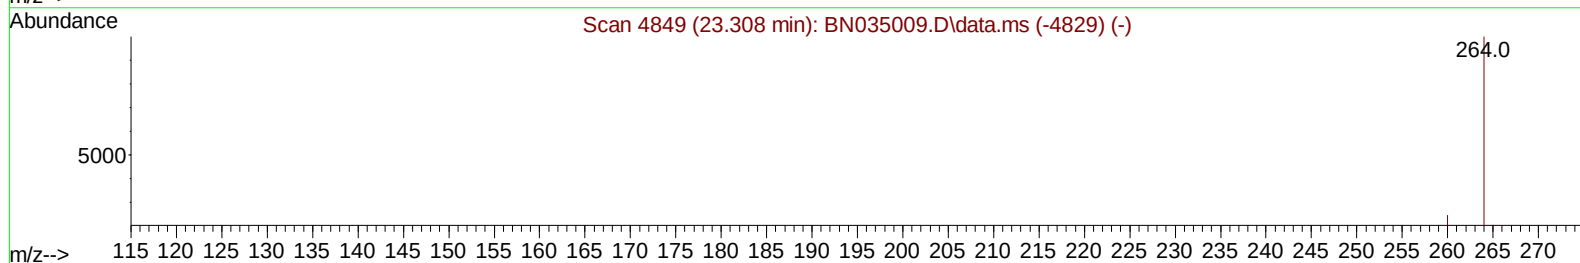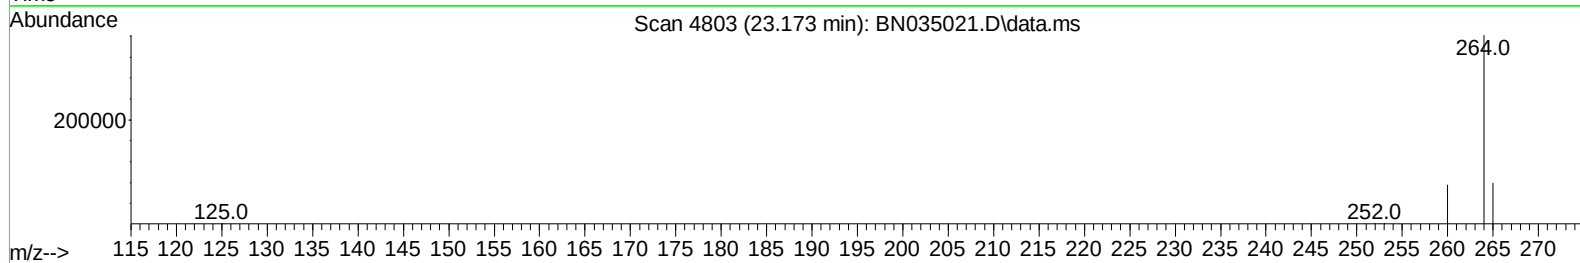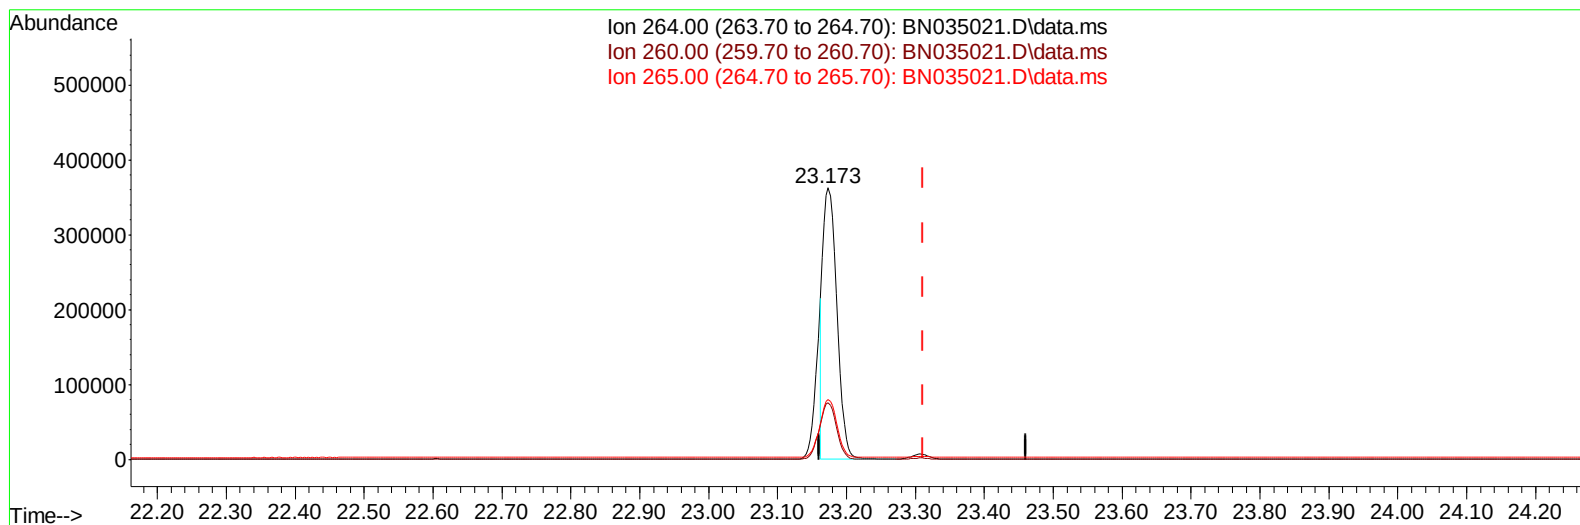

TIC: BN035021.D\data.ms

(23) Perylene-d12 (I)

23.173min (-0.137) 0.40 ng/u1

response 515415

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	20.80#
265.00	52.80	21.99#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035021.D
Acq On : 12 Nov 2024 00:50
Operator : RC/JU
Sample : P4636-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R8

Manual IntegrationsAPPROVED

Quant Time: Nov 12 01:12:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

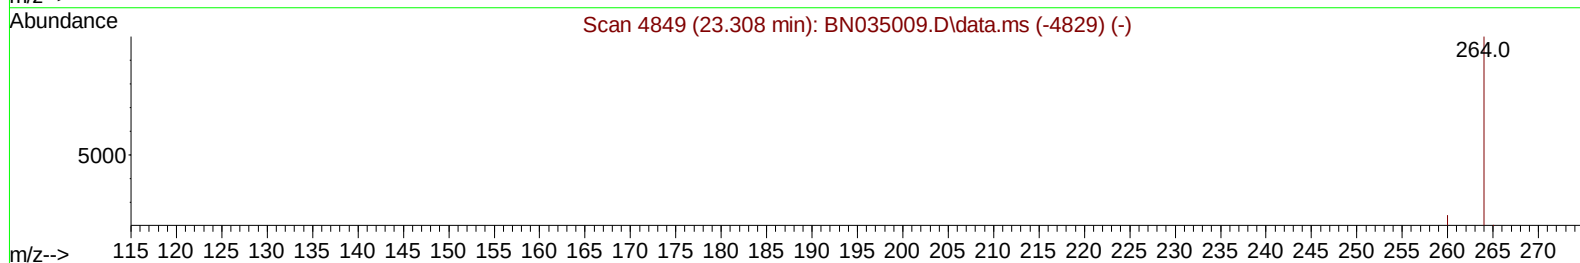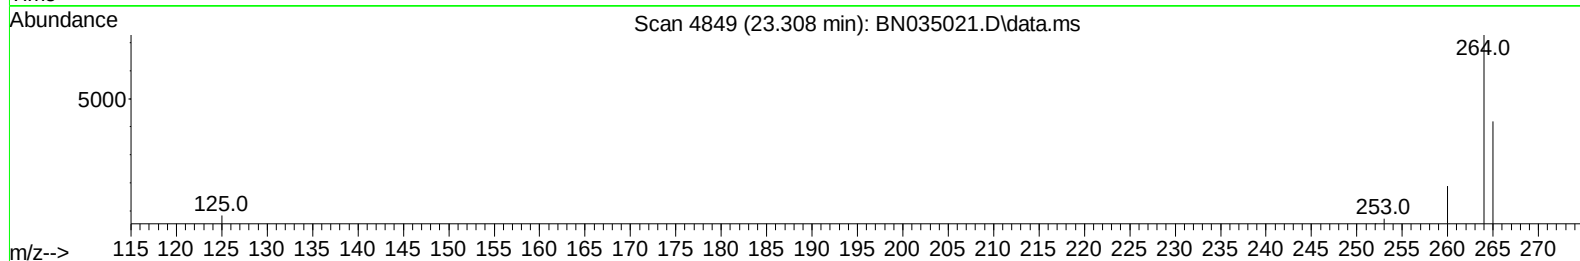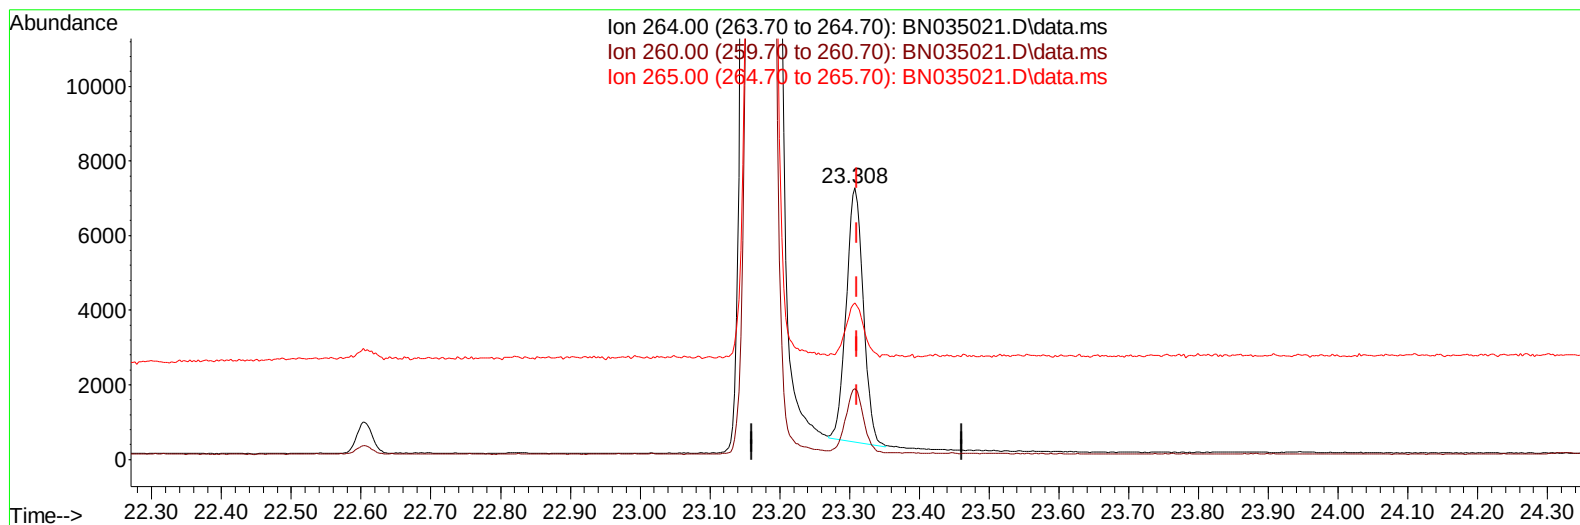

TIC: BN035021.D\data.ms

(23) Perylene-d12 (I)

23.308min (-0.003) 0.40 ng/ul m

response 11581

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	26.04
265.00	52.80	57.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035021.D
 Acq On : 12 Nov 2024 00:50
 Operator : RC/JU
 Sample : P4636-19
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CC0R8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 01:12:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.562	152	2942	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.328	136	7354	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.199	164	4886	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.945	188	10721	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240	10797	0.400	ng/ul	# 0.00
23) Perylene-d12	23.308	264	11581m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	10303	3.680	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152	3028	0.269	ng/ul	-0.01
18) Fluoranthene-d10	18.981	212	7734	0.279	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035021.D
Acq On : 12 Nov 2024 00:50
Operator : RC/JU
Sample : P4636-19
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CC0R8

Manual IntegrationsAPPROVED

Quant Time: Nov 12 01:12:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024

