




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035056.D
Acq On : 13 Nov 2024 03:46
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:17:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

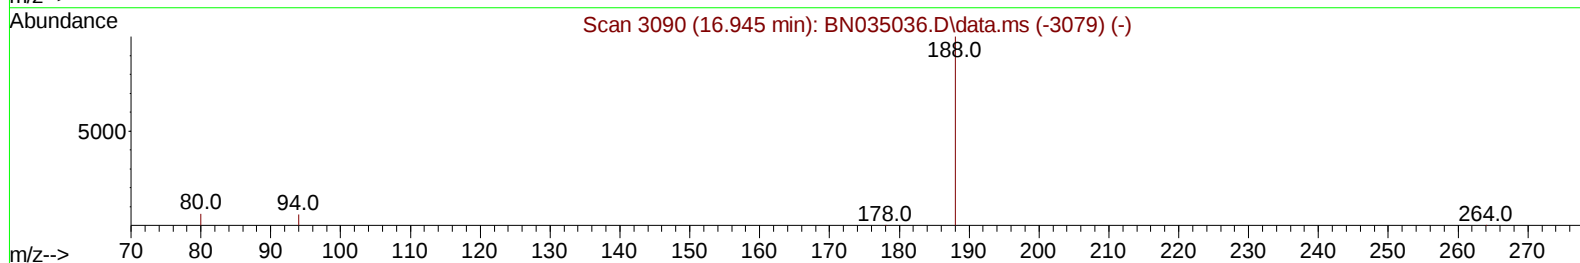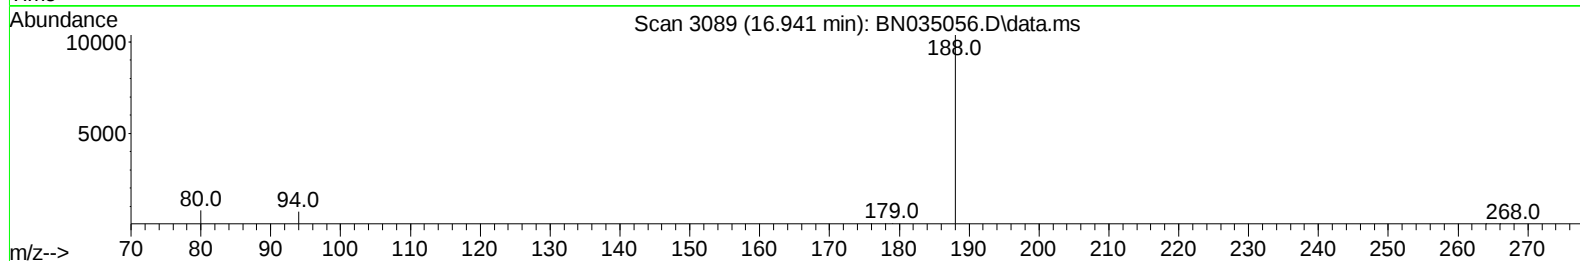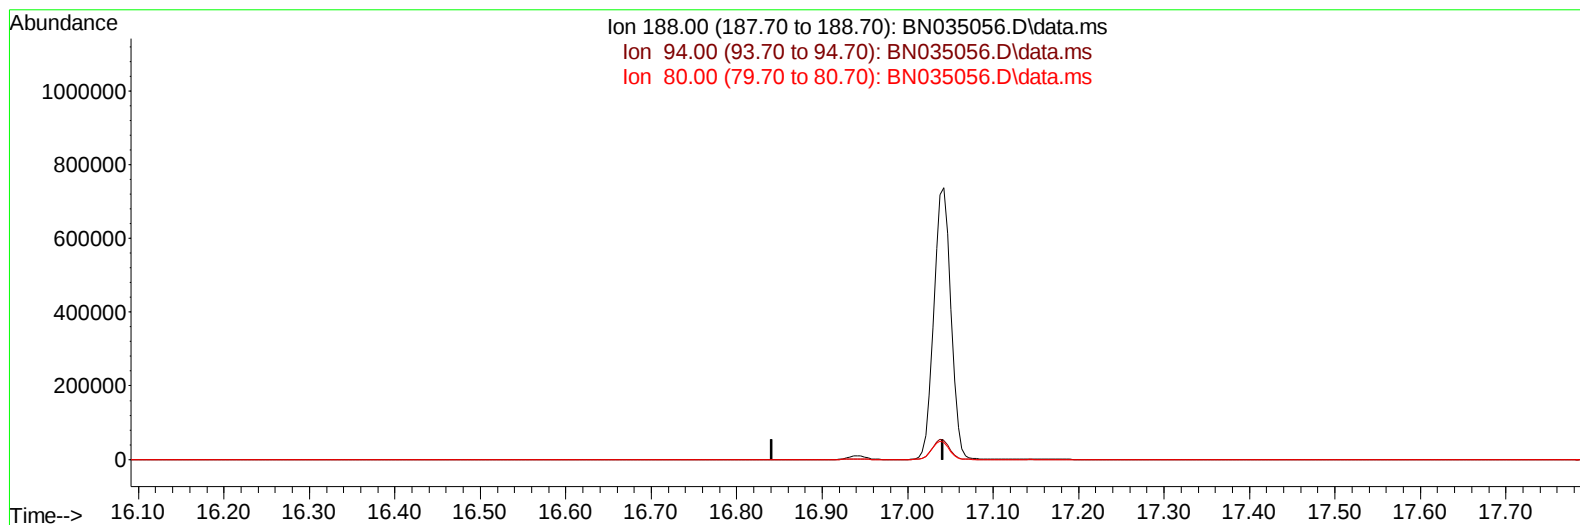

TIC: BN035056.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-16.941) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	6.10	0.00#
80.00	7.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035056.D
Acq On : 13 Nov 2024 03:46
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:17:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

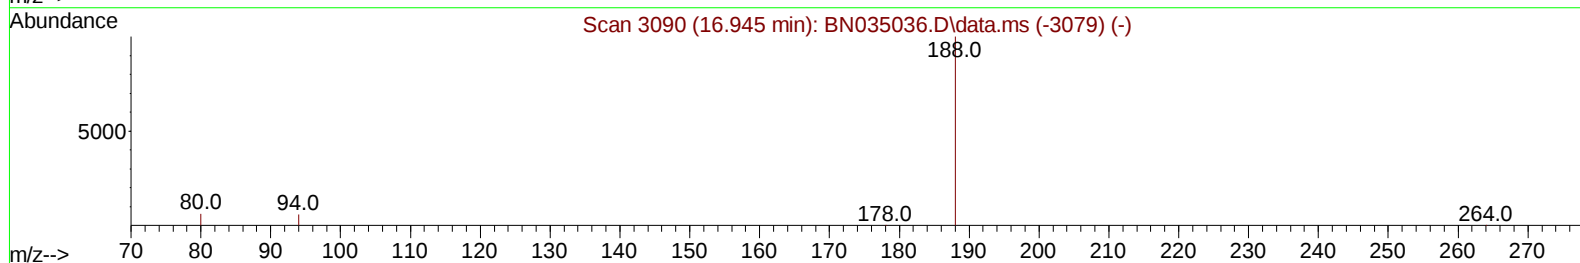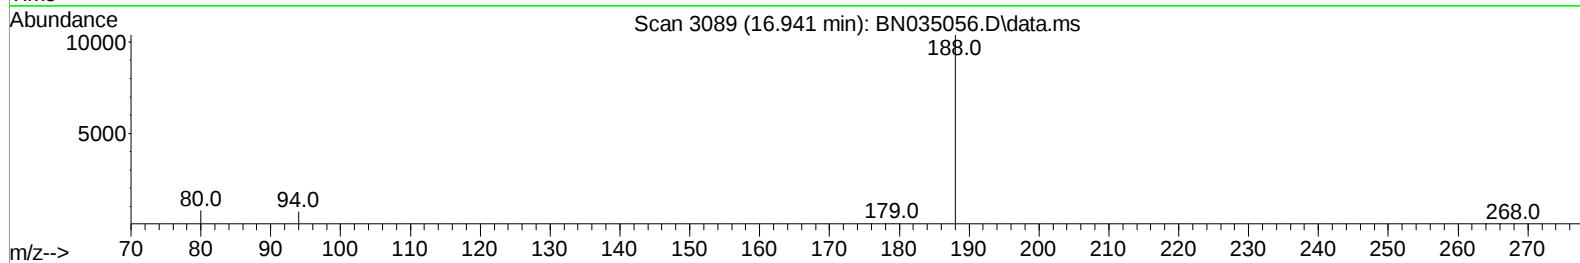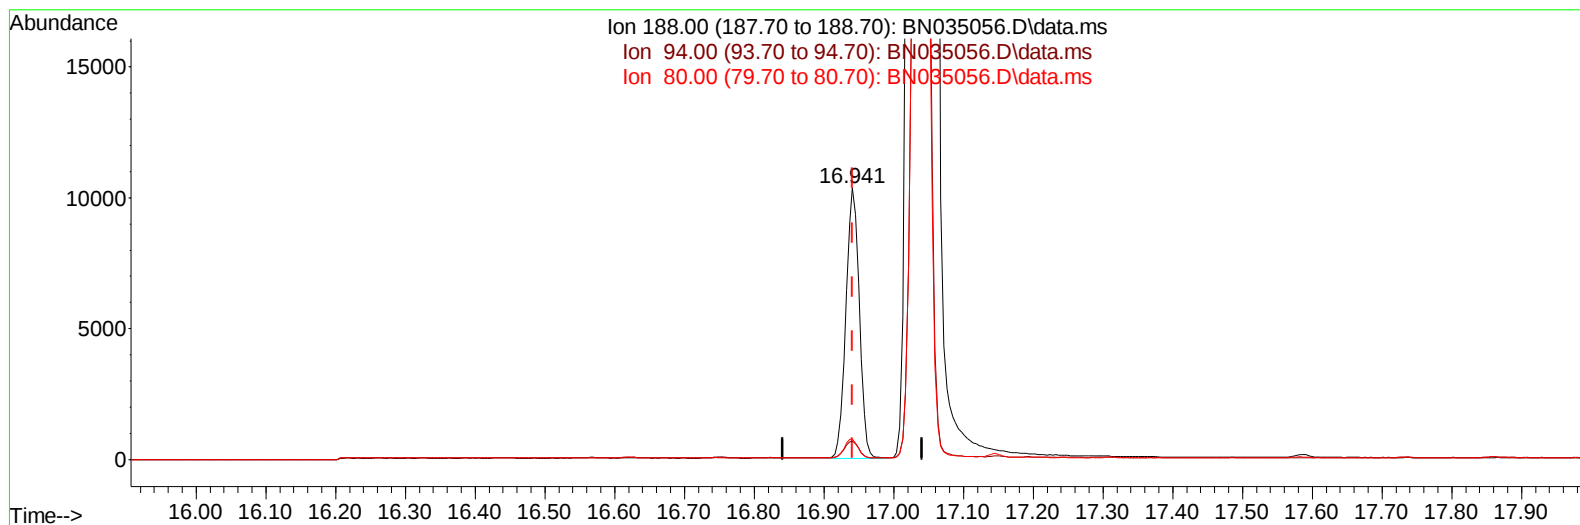

TIC: BN035056.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-0.000) 0.40 ng/ul m

response 13786

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	6.10	6.74
80.00	7.00	7.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035056.D
Acq On : 13 Nov 2024 03:46
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 04:17:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

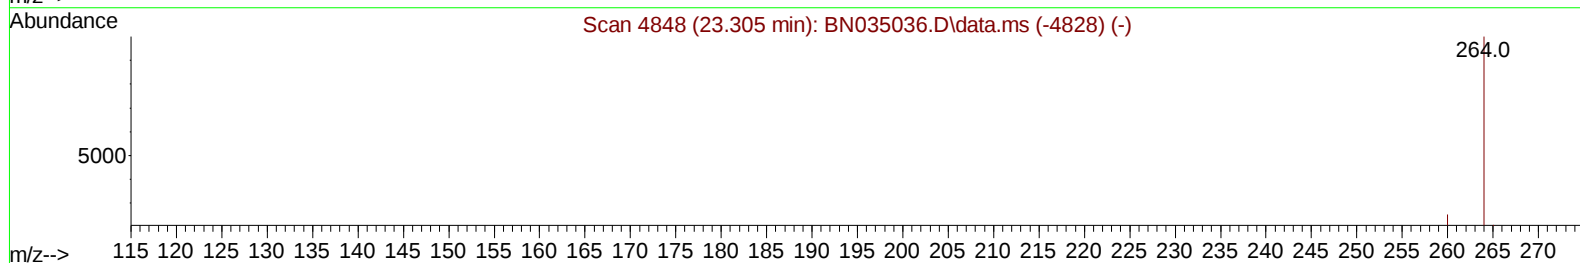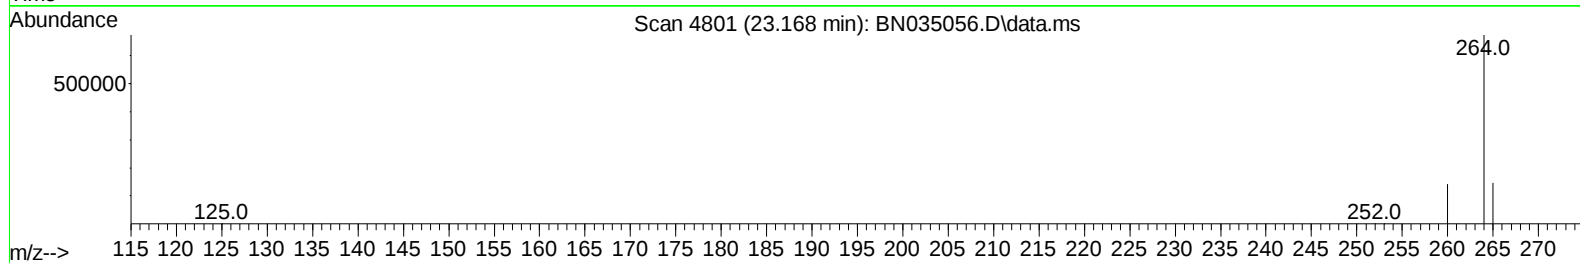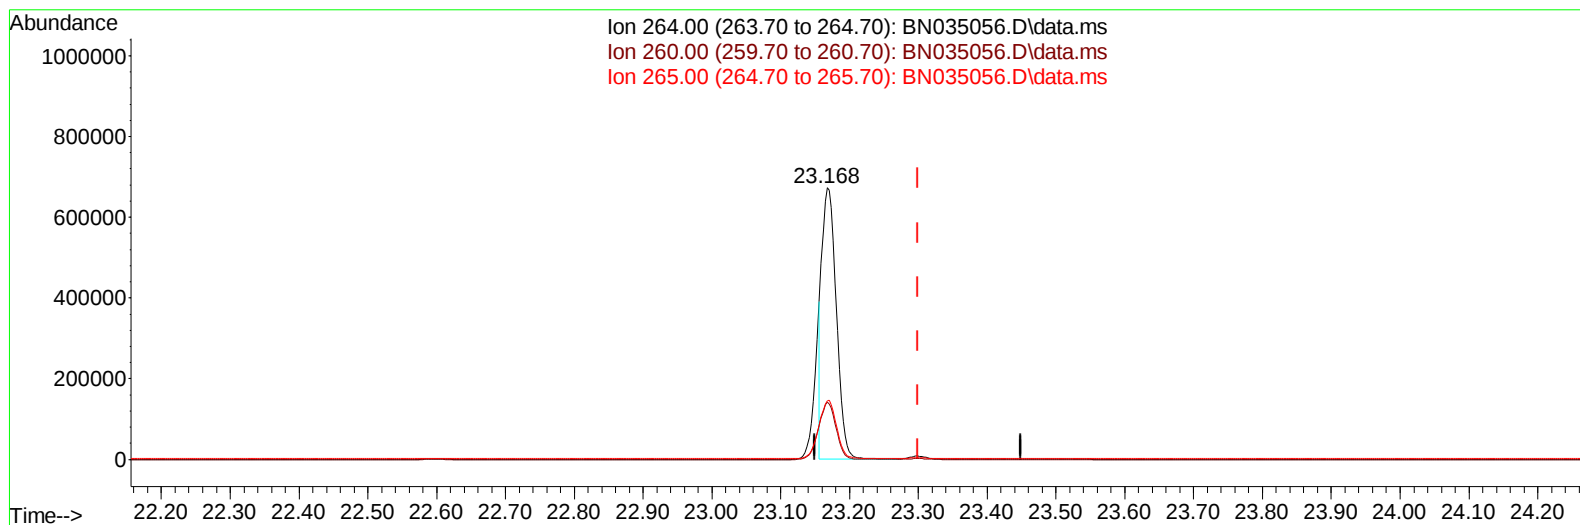

TIC: BN035056.D\data.ms

(23) Perylene-d12 (I)

23.168min (-0.132) 0.40 ng/u1

response 975375

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	21.08#
265.00	52.80	21.64#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035056.D
Acq On : 13 Nov 2024 03:46
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:17:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

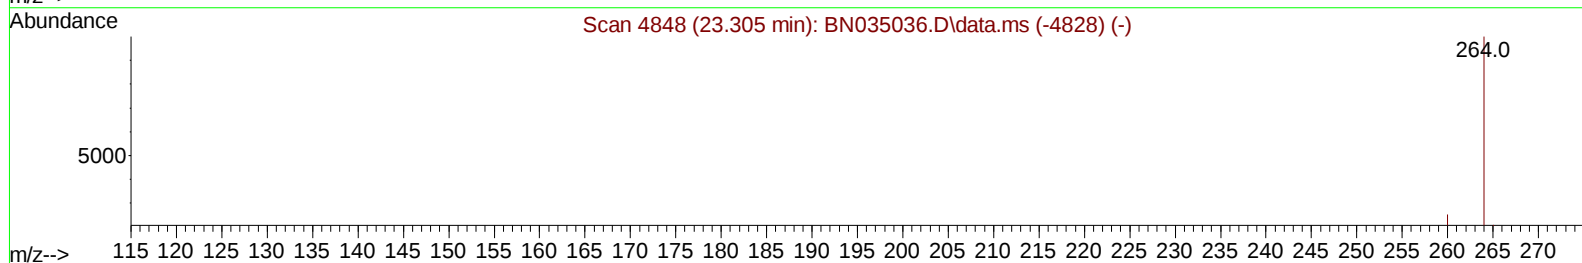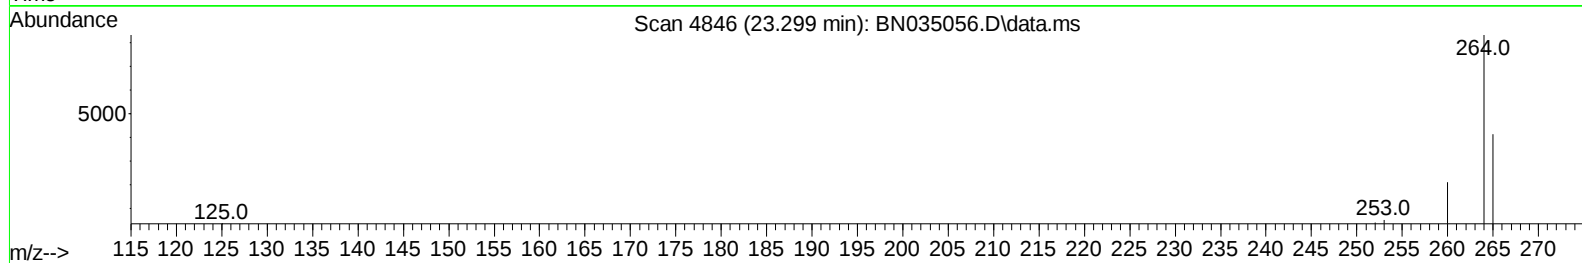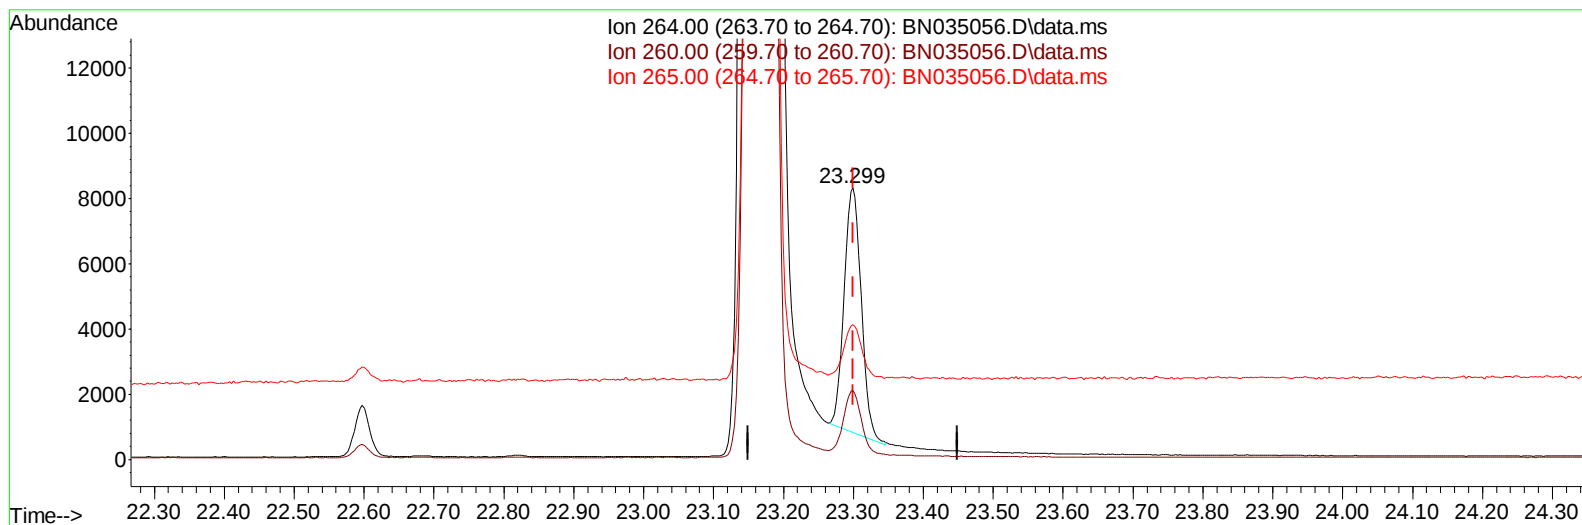

TIC: BN035056.D\data.ms

(23) Perylene-d12 (I)

23.299min (-0.000) 0.40 ng/ul m

response 12704

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.40	25.39
265.00	52.80	49.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035056.D
 Acq On : 13 Nov 2024 03:46
 Operator : RC/JU
 Sample : P4714-07
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 04:17:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 00:41:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	3569	0.400	ng/ul	0.00
4) Naphthalene-d8	10.322	136	8809	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.194	164	6149	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.941	188	13786m	0.400	ng/ul	0.00
17) Chrysene-d12	21.136	240	12639	0.400	ng/ul	# 0.00
23) Perylene-d12	23.299	264	12704m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.144	96	13446	3.959	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.917	152	4101	0.304	ng/ul	0.00
18) Fluoranthene-d10	18.972	212	14529	0.448	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035056.D
Acq On : 13 Nov 2024 03:46
Operator : RC/JU
Sample : P4714-07
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AG4

Manual IntegrationsAPPROVED

Quant Time: Nov 13 04:17:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

