

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035023.D
 Acq On : 12 Nov 2024 02:02
 Operator : RC/JU
 Sample : P4717-07
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF0

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 02:40:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.562	152	3199	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.328	136	7655	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.199	164	5137	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.945	188	11093m	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240	10695	0.400	ng/ul	# 0.00
23) Perylene-d12	23.308	264	11123m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	12894	4.236	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152	3676	0.314	ng/ul	-0.01
18) Fluoranthene-d10	18.981	212	12225	0.445	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.182	88	527	0.158	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035023.D
Acq On : 12 Nov 2024 02:02
Operator : RC/JU
Sample : P4717-07
Misc :
ALS Vial : 33 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AF0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024


Quant Time: Nov 12 02:40:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

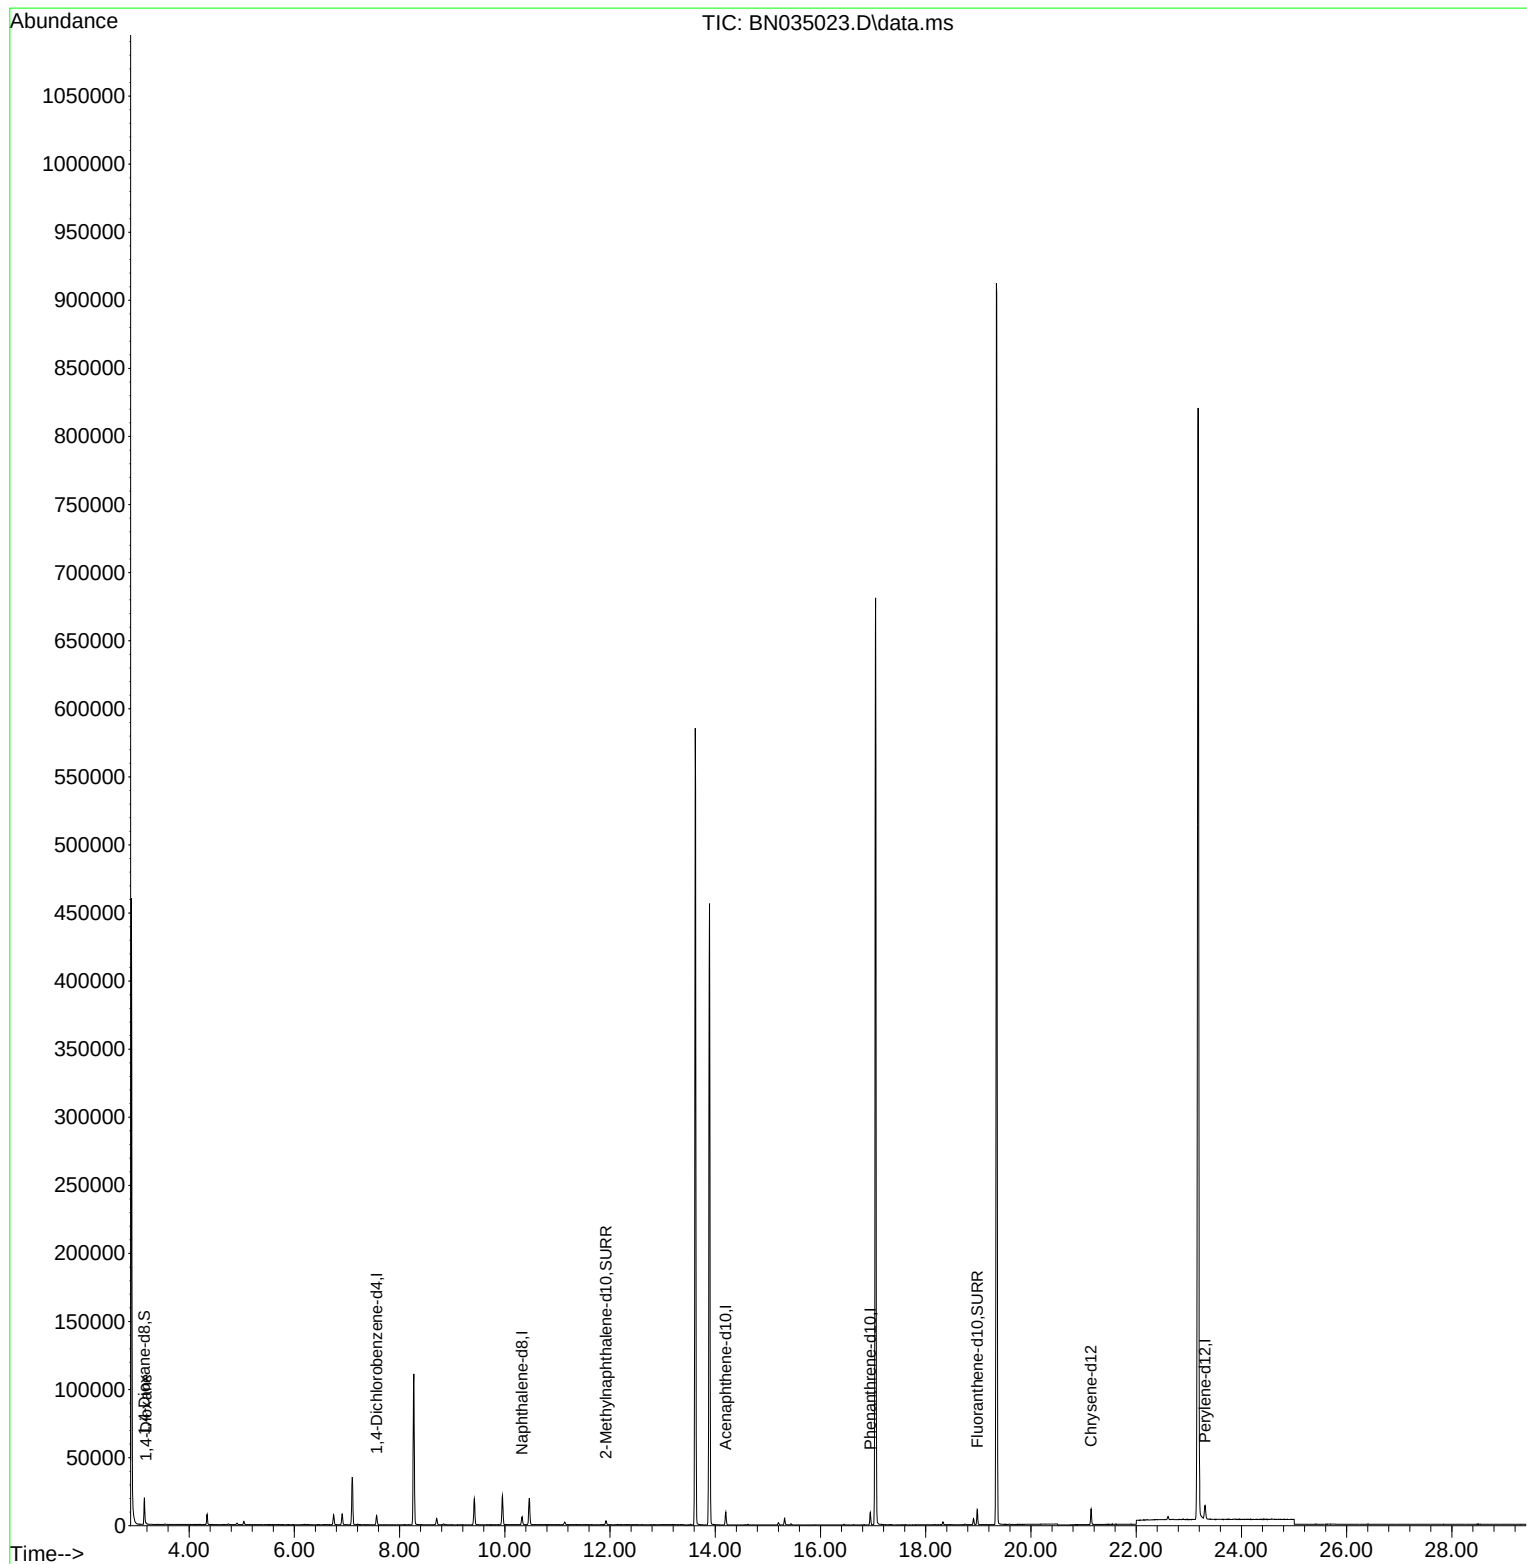

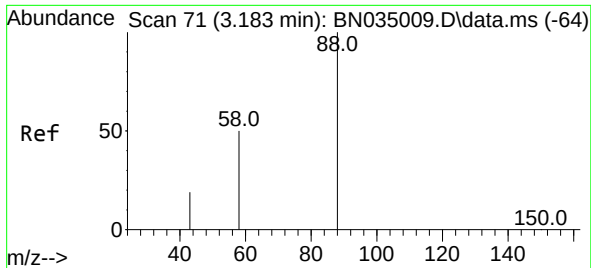

#2
 1,4-Dioxane
 Concen: 0.158 ng/ul
 RT: 3.182 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BN035023.D
 Acq: 12 Nov 2024 02:02

Instrument :
 BNA_N
 ClientSampleId :
 C0AF0

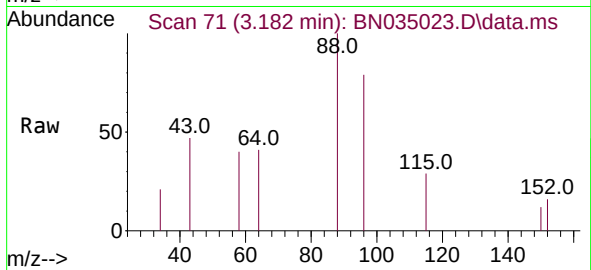

Tgt Ion: 88 Resp: 52

Ion	Ratio	Lower	Upper
88	100		
43	46.8	23.3	34.9
58	40.1	35.4	53.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

