

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035024.D
 Acq On : 12 Nov 2024 02:38
 Operator : RC/JU
 Sample : P4717-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AF1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 03:02:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.562	152	3214	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.328	136	8094	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.199	164	5245	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.945	188	10611m	0.400	ng/ul	0.00
17) Chrysene-d12	21.142	240	9569	0.400	ng/ul	# 0.00
23) Perylene-d12	23.308	264	10036m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13339	4.362	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.923	152	4123	0.333	ng/ul	-0.01
18) Fluoranthene-d10	18.977	212	11729	0.477	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.182	88	5528	1.649	ng/ul#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035024.D
Acq On : 12 Nov 2024 02:38
Operator : RC/JU
Sample : P4717-08
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AF1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/12/2024
Supervised By :mohammad ahmed 11/14/2024


Quant Time: Nov 12 03:02:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

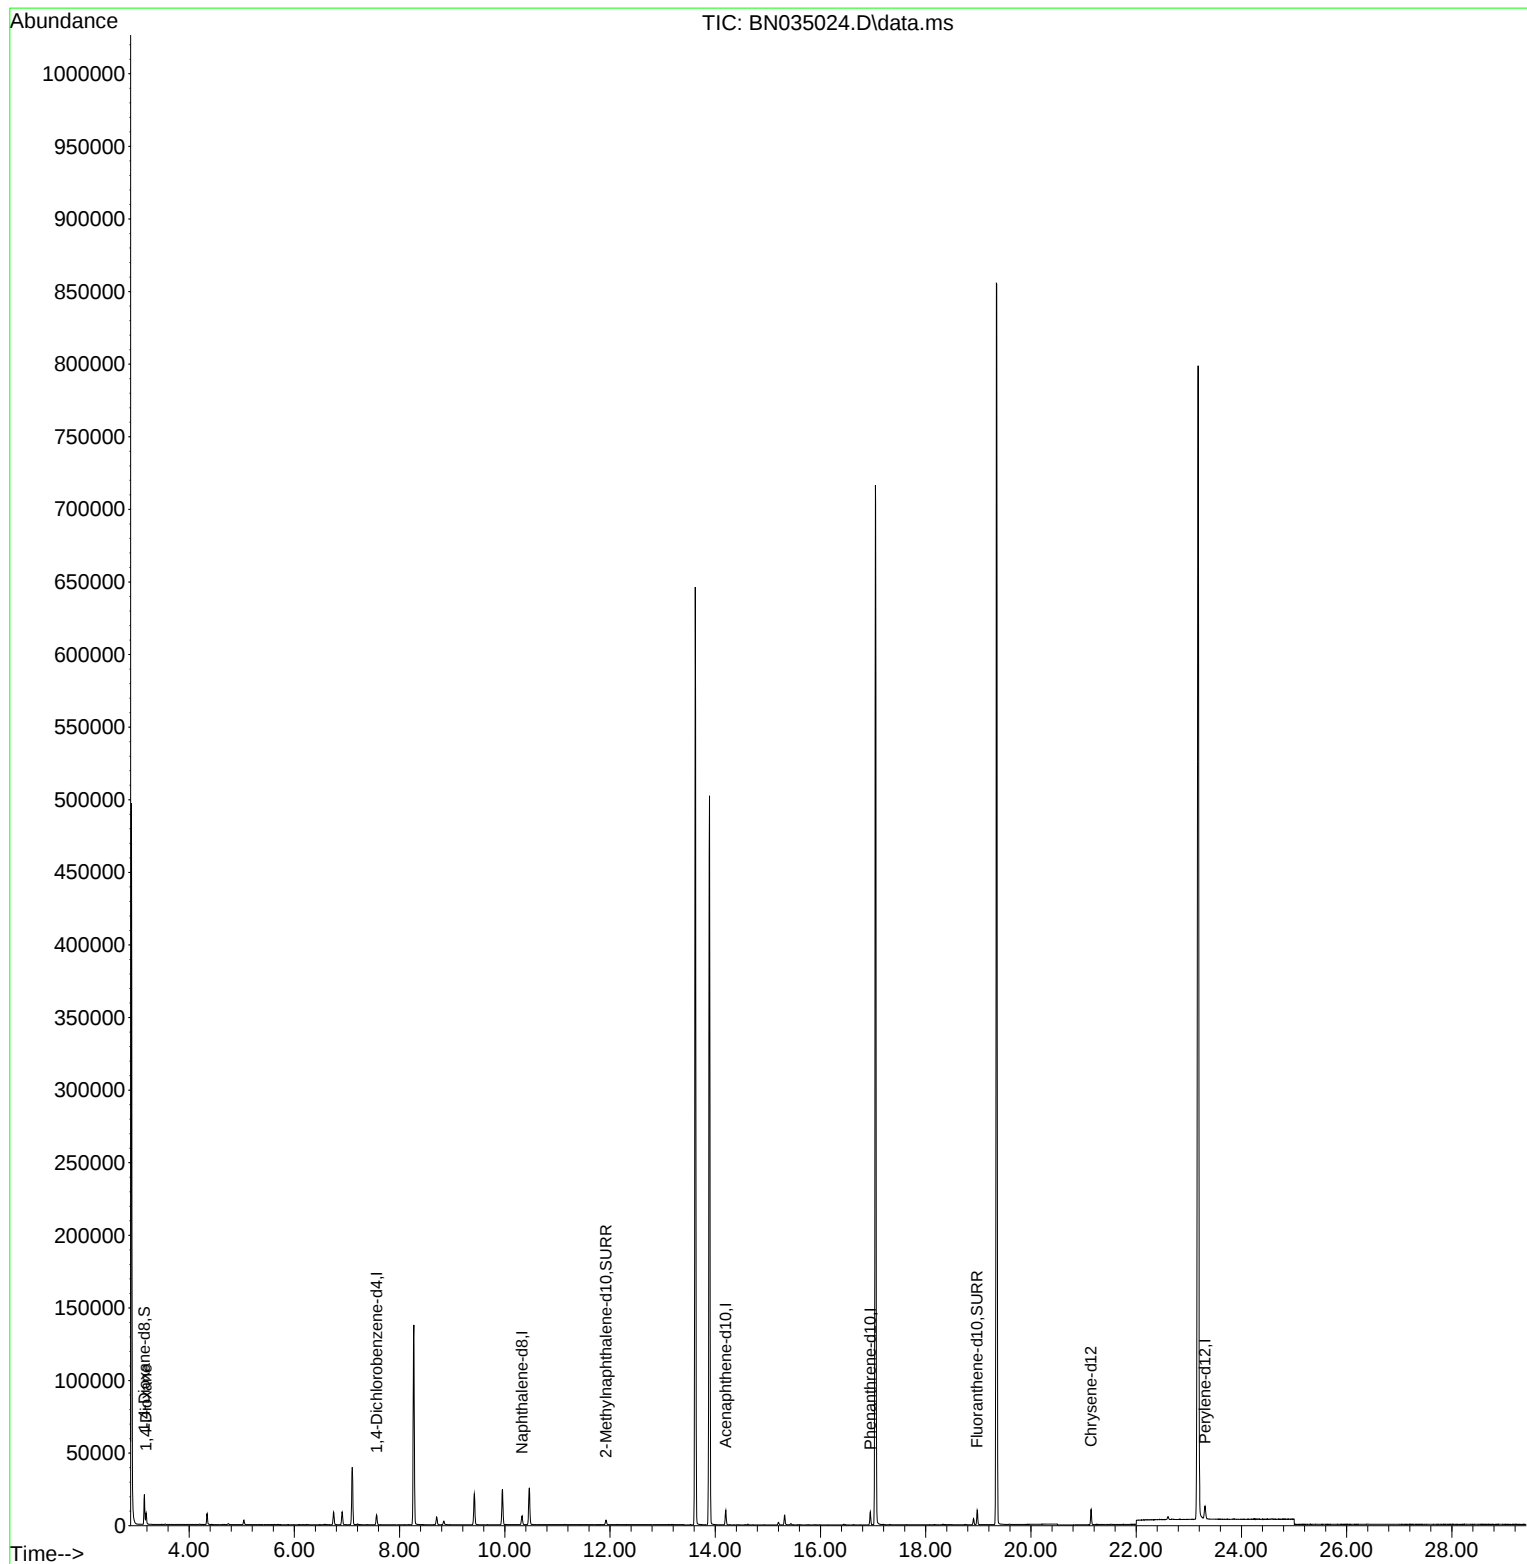

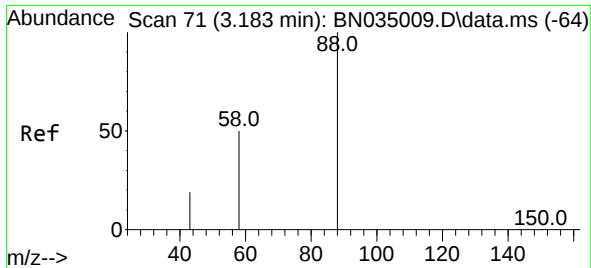

#2
 1,4-Dioxane
 Concen: 1.649 ng/ul
 RT: 3.182 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BN035024.D
 Acq: 12 Nov 2024 02:38

Instrument :
 BNA_N
 ClientSampleId :
 C0AF1

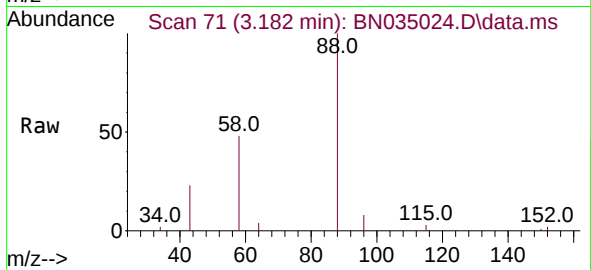

Tgt Ion: 88 Resp: 5528
 Ion Ratio Lower Upper
 88 100
 43 23.0 23.3 34.9
 58 47.7 35.4 53.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/12/2024
 Supervised By :mohammad ahmed 11/14/2024

