

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035033.D
 Acq On : 12 Nov 2024 12:50
 Operator : RC/JU
 Sample : P4714-16
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 14:54:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.562	152	3117	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.322	136	7599	0.400	ng/u1	-0.02
9) Acenaphthene-d10	14.199	164	5145	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.945	188	11401m	0.400	ng/u1	0.00
17) Chrysene-d12	21.139	240	10244	0.400	ng/u1	# 0.00
23) Perylene-d12	23.302	264	10525m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	12184	4.108	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.923	152	3171	0.272	ng/u1	-0.01
18) Fluoranthene-d10	18.977	212	11438	0.435	ng/u1	0.00
Target Compounds						Qvalue
7) 2-Methylnaphthalene	11.994	142	494	0.035	ng/u1	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035033.D
Acq On : 12 Nov 2024 12:50
Operator : RC/JU
Sample : P4714-16
Misc :
ALS Vial : 51 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AJ1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024


Quant Time: Nov 12 14:54:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

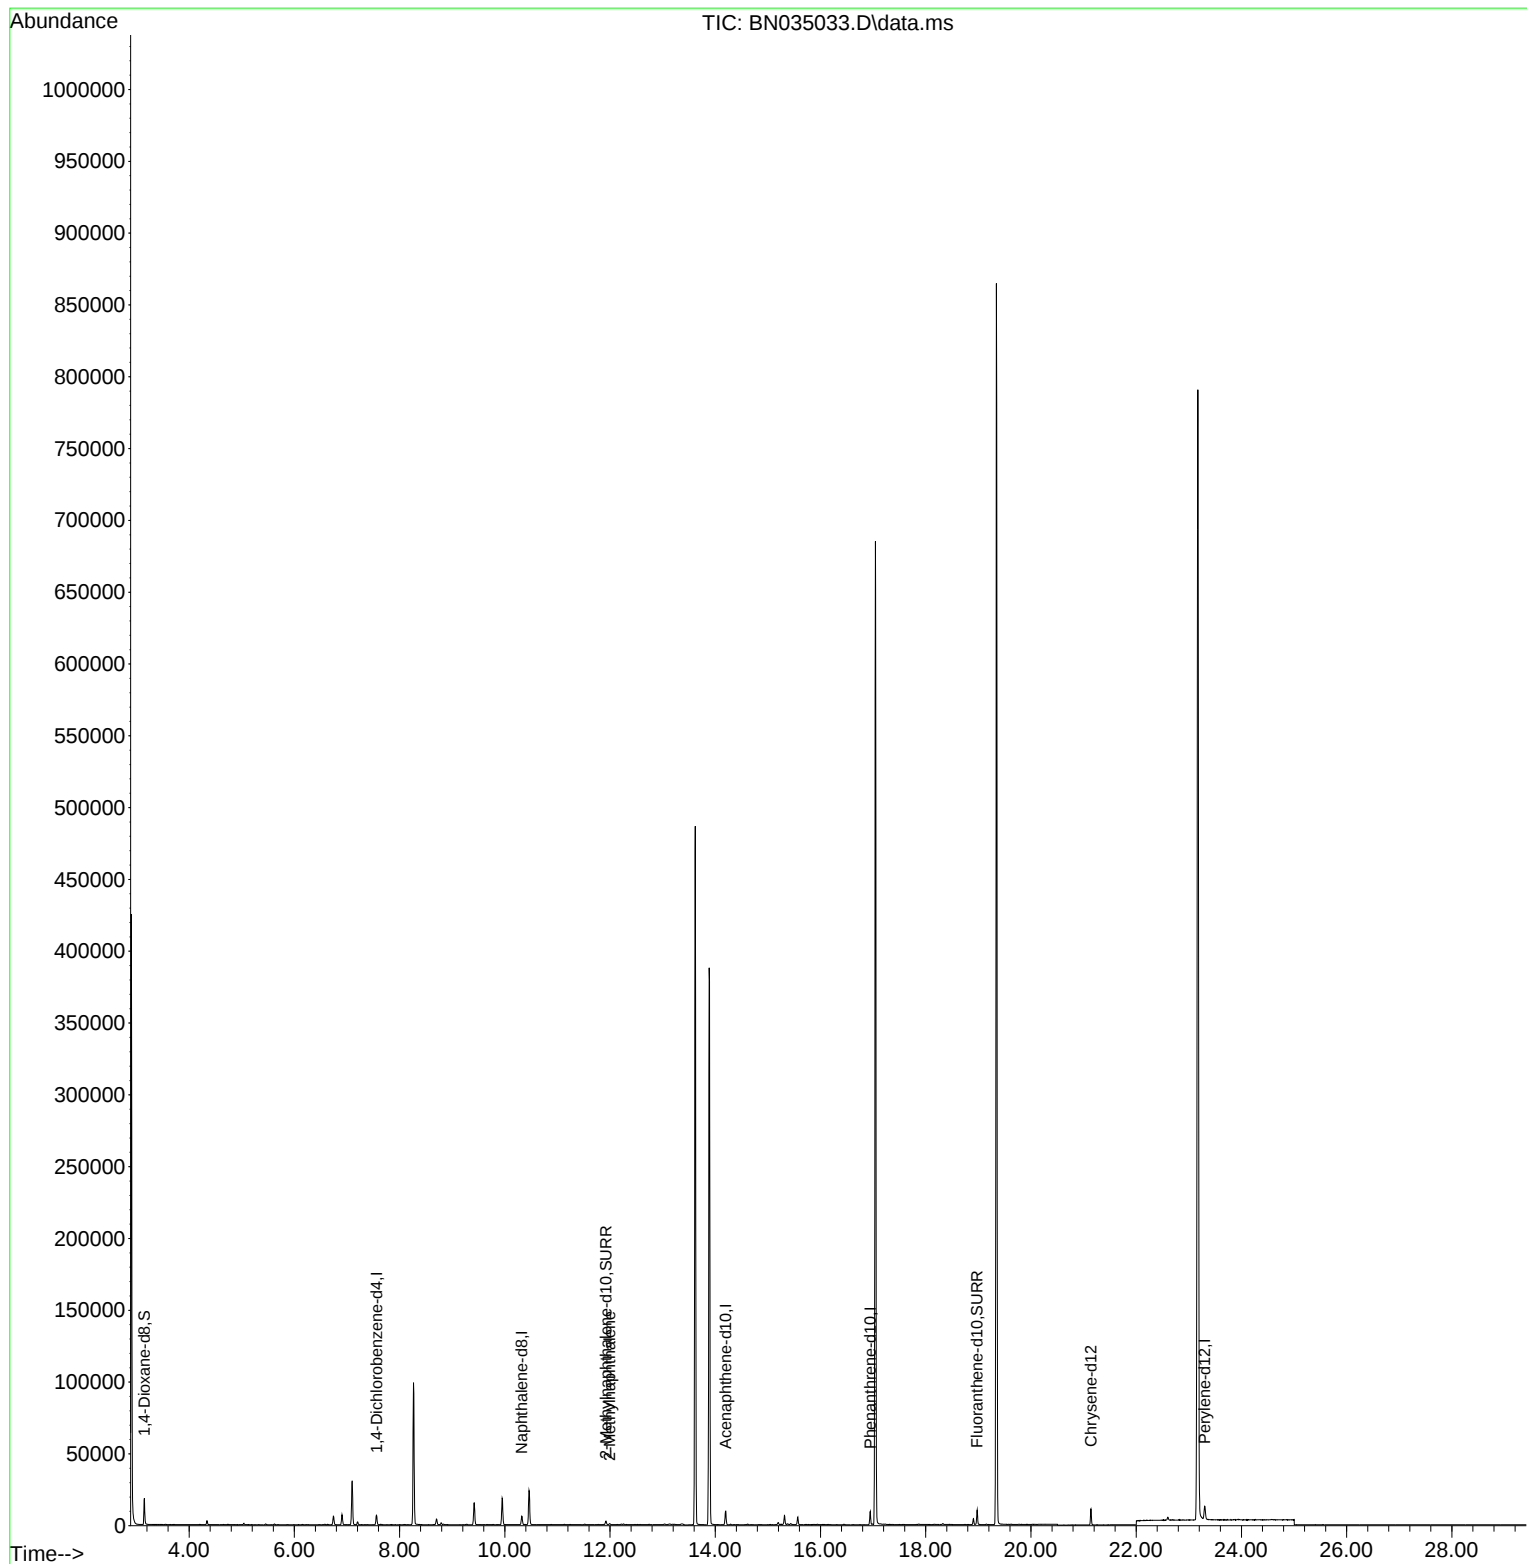

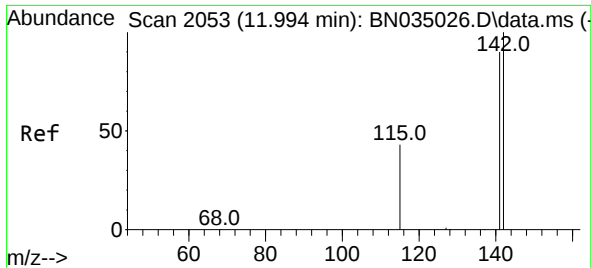

#7
 2-Methylnaphthalene
 Concen: 0.035 ng/ul
 RT: 11.994 min Scan# 2053
 Delta R.T. -0.016 min
 Lab File: BN035033.D
 Acq: 12 Nov 2024 12:50

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ1

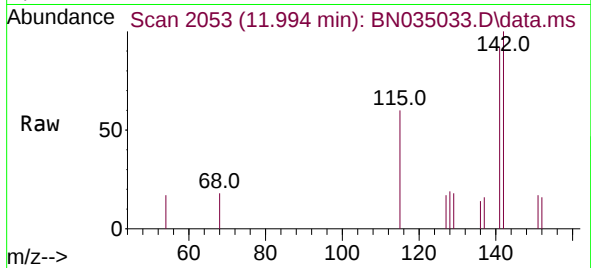

Tgt Ion:142 Resp: 494
 Ion Ratio Lower Upper
 142 100
 141 91.3 70.8 106.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

