

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035038.D
 Acq On : 12 Nov 2024 16:25
 Operator : RC/JU
 Sample : P4714-08
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AG6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 17:08:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.562	152	3503	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.322	136	8589	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.194	164	5907	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.945	188	12999m	0.400	ng/ul	0.00
17) Chrysene-d12	21.139	240	11648	0.400	ng/ul	0.00
23) Perylene-d12	23.305	264	11789m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	12427	3.728	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.917	152	3992	0.303	ng/ul	-0.02
18) Fluoranthene-d10	18.977	212	14124	0.472	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.372	128	746	0.035	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035038.D
Acq On : 12 Nov 2024 16:25
Operator : RC/JU
Sample : P4714-08
Misc :
ALS Vial : 57 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AG6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024


Quant Time: Nov 12 17:08:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

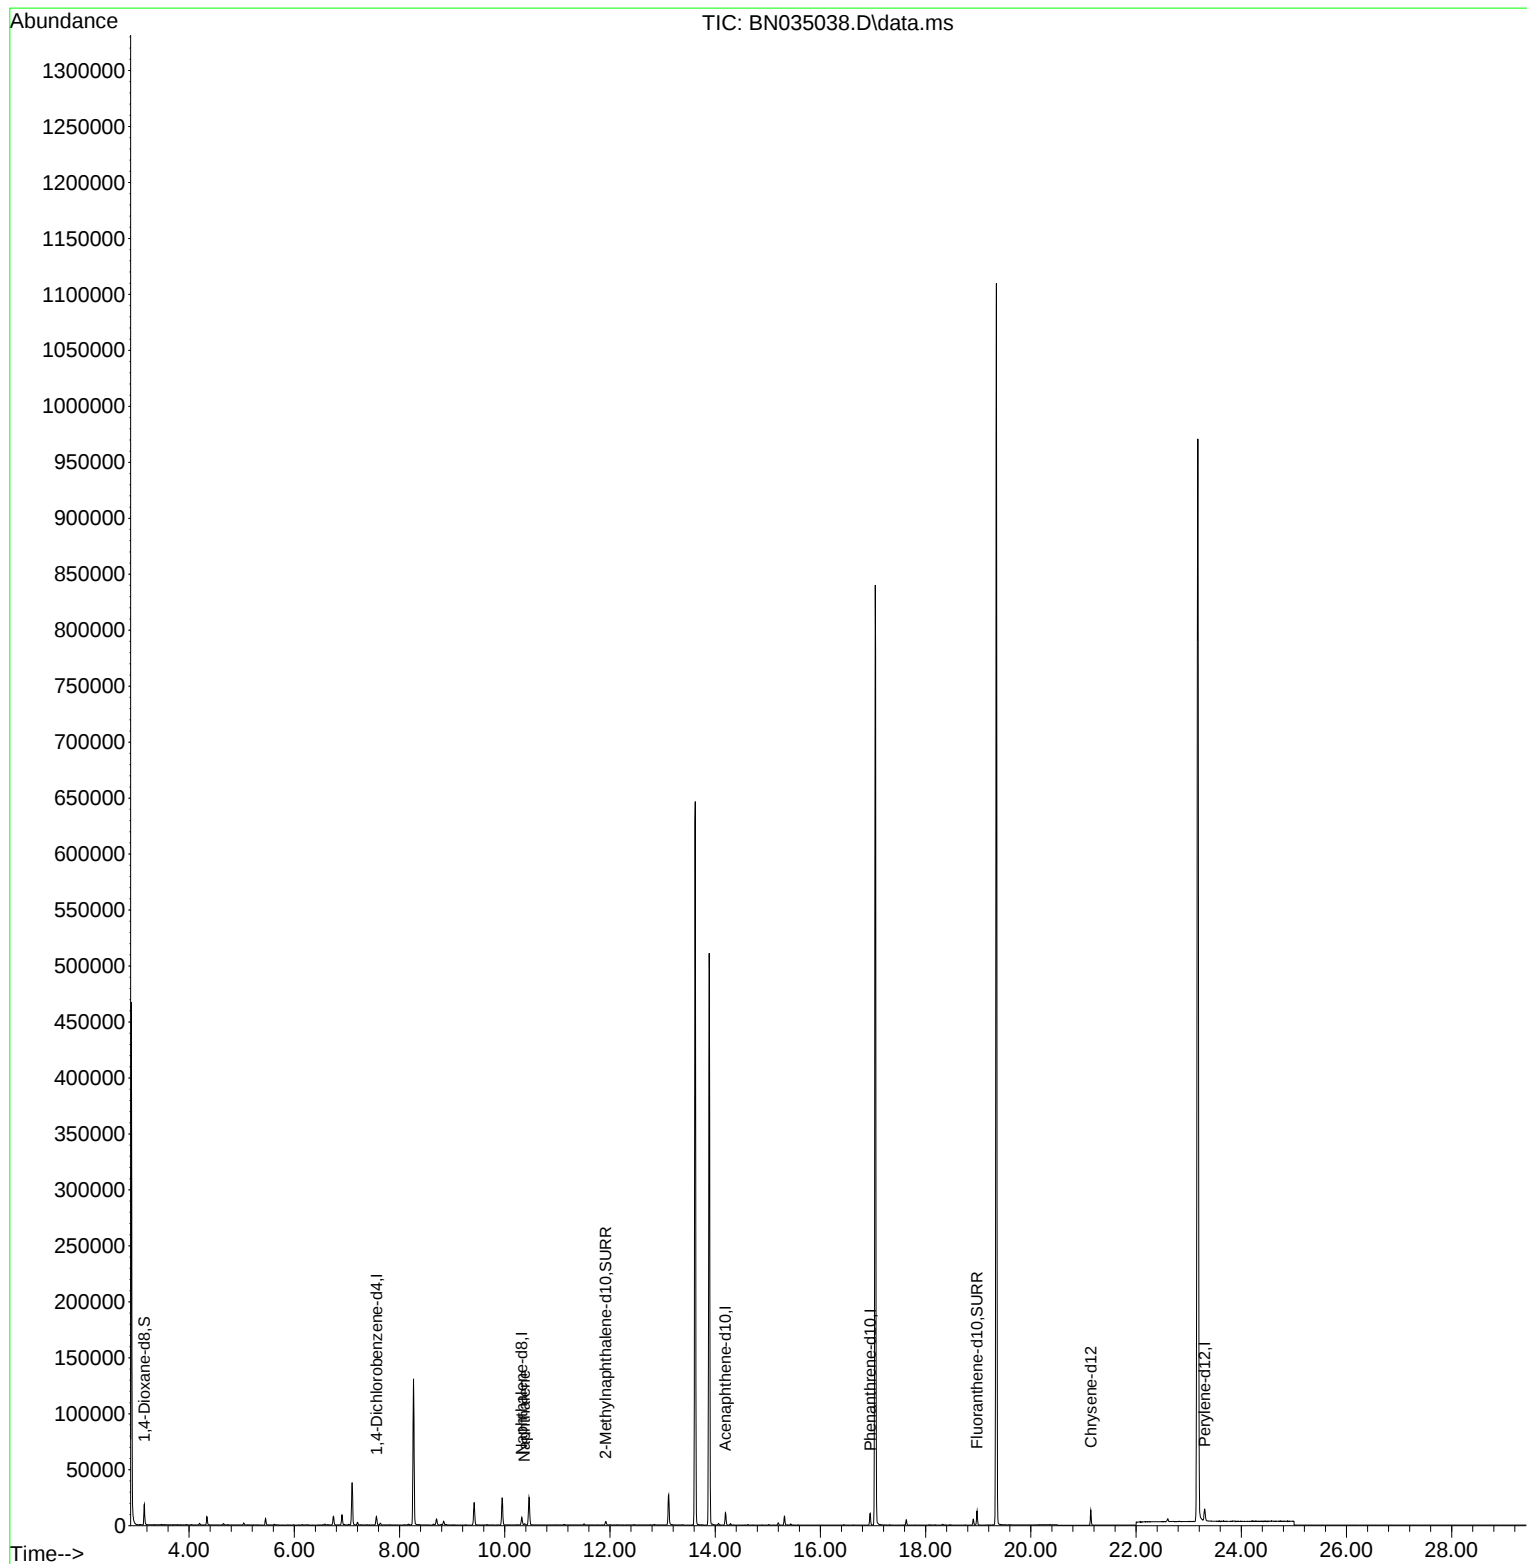

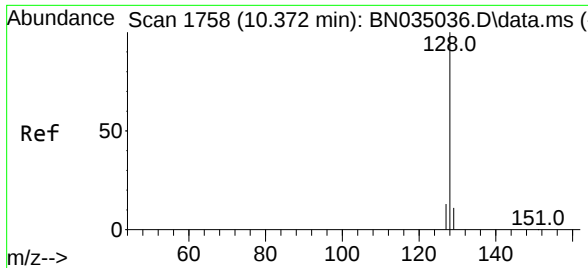

#5
Naphthalene
Concen: 0.035 ng/ul
RT: 10.372 min Scan# 11
Delta R.T. -0.016 min
Lab File: BN035038.D
Acq: 12 Nov 2024 16:25

Instrument :
BNA_N
ClientSampleId :
C0AG6

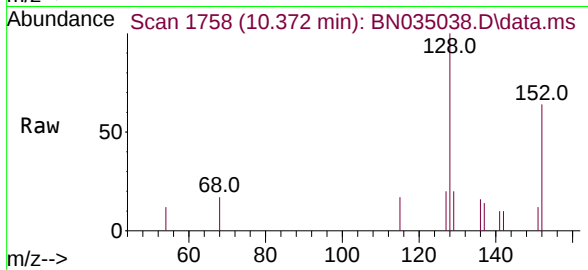

Tgt Ion:128 Resp: 740
Ion Ratio Lower Upper
128 100
129 19.5 10.1 15.1
127 20.3 12.1 18.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

