

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035041.D
 Acq On : 12 Nov 2024 18:13
 Operator : RC/JU
 Sample : P4714-18
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ5

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 21:56:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	3370	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.322	136	8337	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.194	164	5819	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.945	188	12680m	0.400	ng/ul	0.00
17) Chrysene-d12	21.139	240	11803	0.400	ng/ul	# 0.00
23) Perylene-d12	23.305	264	12114m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	13176	4.109	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.917	152	3827	0.300	ng/ul	-0.02
18) Fluoranthene-d10	18.977	212	14598	0.482	ng/ul	0.00
Target Compounds						
5) Naphthalene	10.372	128	733	0.035	ng/ul#	Qvalue 79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035041.D
Acq On : 12 Nov 2024 18:13
Operator : RC/JU
Sample : P4714-18
Misc :
ALS Vial : 60 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AJ5

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024


Quant Time: Nov 12 21:56:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

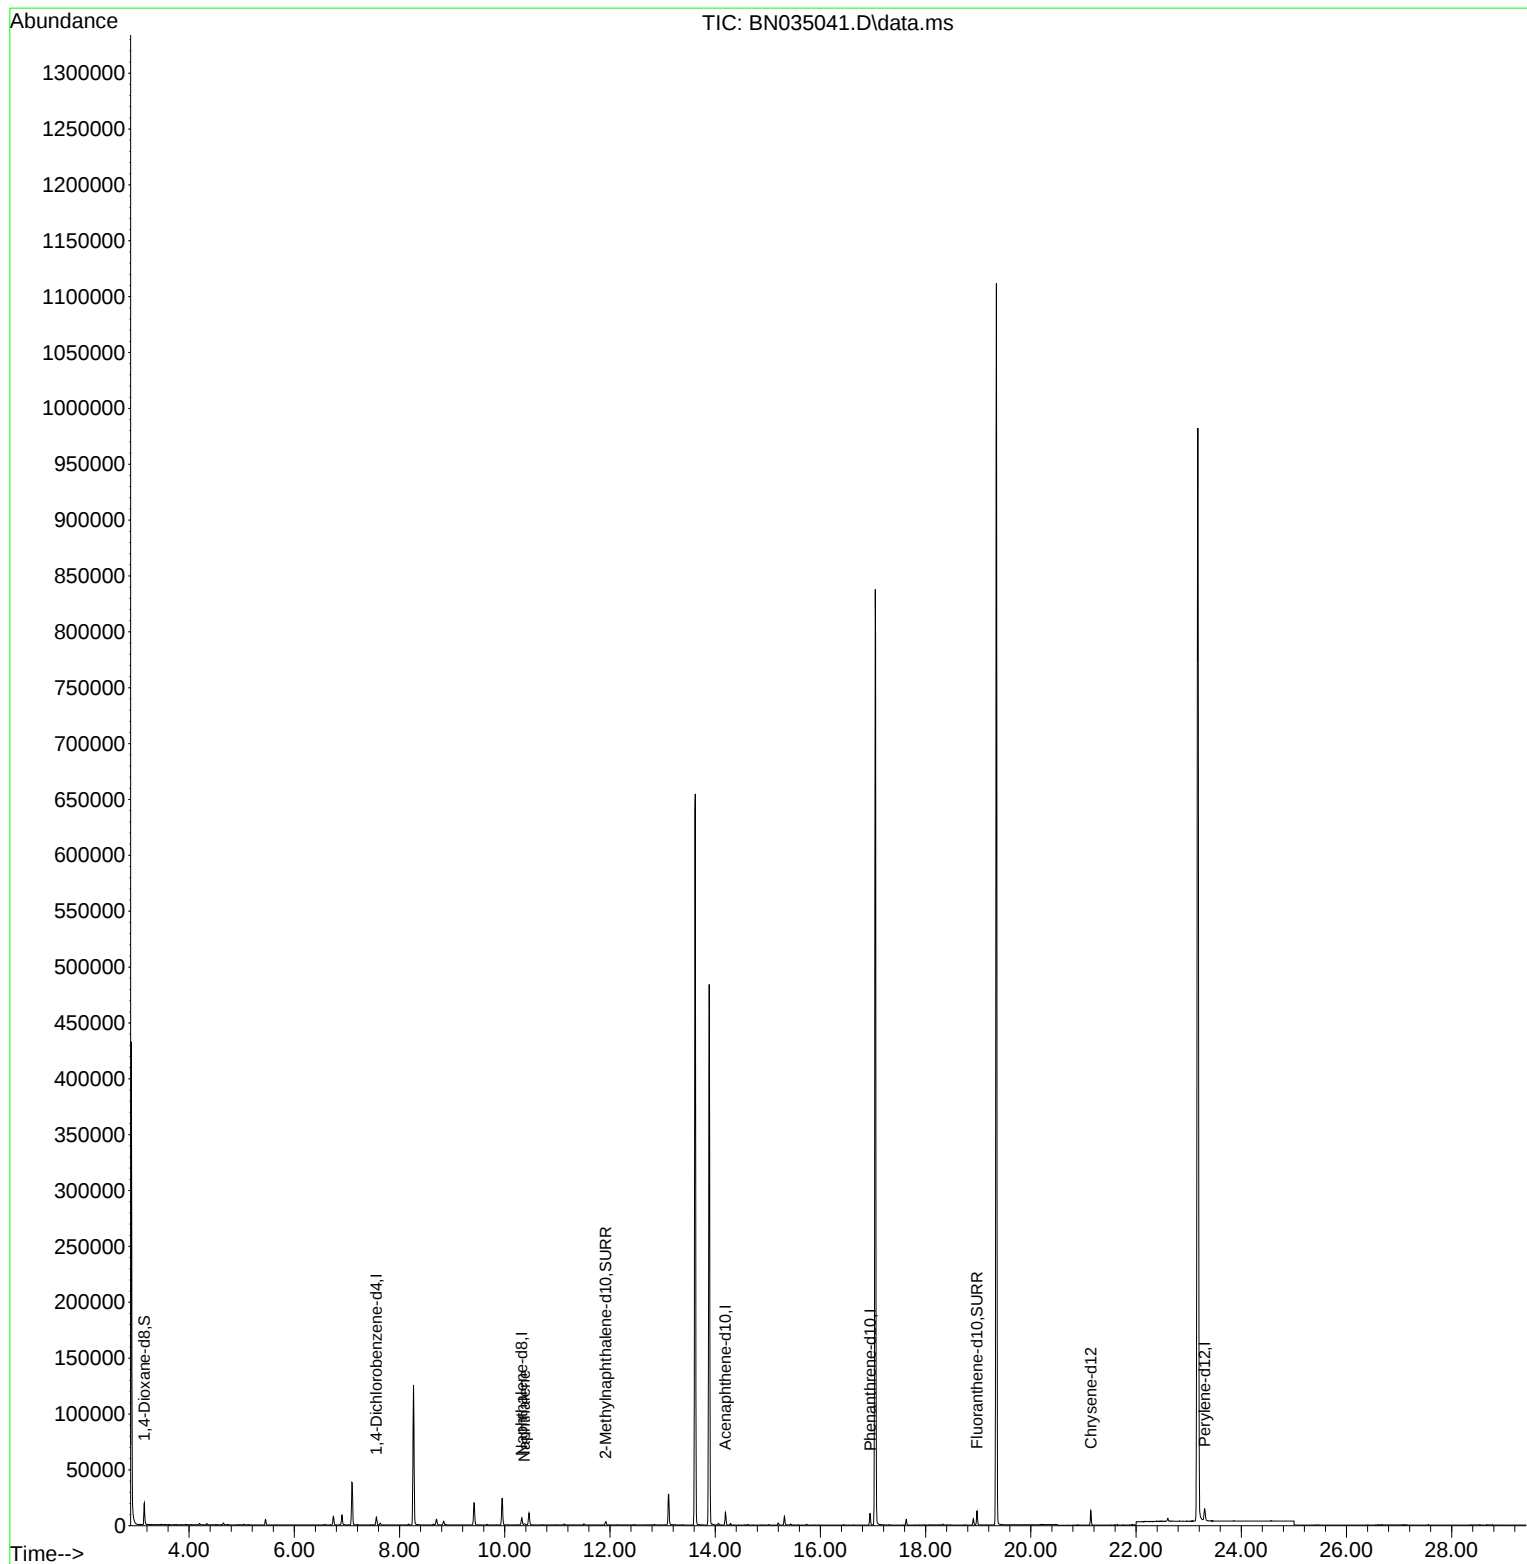

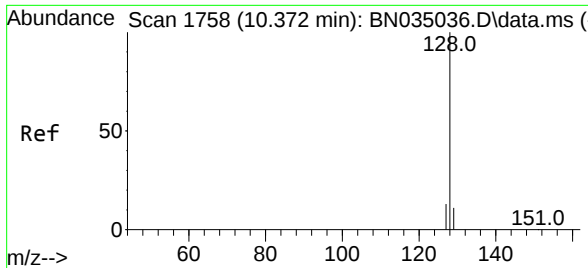

#5
Naphthalene
Concen: 0.035 ng/ul
RT: 10.372 min Scan# 1758
Delta R.T. -0.016 min
Lab File: BN035041.D
Acq: 12 Nov 2024 18:13

Instrument :
BNA_N
ClientSampleId :
C0AJ5

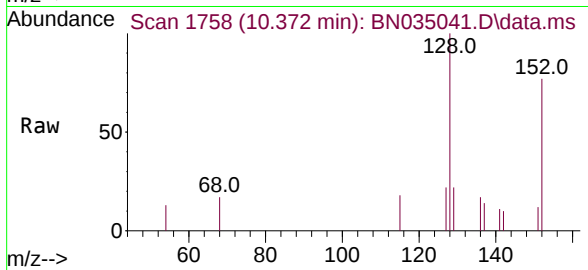

Tgt Ion:	128	Resp:	73
Ion	Ratio	Lower	Upper
128	100		
129	22.4	10.1	15.1
127	22.4	12.1	18.1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

