

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035042.D
 Acq On : 12 Nov 2024 18:49
 Operator : RC/JU
 Sample : P4717-01
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 12 21:56:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 09 00:09:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	3212	0.400	ng/u1	-0.02
4) Naphthalene-d8	10.322	136	7951	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.194	164	5449	0.400	ng/u1	-0.01
13) Phenanthrene-d10	16.945	188	12045m	0.400	ng/u1	0.00
17) Chrysene-d12	21.140	240	11024	0.400	ng/u1	# 0.00
23) Perylene-d12	23.305	264	11314m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.149	96	12608	4.125	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.917	152	3891	0.320	ng/u1	-0.02
18) Fluoranthene-d10	18.977	212	14162	0.500	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.182	88	4035	1.205	ng/u1#	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035042.D
Acq On : 12 Nov 2024 18:49
Operator : RC/JU
Sample : P4717-01
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AE4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :mohammad ahmed 11/14/2024


Quant Time: Nov 12 21:56:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 09 00:09:12 2024
Response via : Initial Calibration

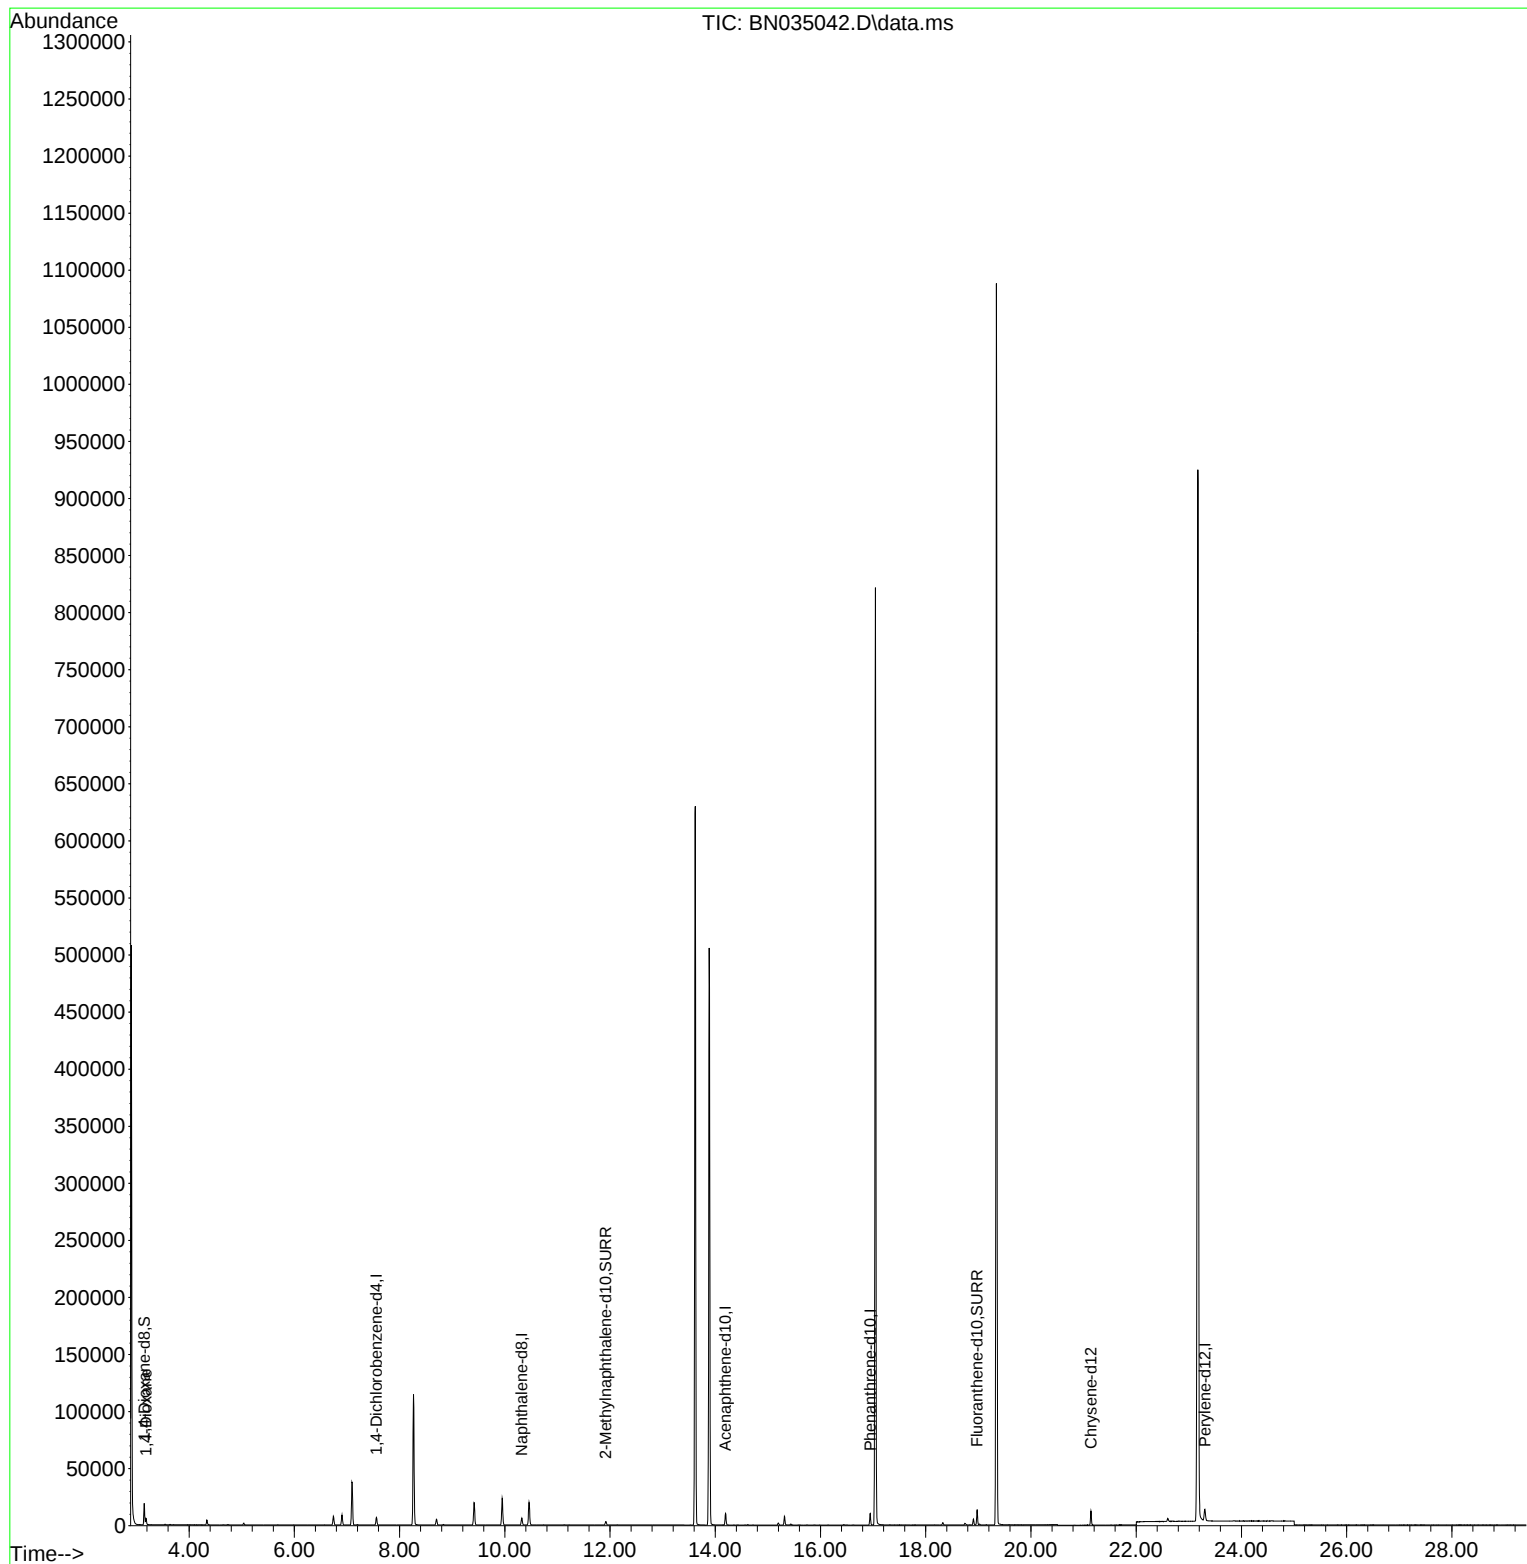

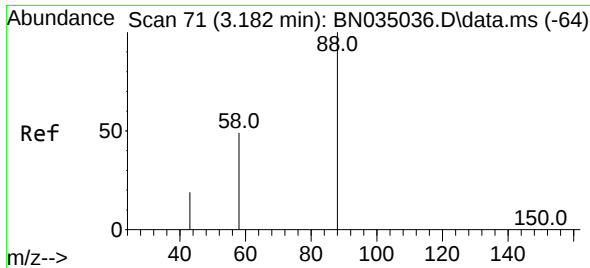

#2
 1,4-Dioxane
 Concen: 1.205 ng/ul
 RT: 3.182 min Scan# 71
 Delta R.T. -0.004 min
 Lab File: BN035042.D
 Acq: 12 Nov 2024 18:49

Instrument :
 BNA_N
 ClientSampleId :
 C0AE4

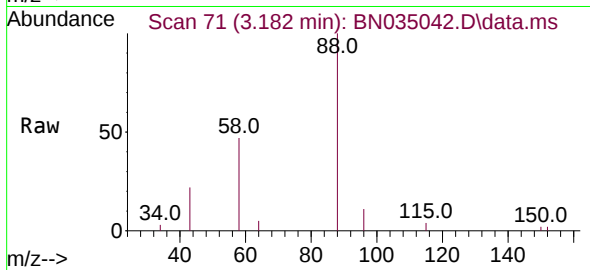

Tgt Ion: 88 Resp: 4035
 Ion Ratio Lower Upper
 88 100
 43 22.1 23.3 34.9
 58 46.8 35.4 53.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

