

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
 Data File : BN035052.D
 Acq On : 13 Nov 2024 01:23
 Operator : RC/JU
 Sample : P4668-06
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 11/13/2024
 Supervised By :mohammad ahmed 11/14/2024

Quant Time: Nov 13 01:45:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 00:41:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.558	152	3659	0.400	ng/ul	0.00
4) Naphthalene-d8	10.322	136	9184	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.194	164	6499	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.941	188	14274m	0.400	ng/ul	0.00
17) Chrysene-d12	21.136	240	13480	0.400	ng/ul	# 0.00
23) Perylene-d12	23.302	264	13382m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.144	96	16681	4.791	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.917	152	4716	0.335	ng/ul	0.00
18) Fluoranthene-d10	18.976	212	13707	0.396	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.372	128	917	0.040	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111124\
Data File : BN035052.D
Acq On : 13 Nov 2024 01:23
Operator : RC/JU
Sample : P4668-06
Misc :
ALS Vial : 72 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0AE2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/13/2024
Supervised By :mohammad ahmed 11/14/2024


Quant Time: Nov 13 01:45:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN110924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 00:41:17 2024
Response via : Initial Calibration

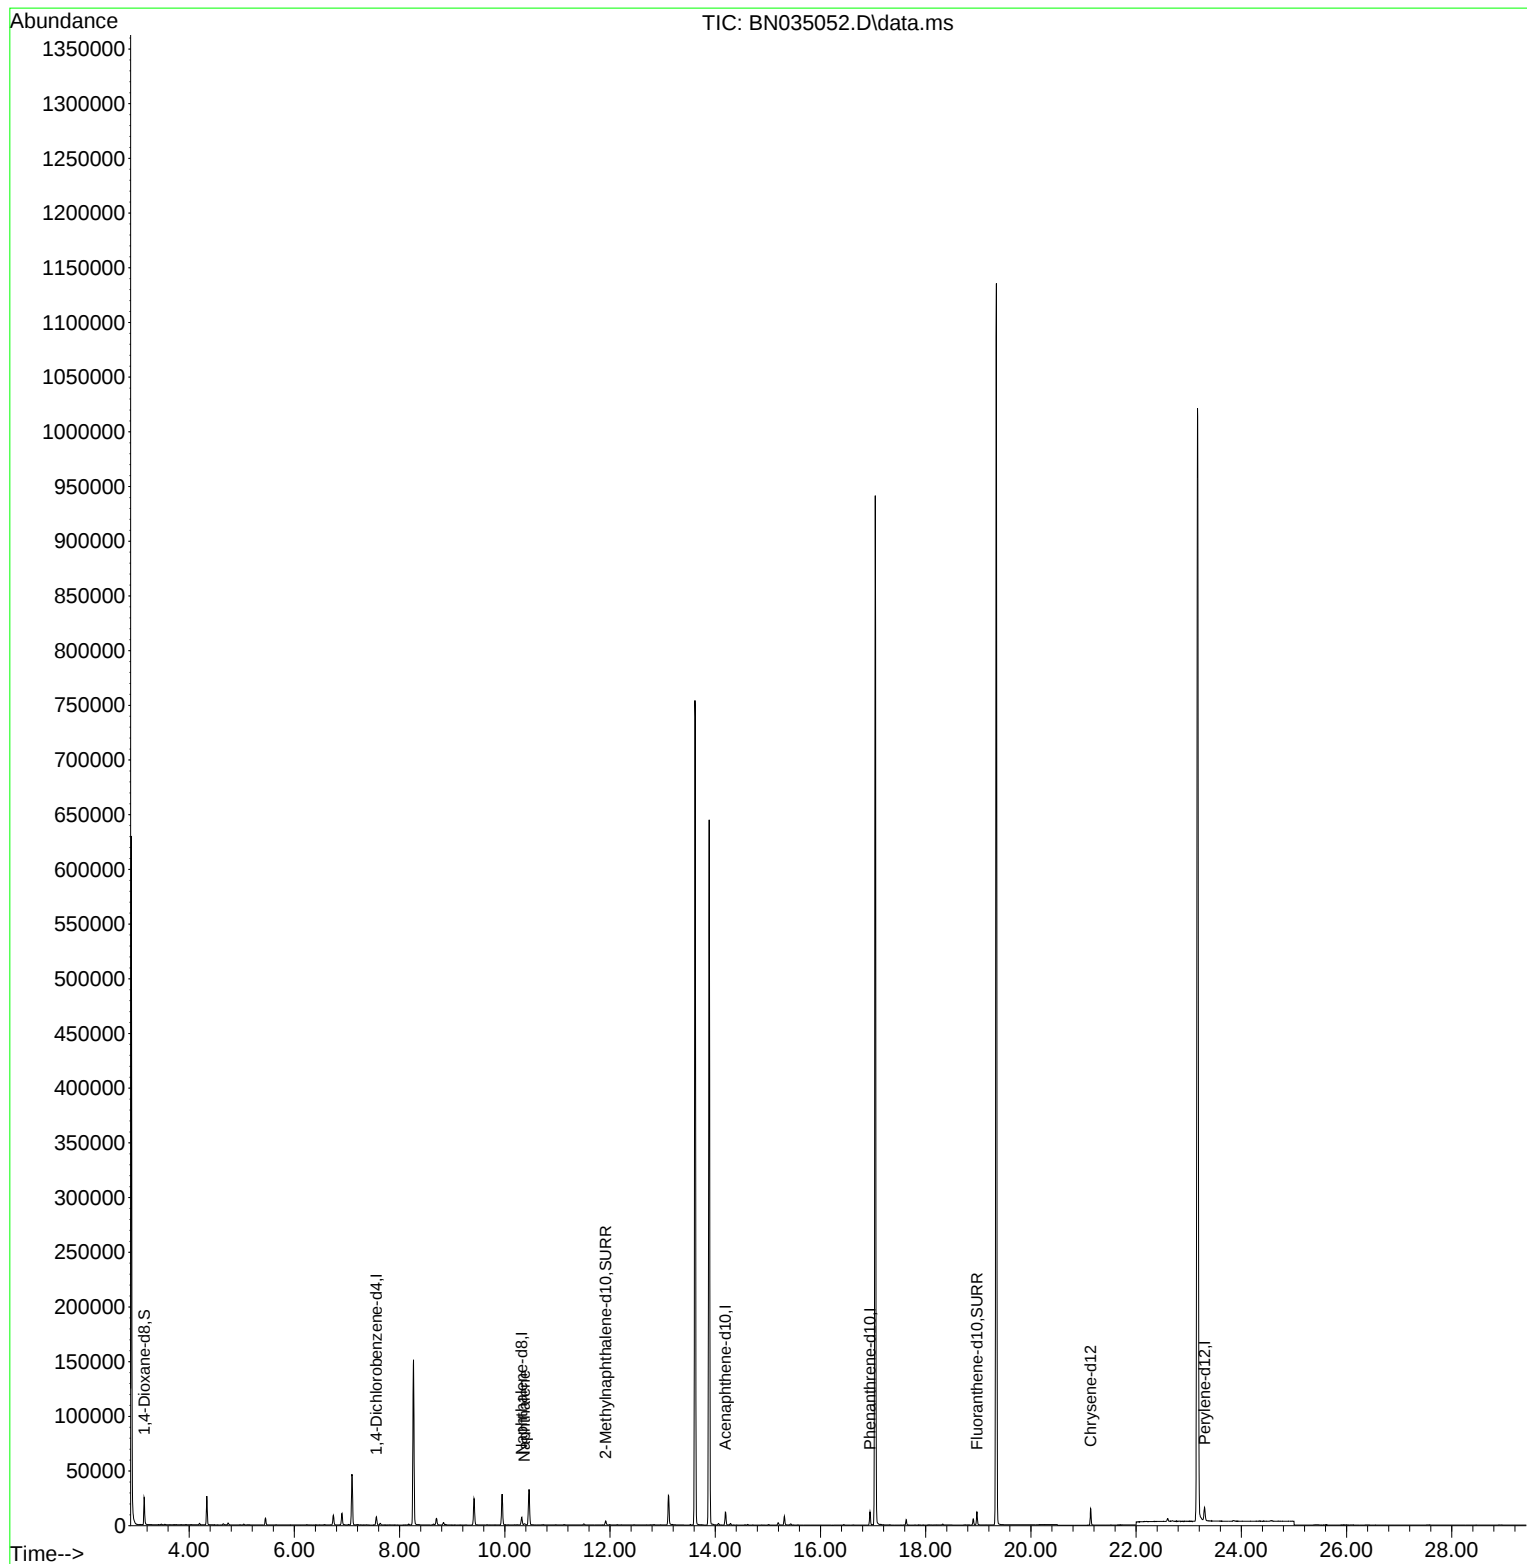

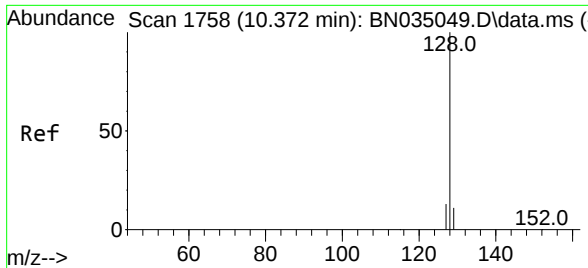

#5
Naphthalene
Concen: 0.040 ng/ul
RT: 10.372 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN035052.D
Acq: 13 Nov 2024 01:23

Instrument :
BNA_N
ClientSampleId :
C0AE2

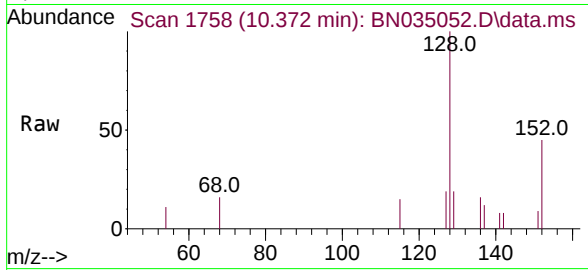

Tgt Ion:128 Resp: 91
Ion Ratio Lower Upper
128 100
129 19.3 10.1 15.1
127 19.3 12.1 18.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 11/13/2024
Supervised By :mohammad ahmed 11/14/2024

