

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022611.D
 Acq On : 11 Nov 2022 14:26
 Operator : CG/JU
 Sample : PB148941BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK941

Quant Time: Nov 11 22:26:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	1894	0.400	ng/ul	0.00
4) Naphthalene-d8	10.723	136	5944	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.577	164	3401	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.336	188	6855	0.400	ng/ul	0.00
17) Chrysene-d12	21.547	240	5263	0.400	ng/ul	0.00
23) Perylene-d12	23.985	264	5001	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	14348	5.829	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.329	152	2670	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	5333	0.302	ng/ul	0.00
Target Compounds						
						Qvalue
12) Fluorene	15.572	166	907	0.061	ng/ul#	18
20) Pyrene	19.742	202	774	0.032	ng/ul#	1
26) Benzo(a)pyrene	23.821	252	1686	0.084	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022611.D
 Acq On : 11 Nov 2022 14:26
 Operator : CG/JU
 Sample : PB148941BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK941

Quant Time: Nov 11 22:26:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration




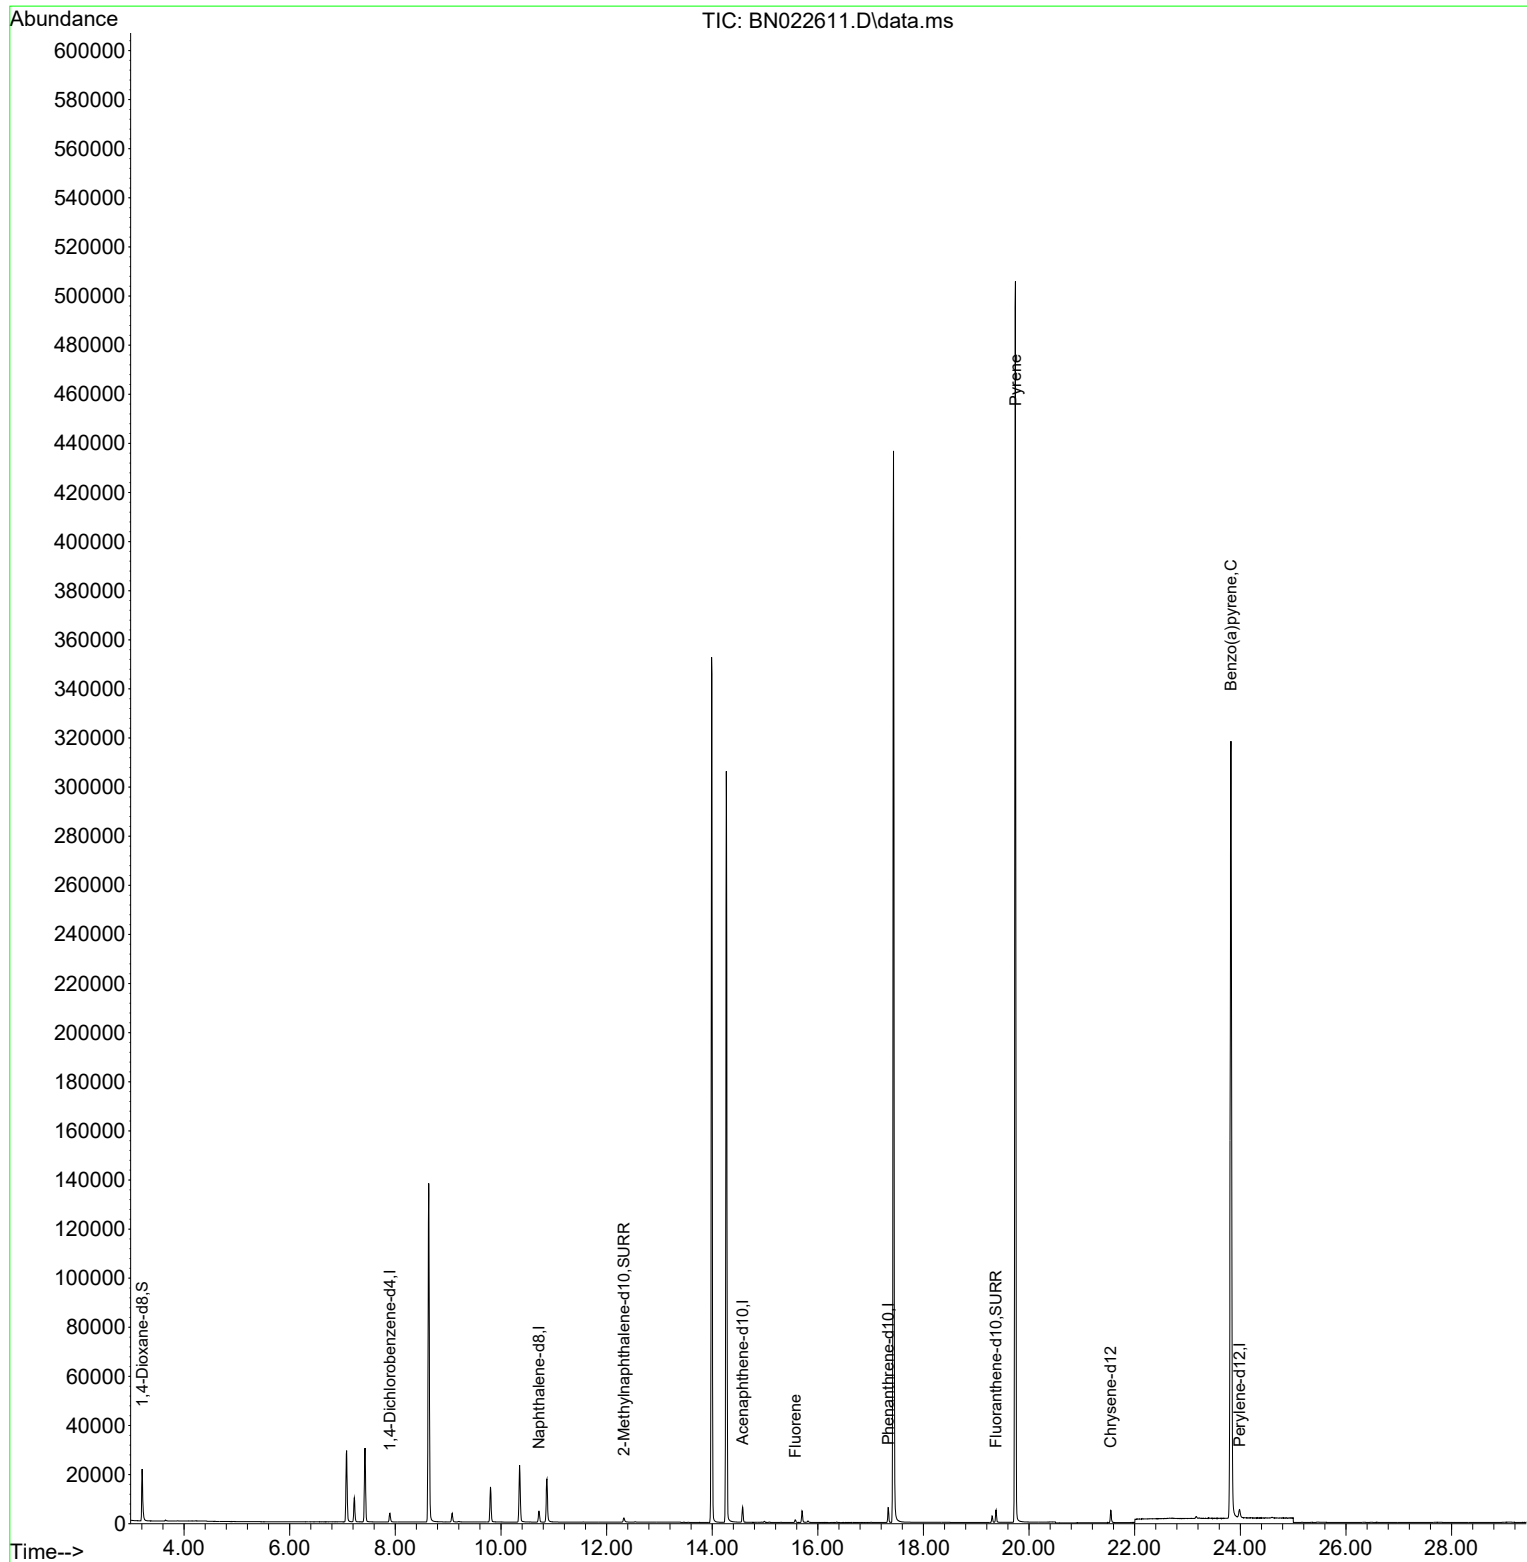


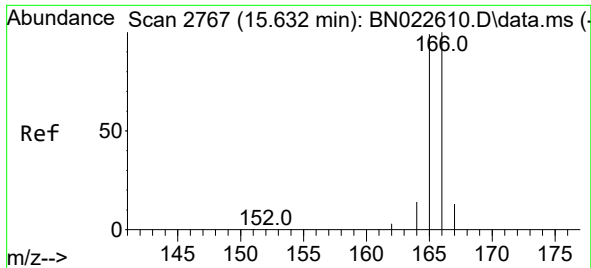

#12
 Fluorene
 Concen: 0.061 ng/u1
 RT: 15.572 min Scan# 21
 Delta R.T. -0.060 min
 Lab File: BN022611.D
 Acq: 11 Nov 2022 14:26




Instrument :
 BNA_N
 ClientSampleId :
 SBLK941


Tgt Ion	Resp	Lower	Upper
166	100		
165	12.5	78.2	117.2#
167	33.7	11.0	16.4#

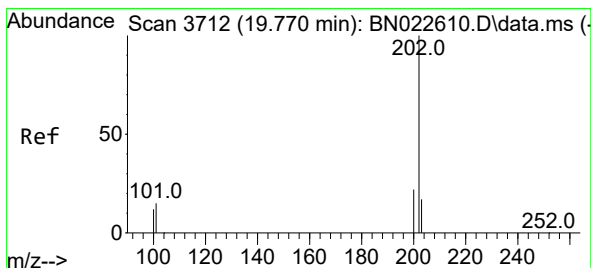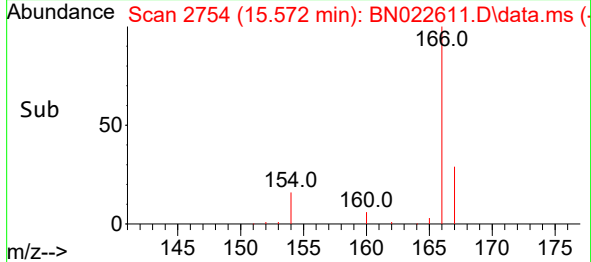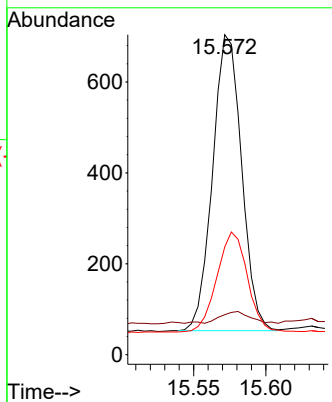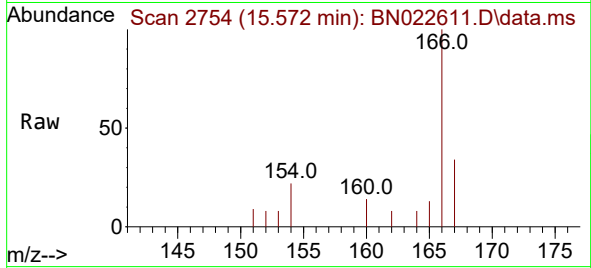

#20
 Pyrene
 Concen: 0.032 ng/u1
 RT: 19.742 min Scan# 3706
 Delta R.T. -0.028 min
 Lab File: BN022611.D
 Acq: 11 Nov 2022 14:26


Tgt Ion	Resp	Lower	Upper
202	100		
101	188.1	13.1	19.7#
100	1320.5	10.6	16.0#

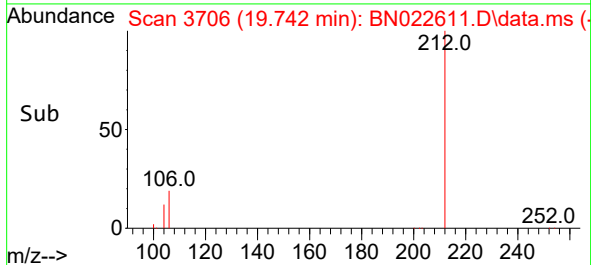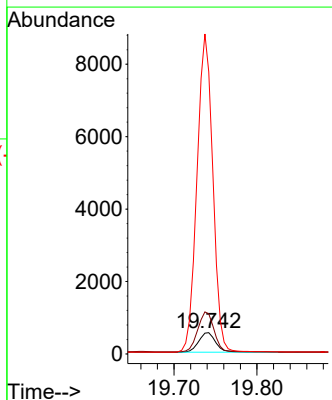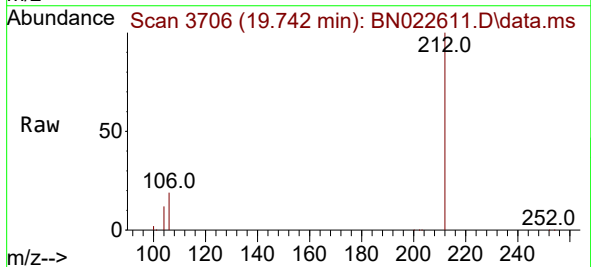

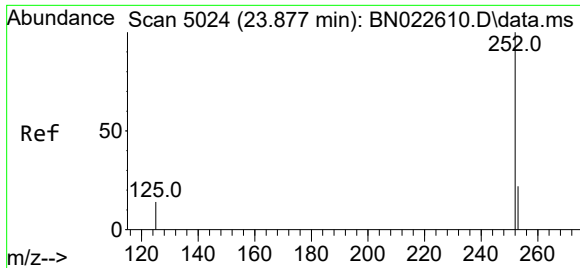

#26
 Benzo(a)pyrene
 Concen: 0.084 ng/ul
 RT: 23.821 min Scan# 50
 Delta R.T. -0.056 min
 Lab File: BN022611.D
 Acq: 11 Nov 2022 14:26

Instrument :
 BNA_N
 ClientSampleId :
 SBLK941

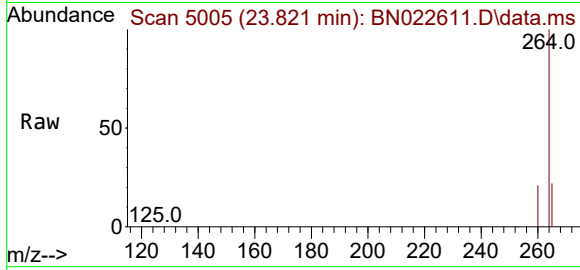

Tgt Ion:252 Resp: 1686

Ion	Ratio	Lower	Upper
252	100		
253	52.5	21.0	31.6#
125	51.1	17.9	26.9#

