

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022614.D
 Acq On : 11 Nov 2022 16:20
 Operator : CG/JU
 Sample : N5493-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AA1

Quant Time: Nov 11 22:27:10 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.894	152	1997	0.400	ng/ul	0.00
4) Naphthalene-d8	10.723	136	6308	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.577	164	3554	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.332	188	7240	0.400	ng/ul	0.00
17) Chrysene-d12	21.547	240	5718	0.400	ng/ul	0.00
23) Perylene-d12	23.985	264	5242	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	10585	4.078	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	2843	0.298	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	6685	0.348	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.245	88	1869	0.701	ng/ul	91
20) Pyrene	19.742	202	1179	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.824	252	2072	0.099	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
Data File : BN022614.D
Acq On : 11 Nov 2022 16:20
Operator : CG/JU
Sample : N5493-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AA1

Quant Time: Nov 11 22:27:10 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:23:04 2022
Response via : Initial Calibration




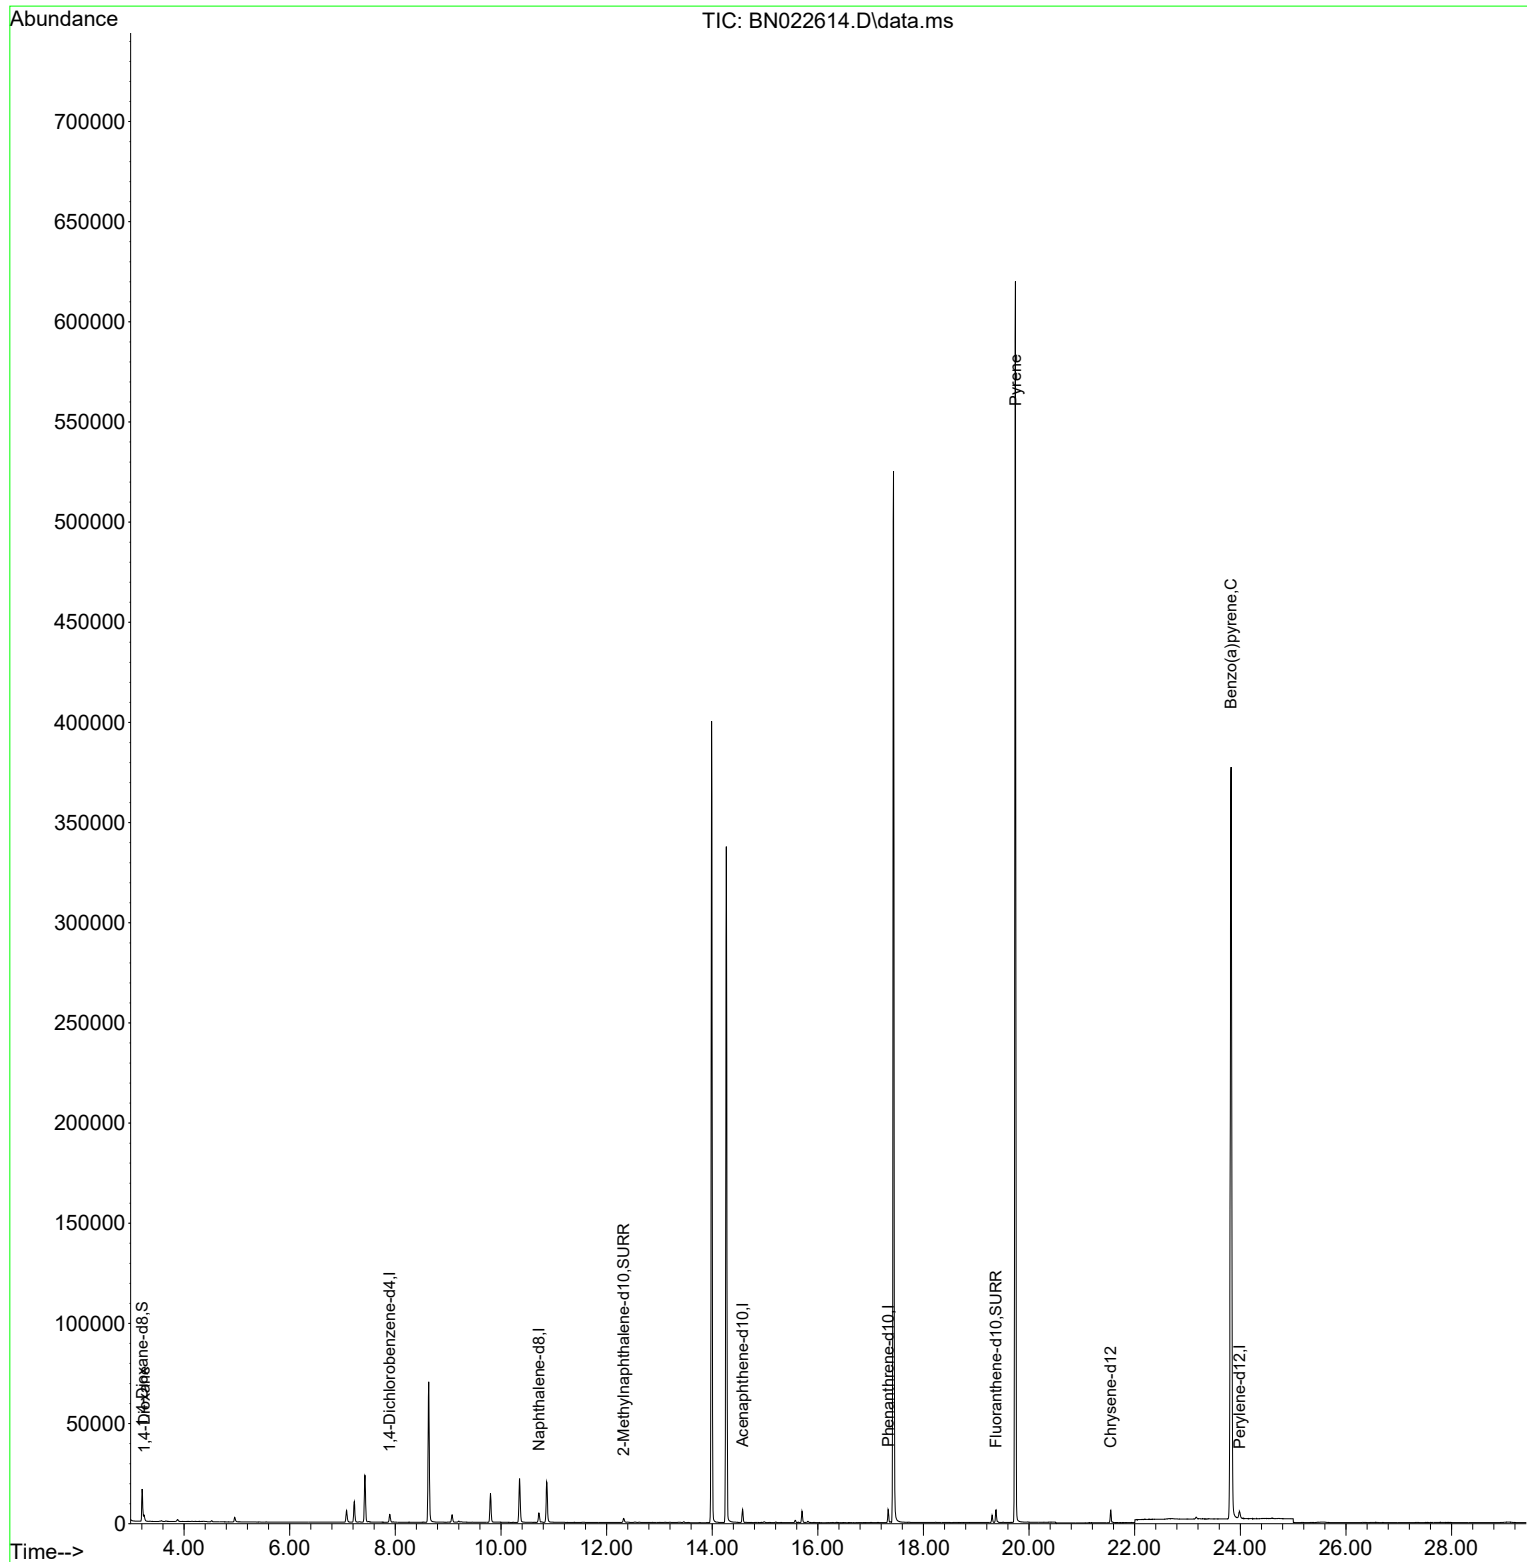


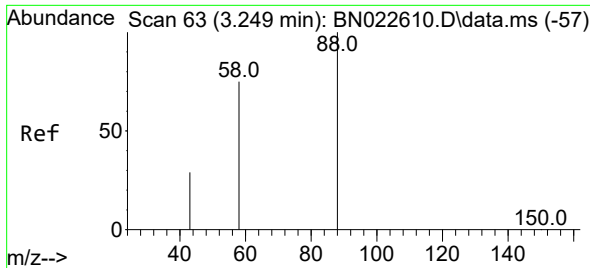

#2
 1,4-Dioxane
 Concen: 0.701 ng/ul
 RT: 3.245 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN022614.D
 Acq: 11 Nov 2022 16:20




Instrument :
 BNA_N
 ClientSampleId :
 H0AA1


Tgt Ion: 88 Resp: 1869
 Ion Ratio Lower Upper
 88 100
 43 38.0 27.4 41.2
 58 68.0 48.2 72.2

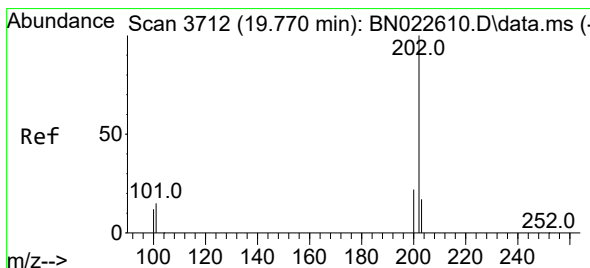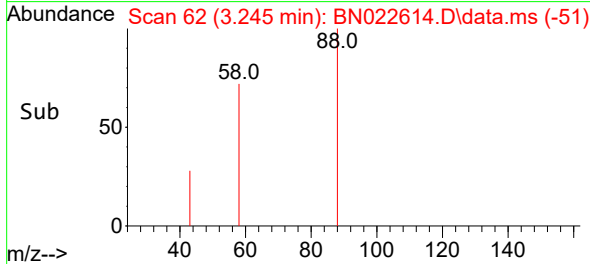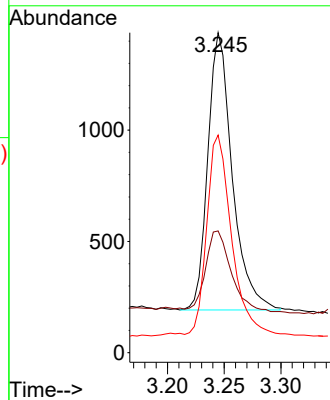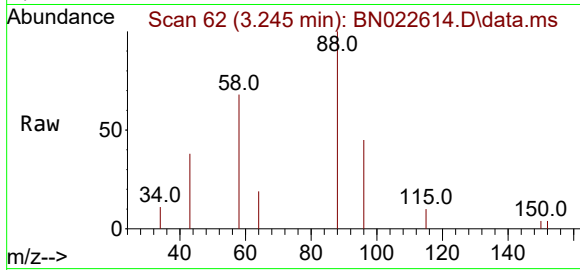

#20
 Pyrene
 Concen: 0.045 ng/ul
 RT: 19.742 min Scan# 3706
 Delta R.T. -0.028 min
 Lab File: BN022614.D
 Acq: 11 Nov 2022 16:20


Tgt Ion: 202 Resp: 1179
 Ion Ratio Lower Upper
 202 100
 101 185.3 13.1 19.7#
 100 1320.3 10.6 16.0#

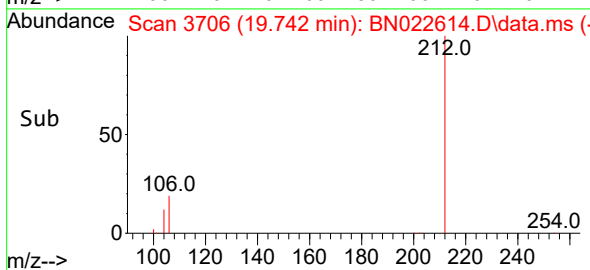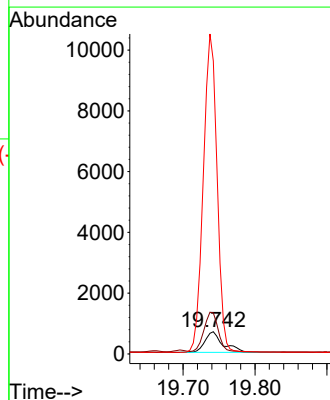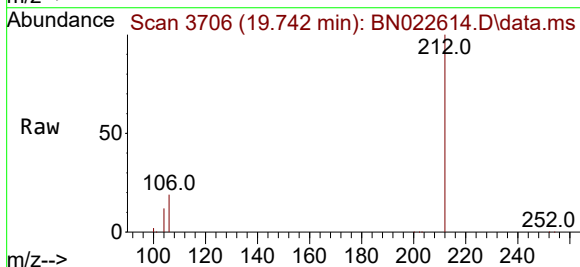

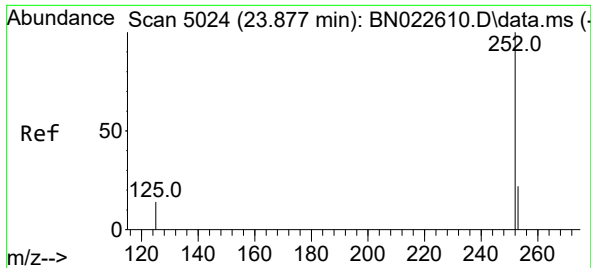

#26
 Benzo(a)pyrene
 Concen: 0.099 ng/ul
 RT: 23.824 min Scan# 50
 Delta R.T. -0.053 min
 Lab File: BN022614.D
 Acq: 11 Nov 2022 16:20

Instrument :
 BNA_N
 ClientSampleId :
 H0AA1

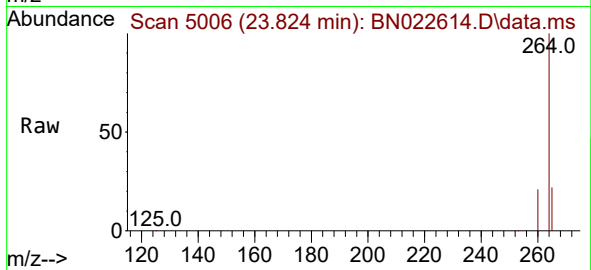

Tgt Ion:252 Resp: 2072
 Ion Ratio Lower Upper
 252 100
 253 49.8 21.0 31.6#
 125 48.7 17.9 26.9#

