

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022615.D
 Acq On : 11 Nov 2022 16:58
 Operator : CG/JU
 Sample : N5493-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AA4

Quant Time: Nov 11 22:27:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.894	152	1882	0.400	ng/ul	0.00
4) Naphthalene-d8	10.717	136	6004	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.577	164	3430	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.332	188	6911	0.400	ng/ul	0.00
17) Chrysene-d12	21.541	240	5430	0.400	ng/ul	0.00
23) Perylene-d12	23.979	264	5027	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	10693	4.372	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.323	152	3134	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.375	212	6512	0.357	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.245	88	2293	0.913	ng/ul	92
20) Pyrene	19.737	202	1003	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.821	252	1925	0.096	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
Data File : BN022615.D
Acq On : 11 Nov 2022 16:58
Operator : CG/JU
Sample : N5493-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AA4

Quant Time: Nov 11 22:27:16 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:23:04 2022
Response via : Initial Calibration




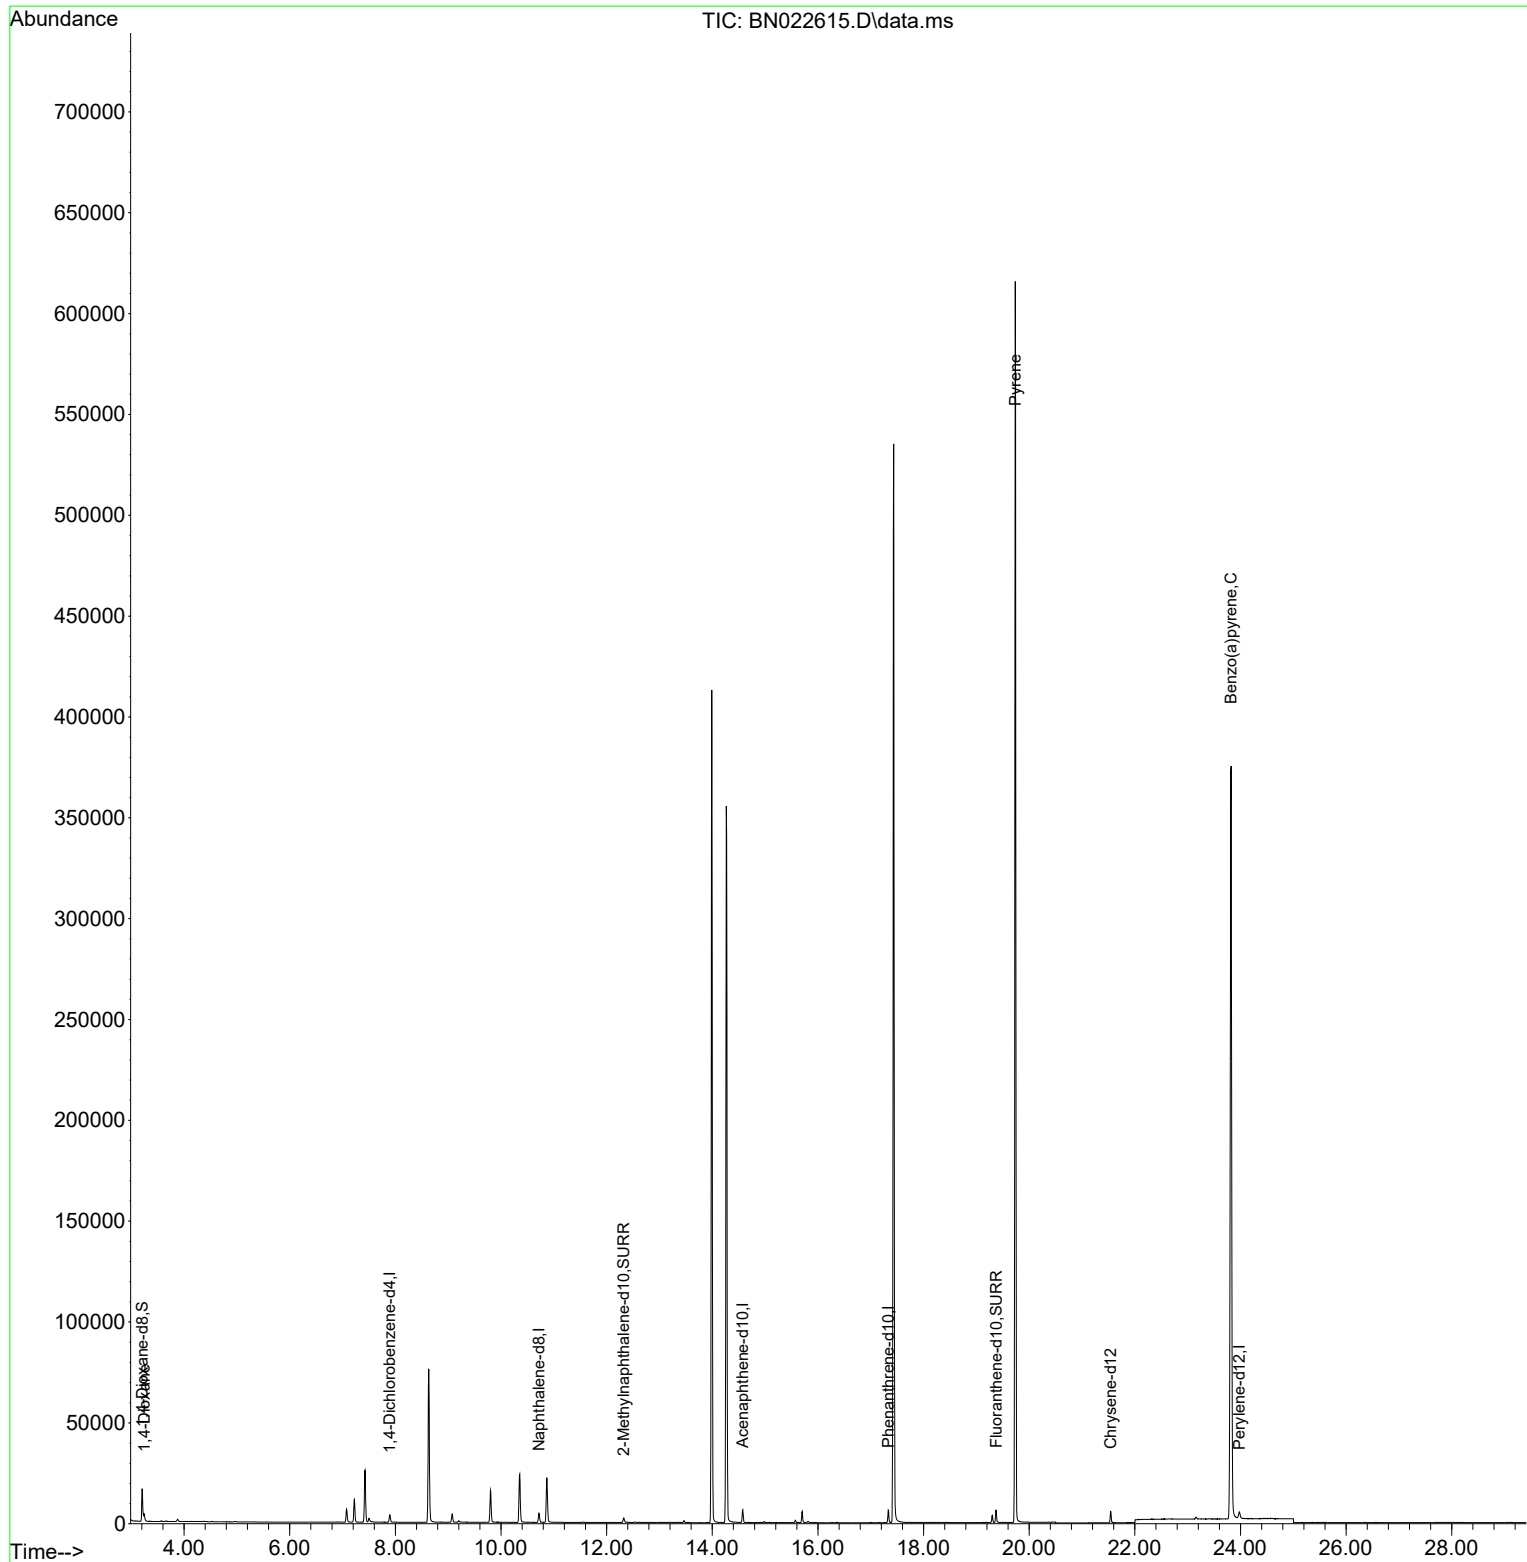


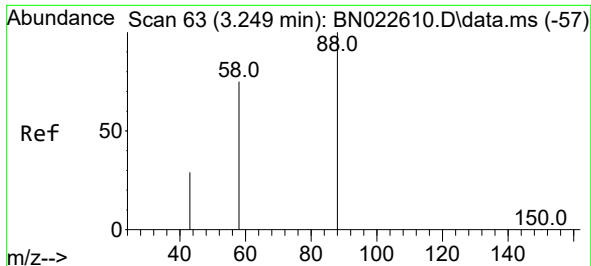

#2
1,4-Dioxane
Concen: 0.913 ng/ul
RT: 3.245 min Scan# 61
Delta R.T. -0.004 min
Lab File: BN022615.D
Acq: 11 Nov 2022 16:58




Instrument :
BNA_N
ClientSampleId :
H0AA4


Tgt Ion: 88 Resp: 2293
Ion Ratio Lower Upper
88 100
43 35.7 27.4 41.2
58 69.1 48.2 72.2

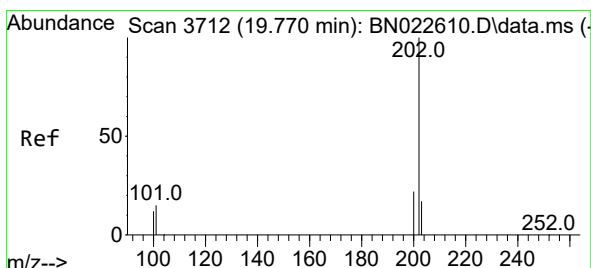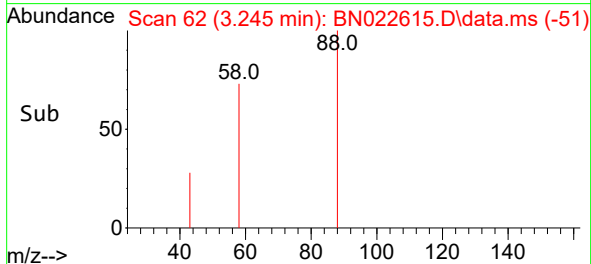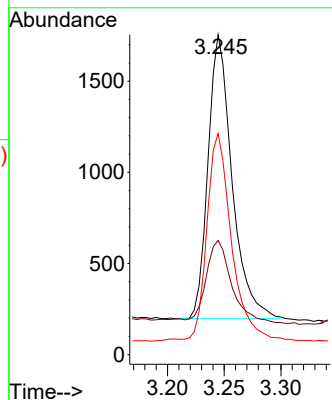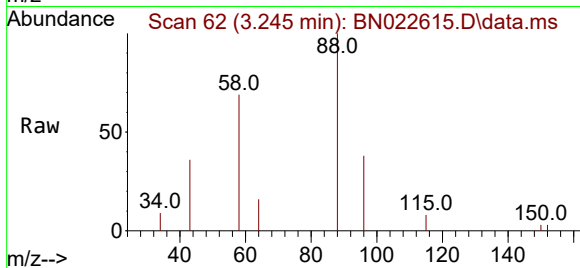

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.737 min Scan# 3705
Delta R.T. -0.032 min
Lab File: BN022615.D
Acq: 11 Nov 2022 16:58


Tgt Ion: 202 Resp: 1003
Ion Ratio Lower Upper
202 100
101 199.0 13.1 19.7#
100 1463.2 10.6 16.0#

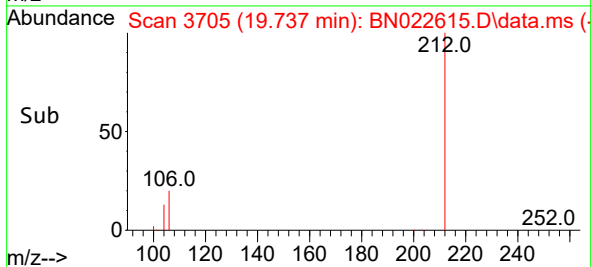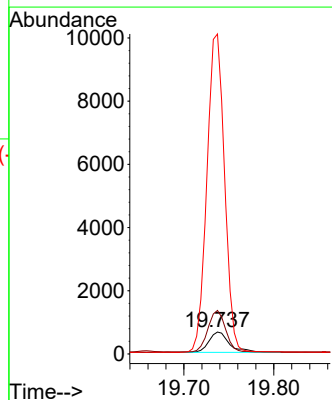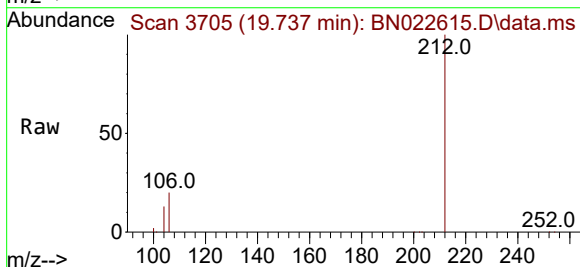

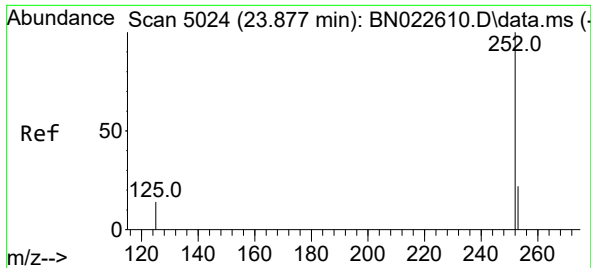

#26
 Benzo(a)pyrene
 Concen: 0.096 ng/ul
 RT: 23.821 min Scan# 50
 Delta R.T. -0.055 min
 Lab File: BN022615.D
 Acq: 11 Nov 2022 16:58

Instrument :
 BNA_N
 ClientSampleId :
 H0AA4

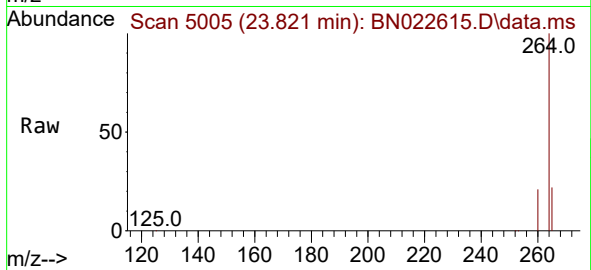

Tgt Ion:252 Resp: 1925
 Ion Ratio Lower Upper
 252 100
 253 51.4 21.0 31.6#
 125 49.4 17.9 26.9#

