

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022616.D
 Acq On : 11 Nov 2022 17:37
 Operator : CG/JU
 Sample : N5493-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AA5

Quant Time: Nov 11 22:27:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	1777	0.400	ng/u1	0.00
4) Naphthalene-d8	10.723	136	5665	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.577	164	3183	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.336	188	6500	0.400	ng/u1	0.00
17) Chrysene-d12	21.544	240	5049	0.400	ng/u1	0.00
23) Perylene-d12	23.979	264	4782	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.206	96	10657	4.615	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.323	152	2808	0.328	ng/u1	0.00
18) Fluoranthene-d10	19.375	212	6302	0.372	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.244	88	3911	1.649	ng/u1	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
Data File : BN022616.D
Acq On : 11 Nov 2022 17:37
Operator : CG/JU
Sample : N5493-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AA5


Quant Time: Nov 11 22:27:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:23:04 2022
Response via : Initial Calibration

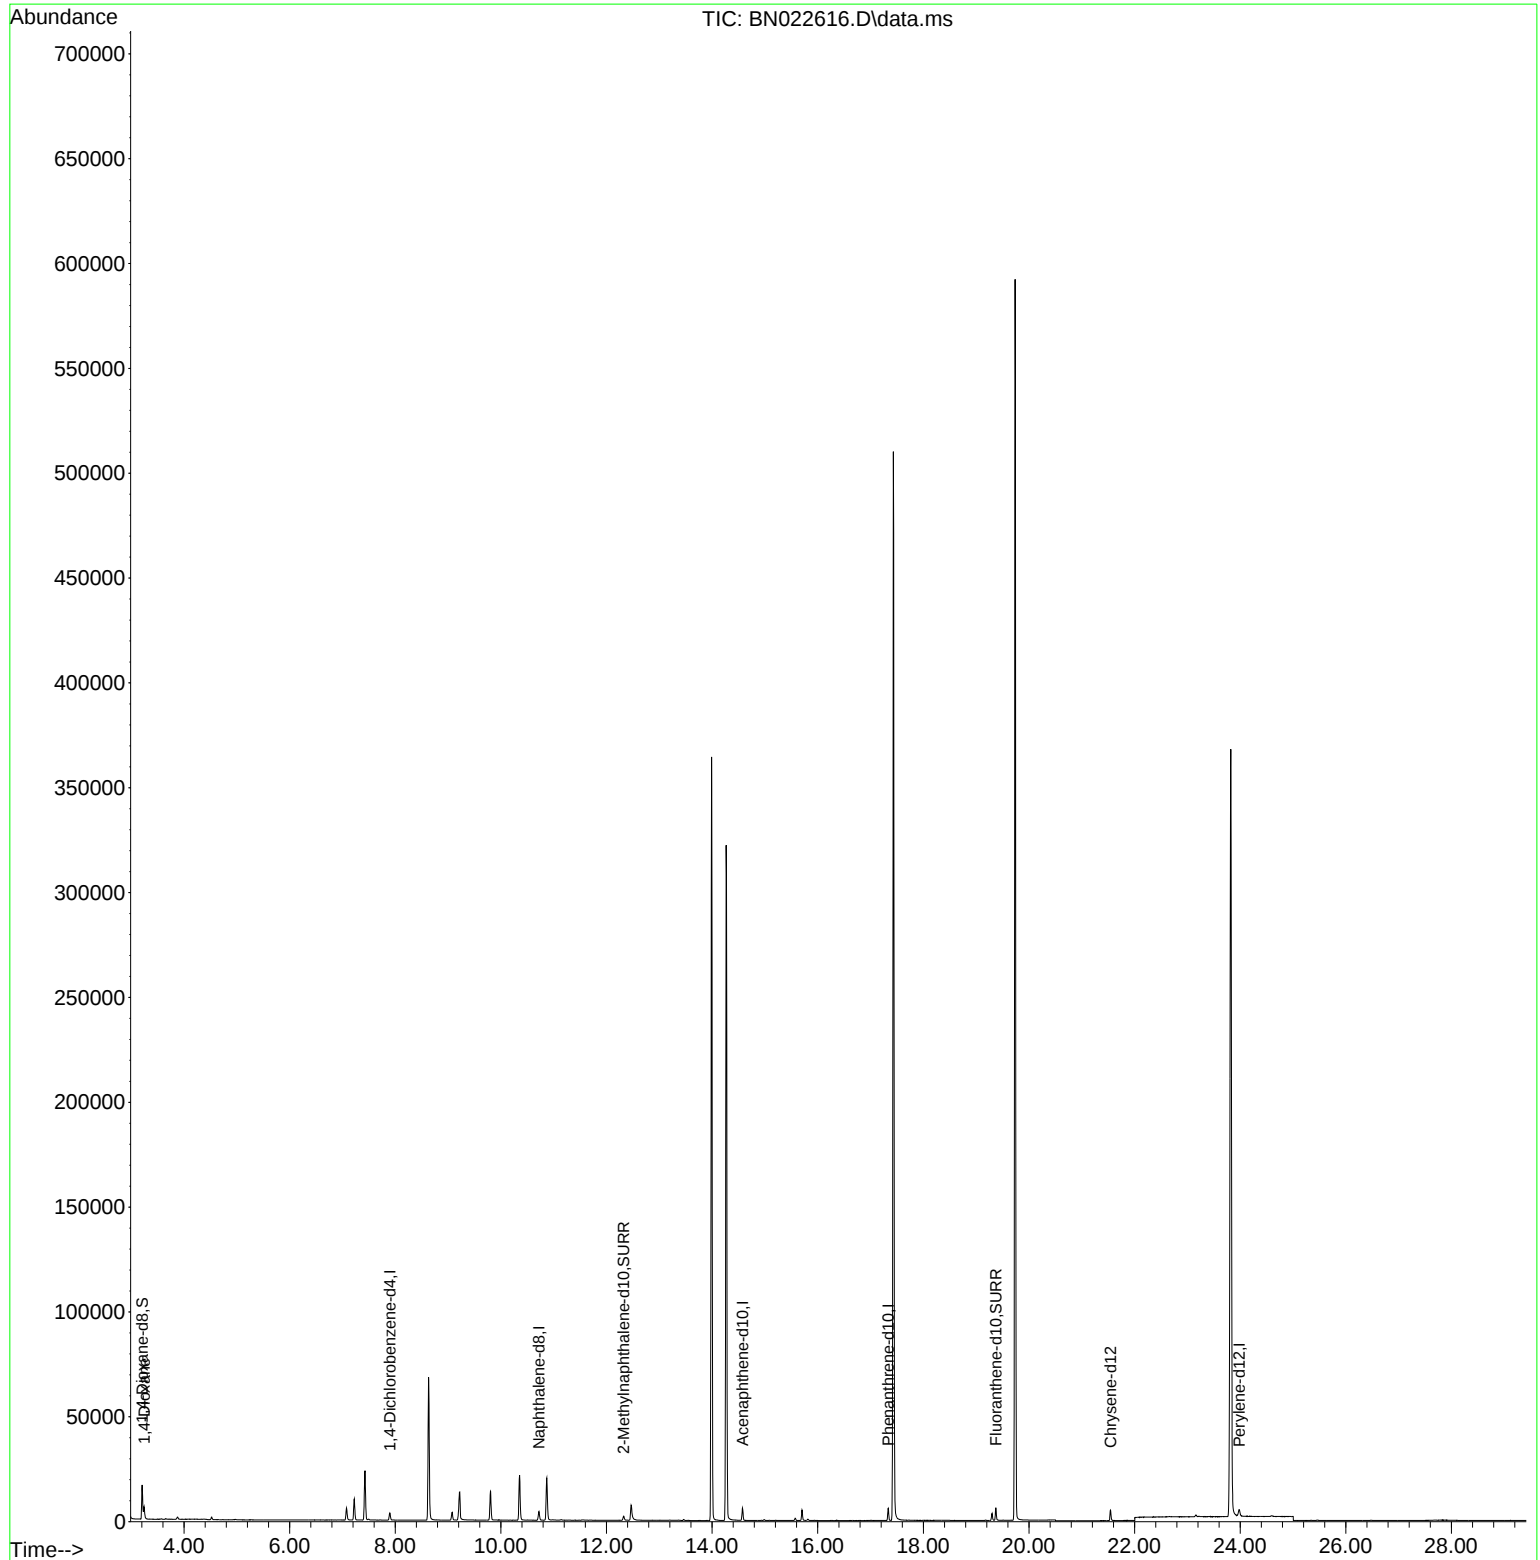

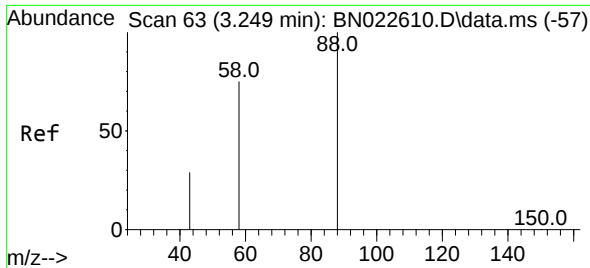

#2
 1,4-Dioxane
 Concen: 1.649 ng/ul
 RT: 3.244 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN022616.D
 Acq: 11 Nov 2022 17:37

Instrument :
 BNA_N
 ClientSampleId :
 H0AA5

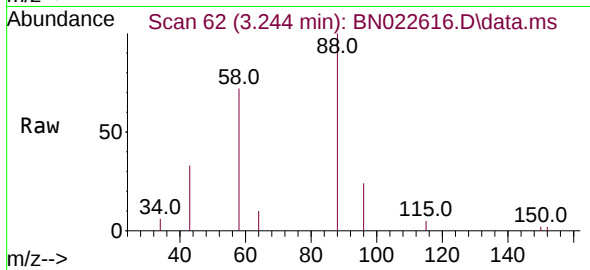

Tgt Ion:	88	Resp:	3911
Ion	Ratio	Lower	Upper
88	100		
43	33.2	27.4	41.2
58	72.0	48.2	72.2

