

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022617.D
 Acq On : 11 Nov 2022 18:15
 Operator : CG/JU
 Sample : N5493-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AA6

Quant Time: Nov 11 22:27:30 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	1905	0.400	ng/ul	0.00
4) Naphthalene-d8	10.722	136	5988	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.576	164	3357	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.335	188	6920	0.400	ng/ul	0.00
17) Chrysene-d12	21.547	240	5500	0.400	ng/ul	0.00
23) Perylene-d12	23.982	264	5084	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	11361	4.589	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.327	152	2945	0.325	ng/ul	0.00
18) Fluoranthene-d10	19.374	212	7040	0.381	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.245	88	648	0.255	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
Data File : BN022617.D
Acq On : 11 Nov 2022 18:15
Operator : CG/JU
Sample : N5493-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AA6


Quant Time: Nov 11 22:27:30 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:23:04 2022
Response via : Initial Calibration

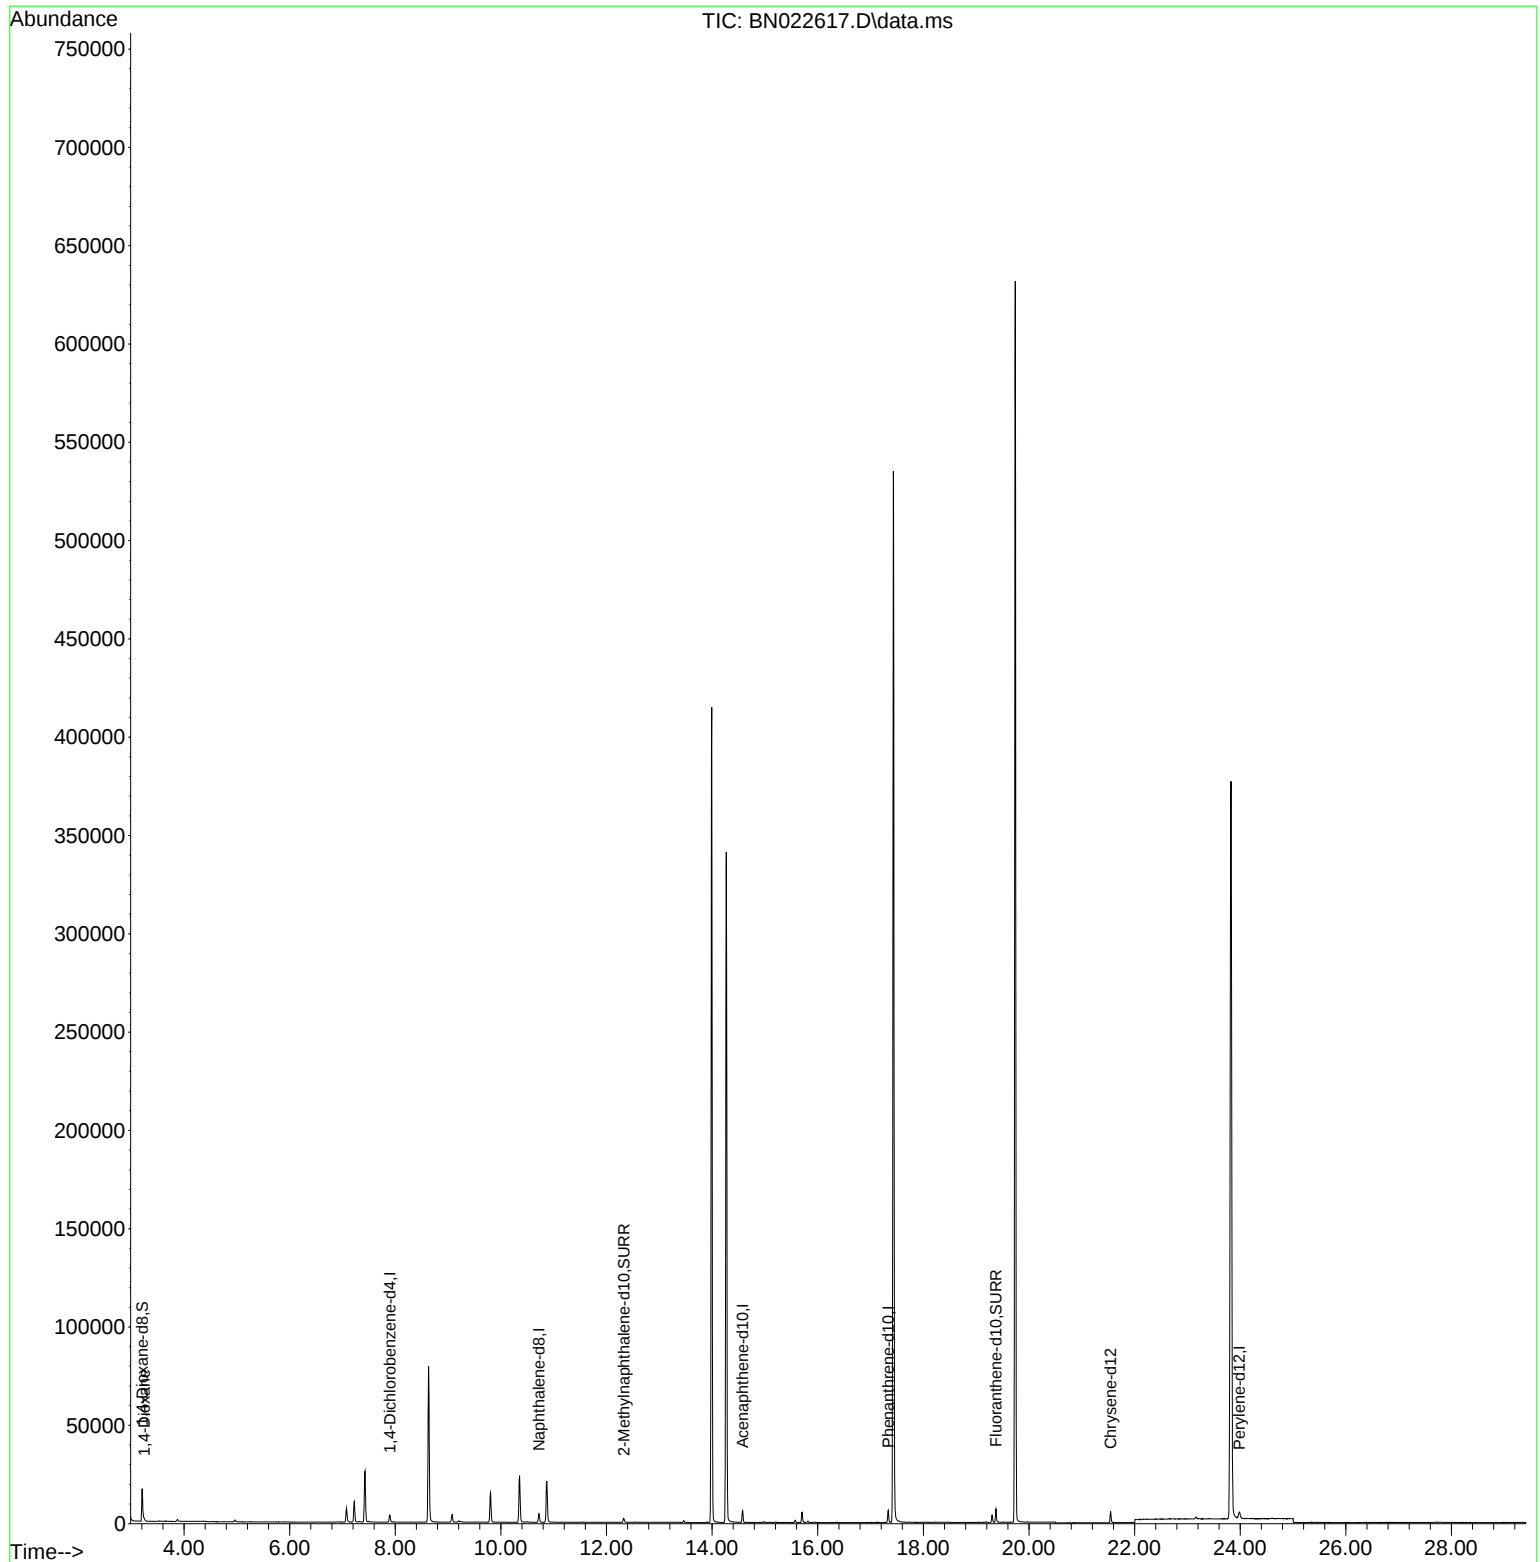

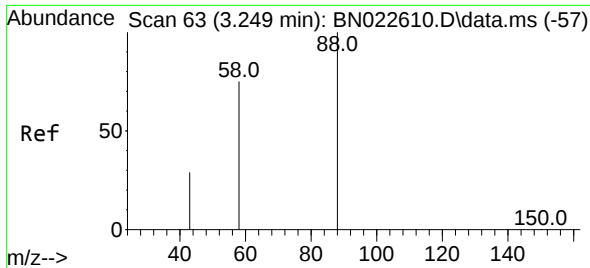

#2
 1,4-Dioxane
 Concen: 0.255 ng/ul
 RT: 3.245 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN022617.D
 Acq: 11 Nov 2022 18:15

Instrument :
 BNA_N
 ClientSampleId :
 H0AA6

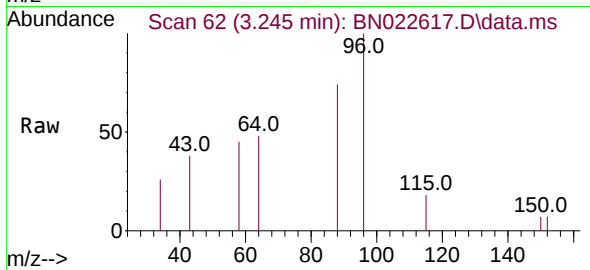

Tgt Ion: 88 Resp: 648
 Ion Ratio Lower Upper
 88 100
 43 52.2 27.4 41.2#
 58 61.8 48.2 72.2

