

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022618.D
 Acq On : 11 Nov 2022 18:53
 Operator : CG/JU
 Sample : N5493-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AC5

Quant Time: Nov 11 22:27:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	2046	0.400	ng/u1	0.00
4) Naphthalene-d8	10.723	136	6602	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.577	164	3875	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.336	188	7811	0.400	ng/u1	0.00
17) Chrysene-d12	21.547	240	6392	0.400	ng/u1	0.00
23) Perylene-d12	23.985	264	5940	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	10731	4.036	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.323	152	2754	0.276	ng/u1	0.00
18) Fluoranthene-d10	19.375	212	7040	0.328	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.249	88	888	0.325	ng/u1	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
Data File : BN022618.D
Acq On : 11 Nov 2022 18:53
Operator : CG/JU
Sample : N5493-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AC5


Quant Time: Nov 11 22:27:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:23:04 2022
Response via : Initial Calibration

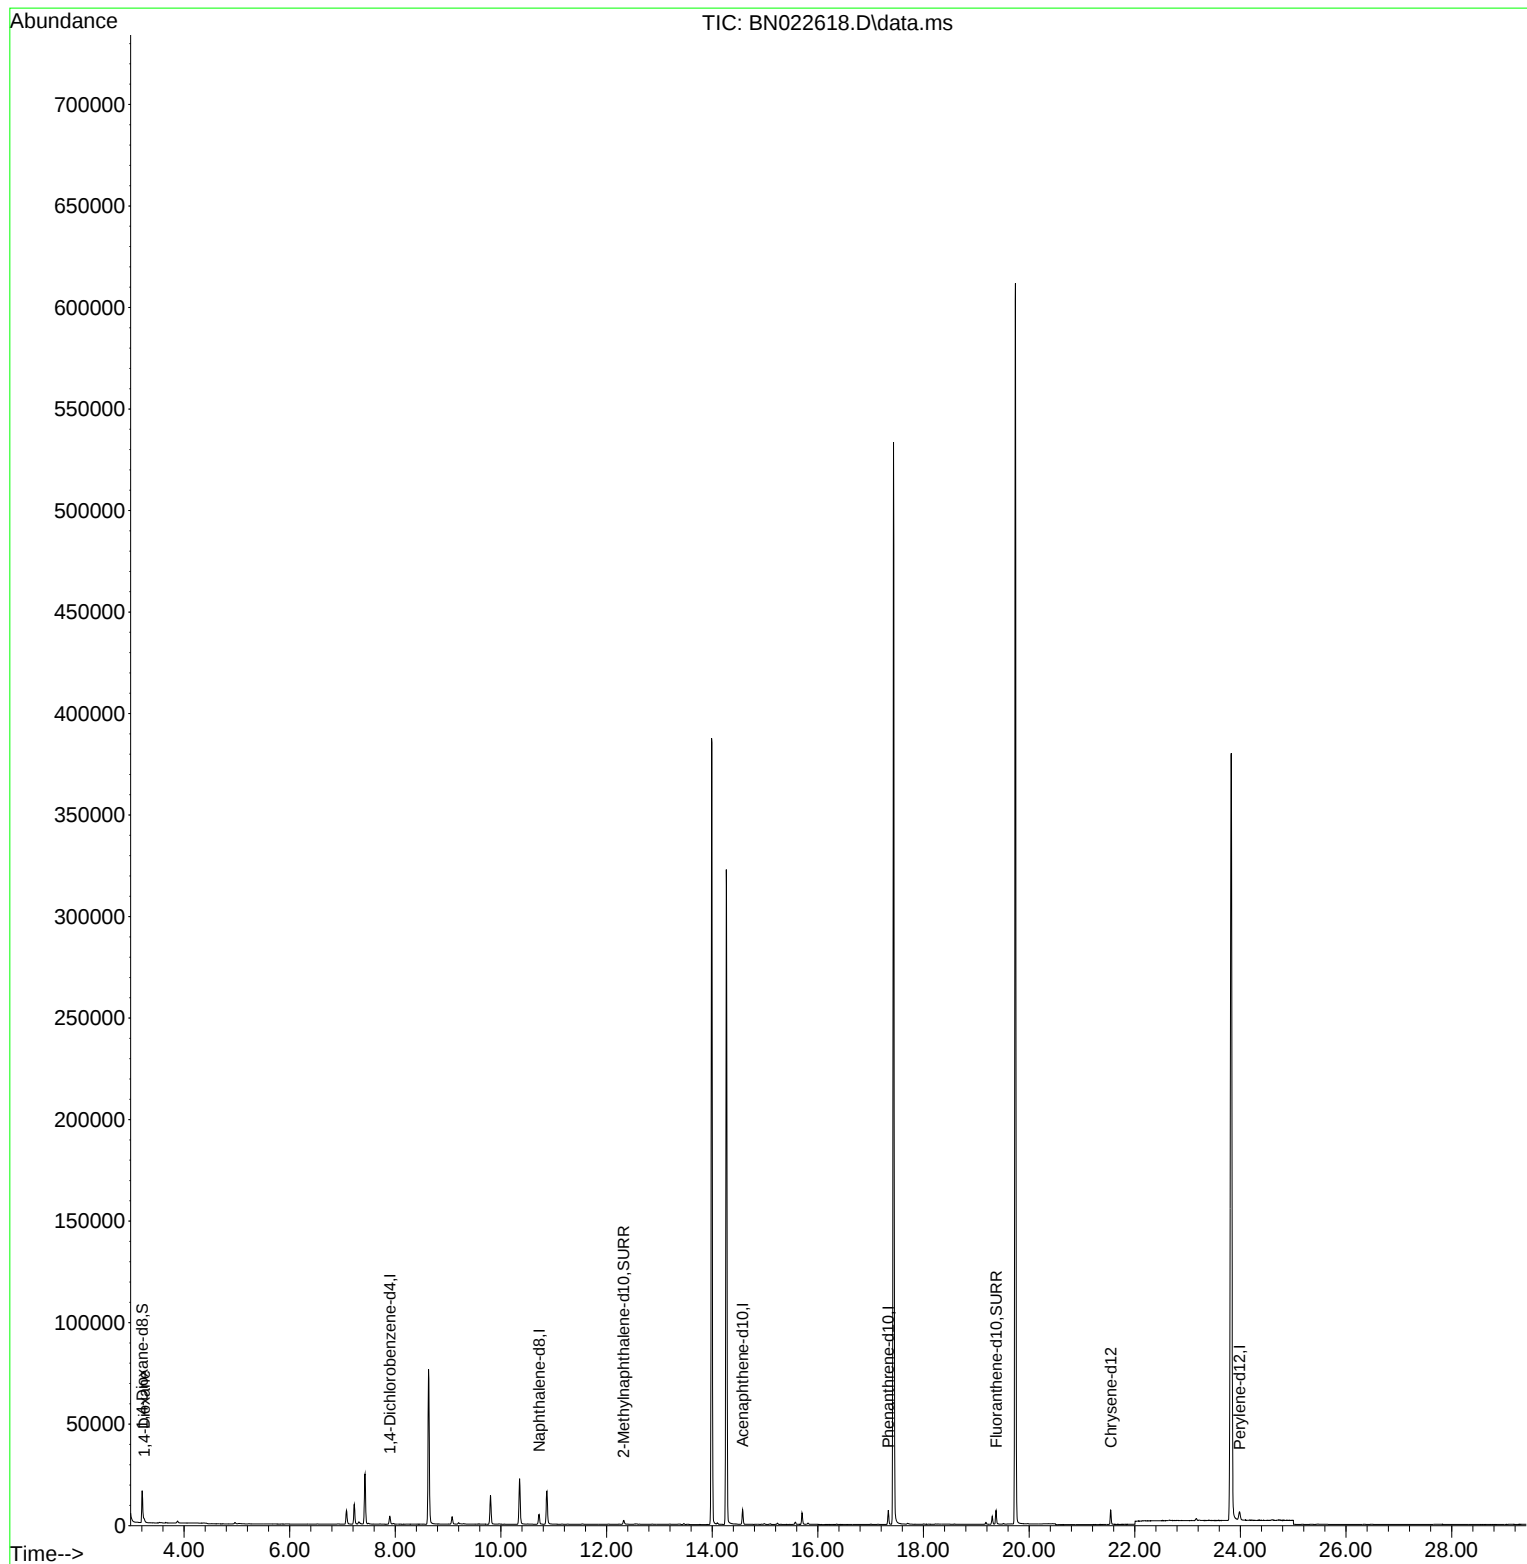

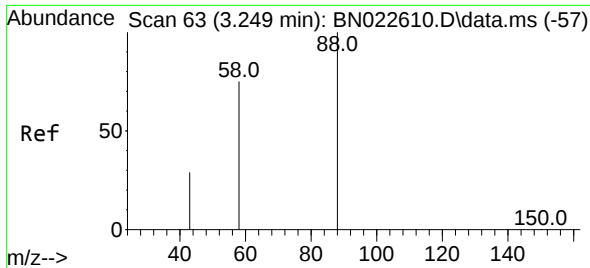

#2
 1,4-Dioxane
 Concen: 0.325 ng/ul
 RT: 3.249 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN022618.D
 Acq: 11 Nov 2022 18:53

Instrument :
 BNA_N
 ClientSampleId :
 H0AC5

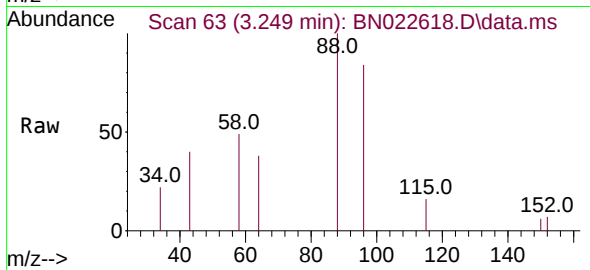

Tgt Ion:	88	Resp:	888
Ion	Ratio	Lower	Upper
88	100		
43	39.5	27.4	41.2
58	49.0	48.2	72.2

