

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
 Data File : BN022619.D
 Acq On : 11 Nov 2022 19:32
 Operator : CG/JU
 Sample : N5493-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0AC6

Quant Time: Nov 11 22:27:41 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 11 22:23:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.898	152	1926	0.400	ng/u1	0.00
4) Naphthalene-d8	10.723	136	6105	0.400	ng/u1	0.00
9) Acenaphthene-d10	14.577	164	3530	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.336	188	7286	0.400	ng/u1	0.00
17) Chrysene-d12	21.547	240	5861	0.400	ng/u1	0.00
23) Perylene-d12	23.985	264	5491	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	12214	4.880	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.323	152	3530	0.382	ng/u1	0.00
18) Fluoranthene-d10	19.375	212	7779	0.395	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.245	88	5604	2.180	ng/u1	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111222\
Data File : BN022619.D
Acq On : 11 Nov 2022 19:32
Operator : CG/JU
Sample : N5493-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0AC6


Quant Time: Nov 11 22:27:41 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 11 22:23:04 2022
Response via : Initial Calibration

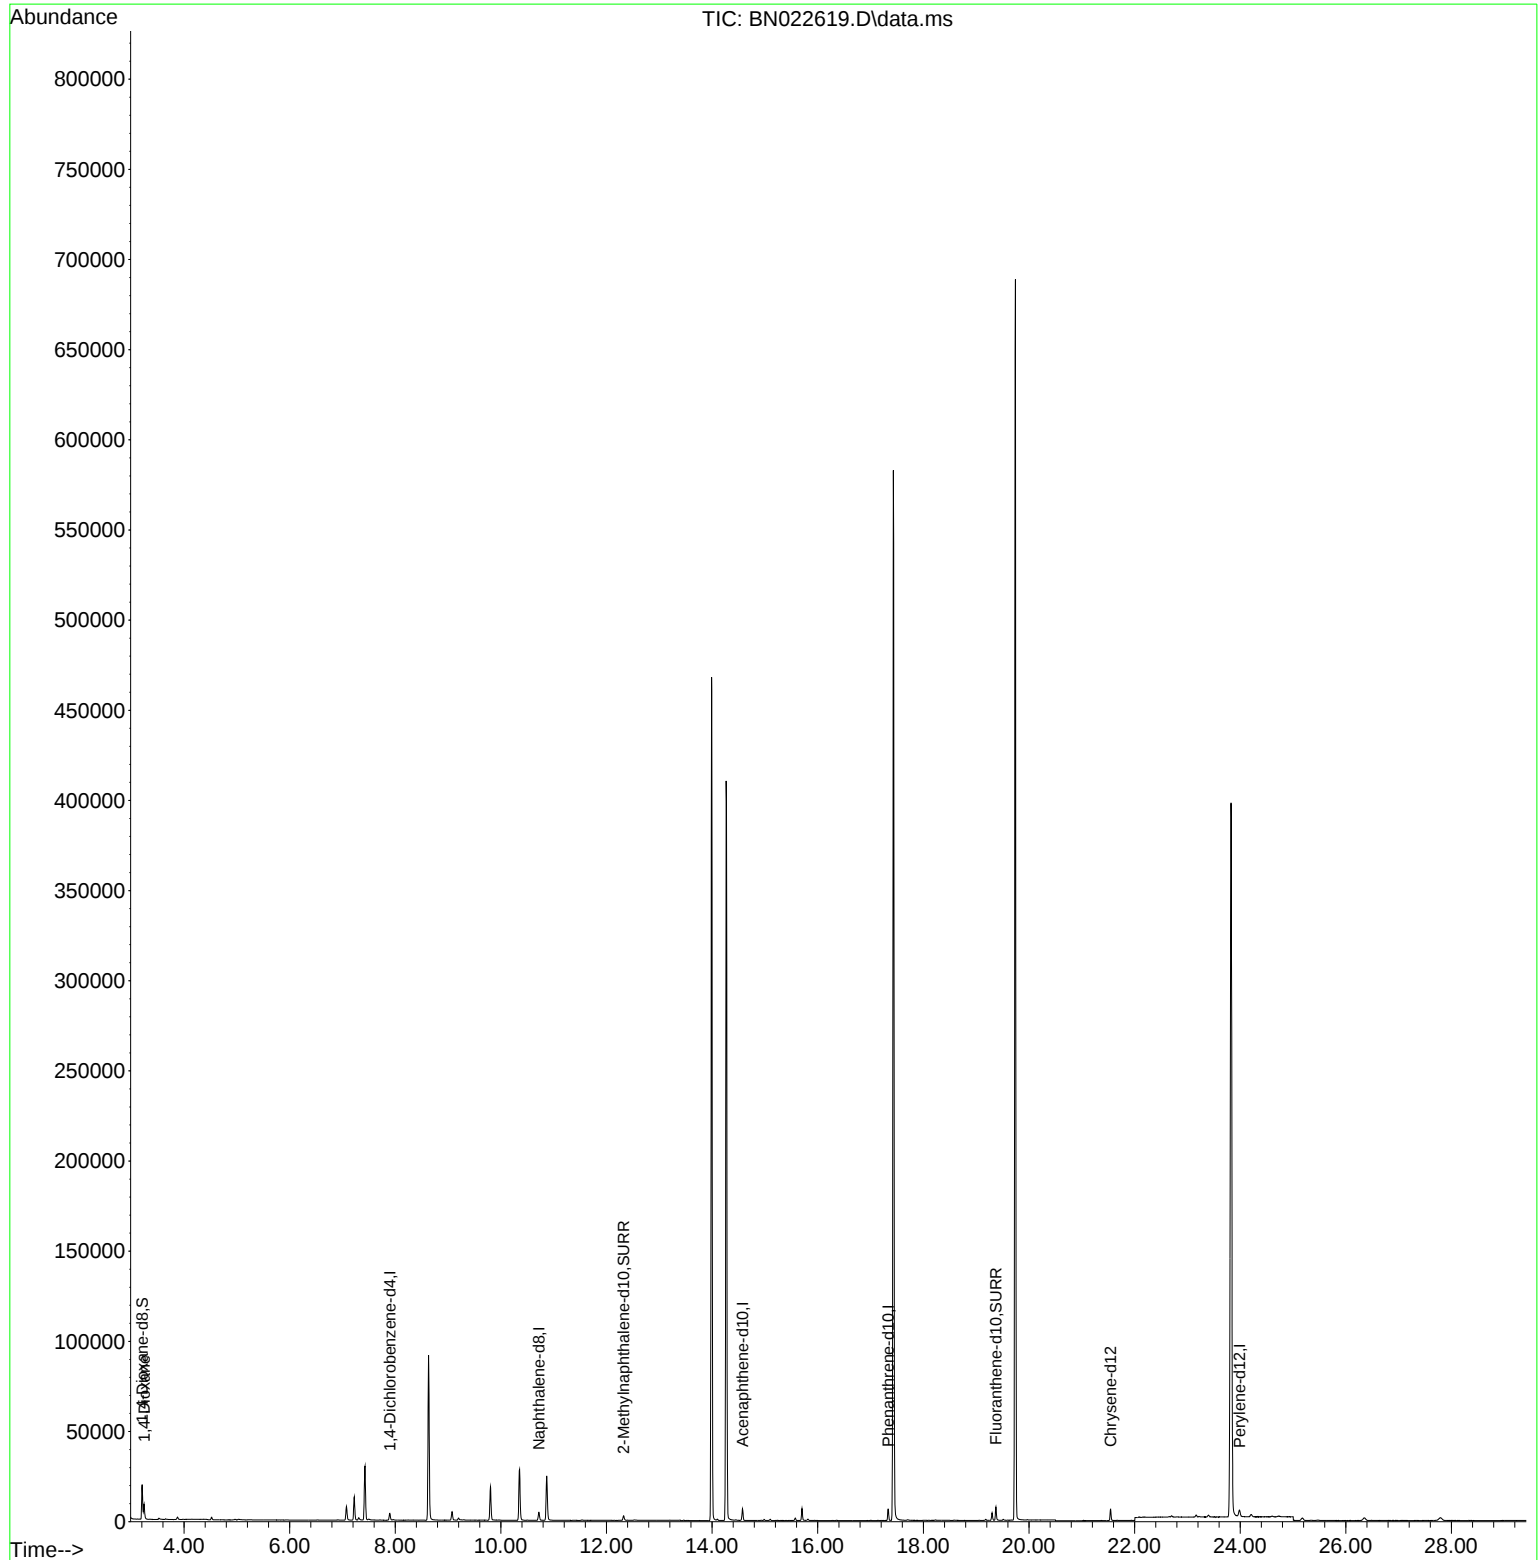

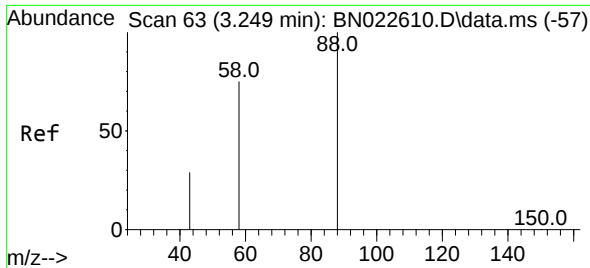

#2
 1,4-Dioxane
 Concen: 2.180 ng/ul
 RT: 3.245 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN022619.D
 Acq: 11 Nov 2022 19:32

Instrument :
 BNA_N
 ClientSampleId :
 H0AC6

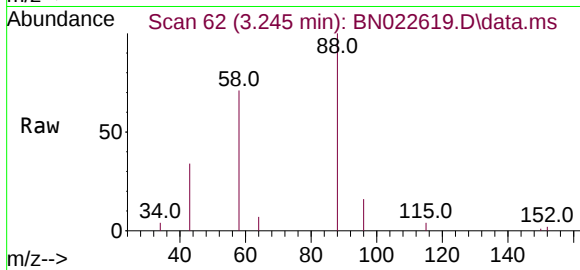

Tgt Ion:	88	Resp:	5604
Ion	Ratio	Lower	Upper
88	100		
43	33.8	27.4	41.2
58	71.3	48.2	72.2

