
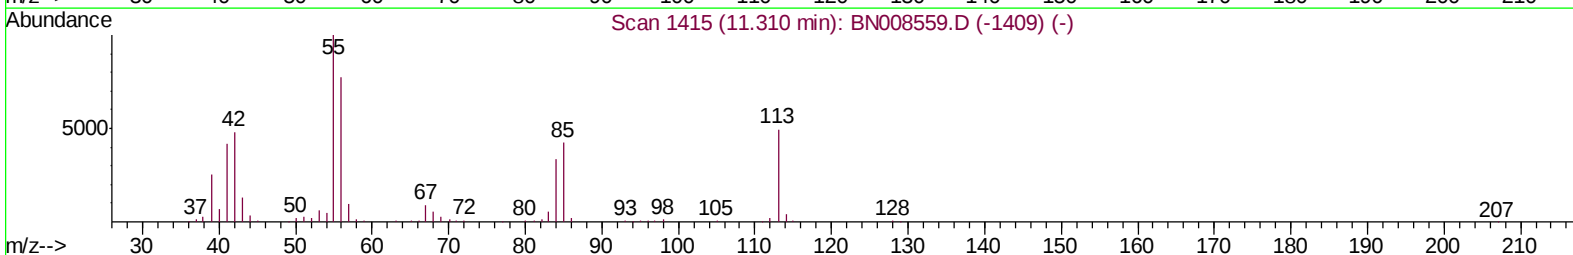
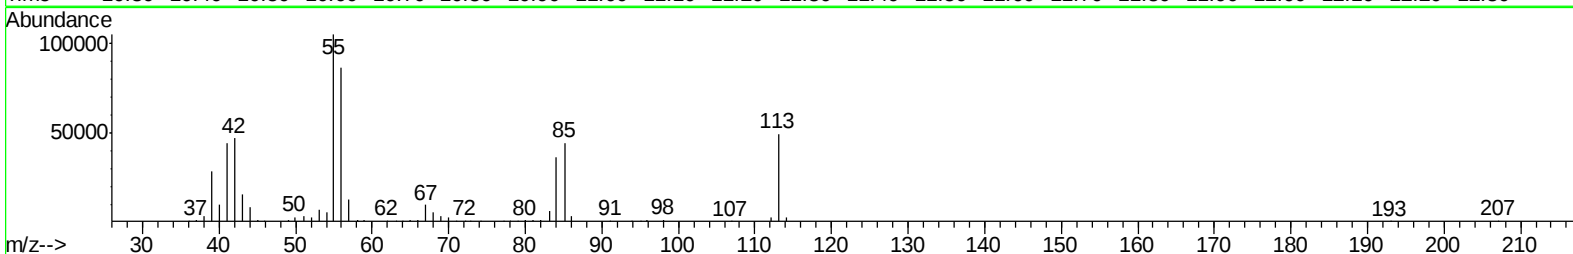


Data File : BN008573.D
Acq On : 15 Nov 2019 01:07
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Nov 15 04:31:54 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 04:28:01 2019
Response via : Initial Calibration

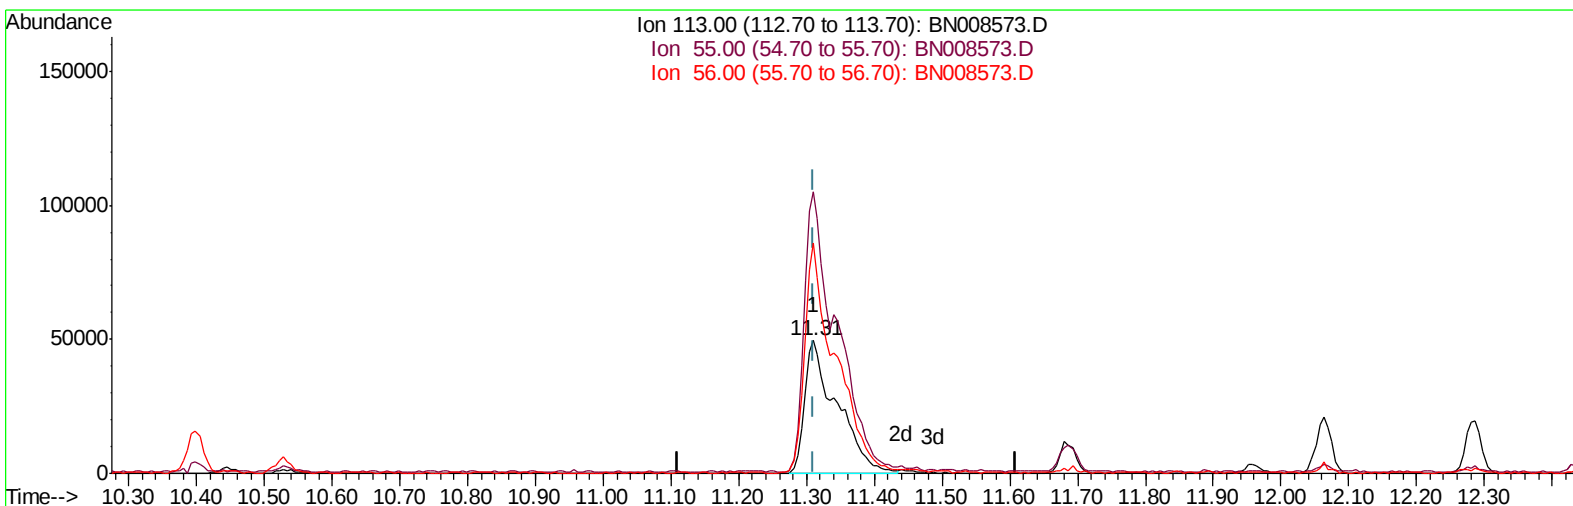

TIC: BN008573.D

(32) Caprolactam

11.310min (+0.000) 18.54ng/ul m

response 164749

Ion	Exp%	Act%
113.00	100	100
55.00	204.80	212.35
56.00	166.90	174.17
0.00	0.00	0.00