

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111319\
 Data File : BN008526.D
 Acq On : 13 Nov 2019 17:24
 Operator : JU
 Sample : PB124539BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 14 03:28:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 15:23:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	250662	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1052718	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	700744	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	1520497	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1460269	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	1635280	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.22	96	43159	6.98	ng/uL	0.00
5) Phenol-d5	6.81	99	789421	35.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	514491	38.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	604722	35.80	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	617206	36.12	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	279503	38.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	269107	39.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	596570	34.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	885230	43.98	ng/ul	0.00
43) Dimethylphthalate-d6	13.68	166	2126799	38.35	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	2334225	36.89	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	294545	34.26	ng/ul	0.00
57) Fluorene-d10	15.26	176	1730247	37.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	165178	28.46	ng/ul	0.00
70) Anthracene-d10	17.10	188	2716659	37.70	ng/ul	0.00
78) Pyrene-d10	19.40	212	3036745	36.42	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	3184889	37.50	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.33	70	18030	1.249	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111319\
Data File : BN008526.D
Acq On : 13 Nov 2019 17:24
Operator : JU
Sample : PB124539BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Nov 14 03:28:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 15:23:53 2019
Response via : Initial Calibration

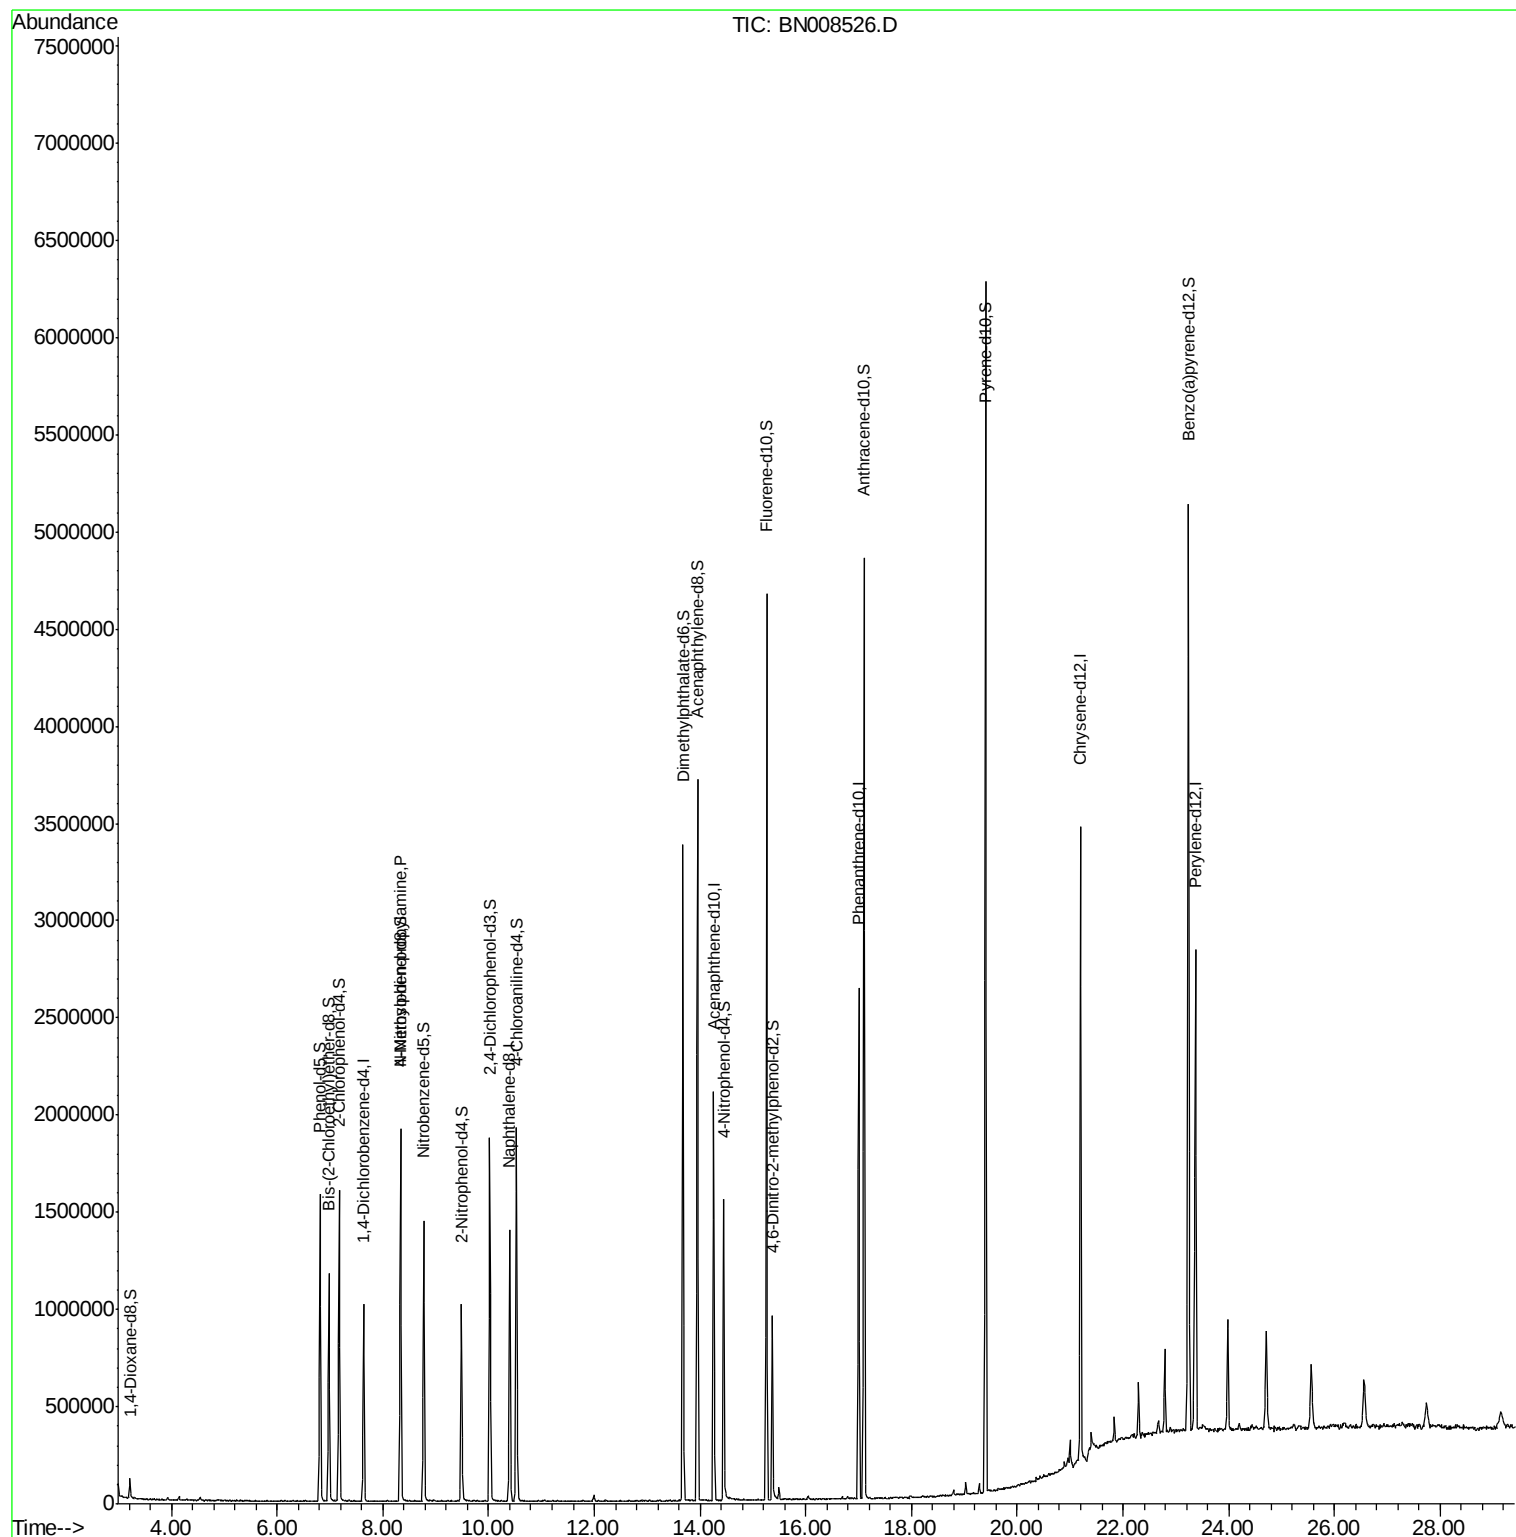

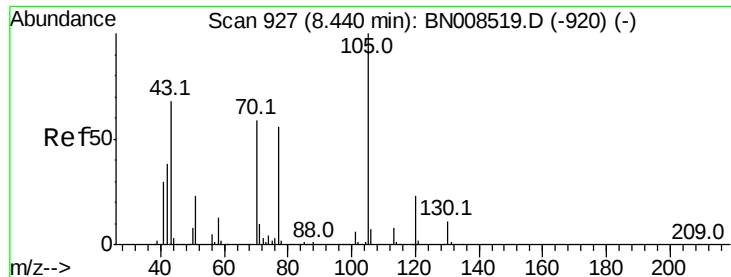

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.249 ng/ul
 RT: 8.33 min Scan# 908
 Delta R.T. -0.11 min
 Lab File: BN008526.D
 Acq: 13 Nov 2019 17:24

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 18030
 Ion Ratio Lower Upper
 70 100
 42 375.6 52.0 78.0#
 101 0.0 7.5 11.3#
 130 0.0 14.9 22.3#

