

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111319\
 Data File : BN008532.D
 Acq On : 13 Nov 2019 21:00
 Operator : JU
 Sample : K5627-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BEJR2

Quant Time: Nov 14 03:29:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 15:23:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	260754	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1084846	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	716543	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	1550649	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	1480605	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	1620383	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	36954	5.75	ng/uL	0.00
5) Phenol-d5	6.81	99	152171	6.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	405515	28.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	412789	23.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	275840	15.52	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	228988	30.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	220182	31.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	463333	26.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	39461	1.90	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	1835920	32.37	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1993777	30.81	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	51053	5.81	ng/ul	0.00
57) Fluorene-d10	15.26	176	1507404	31.99	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	162547	27.46	ng/ul	0.00
70) Anthracene-d10	17.10	188	2575703	35.05	ng/ul	0.00
78) Pyrene-d10	19.39	212	2970749	35.14	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.23	264	3030089	36.01	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.84	94	28266	1.197 ng/ul	96
44) Dimethylphthalate	13.72	163	154046	2.805 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111319\
Data File : BN008532.D
Acq On : 13 Nov 2019 21:00
Operator : JU
Sample : K5627-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BEJR2

Quant Time: Nov 14 03:29:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 15:23:53 2019
Response via : Initial Calibration

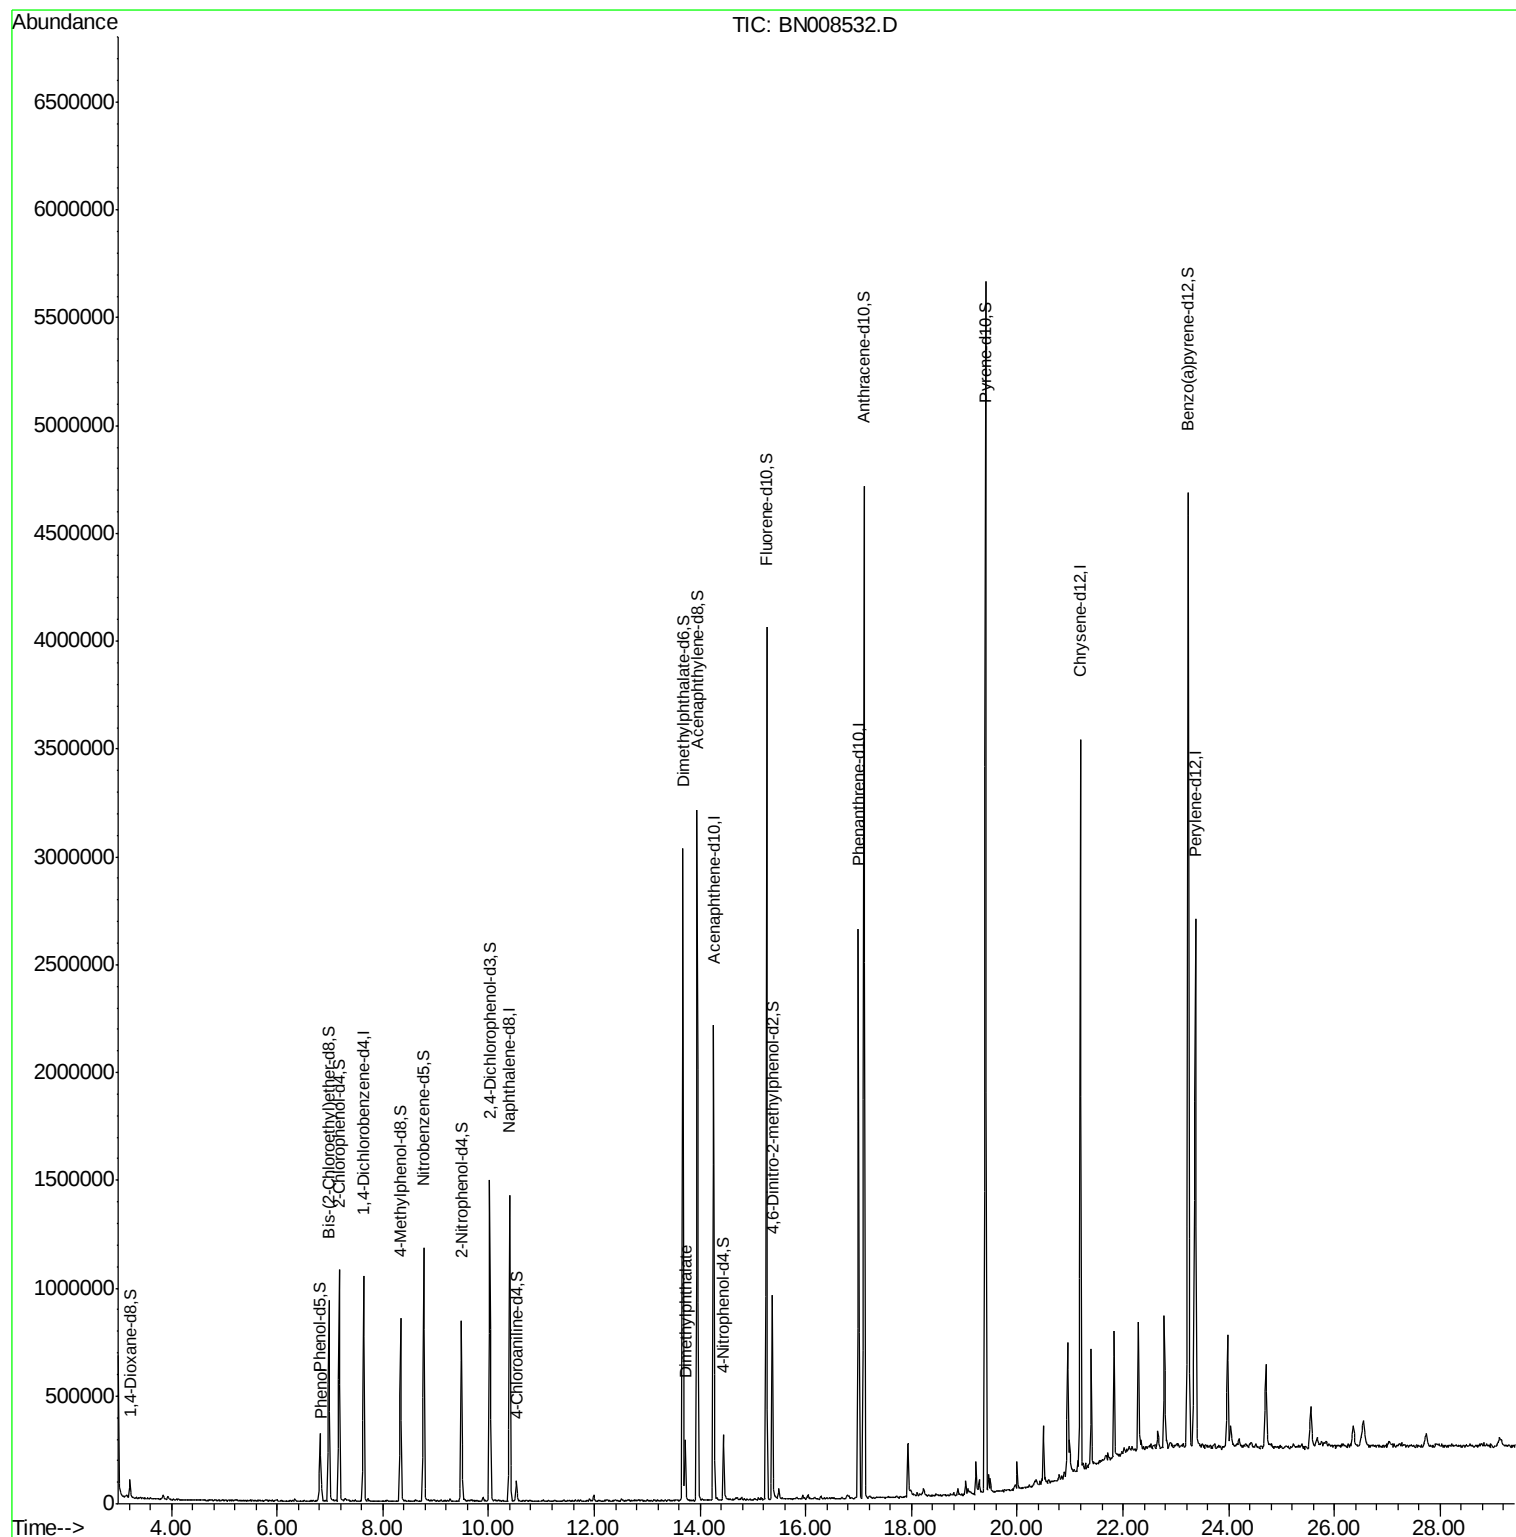

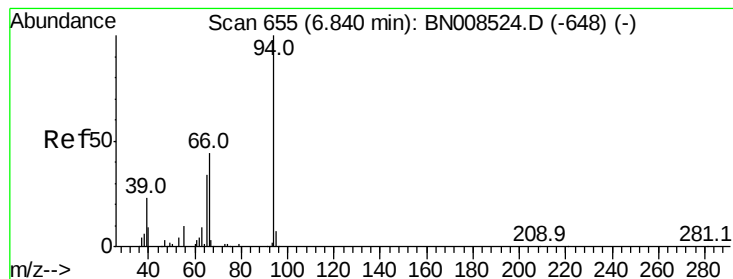





#6

Phenol

Concen: 1.197 ng/ul
 RT: 6.84 min Scan# 655
 Delta R.T. -0.00 min
 Lab File: BN008532.D
 Acq: 13 Nov 2019 21:00

Instrument :
 BNA_N
 ClientSampleId :
 BEJR2

Tot Ion: 94 Resp: 28266
 Ion Ratio Lower Upper
 94 100
 65 33.1 27.7 41.5
 66 50.1 37.0 55.6

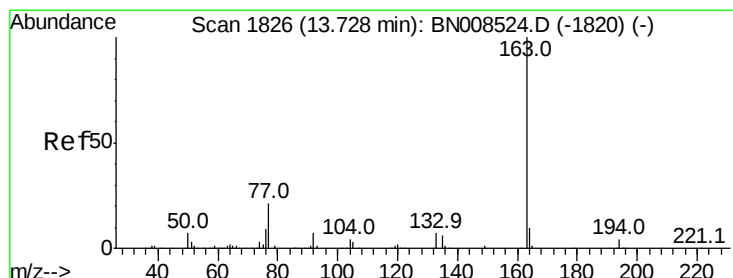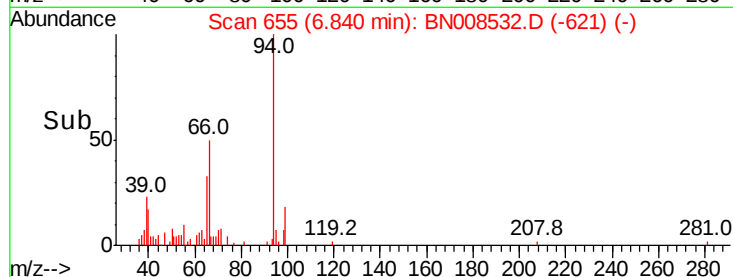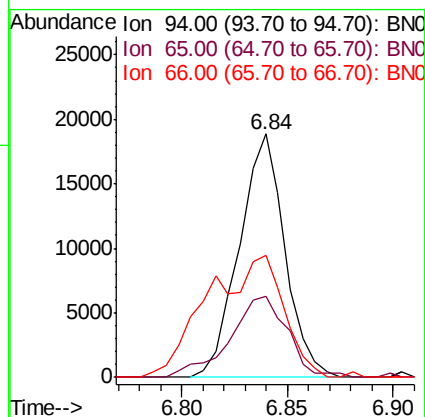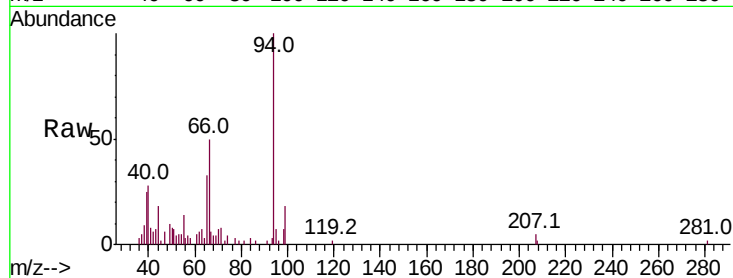

#44

Dimethylphthalate

Concen: 2.805 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BN008532.D
 Acq: 13 Nov 2019 21:00

Tgt Ion: 163 Resp: 154046
 Ion Ratio Lower Upper
 163 100
 194 5.0 3.6 5.4
 164 10.7 8.1 12.1

