

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111319\
 Data File : BN008540.D
 Acq On : 14 Nov 2019 02:24
 Operator : JU
 Sample : K5679-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0CM6

Quant Time: Nov 14 03:30:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 15:23:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	293723	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1223127	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	803151	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	1725886	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	1591326	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	1770029	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	41029	5.66	ng/uL	0.00
5) Phenol-d5	6.81	99	111468	4.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	276013	17.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	284005	14.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	194075	9.69	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	151002	18.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	152844	19.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	331556	16.60	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	21410	0.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	1234920	19.43	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1319864	18.20	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	36169	3.67	ng/ul	0.00
57) Fluorene-d10	15.25	176	1000167	18.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	102987	15.63	ng/ul	0.00
70) Anthracene-d10	17.10	188	1630802	19.94	ng/ul	0.00
78) Pyrene-d10	19.39	212	1893115	20.83	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.23	264	1944404	21.15	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.83	94	51273	1.927 ng/ul	95
44) Dimethylphthalate	13.72	163	199709	3.245 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111319\
Data File : BN008540.D
Acq On : 14 Nov 2019 02:24
Operator : JU
Sample : K5679-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0CM6

Quant Time: Nov 14 03:30:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 15:23:53 2019
Response via : Initial Calibration

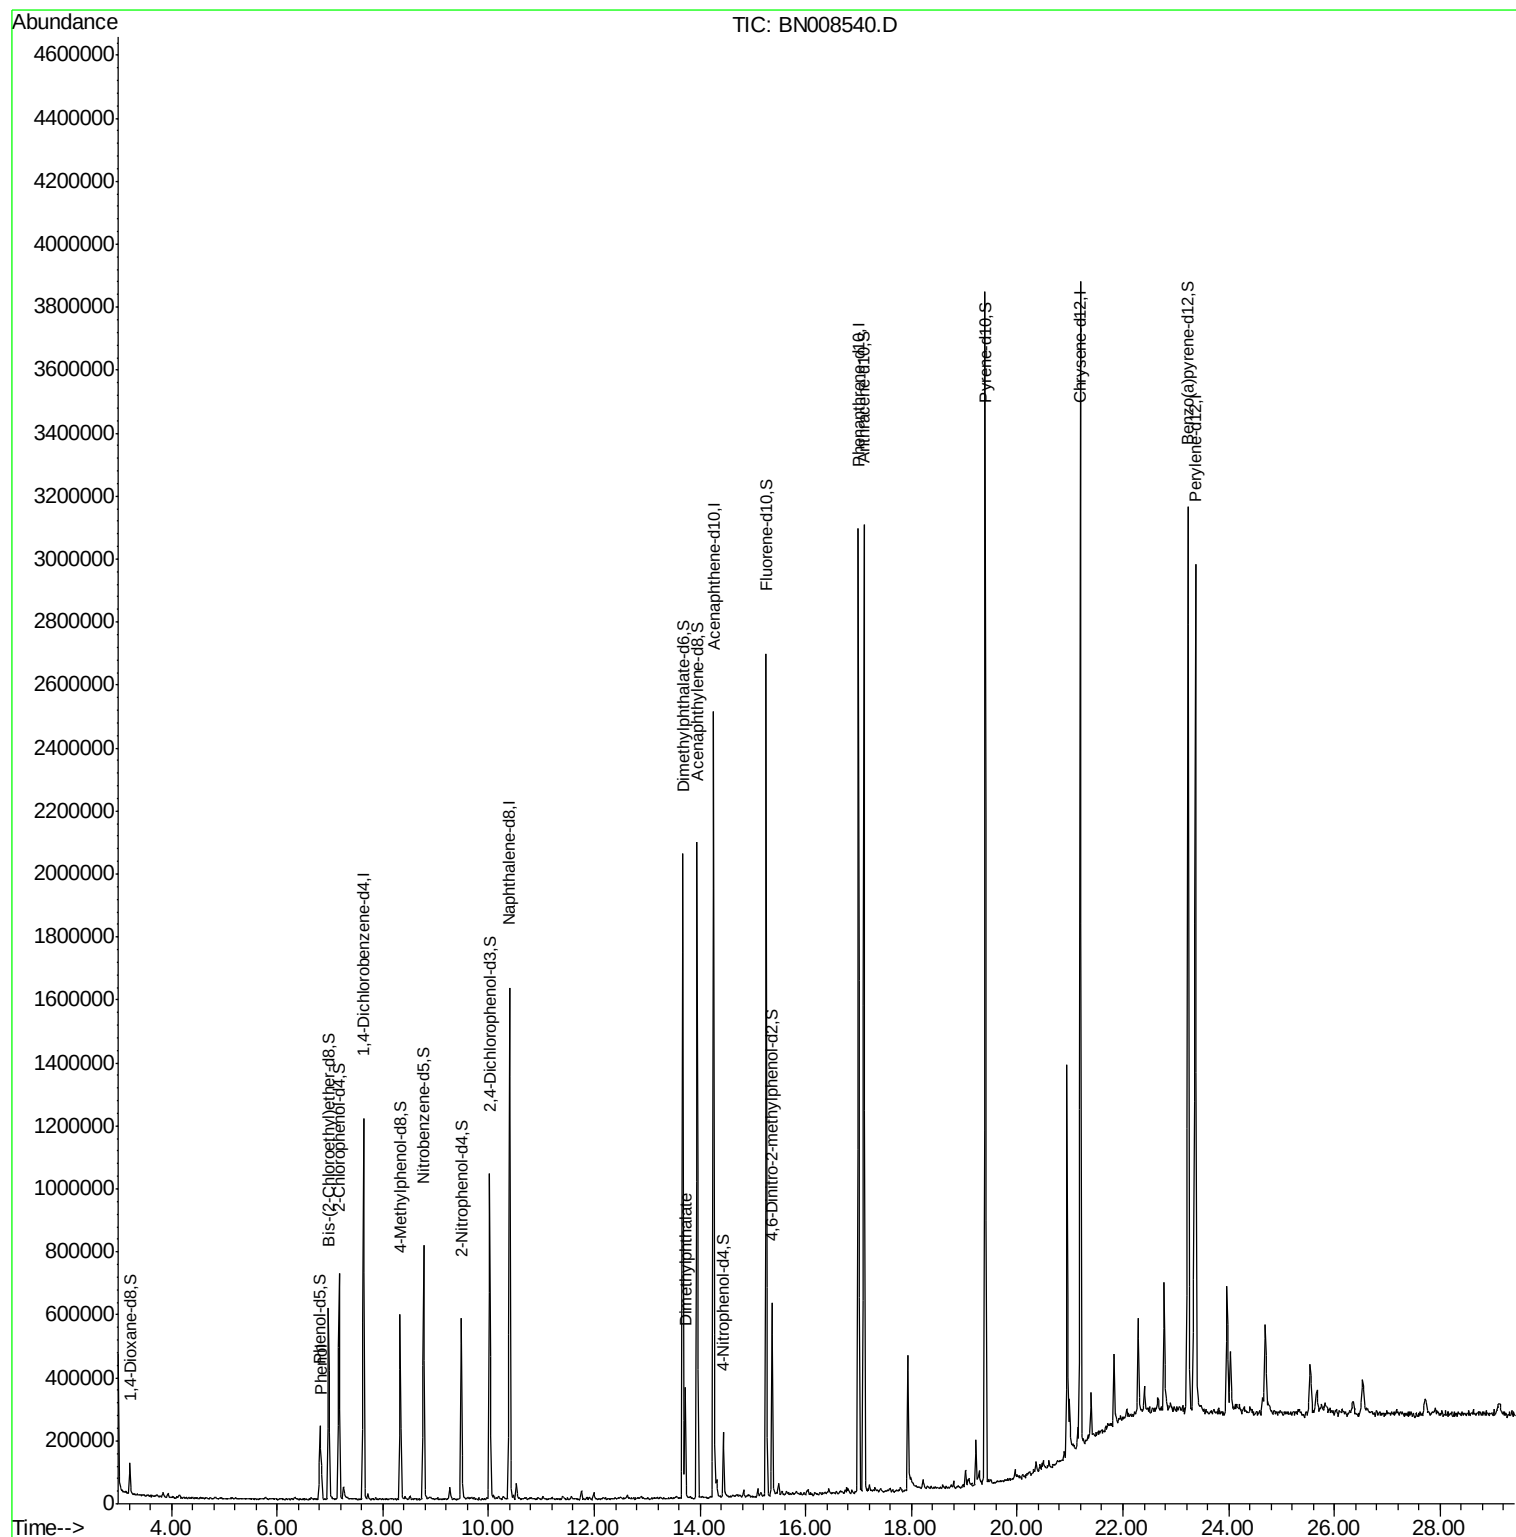

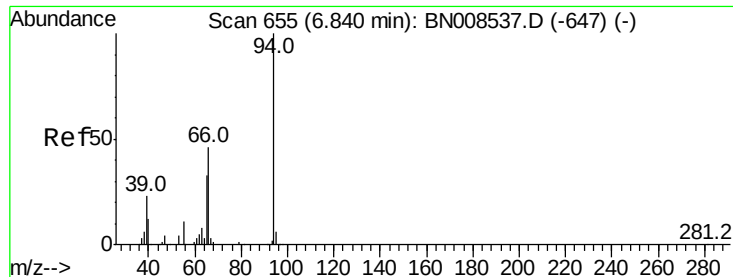





#6

Phenol

Concen: 1.927 ng/ul
 RT: 6.83 min Scan# 654
 Delta R.T. -0.01 min
 Lab File: BN008540.D
 Acq: 14 Nov 2019 02:24

Instrument :
 BNA_N
 ClientSampleId :
 C0CM6

Tot Ion: 94 Resp: 51273
 Ion Ratio Lower Upper
 94 100
 65 32.8 27.7 41.5
 66 42.0 37.0 55.6

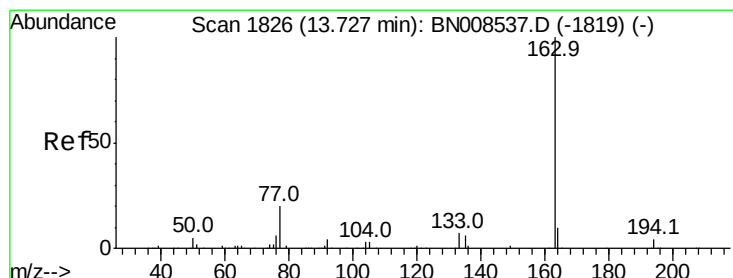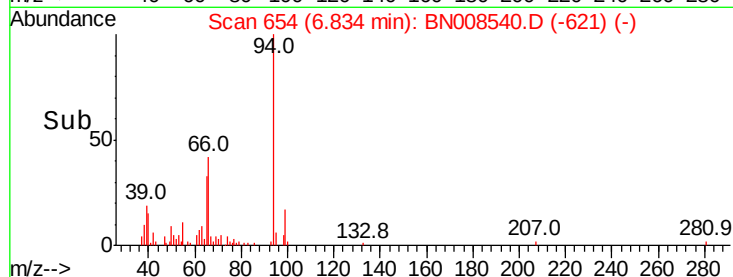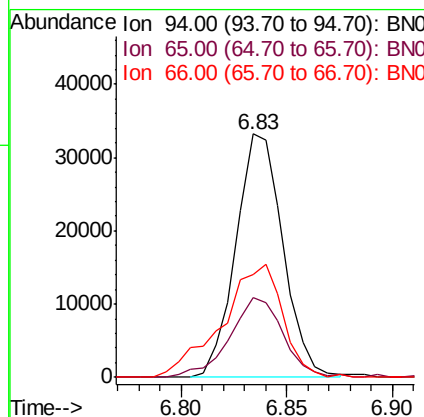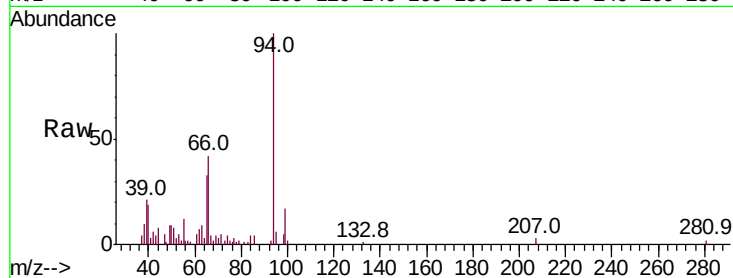

#44

Dimethylphthalate

Concen: 3.245 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BN008540.D
 Acq: 14 Nov 2019 02:24

Tgt Ion: 163 Resp: 199709
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.6 5.4
 164 9.7 8.1 12.1

