

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111319\
 Data File : BN008541.D
 Acq On : 14 Nov 2019 03:00
 Operator : JU
 Sample : K5679-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0CM7

Quant Time: Nov 14 04:39:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Nov 13 15:23:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	307887	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	1309146	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	850295	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	1842858	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	1740178	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	1842653	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	41972	5.53	ng/uL	0.00
5) Phenol-d5	6.81	99	118451	4.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	296876	17.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	299621	14.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	225102	10.72	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	165458	18.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	163662	19.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	382726	17.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	25629	1.02	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	1445796	21.48	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	1547187	20.15	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	41267	3.96	ng/ul	0.00
57) Fluorene-d10	15.25	176	1175997	21.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	121224	17.23	ng/ul	0.00
70) Anthracene-d10	17.10	188	1898128	21.73	ng/ul	0.00
78) Pyrene-d10	19.40	212	2159877	21.74	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	2155929	22.53	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.84	94	44165	1.584 ng/ul	91
44) Dimethylphthalate	13.72	163	212475	3.261 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111319\
Data File : BN008541.D
Acq On : 14 Nov 2019 03:00
Operator : JU
Sample : K5679-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0CM7

Quant Time: Nov 14 04:39:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Nov 13 15:23:53 2019
Response via : Initial Calibration

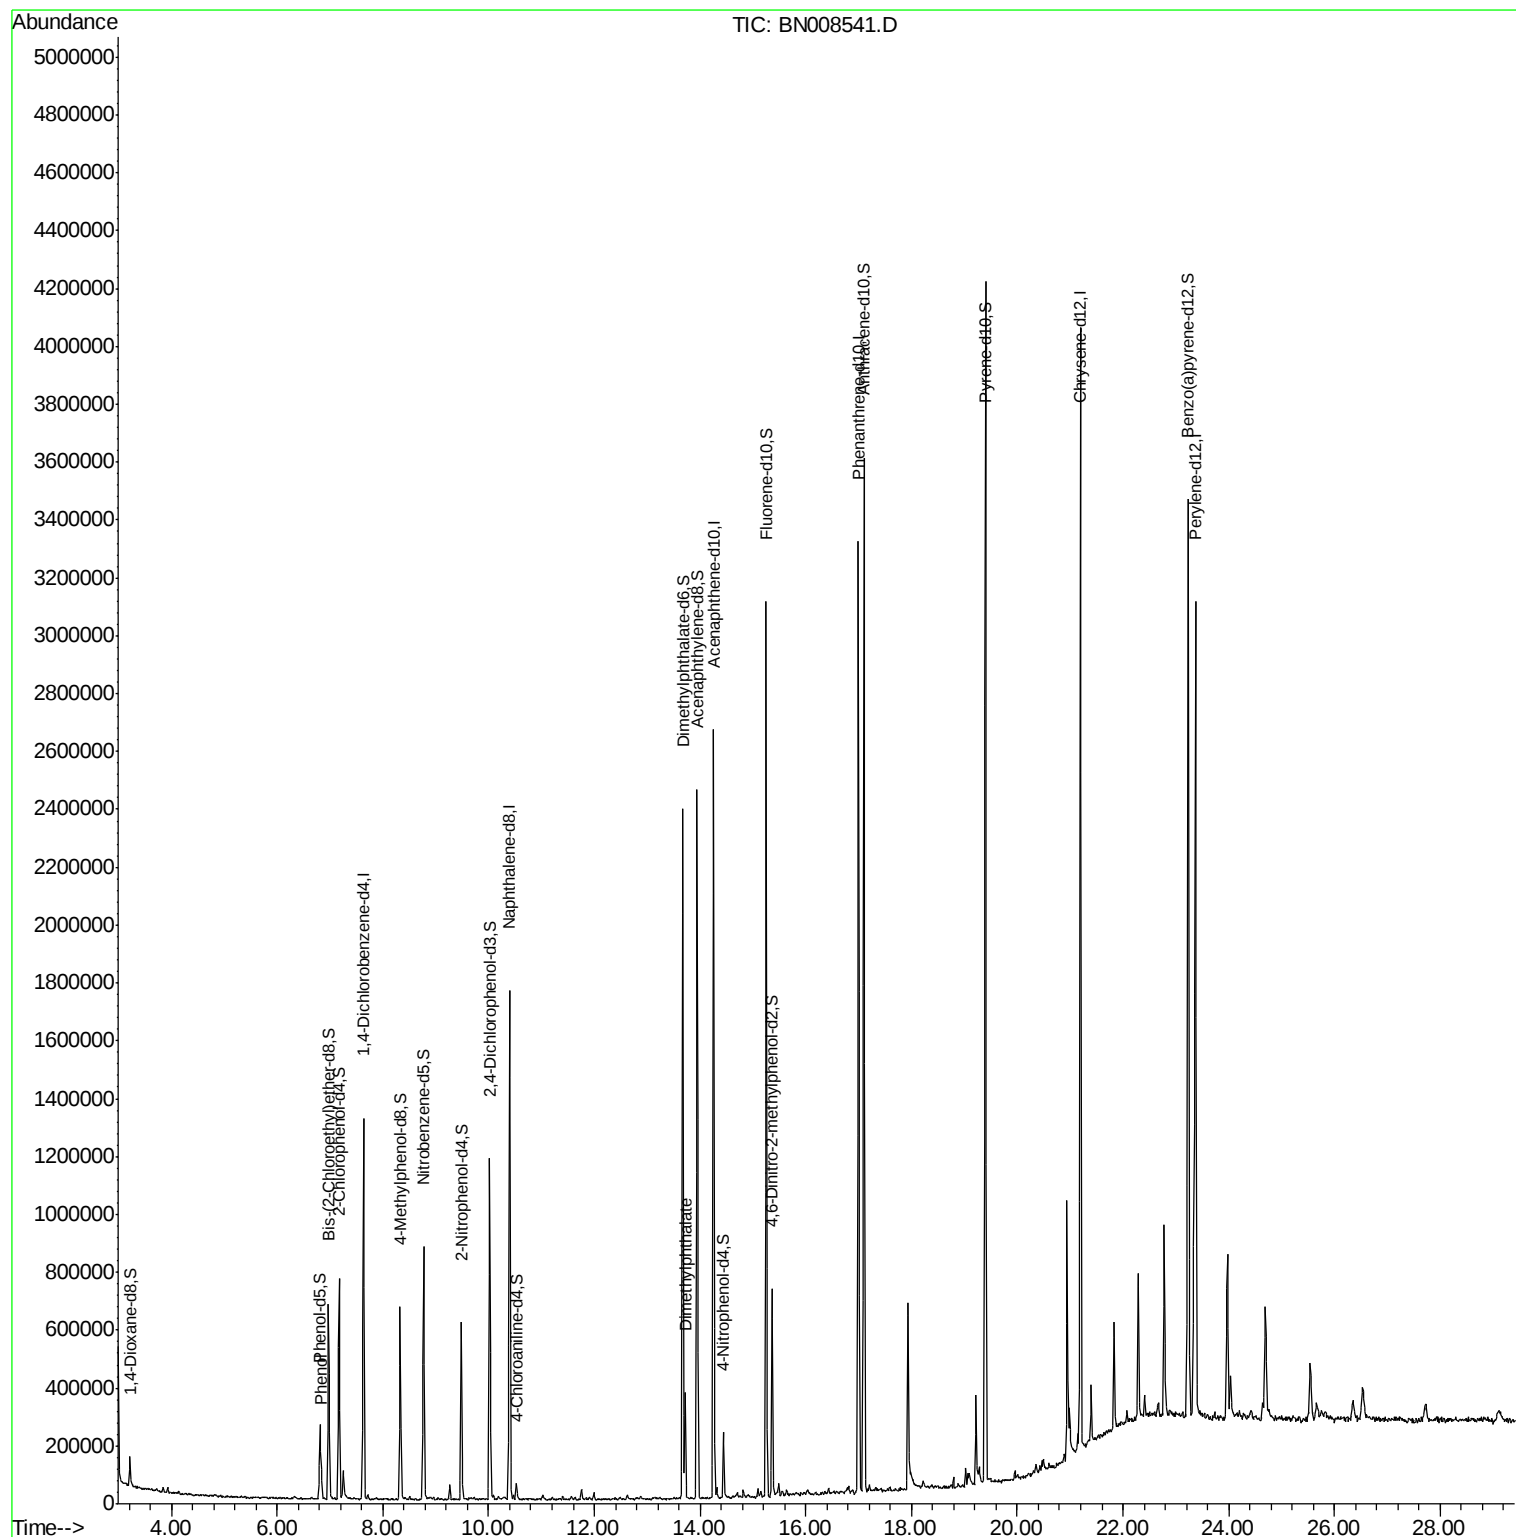

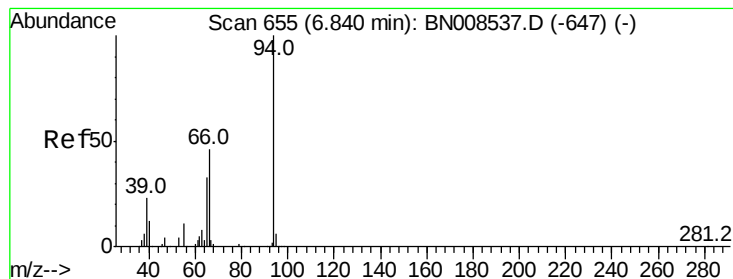





#6

Phenol

Concen: 1.584 ng/ul
 RT: 6.84 min Scan# 655
 Delta R.T. -0.00 min
 Lab File: BN008541.D
 Acq: 14 Nov 2019 03:00

Instrument :
 BNA_N
 ClientSampleId :
 C0CM7

Tot Ion: 94 Resp: 44165
 Ion Ratio Lower Upper
 94 100
 65 32.4 27.7 41.5
 66 37.2 37.0 55.6

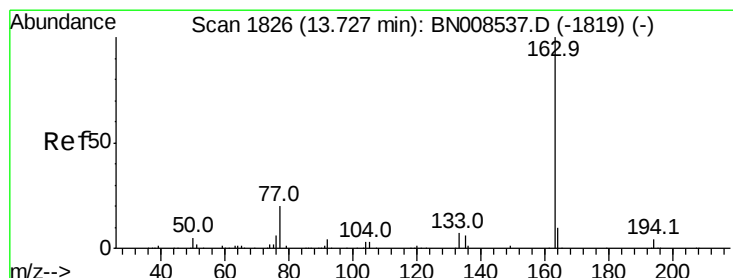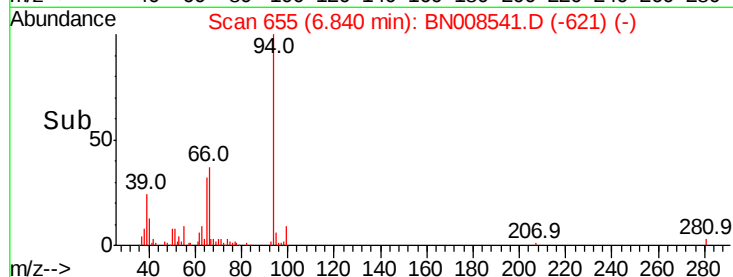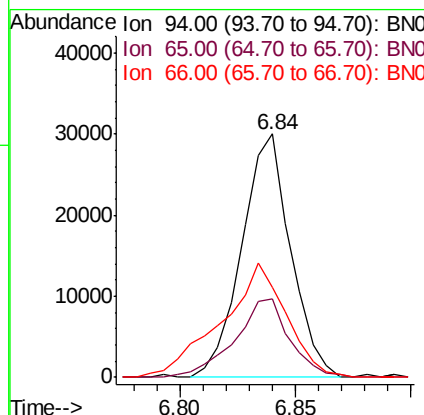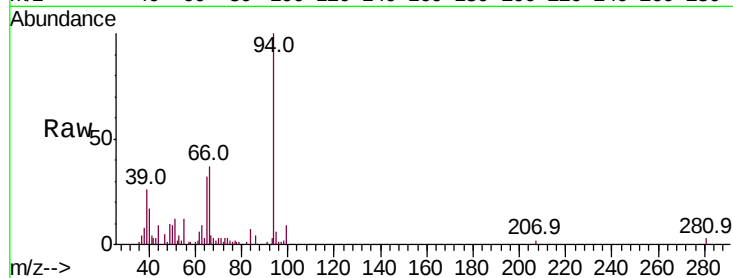

#44

Dimethylphthalate

Concen: 3.261 ng/ul
 RT: 13.72 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BN008541.D
 Acq: 14 Nov 2019 03:00

Tgt Ion: 163 Resp: 212475
 Ion Ratio Lower Upper
 163 100
 194 4.5 3.6 5.4
 164 10.3 8.1 12.1

