

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN111319\
 Data File : BN008562.D
 Acq On : 14 Nov 2019 18:31
 Operator : JU
 Sample : K5656-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A5451

Quant Time: Nov 15 04:30:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 15 04:28:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	549984	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	2314094	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.26	164	1508898	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	3214083	20.00	ng/ul	0.00
77) Chrysene-d12	21.20	240	2875449	20.00	ng/ul	0.00
85) Perylene-d12	23.38	264	3093556	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	54915	4.05	ng/uL	0.00
5) Phenol-d5	6.82	99	191658	3.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	426453	14.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	476813	12.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	338013	9.01	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	284543	18.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	315190	21.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.02	165	566989	15.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	52055	1.18	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	2016776	16.89	ng/ul	0.00
46) Acenaphthylene-d8	13.95	160	2253070	16.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	83197	4.49	ng/ul	0.00
57) Fluorene-d10	15.26	176	1734986	17.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.37	200	238108	19.41	ng/ul	0.00
70) Anthracene-d10	17.10	188	2747733	18.04	ng/ul	0.00
78) Pyrene-d10	19.40	212	3039180	18.51	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.24	264	2910764	18.12	ng/ul	0.00

Target Compounds


				Ovalue	
44) Dimethylphthalate	13.72	163	131529	1.137	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111319\
Data File : BN008562.D
Acq On : 14 Nov 2019 18:31
Operator : JU
Sample : K5656-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A5451

Quant Time: Nov 15 04:30:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 04:28:01 2019
Response via : Initial Calibration

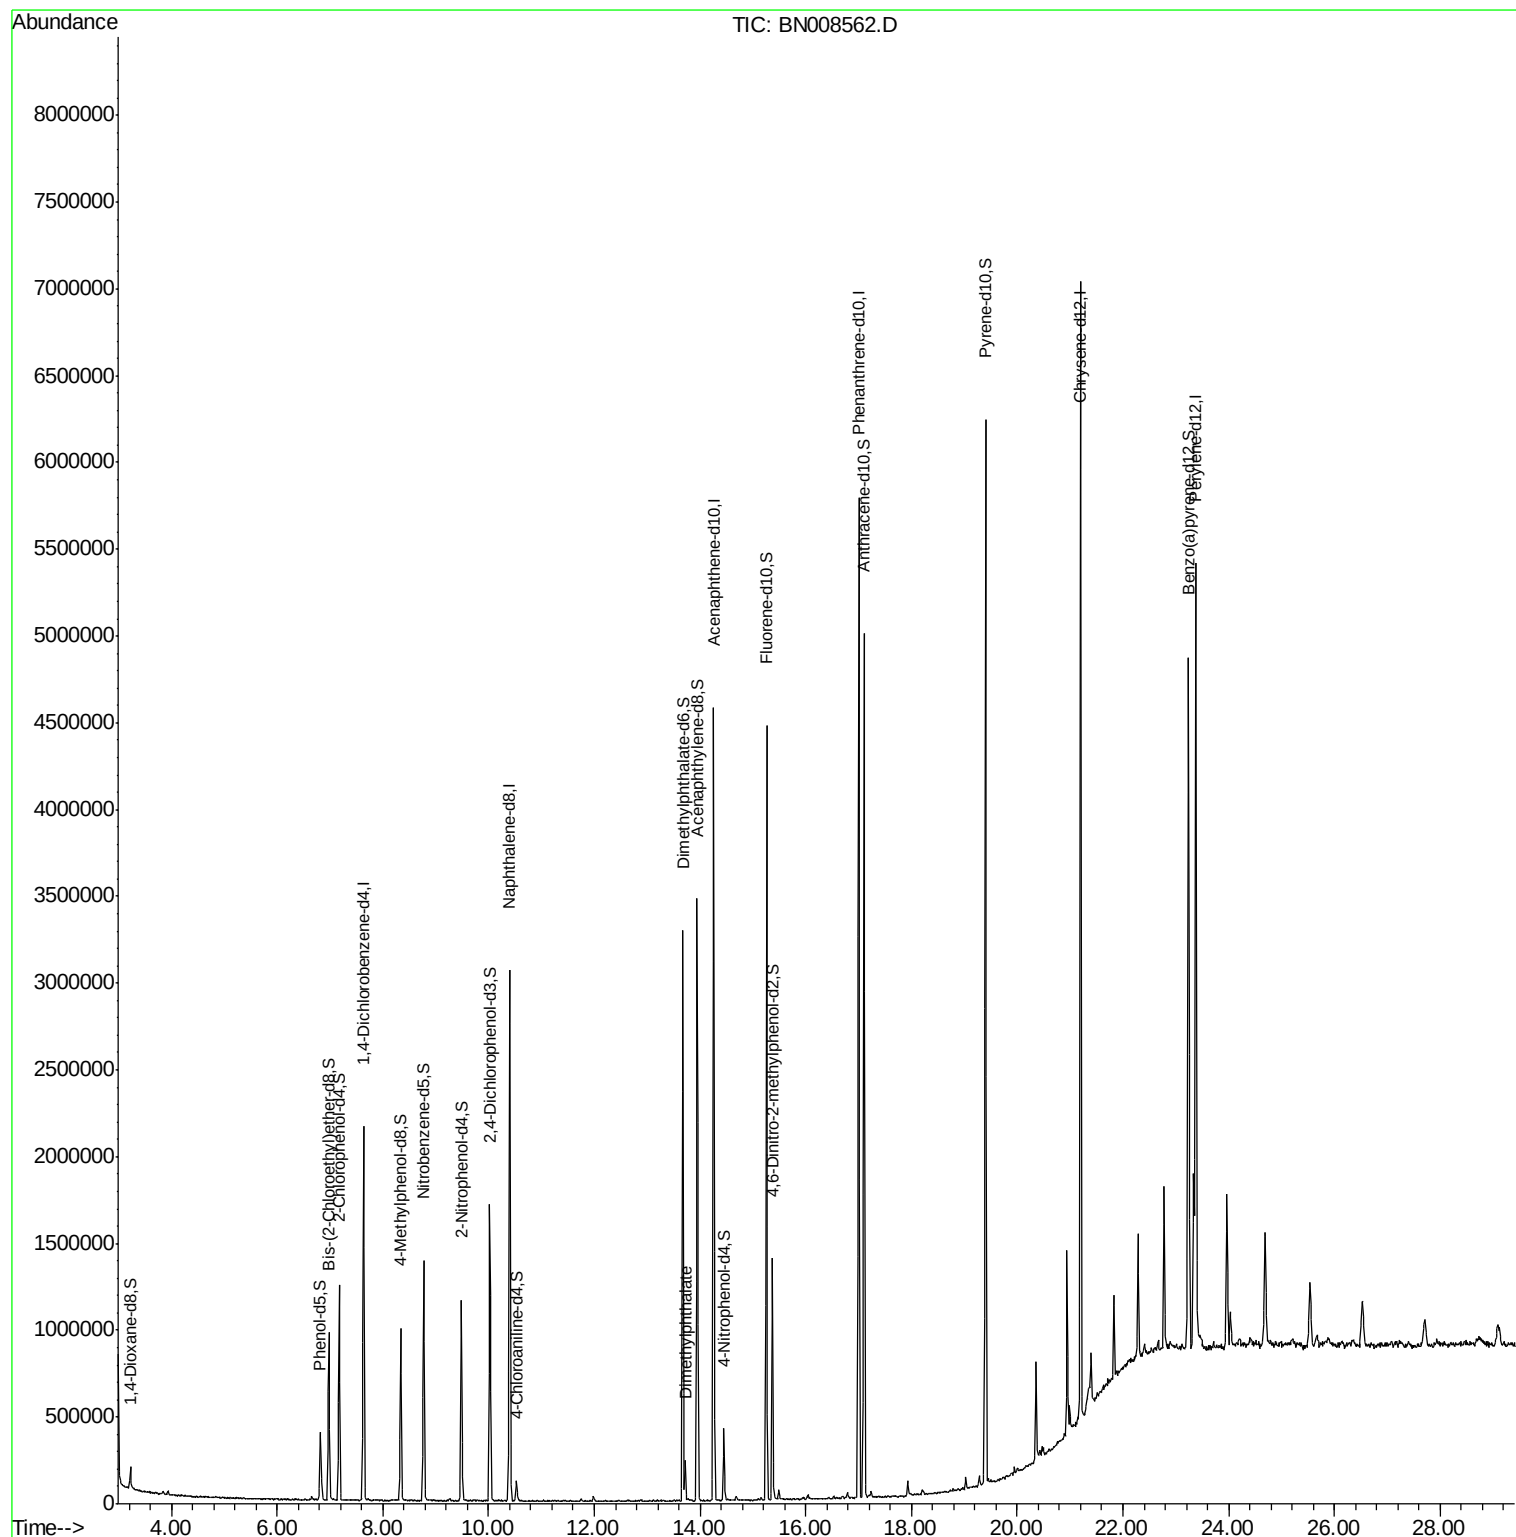

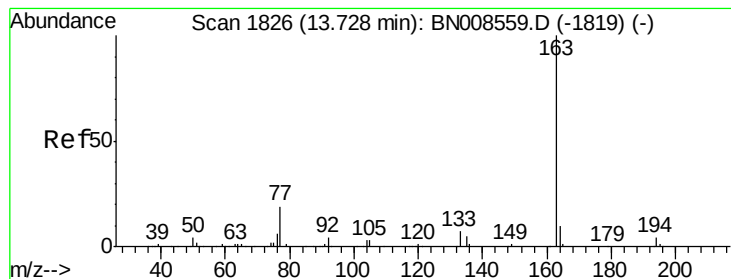

#44

Dimethylphthalate

Concen: 1.137 ng/ul

RT: 13.72 min Scan# 1825

Delta R.T. -0.01 min

Lab File: BN008562.D

Acq: 14 Nov 2019 18:31

Instrument :

BNA_N

ClientSampleId :

A5451


Tot Ion:163 Resp: 131529

Ion Ratio Lower Upper

163 100

194 4.6 3.6 5.4

164 11.3 8.1 12.1

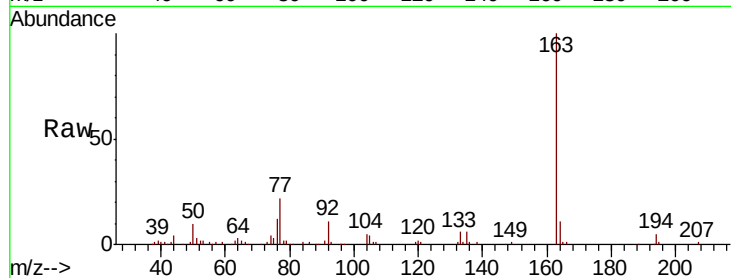

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

