

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111319\
 Data File : BN008583.D
 Acq On : 15 Nov 2019 09:59
 Operator : JU
 Sample : K5739-03DL 5X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0CR1DL

Quant Time: Nov 15 12:41:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Nov 15 04:28:01 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.63	152	397005	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.39	136	1622836	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.25	164	1092362	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.00	188	2310157	20.00	ng/ul	0.00
77) Chrysene-d12	21.19	240	2103798	20.00	ng/ul	0.00
85) Perylene-d12	23.37	264	2194840	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
5) Phenol-d5	6.81	99	38126	1.09	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.98	67	101791	4.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.17	132	100757	3.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.33	113	71730	2.65	ng/ul	-0.01
19) Nitrobenzene-d5	8.76	128	63006	5.70	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.48	143	62677	6.04	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.02	165	122026	4.61	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.53	131	10638	0.34	ng/ul	0.00
43) Dimethylphthalate-d6	13.67	166	476991	5.52	ng/ul	-0.01
46) Acenaphthylene-d8	13.94	160	502902	5.10	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.45	143	14075	1.05	ng/ul	-0.01
57) Fluorene-d10	15.25	176	400192	5.57	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	40899	4.64	ng/ul	-0.01
70) Anthracene-d10	17.09	188	644064	5.88	ng/ul	0.00
78) Pyrene-d10	19.39	212	706985	5.88	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.23	264	676168	5.93	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
20) Nitrobenzene	8.80	77	643307	21.153	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN111319\
Data File : BN008583.D
Acq On : 15 Nov 2019 09:59
Operator : JU
Sample : K5739-03DL 5X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0CR1DL

Quant Time: Nov 15 12:41:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN111319MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Nov 15 04:28:01 2019
Response via : Initial Calibration

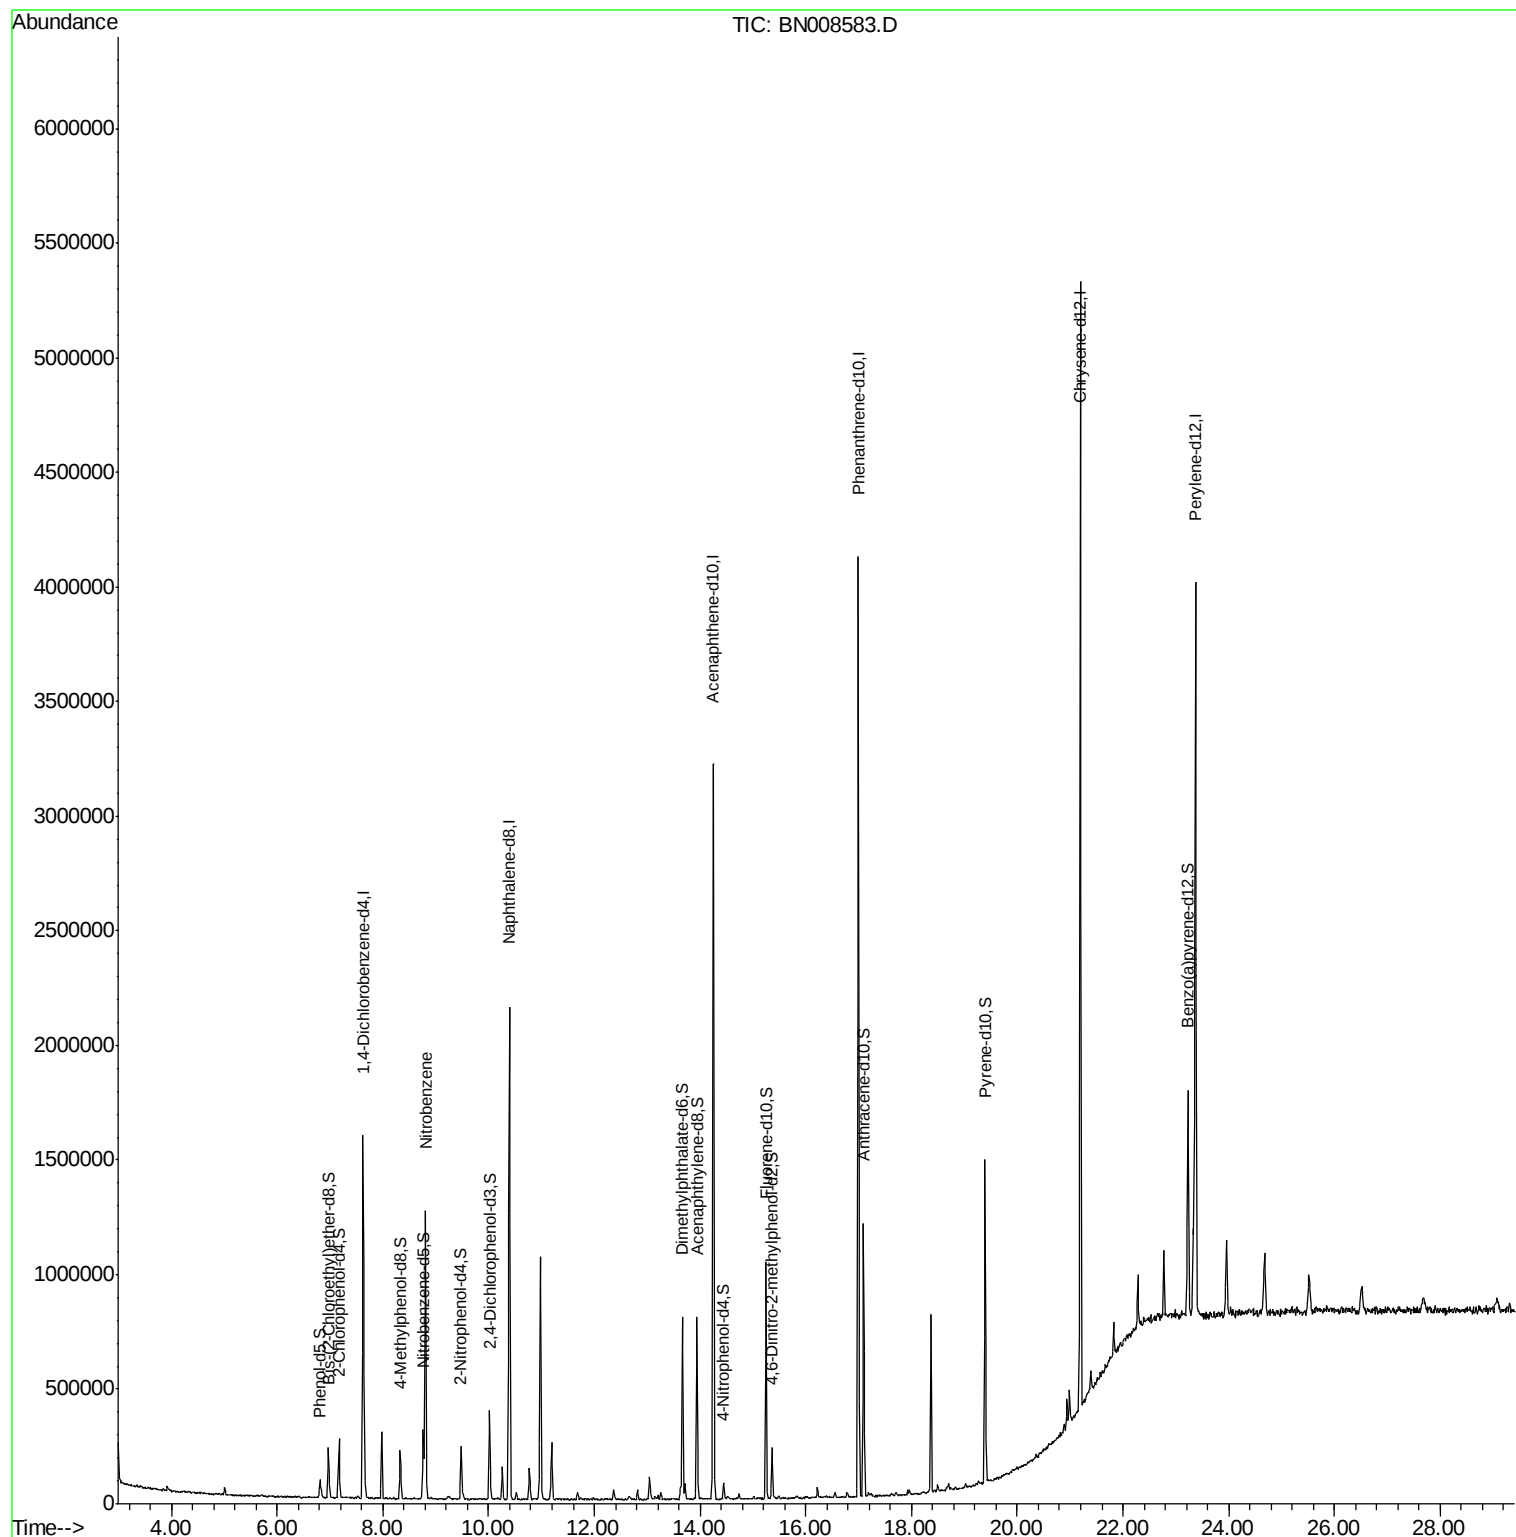

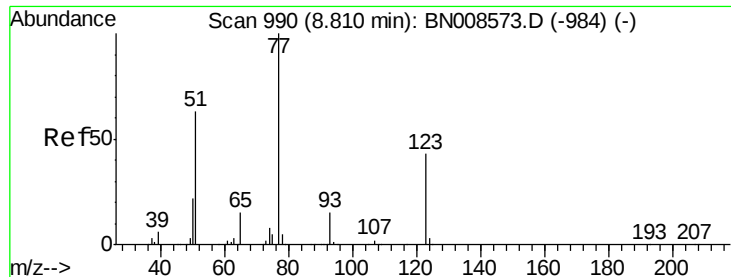

#20
 Nitrobenzene
 Concen: 21.153 ng/ul
 RT: 8.80 min Scan# 989
 Delta R.T. -0.01 min
 Lab File: BN008583.D
 Acq: 15 Nov 2019 09:59

Instrument :
 BNA_N
 ClientSampleId :
 C0CR1DL

Tot Ion	Ion	Ratio	Lower	Upper
77	100			
123	39.8	31.3	46.9	
65	14.8	12.5	18.7	

