

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
 Data File : BN017407.D
 Acq On : 14 Nov 2021 01:01
 Operator : CG/JU
 Sample : M4524-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG397

Quant Time: Nov 15 04:30:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 02:31:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.877	152	6914	0.400	ng/ul	0.00
4) Naphthalene-d8	10.669	136	25657	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.509	164	16545	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.249	188	34209	0.400	ng/ul	0.00
17) Chrysene-d12	21.431	240	24586	0.400	ng/ul	0.00
23) Perylene-d12	23.807	264	22247	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.333	96	25375	3.346	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.264	152	13303	0.336	ng/ul	0.00
18) Fluoranthene-d10	19.278	212	37330	0.422	ng/ul	0.00
Target Compounds						
					Qvalue	
28) Dibenzo(a,h)anthracene	26.294	278	1106	0.023	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
Data File : BN017407.D
Acq On : 14 Nov 2021 01:01
Operator : CG/JU
Sample : M4524-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG397


Quant Time: Nov 15 04:30:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 02:31:43 2021
Response via : Initial Calibration

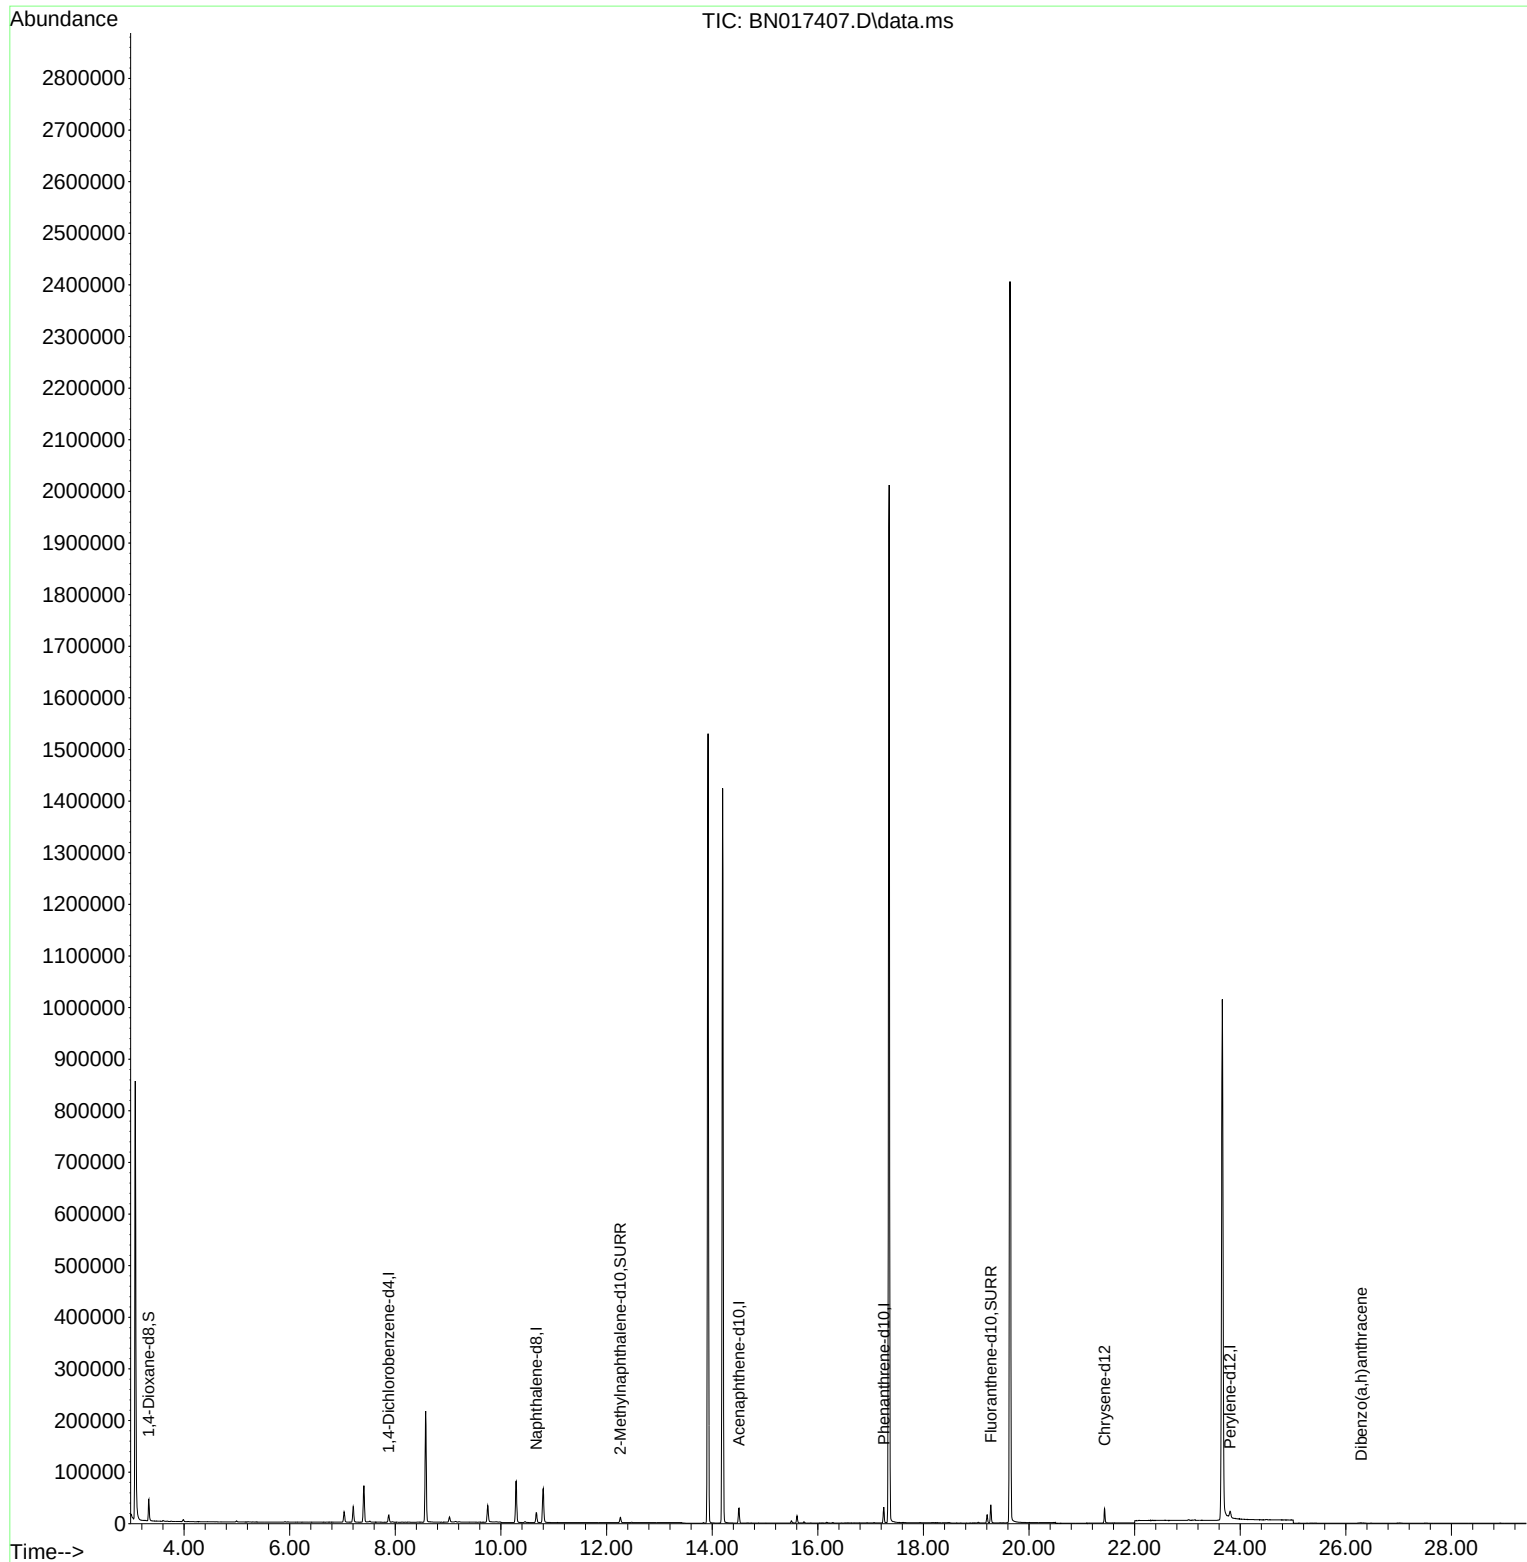

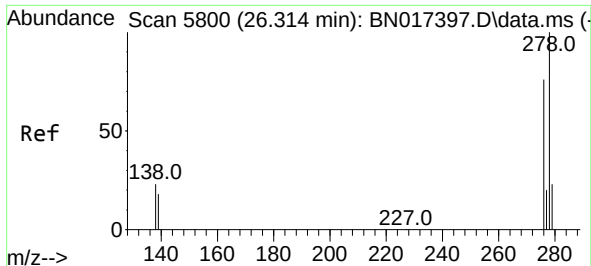

#28
 Dibenzo(a,h)anthracene
 Concen: 0.023 ng/ul
 RT: 26.294 min Scan# 51
 Delta R.T. -0.020 min
 Lab File: BN017407.D
 Acq: 14 Nov 2021 01:01

Instrument :
 BNA_N
 ClientSampleId :
 BG397

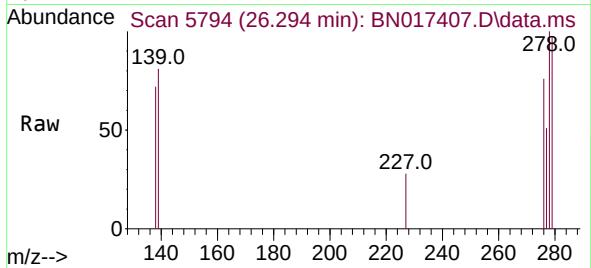

Tgt Ion:278 Resp: 1106
 Ion Ratio Lower Upper
 278 100
 139 81.3 21.8 32.8#
 279 96.6 26.3 39.5#

