

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
 Data File : BN017417.D
 Acq On : 14 Nov 2021 07:37
 Operator : CG/JU
 Sample : M4522-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG396

Quant Time: Nov 15 04:42:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 02:31:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.868	152	7101	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.667	136	27004	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.503	164	17497	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.243	188	34753	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	23461	0.400	ng/ul	-0.01
23) Perylene-d12	23.800	264	19819	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	37478	4.811	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.257	152	16330	0.392	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	41996	0.498	ng/ul	-0.01
Target Compounds						
					Qvalue	
27) Indeno(1,2,3-cd)pyrene	26.252	276	1394	0.024	ng/ul#	95
28) Dibenzo(a,h)anthracene	26.279	278	1068	0.025	ng/ul#	6
29) Benzo(g,h,i)perylene	27.000	276	1122	0.021	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
Data File : BN017417.D
Acq On : 14 Nov 2021 07:37
Operator : CG/JU
Sample : M4522-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG396

Quant Time: Nov 15 04:42:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 02:31:43 2021
Response via : Initial Calibration




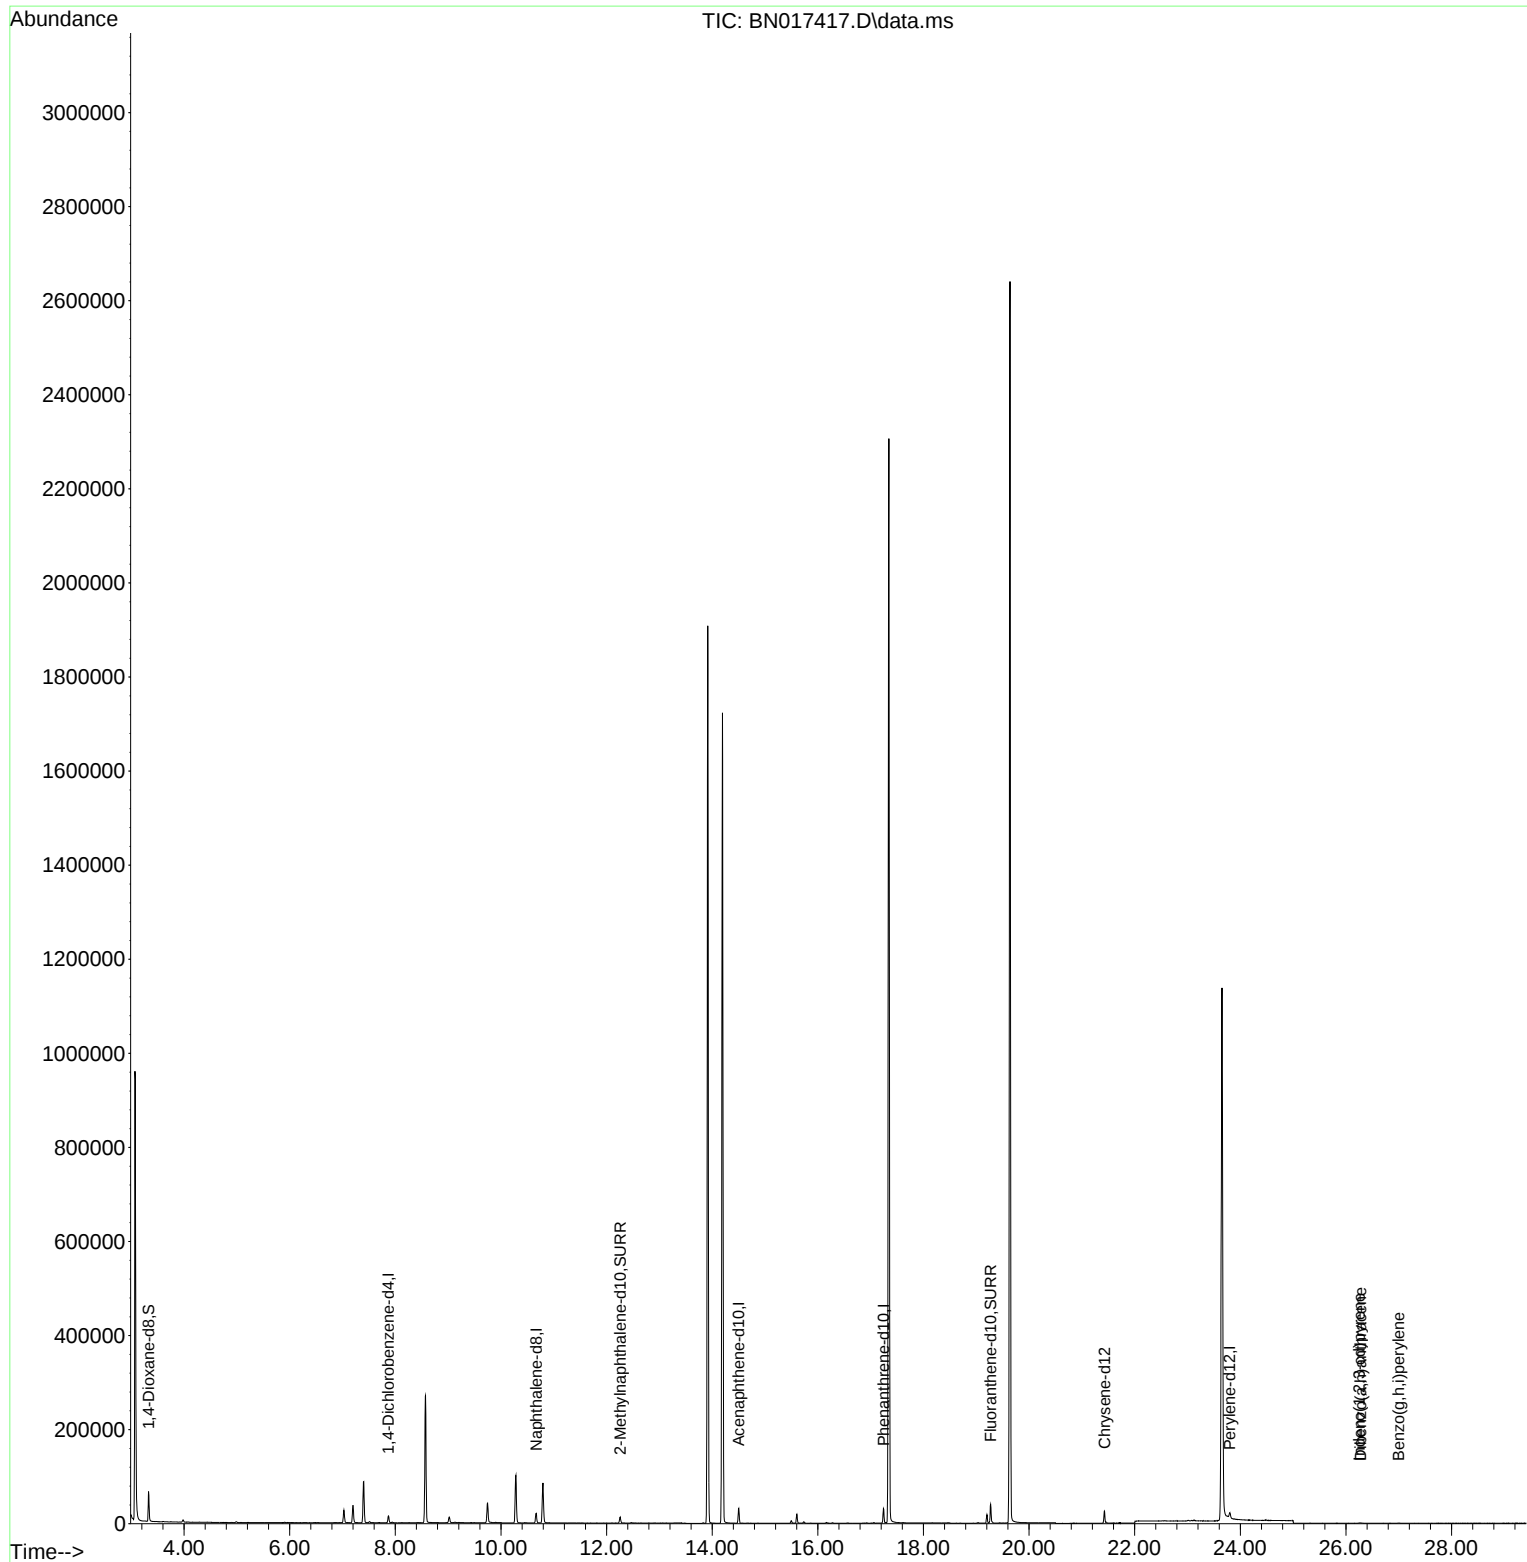


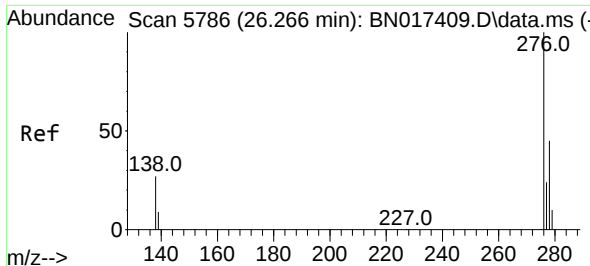

#27
 Indeno(1,2,3-cd)pyrene
 Concen: 0.024 ng/ul
 RT: 26.252 min Scan# 51
 Delta R.T. -0.035 min
 Lab File: BN017417.D
 Acq: 14 Nov 2021 07:37




Instrument :
 BNA_N
 ClientSampleId :
 BG396


Tgt Ion:276 Resp: 1394
 Ion Ratio Lower Upper
 276 100
 138 10.8 0.1 0.1#
 227 0.0 0.0 0.0

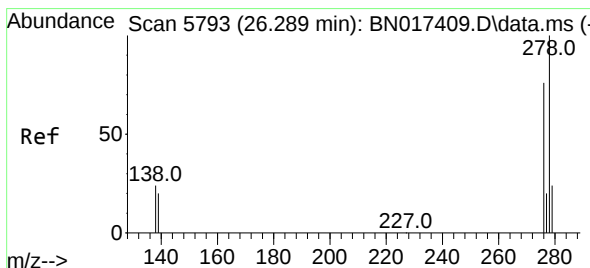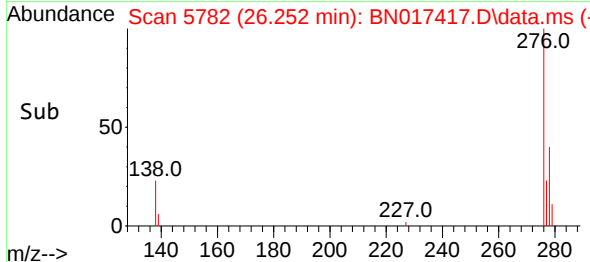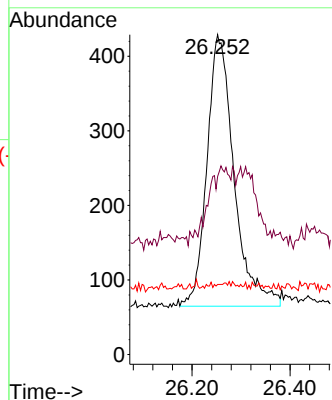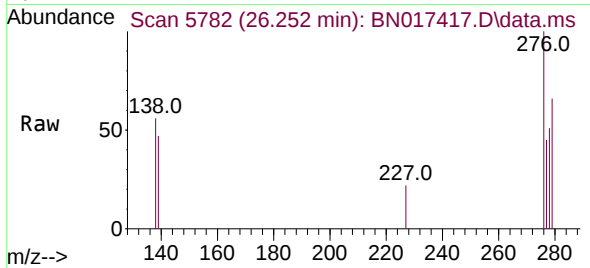

#28
 Dibenzo(a,h)anthracene
 Concen: 0.025 ng/ul
 RT: 26.279 min Scan# 5790
 Delta R.T. -0.035 min
 Lab File: BN017417.D
 Acq: 14 Nov 2021 07:37


Tgt Ion:278 Resp: 1068
 Ion Ratio Lower Upper
 278 100
 139 77.0 21.8 32.8#
 279 84.7 26.3 39.5#

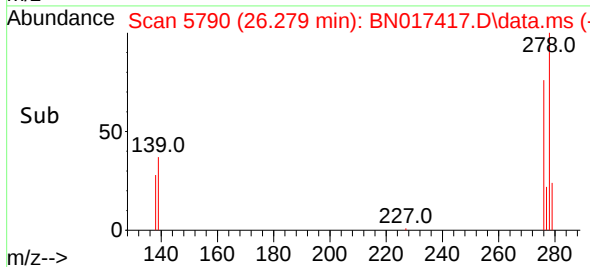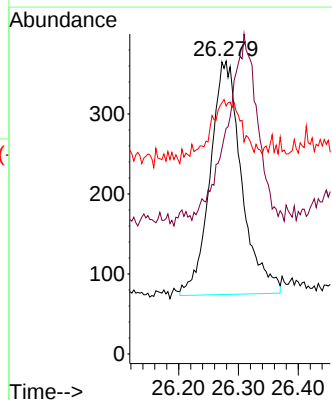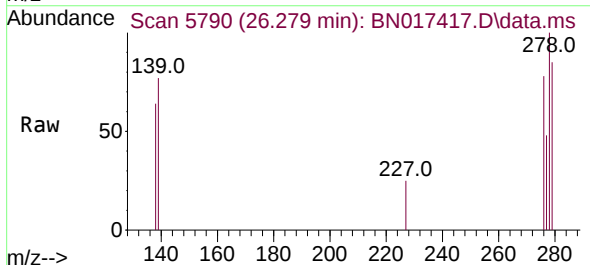

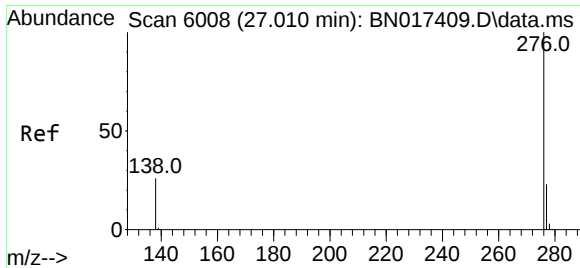

#29
 Benzo(g,h,i)perylene
 Concen: 0.021 ng/ul
 RT: 27.000 min Scan# 6005
 Delta R.T. -0.038 min
 Lab File: BN017417.D
 Acq: 14 Nov 2021 07:37

Instrument :
 BNA_N
 ClientSampleId :
 BG396

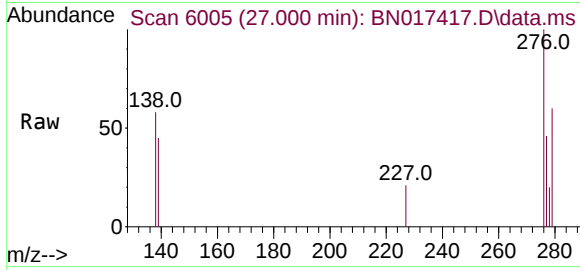

Tgt Ion:276 Resp: 1122
 Ion Ratio Lower Upper
 276 100
 138 57.7 24.5 36.7#
 277 46.1 21.2 31.8#

