

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
 Data File : BN017422.D
 Acq On : 14 Nov 2021 10:36
 Operator : CG/JU
 Sample : M4522-08
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG398

Quant Time: Nov 15 04:47:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 02:31:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.872	152	7755	0.400	ng/ul	0.00
4) Naphthalene-d8	10.663	136	28795	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.499	164	18459	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.244	188	38211	0.400	ng/ul	0.00
17) Chrysene-d12	21.425	240	28462	0.400	ng/ul	#-0.01
23) Perylene-d12	23.799	264	25951	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	47243	5.554	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.253	152	16356	0.368	ng/ul	-0.01
18) Fluoranthene-d10	19.269	212	47711	0.466	ng/ul	-0.01
Target Compounds						
15) Phenanthrene	17.282	178	2363	0.021	ng/ul#	Qvalue 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
Data File : BN017422.D
Acq On : 14 Nov 2021 10:36
Operator : CG/JU
Sample : M4522-08
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG398


Quant Time: Nov 15 04:47:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 02:31:43 2021
Response via : Initial Calibration

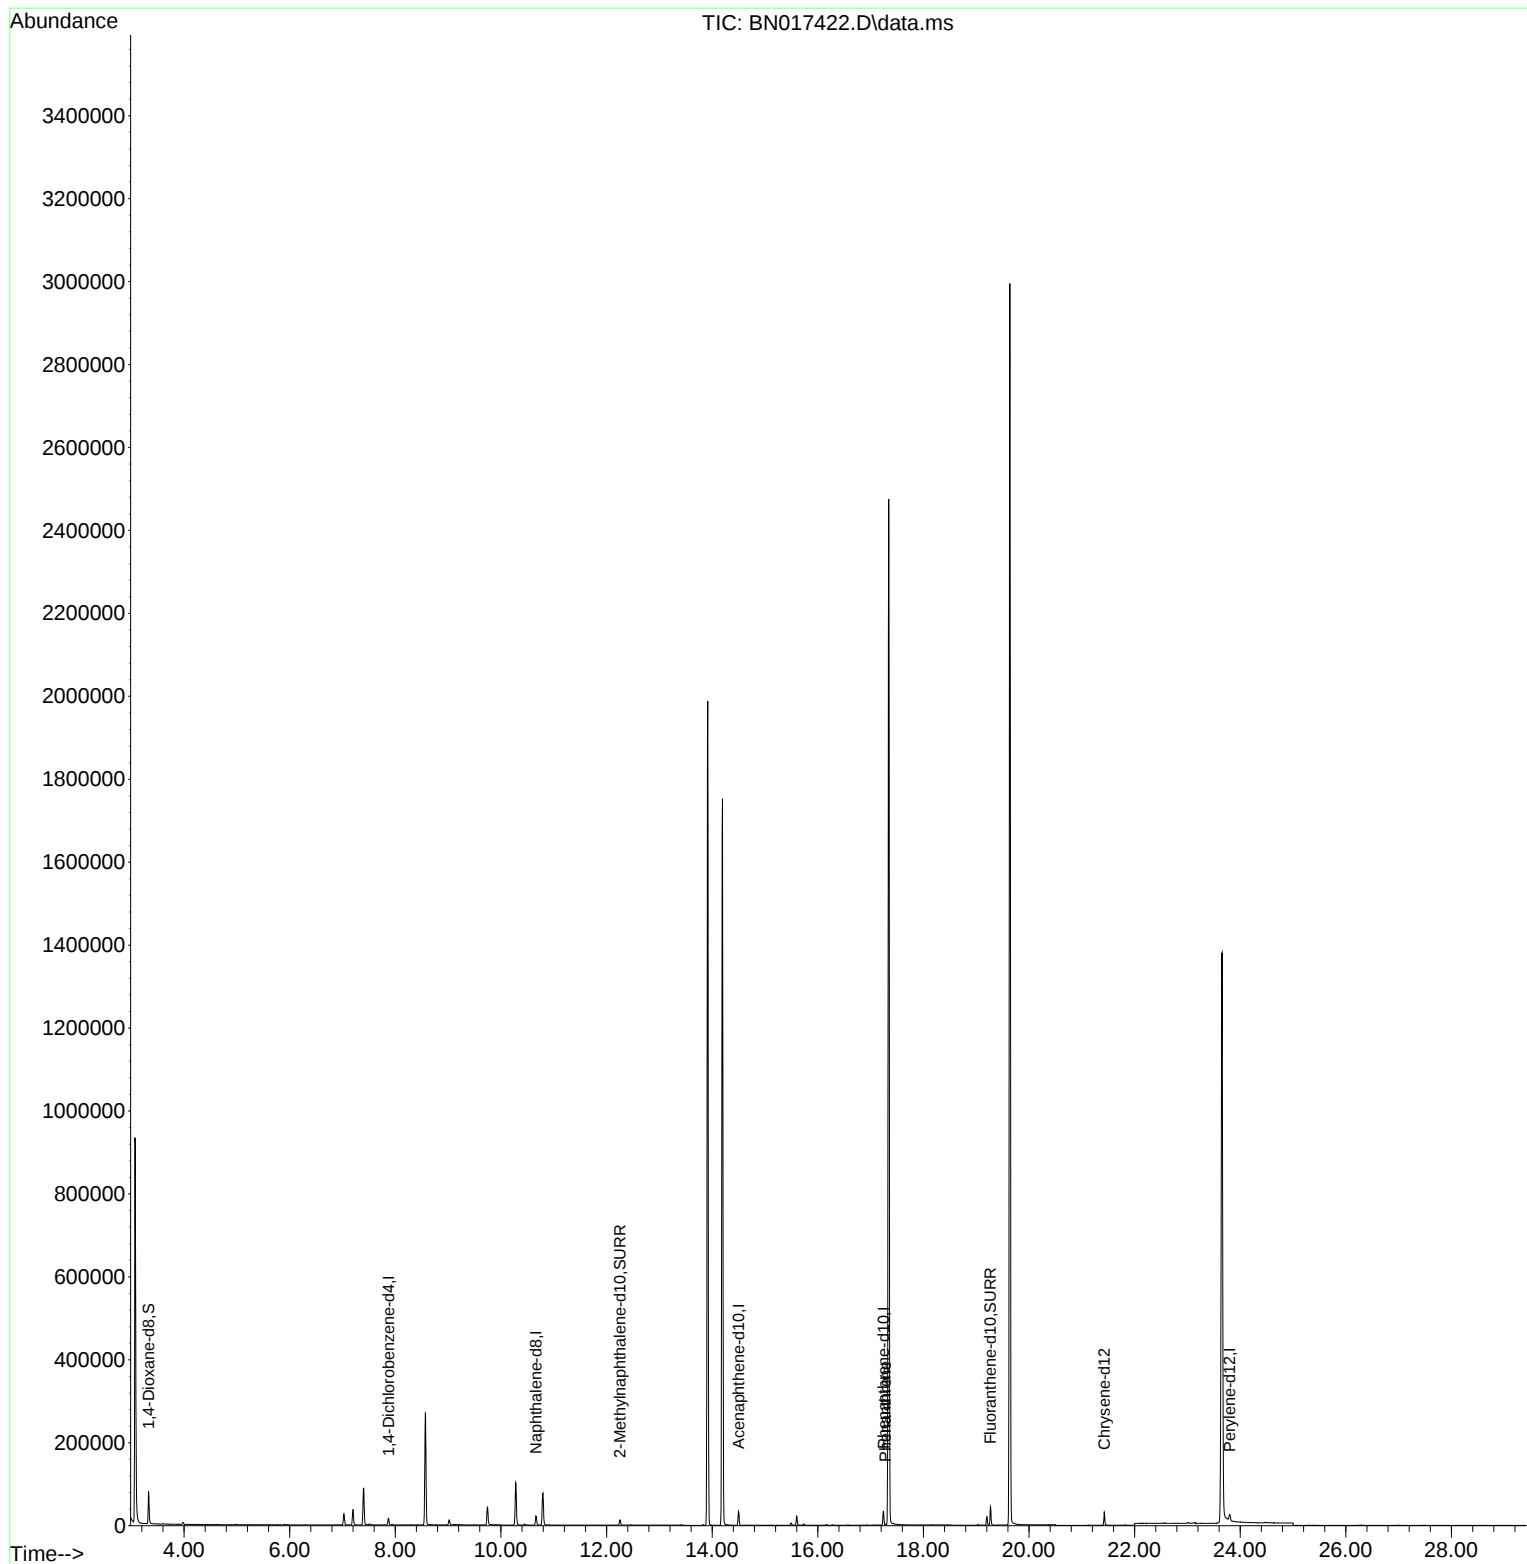

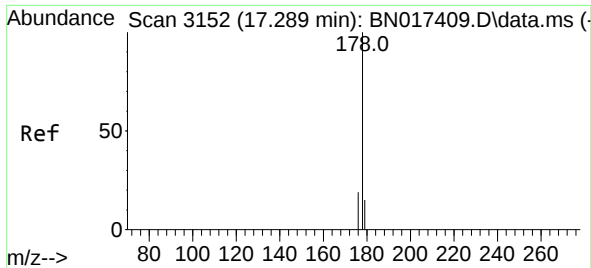

#15
 Phenanthrene
 Concen: 0.021 ng/ul
 RT: 17.282 min Scan# 3150
 Delta R.T. -0.012 min
 Lab File: BN017422.D
 Acq: 14 Nov 2021 10:36

Instrument :
 BNA_N
 ClientSampleId :
 BG398

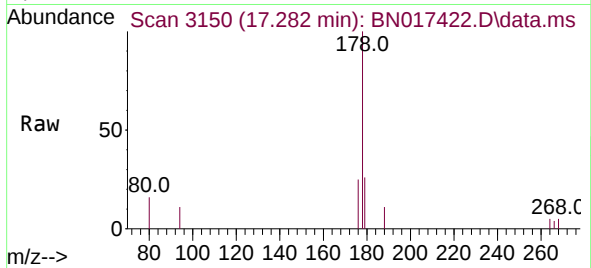

Tgt Ion:178 Resp: 2363

Ion	Ratio	Lower	Upper
178	100		
179	26.1	13.0	19.4#
176	25.3	15.6	23.4#

