

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
 Data File : BN017423.D
 Acq On : 14 Nov 2021 11:12
 Operator : CG/JU
 Sample : M4524-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3A0

Quant Time: Nov 15 04:47:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 02:31:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.868	152	7742	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.667	136	28693	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.502	164	19341	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.243	188	37994	0.400	ng/ul	0.00
17) Chrysene-d12	21.426	240	27013	0.400	ng/ul	#-0.01
23) Perylene-d12	23.800	264	23171	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	31295	3.685	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.257	152	14935	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	44032	0.453	ng/ul	-0.01
Target Compounds						
15) Phenanthrene	17.285	178	3221	0.028	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
Data File : BN017423.D
Acq On : 14 Nov 2021 11:12
Operator : CG/JU
Sample : M4524-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3A0

Quant Time: Nov 15 04:47:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 02:31:43 2021
Response via : Initial Calibration

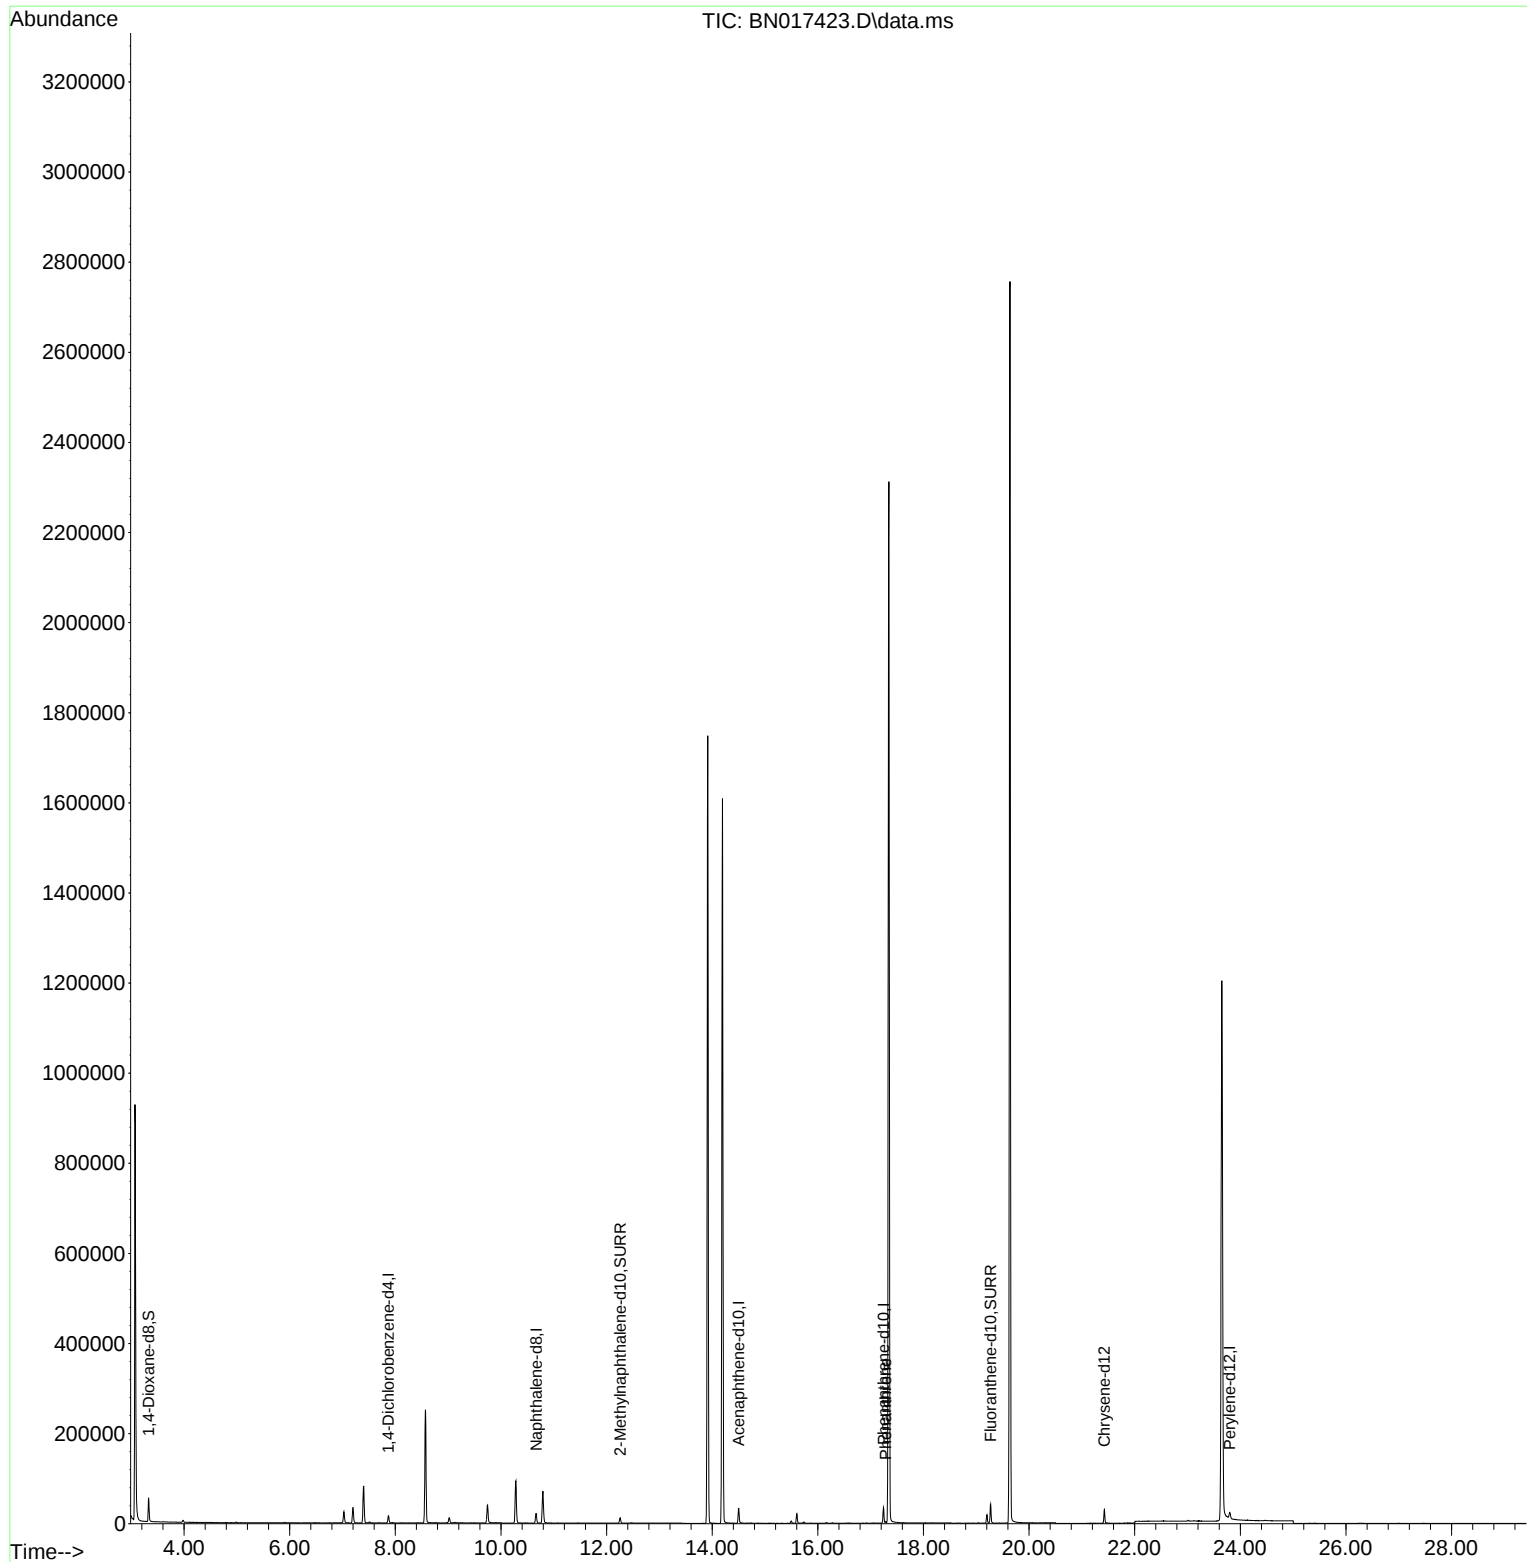

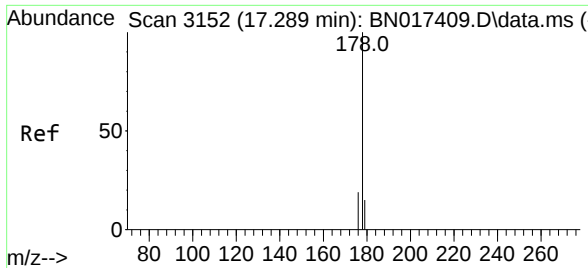

#15
 Phenanthrene
 Concen: 0.028 ng/ul
 RT: 17.285 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: BN017423.D
 Acq: 14 Nov 2021 11:12

Instrument :
 BNA_N
 ClientSampleId :
 BG3A0

Tgt Ion:178 Resp: 3221
 Ion Ratio Lower Upper
 178 100
 179 22.1 13.0 19.4#
 176 23.9 15.6 23.4#

