

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
 Data File : BN017424.D
 Acq On : 14 Nov 2021 11:47
 Operator : CG/JU
 Sample : M4522-10
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3A0

Quant Time: Nov 15 04:48:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 02:31:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.868	152	7897	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.668	136	29812	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.503	164	19779	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.243	188	36592	0.400	ng/ul	0.00
17) Chrysene-d12	21.427	240	23080	0.400	ng/ul	#-0.01
23) Perylene-d12	23.800	264	20262	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.328	96	36106	4.168	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.257	152	15874	0.345	ng/ul	0.00
18) Fluoranthene-d10	19.272	212	41209	0.497	ng/ul	-0.01
Target Compounds						
15) Phenanthrene	17.285	178	3202	0.029	ng/ul#	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
Data File : BN017424.D
Acq On : 14 Nov 2021 11:47
Operator : CG/JU
Sample : M4522-10
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3A0

Quant Time: Nov 15 04:48:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 02:31:43 2021
Response via : Initial Calibration

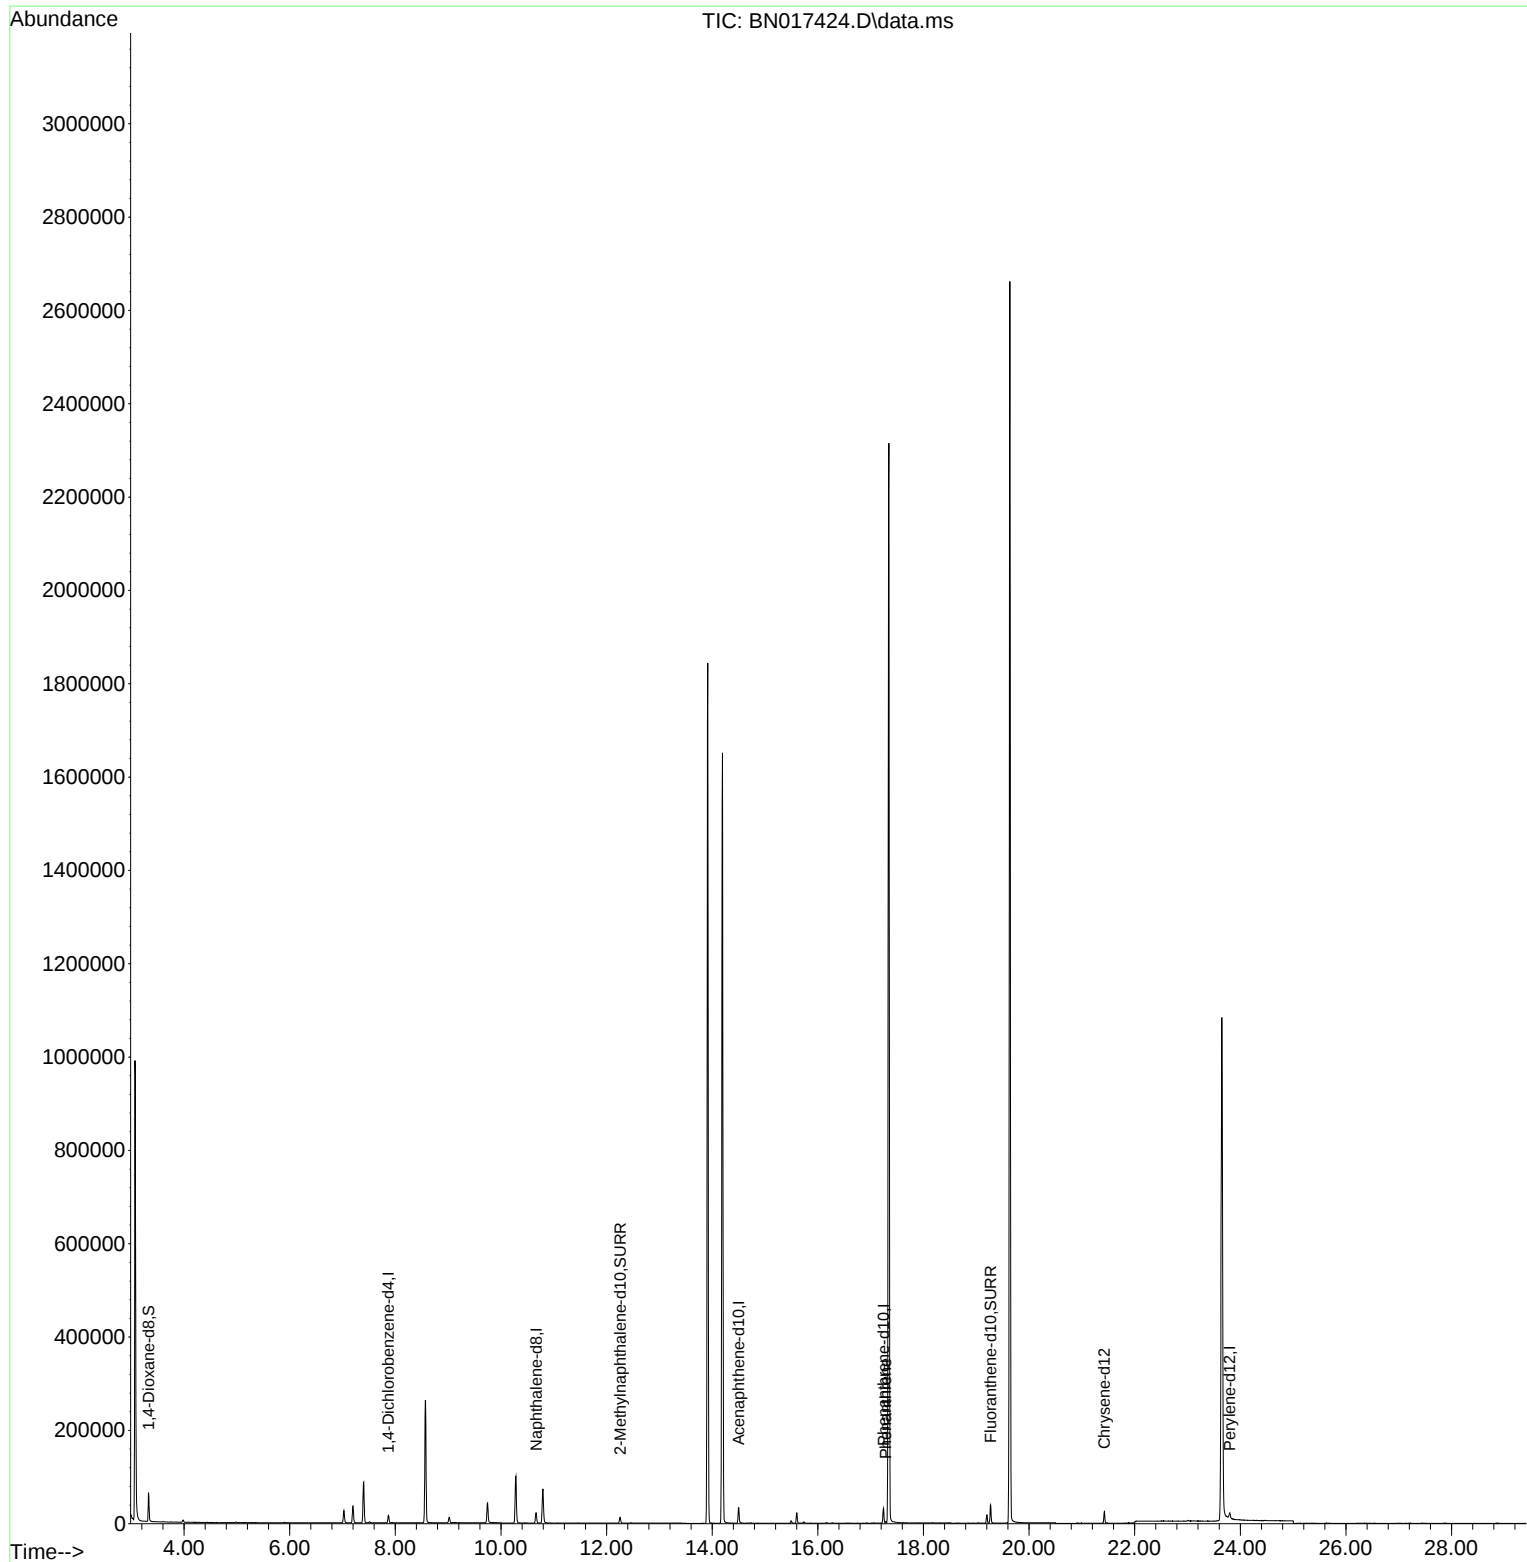

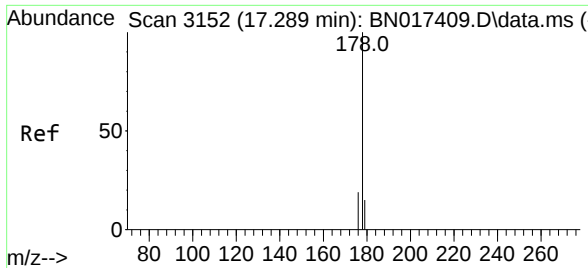

#15
 Phenanthrene
 Concen: 0.029 ng/ul
 RT: 17.285 min Scan# 31
 Delta R.T. -0.009 min
 Lab File: BN017424.D
 Acq: 14 Nov 2021 11:47

Instrument :
 BNA_N
 ClientSampleId :
 BG3A0

Tgt Ion:178 Resp: 3202
 Ion Ratio Lower Upper
 178 100
 179 21.9 13.0 19.4#
 176 23.5 15.6 23.4#

