

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
 Data File : BN017450.D
 Acq On : 15 Nov 2021 04:37
 Operator : CG/JU
 Sample : M4446-18
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3A5

Quant Time: Nov 15 05:47:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 15 02:31:43 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	7372	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.658	136	25910	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.499	164	15158	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.240	188	30758	0.400	ng/ul	-0.01
17) Chrysene-d12	21.422	240	22443	0.400	ng/ul	-0.02
23) Perylene-d12	23.793	264	20188	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.324	96	30149	3.728	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.253	152	13010	0.325	ng/ul	-0.01
18) Fluoranthene-d10	19.269	212	33775	0.419	ng/ul	-0.01
Target Compounds						
					Qvalue	
28) Dibenzo(a,h)anthracene	26.267	278	974	0.023	ng/ul#	6


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111321\
Data File : BN017450.D
Acq On : 15 Nov 2021 04:37
Operator : CG/JU
Sample : M4446-18
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3A5


Quant Time: Nov 15 05:47:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN111321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 15 02:31:43 2021
Response via : Initial Calibration

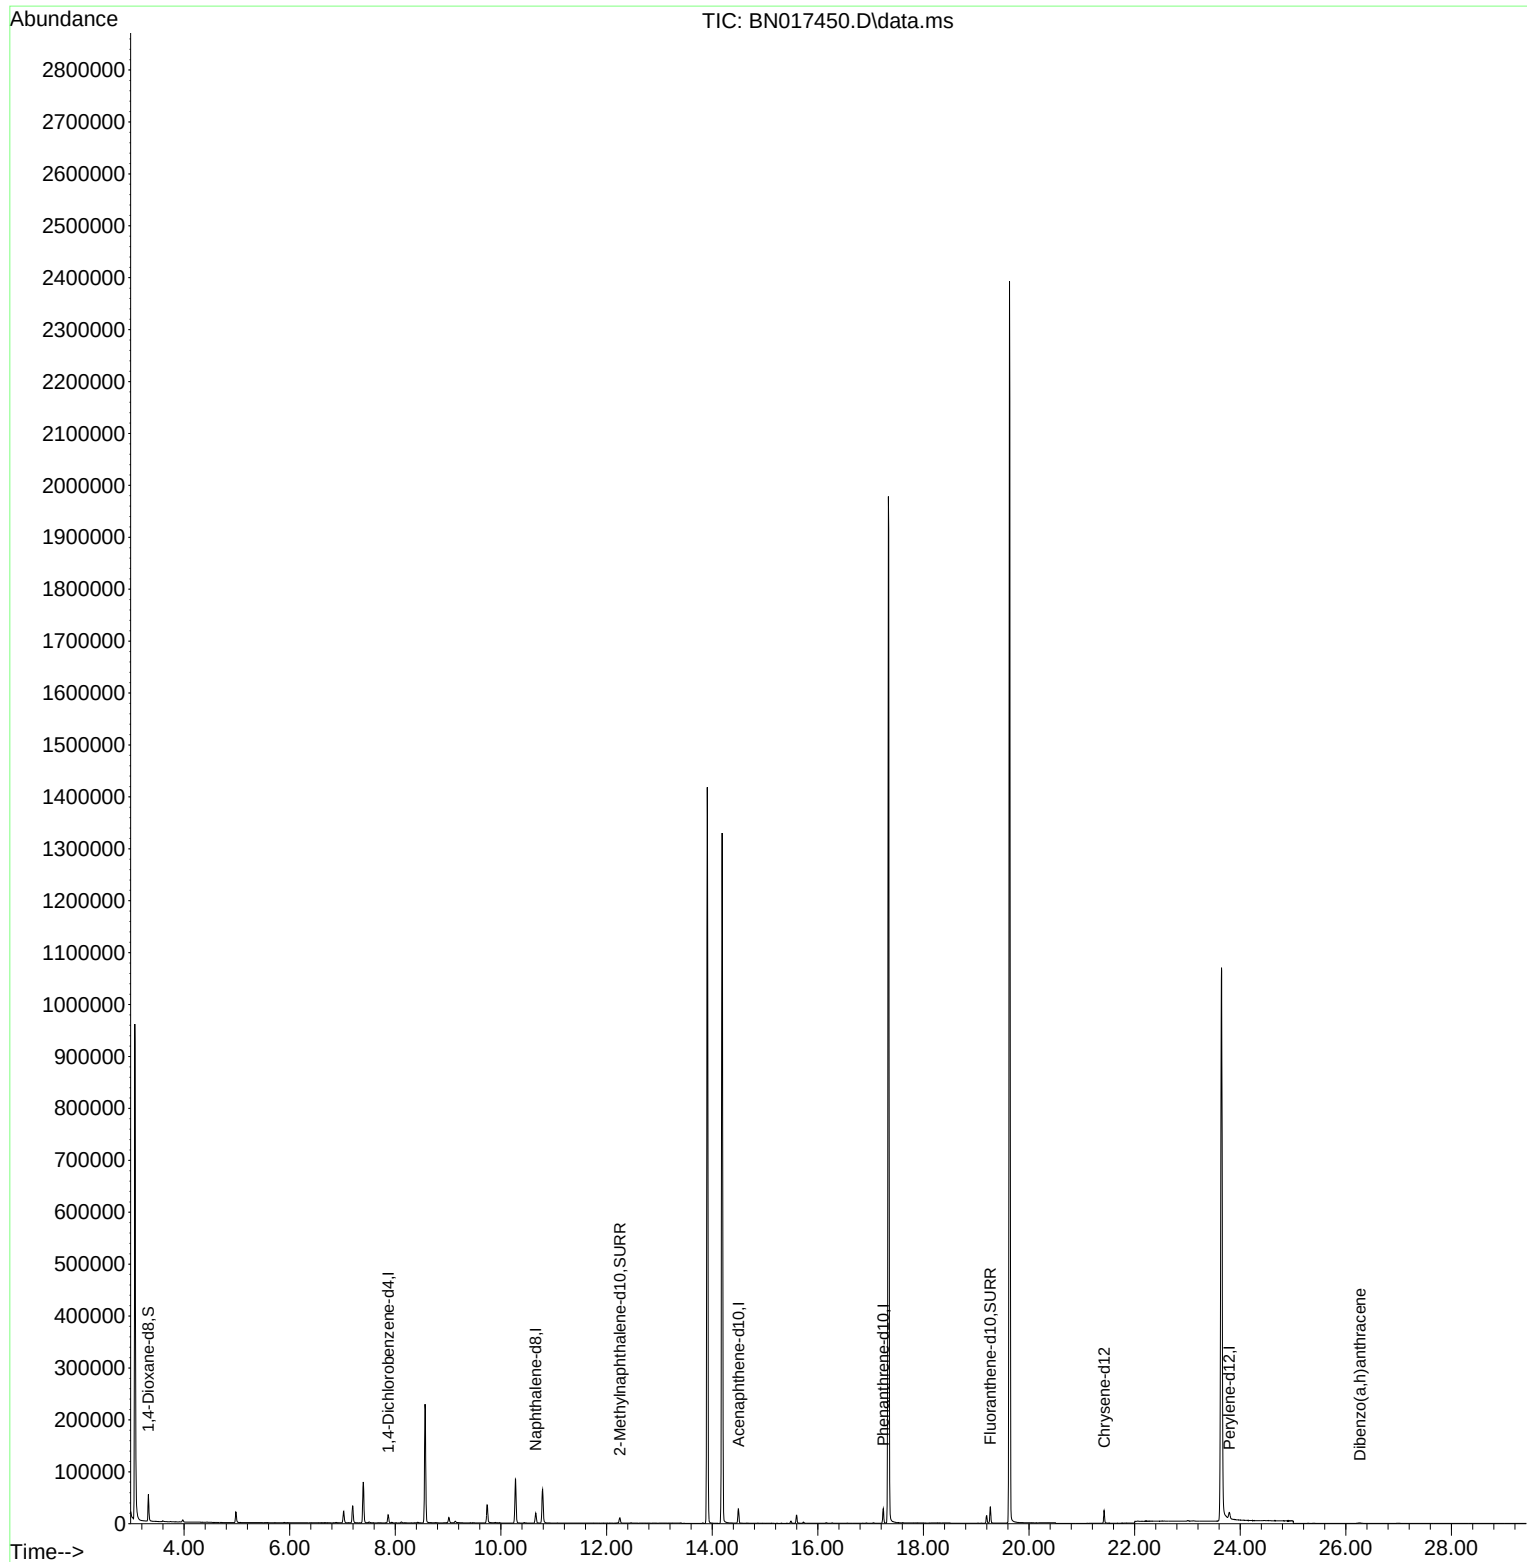

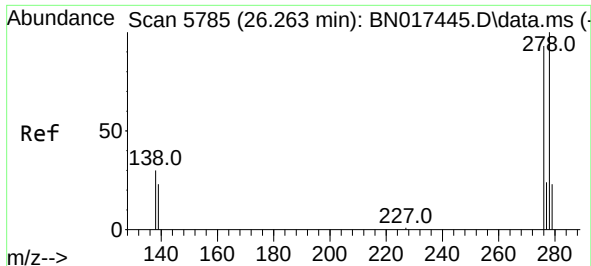

#28
 Dibenzo(a,h)anthracene
 Concen: 0.023 ng/ul
 RT: 26.267 min Scan# 51
 Delta R.T. -0.047 min
 Lab File: BN017450.D
 Acq: 15 Nov 2021 04:37

Instrument :
 BNA_N
 ClientSampleId :
 BG3A5

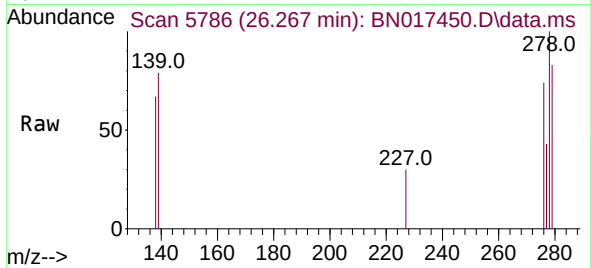

Tgt Ion:278 Resp: 974
 Ion Ratio Lower Upper
 278 100
 139 78.9 21.8 32.8#
 279 83.3 26.3 39.5#

