

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111322\
 Data File : BN022628.D
 Acq On : 12 Nov 2022 14:30
 Operator : CG/JU
 Sample : SSTDICC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

Quant Time: Nov 14 01:38:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Nov 14 01:35:37 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.892	152	1703	0.400	ng	0.00
7) Naphthalene-d8	10.720	136	5384	0.400	ng	0.00
13) Acenaphthene-d10	14.571	164	3348	0.400	ng	0.00
19) Phenanthrene-d10	17.329	188	7194	0.400	ng	# 0.00
29) Chrysene-d12	21.537	240	6464	0.400	ng	0.00
35) Perylene-d12	23.979	264	5654	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.436	112	4140	0.841	ng	0.00
5) Phenol-d6	7.075	99	5157	0.838	ng	0.00
8) Nitrobenzene-d5	9.065	82	4178	0.816	ng	-0.01
11) 2-Methylnaphthalene-d10	12.315	152	6973	0.794	ng	0.00
14) 2,4,6-Tribromophenol	16.075	330	1429	0.882	ng	0.00
15) 2-Fluorobiphenyl	13.192	172	10428	0.765	ng	0.00
27) Fluoranthene-d10	19.369	212	16210	0.818	ng	0.00
31) Terphenyl-d14	19.967	244	15765	0.787	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.233	88	1956	0.814	ng	# 91
3) n-Nitrosodimethylamine	3.580	42	2172	0.885	ng	95
6) bis(2-Chloroethyl)ether	7.314	93	4493	0.830	ng	98
9) Naphthalene	10.763	128	13566	0.854	ng	98
10) Hexachlorobutadiene	11.040	225	2258	0.766	ng	# 100
12) 2-Methylnaphthalene	12.043	142	2941	0.906	ng	# 87
16) Acenaphthylene	14.283	152	12195	0.791	ng	100
17) Acenaphthene	14.636	154	8269	0.783	ng	99
18) Fluorene	15.619	166	11798	0.825	ng	99
20) 4,6-Dinitro-2-methylph...	15.715	198	1078	0.998	ng	# 32
21) 4-Bromophenyl-phenylether	16.510	248	3304	0.779	ng	# 70
22) Hexachlorobenzene	16.621	284	3721	0.753	ng	99
23) Atrazine	16.795	200	3143	0.871	ng	# 94
24) Pentachlorophenol	16.981	266	1708	0.904	ng	99
25) Phenanthrene	17.366	178	18585	0.801	ng	99
26) Anthracene	17.465	178	15776	0.796	ng	100
28) Fluoranthene	19.403	202	20491	0.815	ng	99
30) Pyrene	19.765	202	21086	0.801	ng	100
32) Benzo(a)anthracene	21.519	228	19013	0.800	ng	98
33) Chrysene	21.573	228	19386	0.791	ng	99
34) Bis(2-ethylhexyl)phtha...	21.438	149	13283	0.968	ng	99
36) Indeno(1,2,3-cd)pyrene	26.528	276	18368	0.688	ng	99
37) Benzo(b)fluoranthene	23.227	252	17418	0.761	ng	92
38) Benzo(k)fluoranthene	23.274	252	17853	0.782	ng	93
39) Benzo(a)pyrene	23.865	252	14223	0.765	ng	# 91
40) Dibenzo(a,h)anthracene	26.549	278	14665	0.683	ng	94
41) Benzo(g,h,i)perylene	27.320	276	15252	0.675	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111322\
Data File : BN022628.D
Acq On : 12 Nov 2022 14:30
Operator : CG/JU
Sample : SSTDICC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8

Quant Time: Nov 14 01:38:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 01:35:37 2022
Response via : Initial Calibration




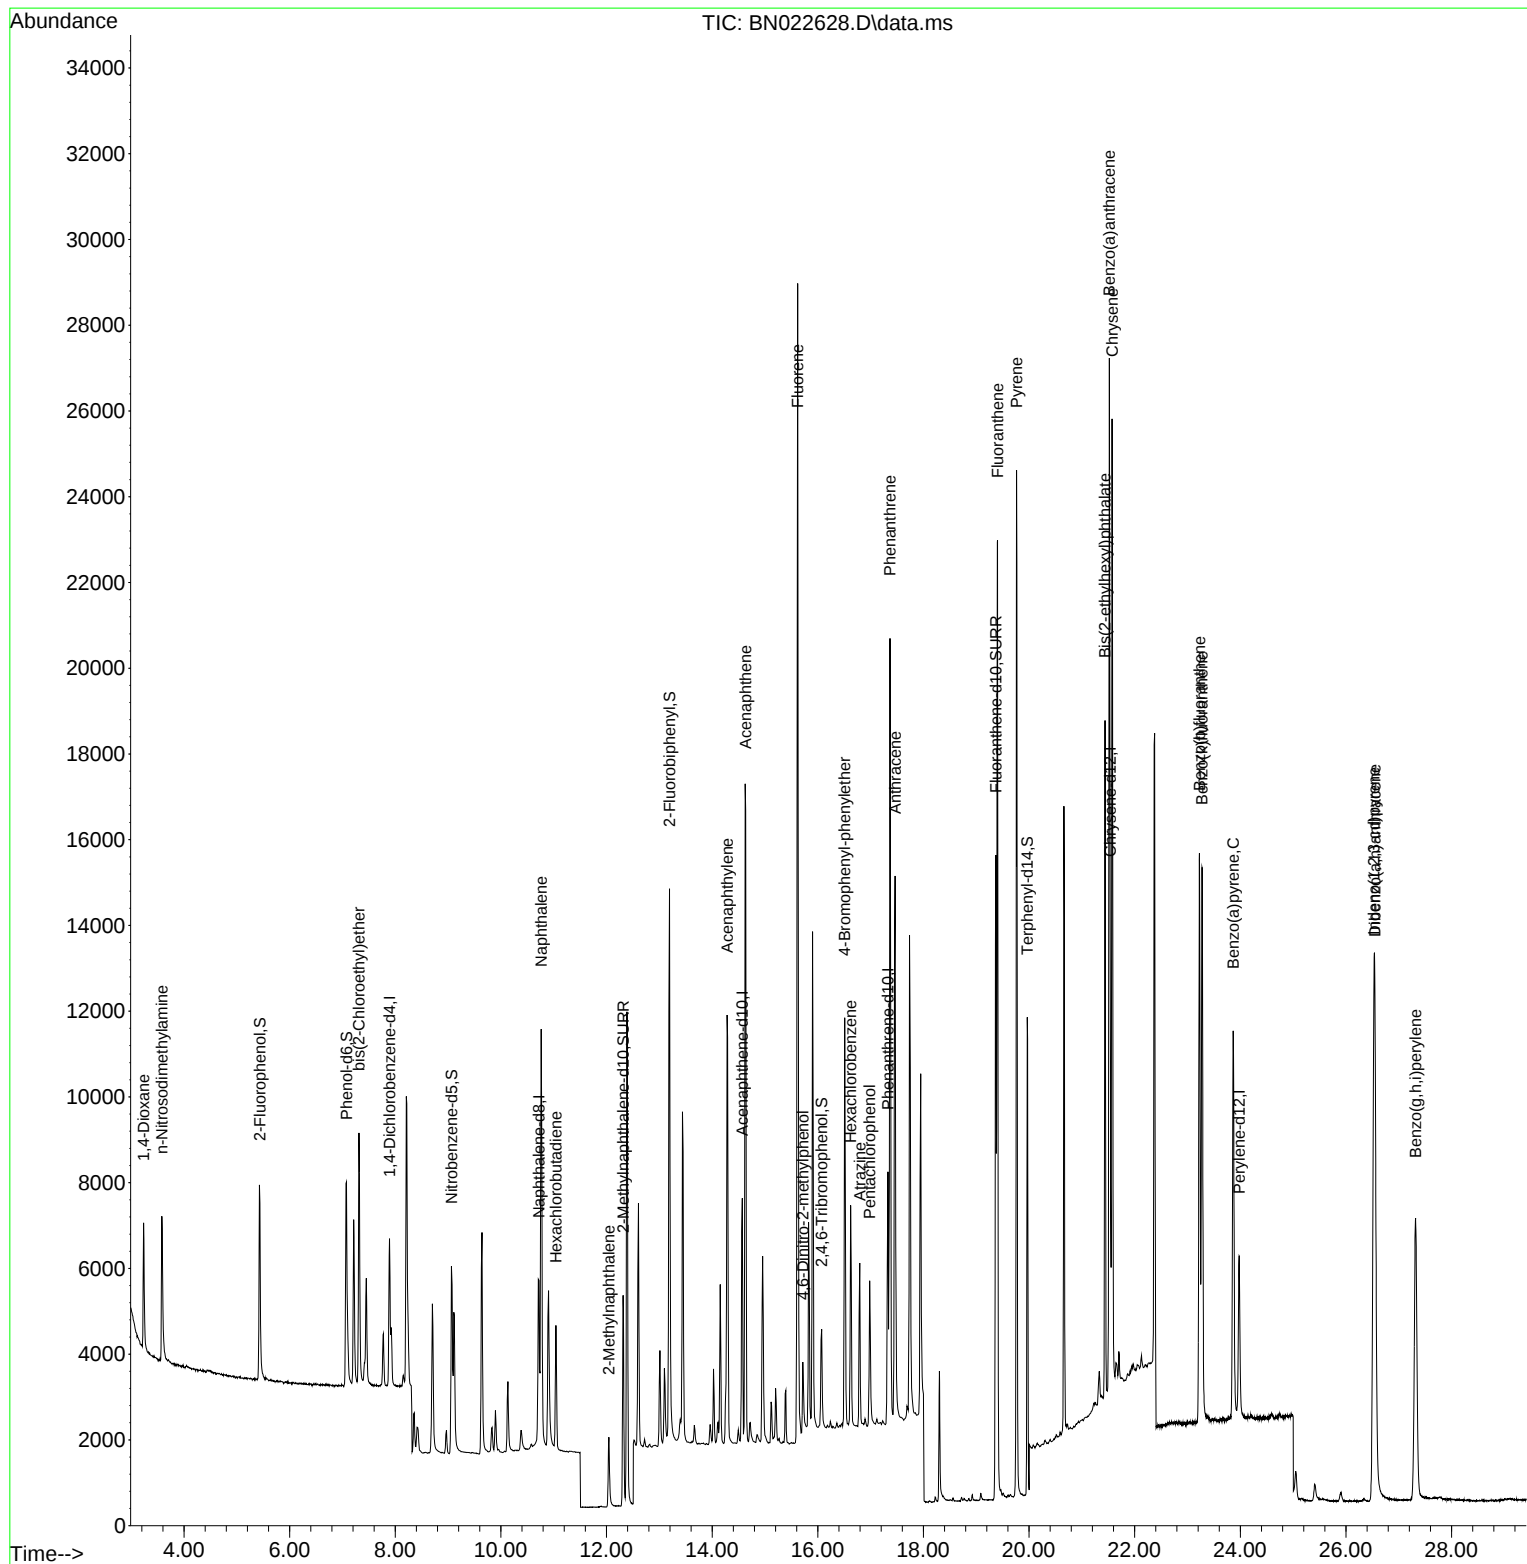




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.892 min Scan# 680
 Delta R.T. -0.000 min
 Lab File: BN022628.D
 Acq: 12 Nov 2022 14:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:152 Resp: 1703
 Ion Ratio Lower Upper
 152 100
 150 151.0 122.2 183.4
 115 69.5 56.3 84.5

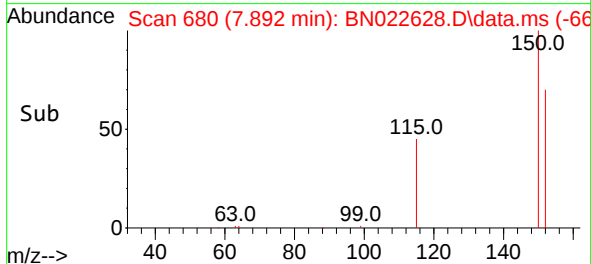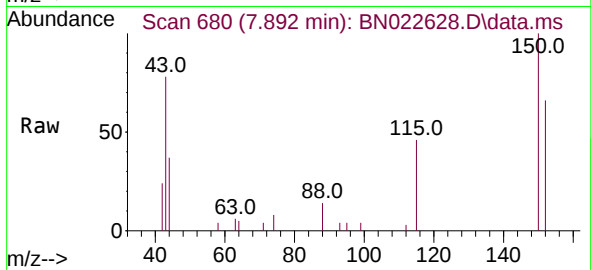

#2
 1,4-Dioxane
 Concen: 0.814 ng
 RT: 3.233 min Scan# 35
 Delta R.T. -0.007 min
 Lab File: BN022628.D
 Acq: 12 Nov 2022 14:30

Tgt Ion: 88 Resp: 1956
 Ion Ratio Lower Upper
 88 100
 43 31.8 34.9 52.3#
 58 76.6 58.8 88.2


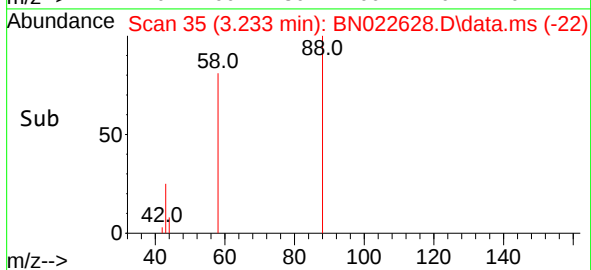




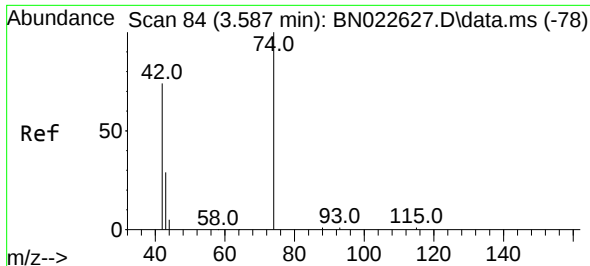

#3
n-Nitrosodimethylamine
Concen: 0.885 ng
RT: 3.580 min Scan# 84
Delta R.T. -0.007 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion: 42 Resp: 2172
Ion Ratio Lower Upper
42 100
74 132.2 101.3 151.9
44 10.9 7.4 11.0

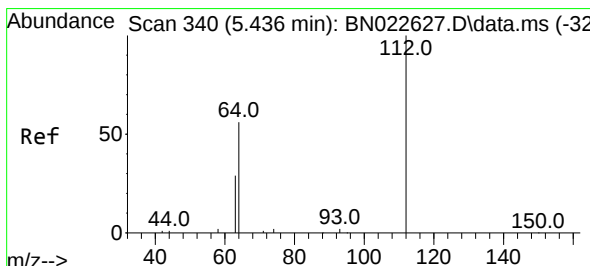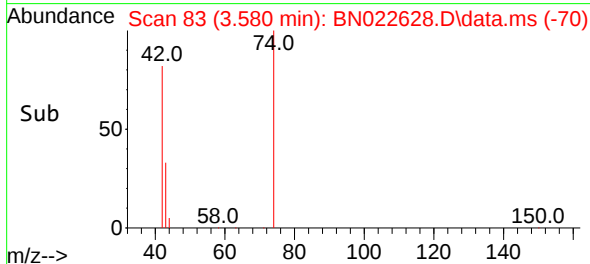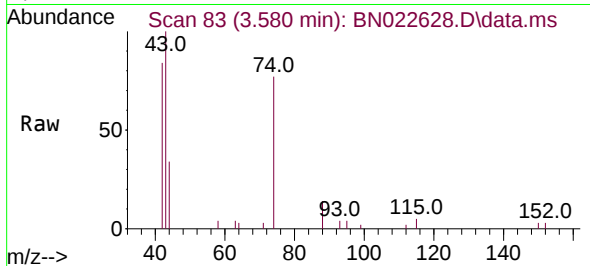

#4
2-Fluorophenol
Concen: 0.841 ng
RT: 5.436 min Scan# 340
Delta R.T. -0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion: 112 Resp: 4140
Ion Ratio Lower Upper
112 100
64 61.6 49.8 74.6
63 33.3 26.0 39.0


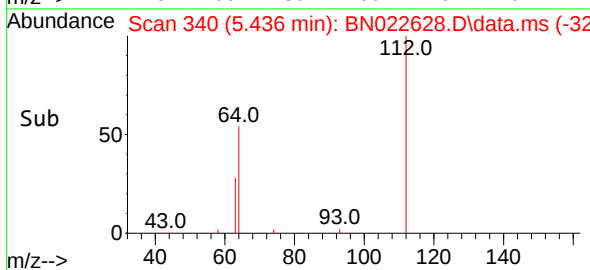

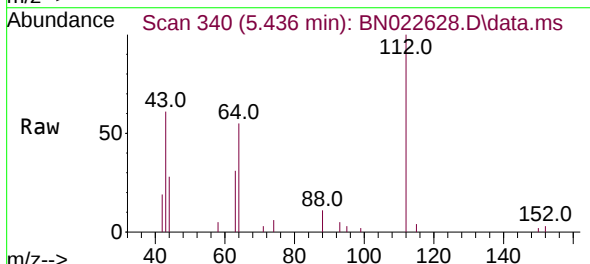




#5
Phenol-d6
Concen: 0.838 ng
RT: 7.075 min Scan# 567
Delta R.T. 0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	99	Resp:	5157
Ion	Ratio	Lower	Upper
99	100		
42	21.8	16.9	25.3
71	38.2	30.2	45.4

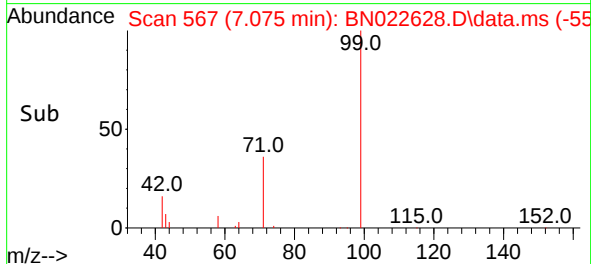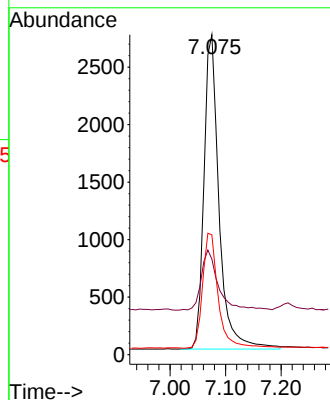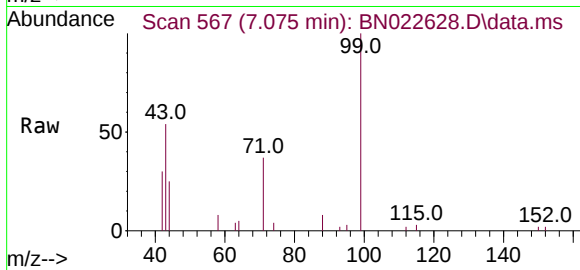

#6
bis(2-Chloroethyl)ether
Concen: 0.830 ng
RT: 7.314 min Scan# 600
Delta R.T. 0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:	93	Resp:	4493
Ion	Ratio	Lower	Upper
93	100		
63	80.1	62.5	93.7
95	33.1	26.1	39.1


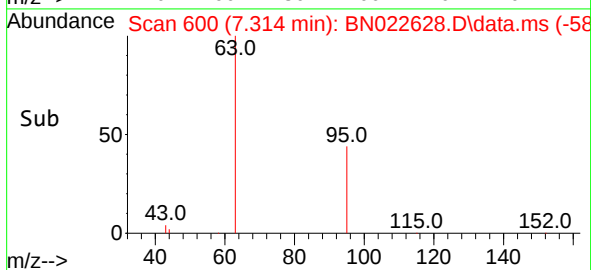
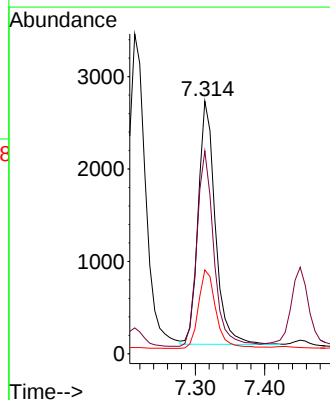
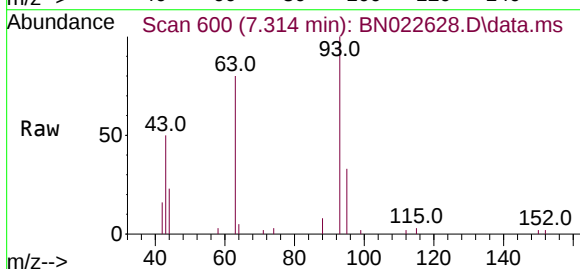


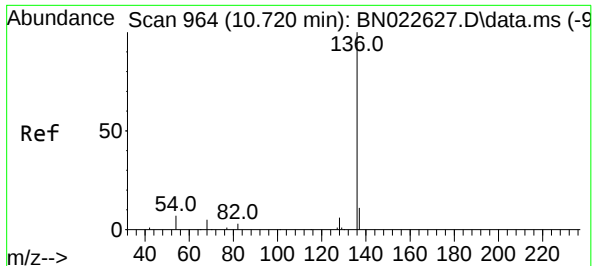

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.720 min Scan# 90
Delta R.T. -0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	136	Resp:	5384
Ion	Ratio	Lower	Upper
136	100		
137	12.1	10.0	15.0
54	7.9	7.0	10.4
68	6.5	5.3	7.9

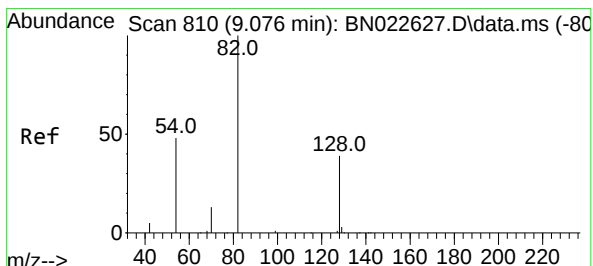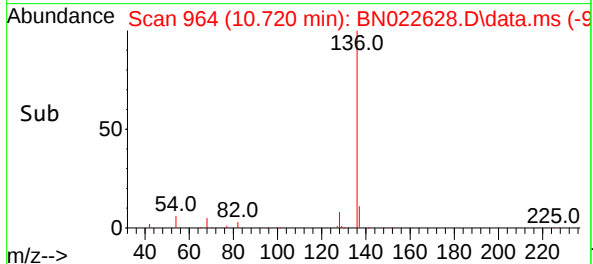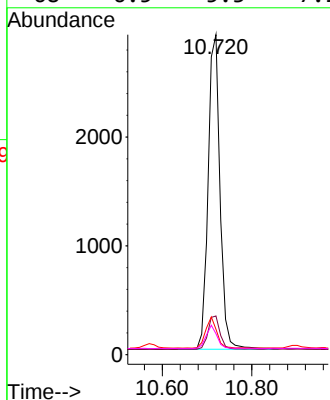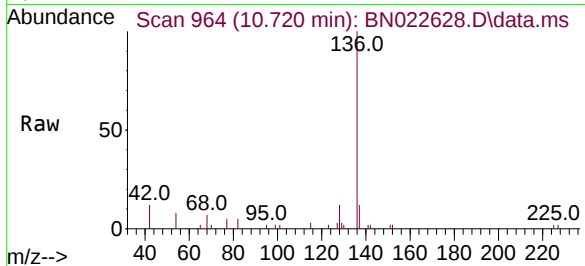

#8
Nitrobenzene-d5
Concen: 0.816 ng
RT: 9.065 min Scan# 809
Delta R.T. -0.011 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:	82	Resp:	4178
Ion	Ratio	Lower	Upper
82	100		
128	35.0	34.6	51.8
54	54.3	40.4	60.6


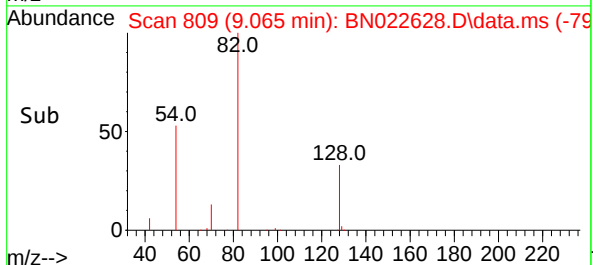
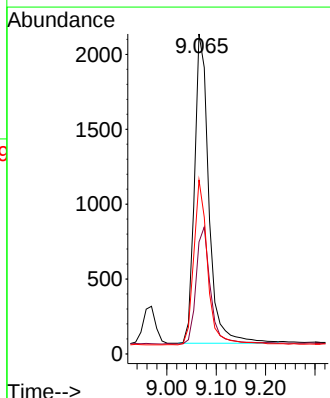
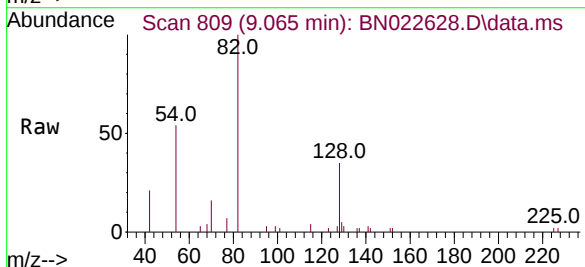


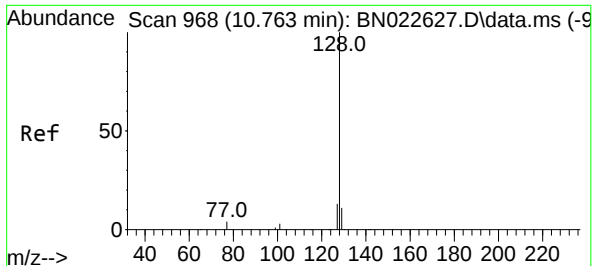

#9
Naphthalene
Concen: 0.854 ng
RT: 10.763 min Scan# 968
Delta R.T. 0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	128	Resp:	13566
Ion	Ratio	Lower	Upper
128	100		
129	11.5	9.9	14.9
127	13.9	11.4	17.2

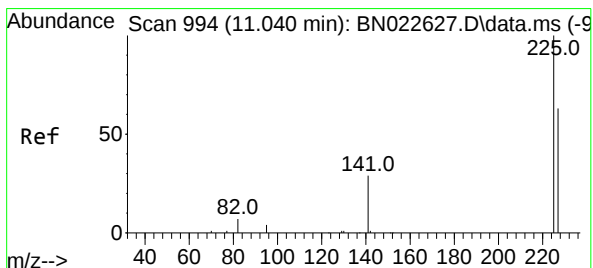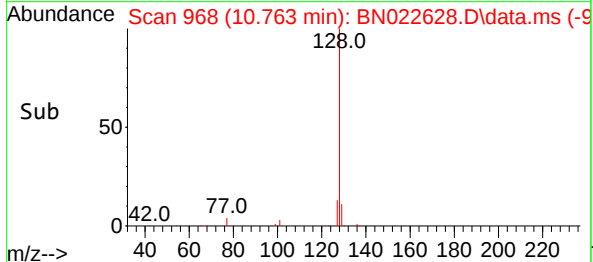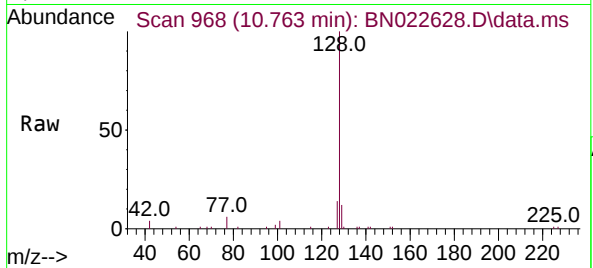

#10
Hexachlorobutadiene
Concen: 0.766 ng
RT: 11.040 min Scan# 994
Delta R.T. 0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:	225	Resp:	2258
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.3	51.3	76.9


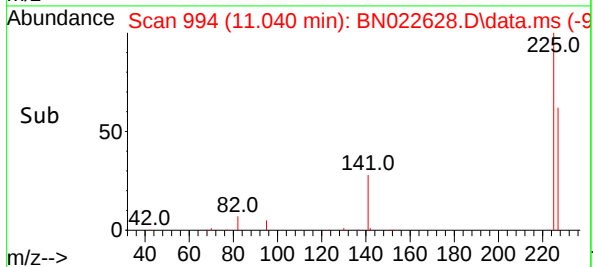

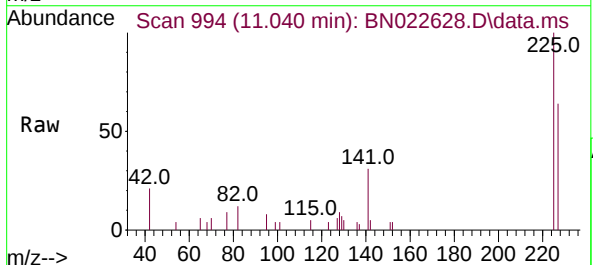




#11
2-Methylnaphthalene-d10
Concen: 0.794 ng
RT: 12.315 min Scan# 1179
Delta R.T. 0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:152 Resp: 6973
Ion Ratio Lower Upper
152 100
151 20.6 16.3 24.5

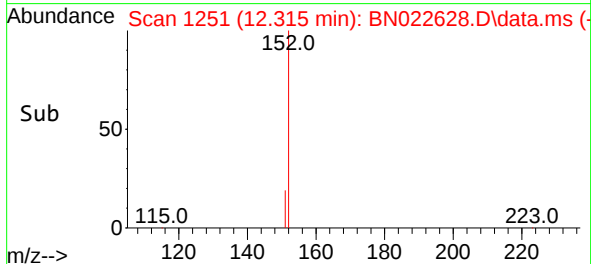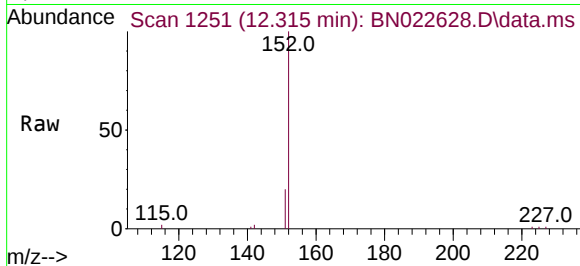

#12
2-Methylnaphthalene
Concen: 0.906 ng
RT: 12.043 min Scan# 1179
Delta R.T. -0.004 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:142 Resp: 2941
Ion Ratio Lower Upper
142 100
141 14.2 14.9 22.3#
115 7.0 11.3 16.9#




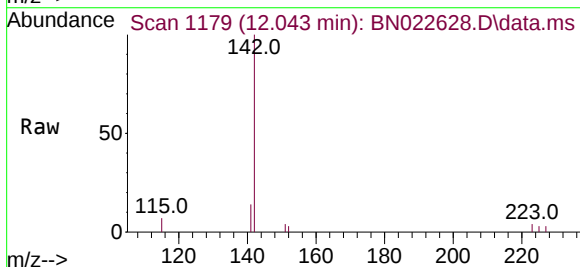


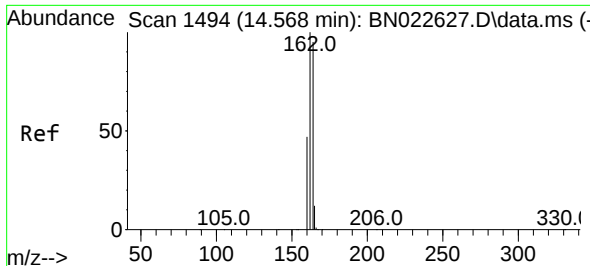

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.571 min Scan# 1495
 Delta R.T. 0.004 min
 Lab File: BN022628.D
 Acq: 12 Nov 2022 14:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:164 Resp: 3348
 Ion Ratio Lower Upper
 164 100
 162 102.4 84.1 126.1
 160 49.2 40.2 60.2

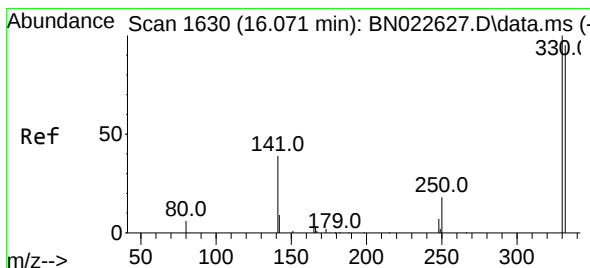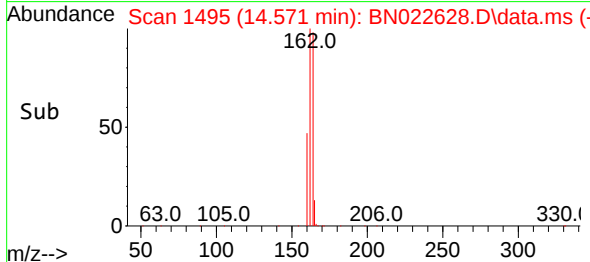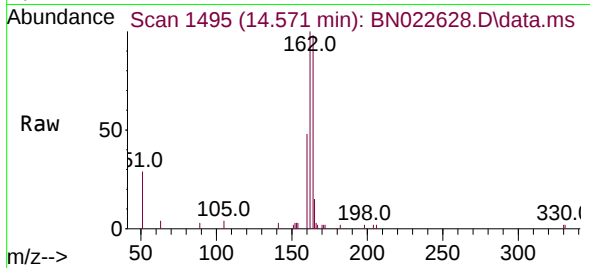

#14
 2,4,6-Tribromophenol
 Concen: 0.882 ng
 RT: 16.075 min Scan# 1631
 Delta R.T. 0.004 min
 Lab File: BN022628.D
 Acq: 12 Nov 2022 14:30

Tgt Ion:330 Resp: 1429
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.2 115.8
 141 49.4 46.2 69.2


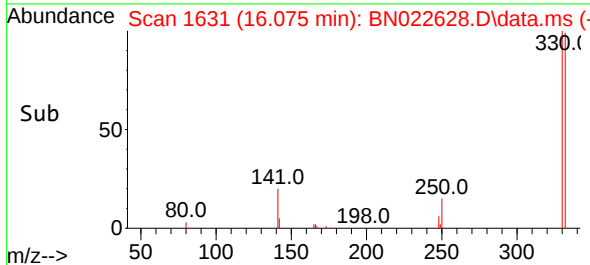

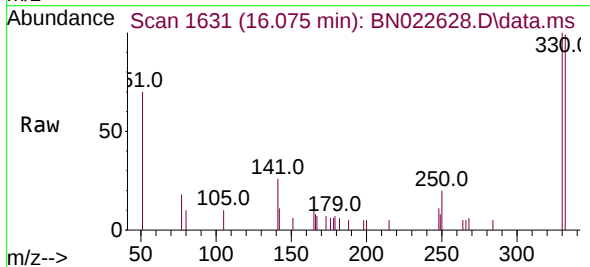




#15
2-Fluorobiphenyl
Concen: 0.765 ng
RT: 13.192 min Scan# 1366
Delta R.T. 0.004 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:172 Resp: 10428
Ion Ratio Lower Upper
172 100
171 35.0 29.0 43.4
170 23.5 20.1 30.1

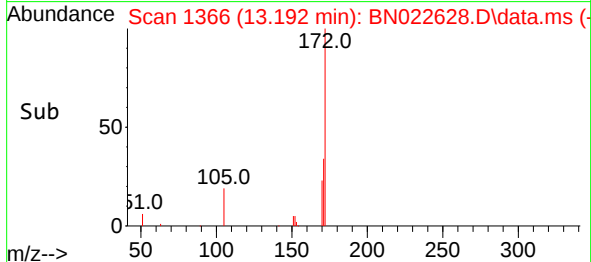

#16
Acenaphthylene
Concen: 0.791 ng
RT: 14.283 min Scan# 1468
Delta R.T. -0.007 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:152 Resp: 12195
Ion Ratio Lower Upper
152 100
151 19.5 15.7 23.5
153 12.8 10.3 15.5

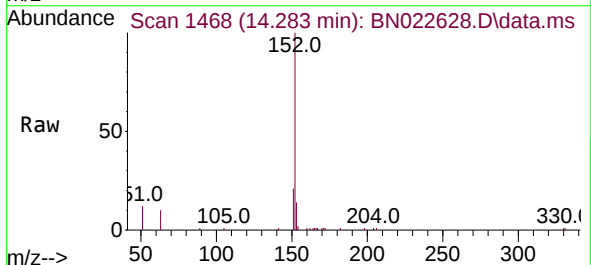



#17

Acenaphthene

Concen: 0.783 ng

RT: 14.636 min Scan# 1501

Delta R.T. 0.004 min

Lab File: BN022628.D

Acq: 12 Nov 2022 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:154 Resp: 8269

Ion Ratio Lower Upper

154 100

153 115.6 91.6 137.4

152 56.8 45.6 68.4

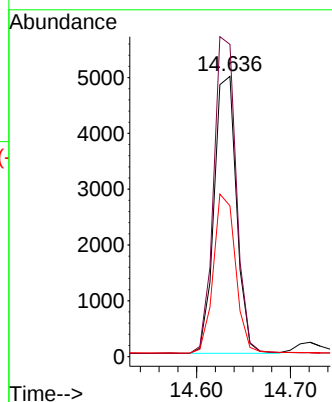

#18

Fluorene

Concen: 0.825 ng

RT: 15.619 min Scan# 1593

Delta R.T. -0.007 min

Lab File: BN022628.D

Acq: 12 Nov 2022 14:30




Tgt Ion:166 Resp: 11798


Ion Ratio Lower Upper

166 100

165 98.6 77.8 116.8

167 12.8 10.2 15.4


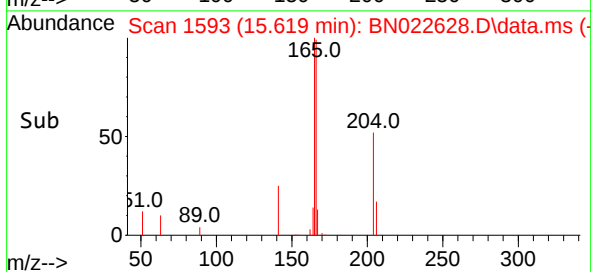
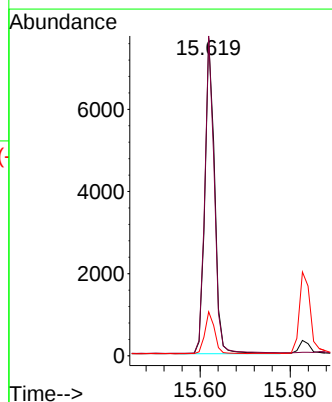





#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.329 min Scan# 1732
Delta R.T. 0.004 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:188 Resp: 7194
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 12.3 12.6 19.0#

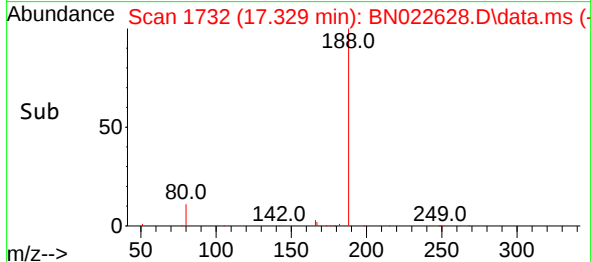

#20
4,6-Dinitro-2-methylphenol
Concen: 0.998 ng
RT: 15.715 min Scan# 1602
Delta R.T. -0.009 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:198 Resp: 1078
Ion Ratio Lower Upper
198 100
51 161.6 266.5 399.7#
105 70.4 64.5 96.7




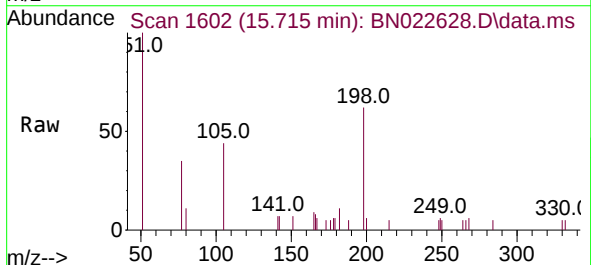


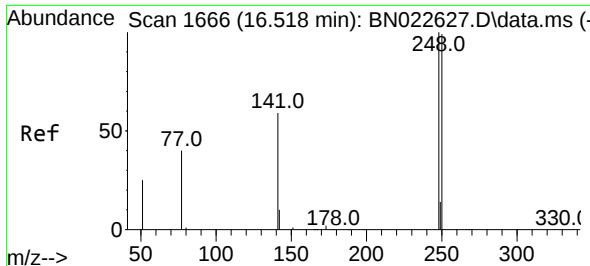

#21
4-Bromophenyl-phenylether
Concen: 0.779 ng
RT: 16.510 min Scan# 1666
Delta R.T. -0.009 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:248 Resp: 3304
Ion Ratio Lower Upper
248 100
250 91.8 79.8 119.6
141 112.0 49.8 74.8#

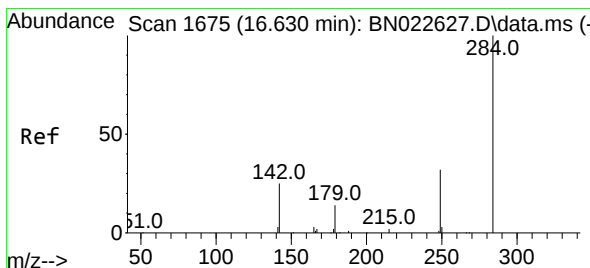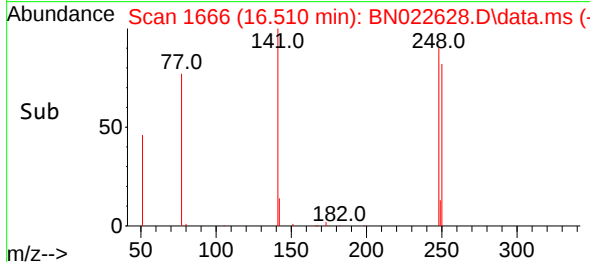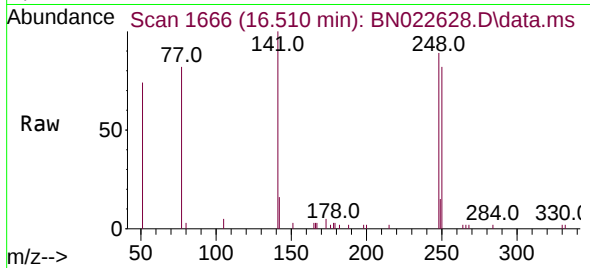

#22
Hexachlorobenzene
Concen: 0.753 ng
RT: 16.621 min Scan# 1675
Delta R.T. -0.009 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:284 Resp: 3721
Ion Ratio Lower Upper
284 100
142 45.6 36.2 54.2
249 33.5 27.6 41.4


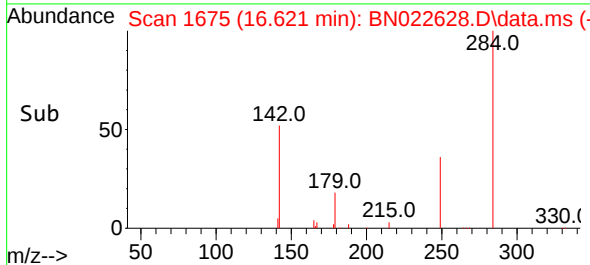

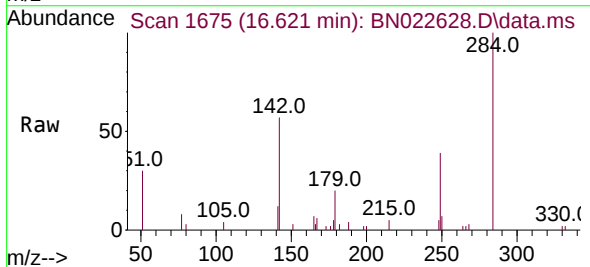


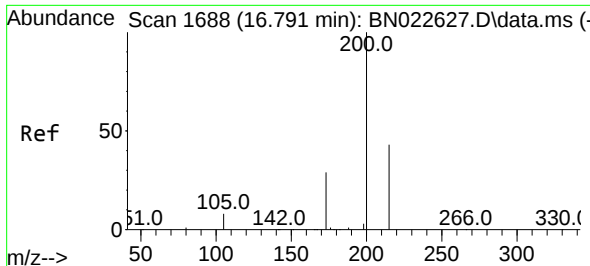

#23
Atrazine
Concen: 0.871 ng
RT: 16.795 min Scan# 1688
Delta R.T. 0.004 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:200 Resp: 3143
Ion Ratio Lower Upper
200 100
173 25.5 26.2 39.4#
215 44.7 36.4 54.6

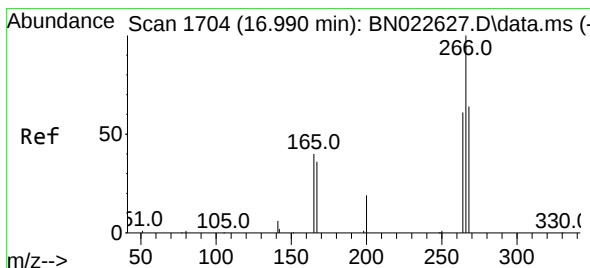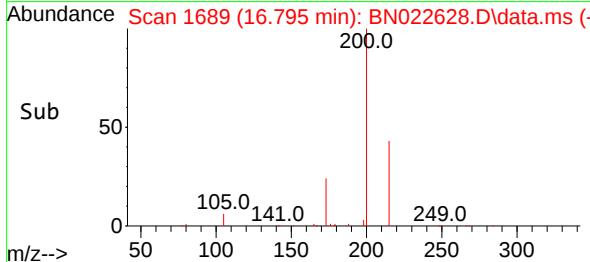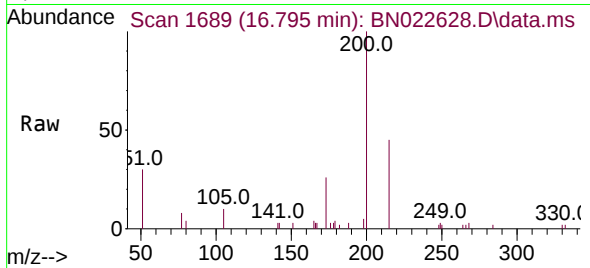

#24
Pentachlorophenol
Concen: 0.904 ng
RT: 16.981 min Scan# 1704
Delta R.T. -0.009 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:266 Resp: 1708
Ion Ratio Lower Upper
266 100
264 64.0 49.6 74.4
268 63.3 50.9 76.3


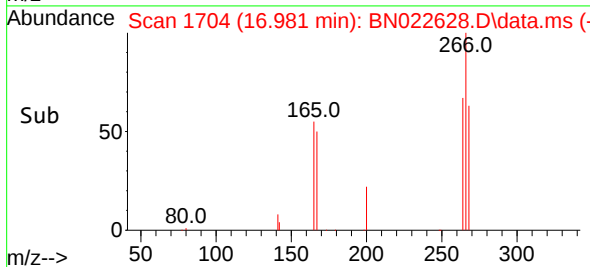

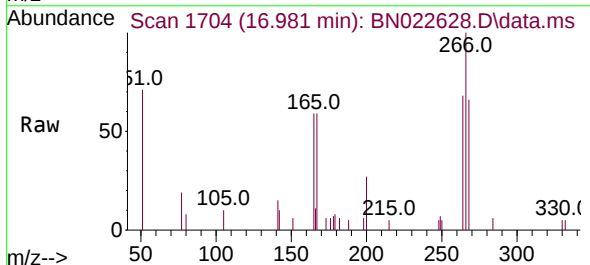




#25
Phenanthrene
Concen: 0.801 ng
RT: 17.366 min Scan# 1735
Delta R.T. -0.009 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:178 Resp: 18585
Ion Ratio Lower Upper
178 100
176 19.5 15.7 23.5
179 15.3 12.6 19.0

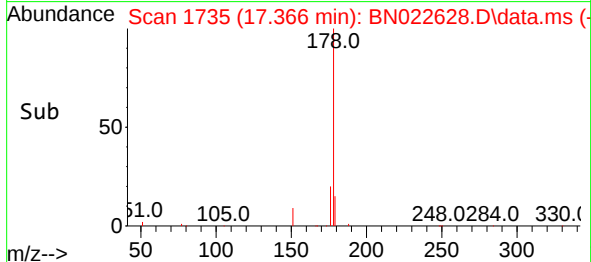

#26
Anthracene
Concen: 0.796 ng
RT: 17.465 min Scan# 1743
Delta R.T. 0.004 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:178 Resp: 15776
Ion Ratio Lower Upper
178 100
176 18.9 15.1 22.7
179 15.0 11.7 17.5




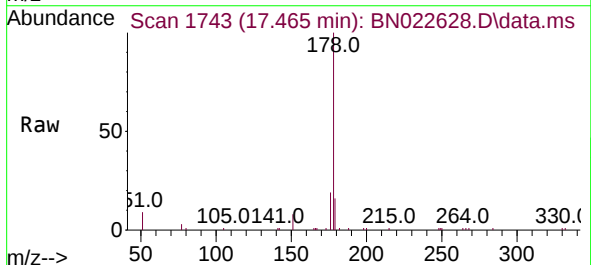




#27
Fluoranthene-d10
Concen: 0.818 ng
RT: 19.369 min Scan# 2108
Delta R.T. -0.004 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:212 Resp: 16210
Ion Ratio Lower Upper
212 100
106 16.3 13.3 19.9
104 9.5 7.8 11.8

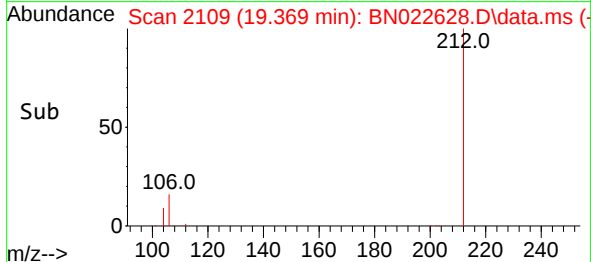

#28
Fluoranthene
Concen: 0.815 ng
RT: 19.403 min Scan# 2117
Delta R.T. -0.000 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:202 Resp: 20491
Ion Ratio Lower Upper
202 100
101 13.4 10.4 15.6
203 17.2 13.9 20.9

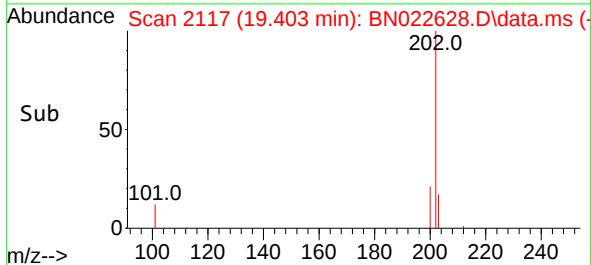



#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.537 min Scan# 2429

Delta R.T. -0.000 min

Lab File: BN022628.D

Acq: 12 Nov 2022 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:240 Resp: 6464

Ion Ratio Lower Upper

240 100

120 15.2 14.0 21.0

236 28.9 23.4 35.2

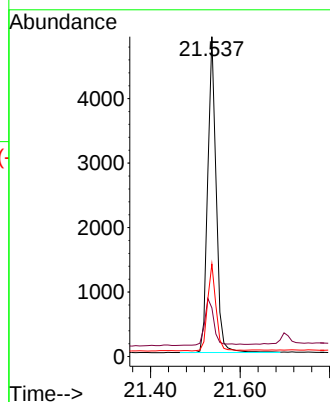

#30

Pyrene

Concen: 0.801 ng

RT: 19.765 min Scan# 2203

Delta R.T. -0.000 min

Lab File: BN022628.D

Acq: 12 Nov 2022 14:30




Tgt Ion:202 Resp: 21086


Ion Ratio Lower Upper

202 100

200 21.3 17.0 25.4

203 18.0 14.6 22.0


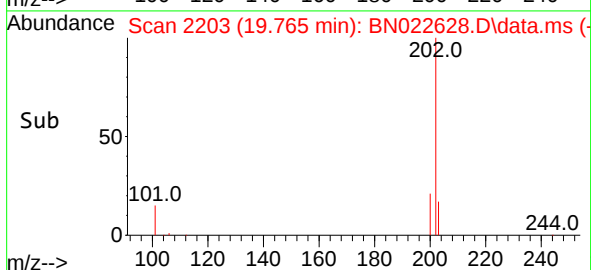
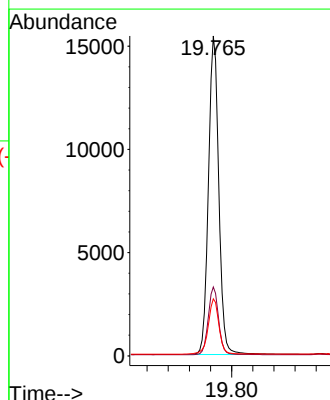





#31
 Terphenyl-d14
 Concen: 0.787 ng
 RT: 19.967 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN022628.D
 Acq: 12 Nov 2022 14:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:244 Resp: 15765
 Ion Ratio Lower Upper
 244 100
 212 9.6 8.3 12.5
 122 0.0 0.0 0.0

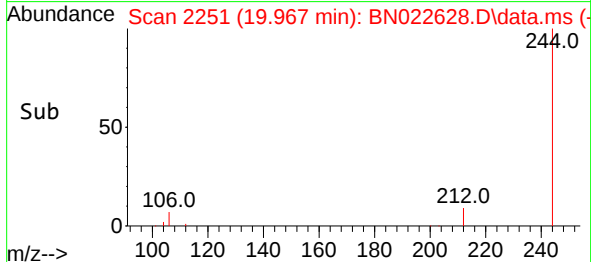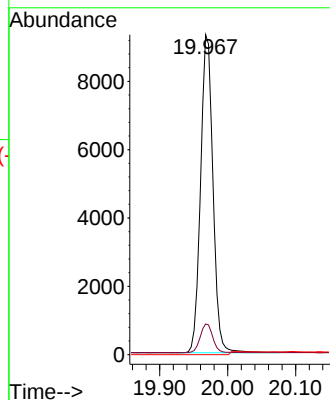

#32
 Benzo(a)anthracene
 Concen: 0.800 ng
 RT: 21.519 min Scan# 2429
 Delta R.T. -0.000 min
 Lab File: BN022628.D
 Acq: 12 Nov 2022 14:30

Tgt Ion:228 Resp: 19013
 Ion Ratio Lower Upper
 228 100
 226 27.8 23.3 34.9
 229 20.1 16.5 24.7

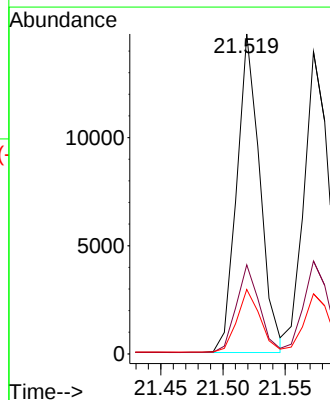

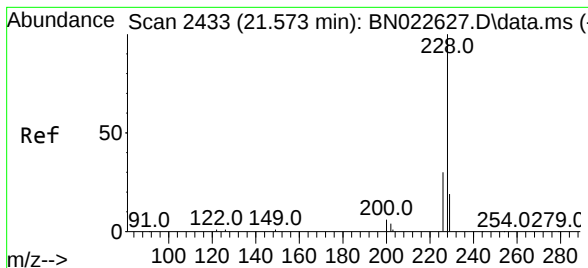

#33

Chrysene

Concen: 0.791 ng

RT: 21.573 min Scan# 2433

Delta R.T. -0.000 min

Lab File: BN022628.D

Acq: 12 Nov 2022 14:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.8





Tgt Ion:228 Resp: 19386

Ion Ratio Lower Upper

228 100

226 30.7 24.9 37.3

229 19.9 16.2 24.2

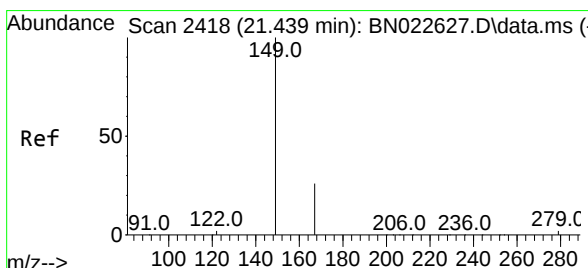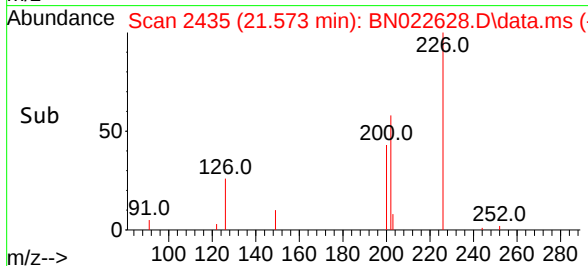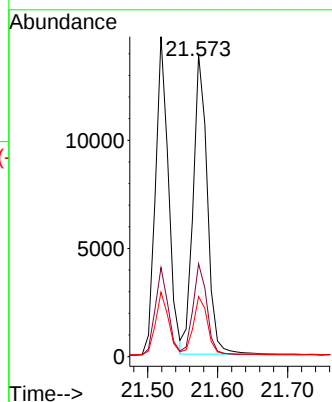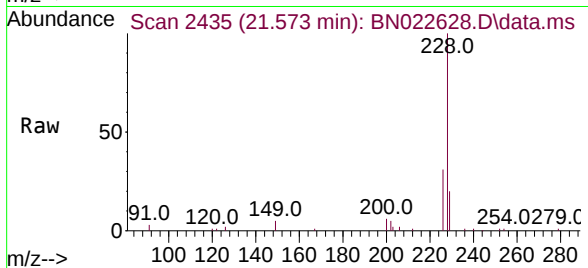

#34

Bis(2-ethylhexyl)phthalate

Concen: 0.968 ng

RT: 21.438 min Scan# 2420

Delta R.T. -0.000 min

Lab File: BN022628.D

Acq: 12 Nov 2022 14:30




Tgt Ion:149 Resp: 13283


Ion Ratio Lower Upper

149 100

167 25.9 21.1 31.7

279 3.1 2.8 4.2


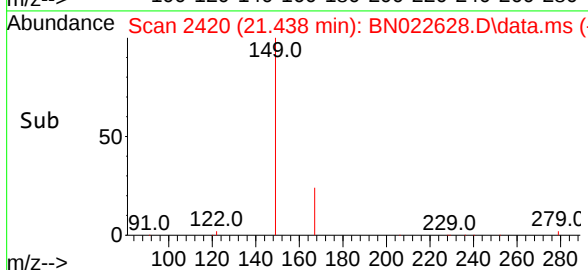

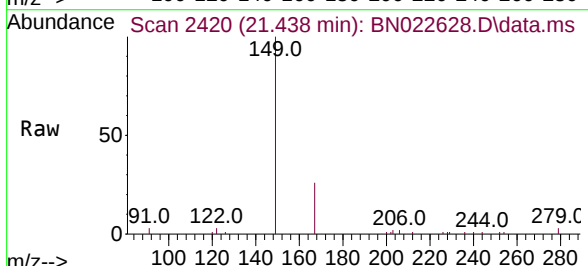




#35
Perylene-d12
Concen: 0.400 ng
RT: 23.979 min Scan# 3066
Delta R.T. -0.003 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	264	Resp:	5654
Ion Ratio	Lower	Upper	
264	100		
260	27.6	22.0	33.0
265	72.5	60.6	90.8

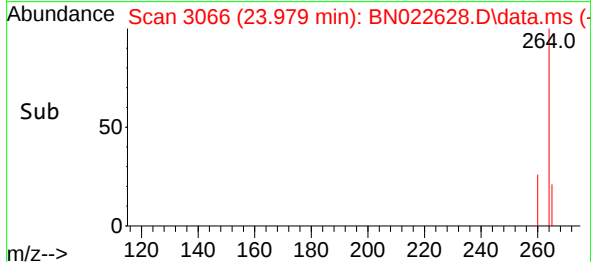

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.688 ng
RT: 26.528 min Scan# 3938
Delta R.T. -0.003 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30


Tgt Ion:	276	Resp:	18368
Ion Ratio	Lower	Upper	
276	100		
138	30.4	23.8	35.8
277	24.8	19.9	29.9

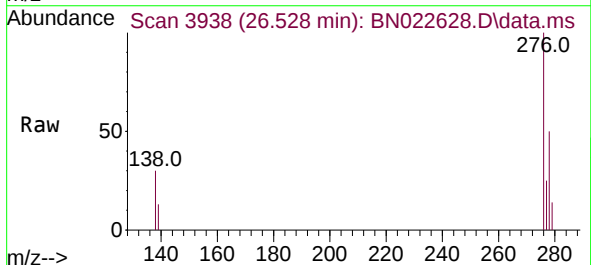






#37
Benzo(b)fluoranthene
Concen: 0.761 ng
RT: 23.227 min Scan# 2809
Delta R.T. -0.003 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8



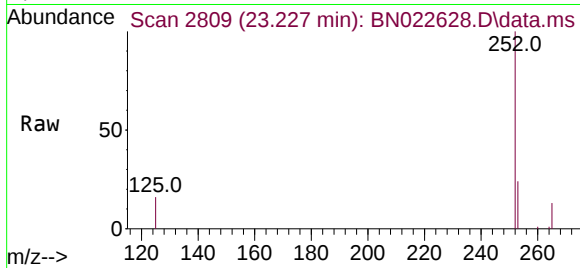



Tgt Ion:252 Resp: 17418
Ion Ratio Lower Upper
252 100
253 24.4 22.7 34.1
125 15.6 15.2 22.8

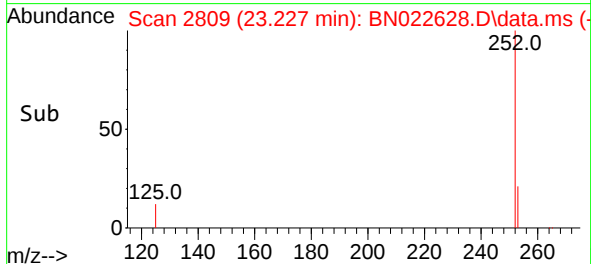

#38
Benzo(k)fluoranthene
Concen: 0.782 ng
RT: 23.274 min Scan# 2825
Delta R.T. -0.006 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30

Tgt Ion:252 Resp: 17853
Ion Ratio Lower Upper
252 100
253 24.4 22.6 33.8
125 15.3 14.9 22.3




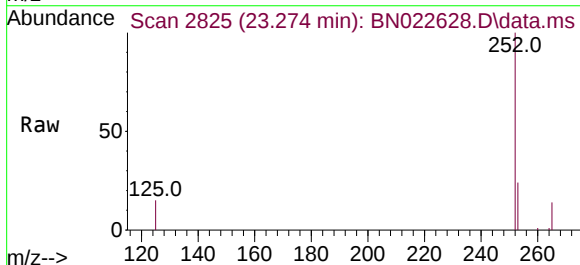




#39
Benzo(a)pyrene
Concen: 0.765 ng
RT: 23.865 min Scan# 3026
Delta R.T. -0.003 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252 Resp: 14223
Ion Ratio Lower Upper
252 100
253 26.2 24.6 36.8
125 19.0 19.4 29.0#

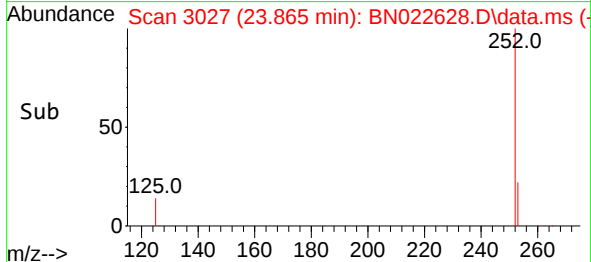

#40
Dibenzo(a,h)anthracene
Concen: 0.683 ng
RT: 26.549 min Scan# 3945
Delta R.T. -0.006 min
Lab File: BN022628.D
Acq: 12 Nov 2022 14:30


Tgt Ion:278 Resp: 14665
Ion Ratio Lower Upper
278 100
139 21.9 19.1 28.7
279 26.6 24.8 37.2

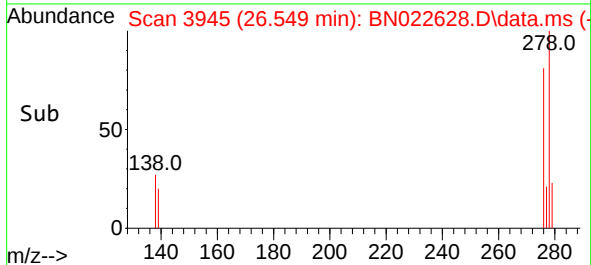

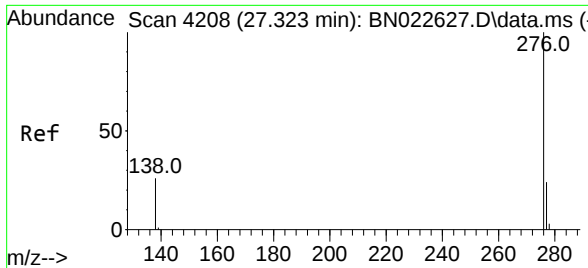

#41
 Benzo(g,h,i)perylene
 Concen: 0.675 ng
 RT: 27.320 min Scan# 41
 Delta R.T. -0.003 min
 Lab File: BN022628.D
 Acq: 12 Nov 2022 14:30

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8

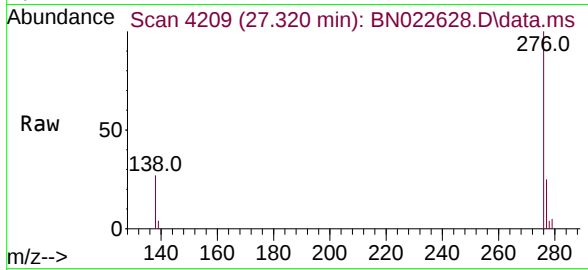

Tgt Ion:	276	Resp:	15252
Ion	Ratio	Lower	Upper
276	100		
277	25.1	21.2	31.8
138	27.3	23.8	35.8

