


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111322\
 Data File : BN022624.D
 Acq On : 12 Nov 2022 11:56
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 14 02:29:35 2022

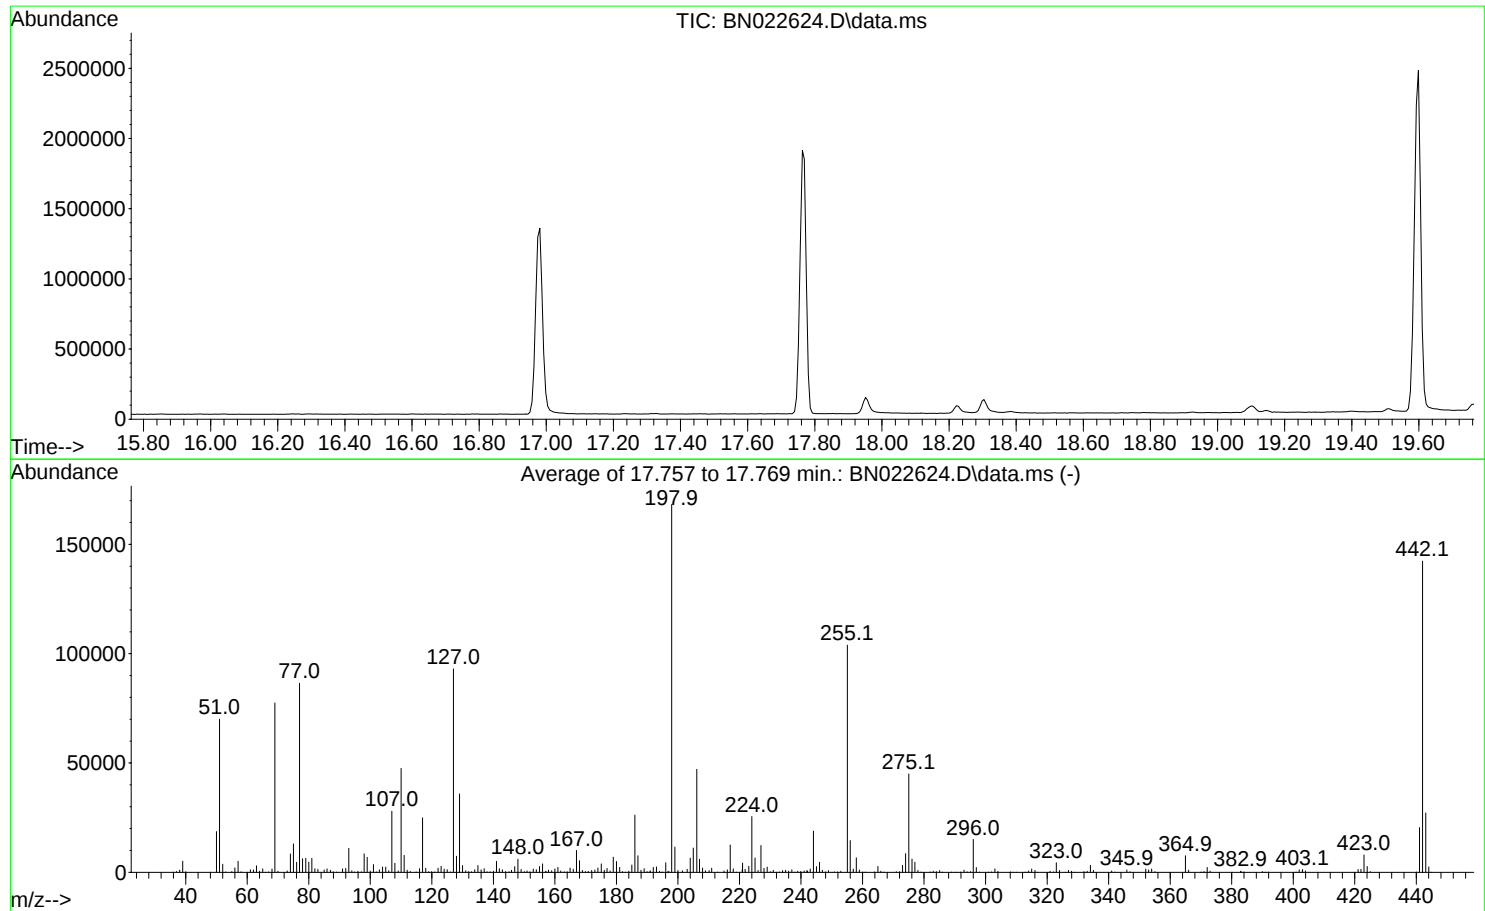




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	70010	PASS
68	69	0.00	2	1.9	1495	PASS
69	198	0.00	100	46.0	77485	PASS
70	69	0.00	2	0.6	489	PASS
127	198	10	80	55.3	93080	PASS
197	198	0.00	2	0.3	465	PASS
198	198	100	100	100.0	168267	PASS
199	198	5	9	6.8	11518	PASS
275	198	10	60	26.7	45011	PASS
365	198	1	100	4.5	7559	PASS
441	198	0.01	100	12.2	20495	PASS
442	442	50	100	100.0	142309	PASS
443	442	15	24	19.1	27156	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111322\
Data File : BN022624.D
Acq On : 12 Nov 2022 11:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 14 08:30:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 08:30:11 2022
Response via : Initial Calibration

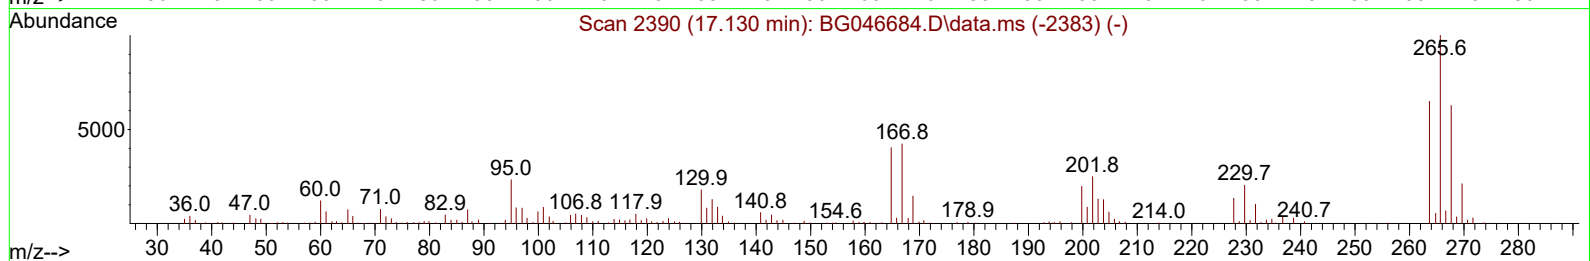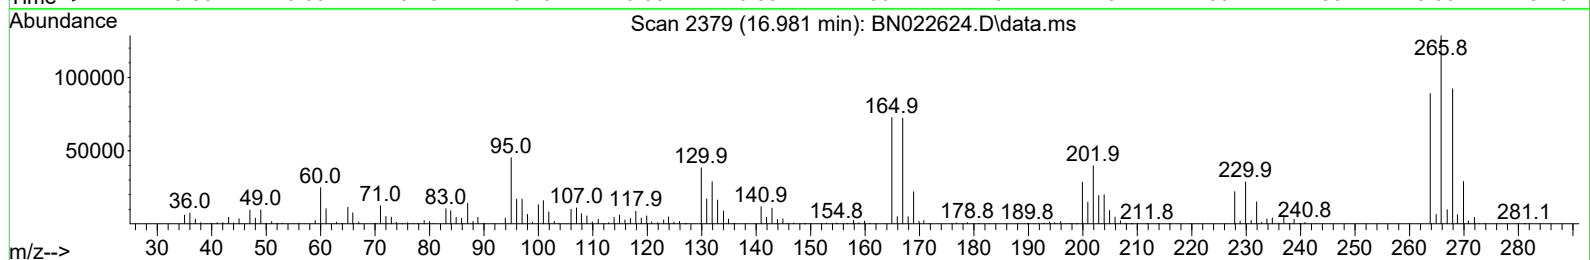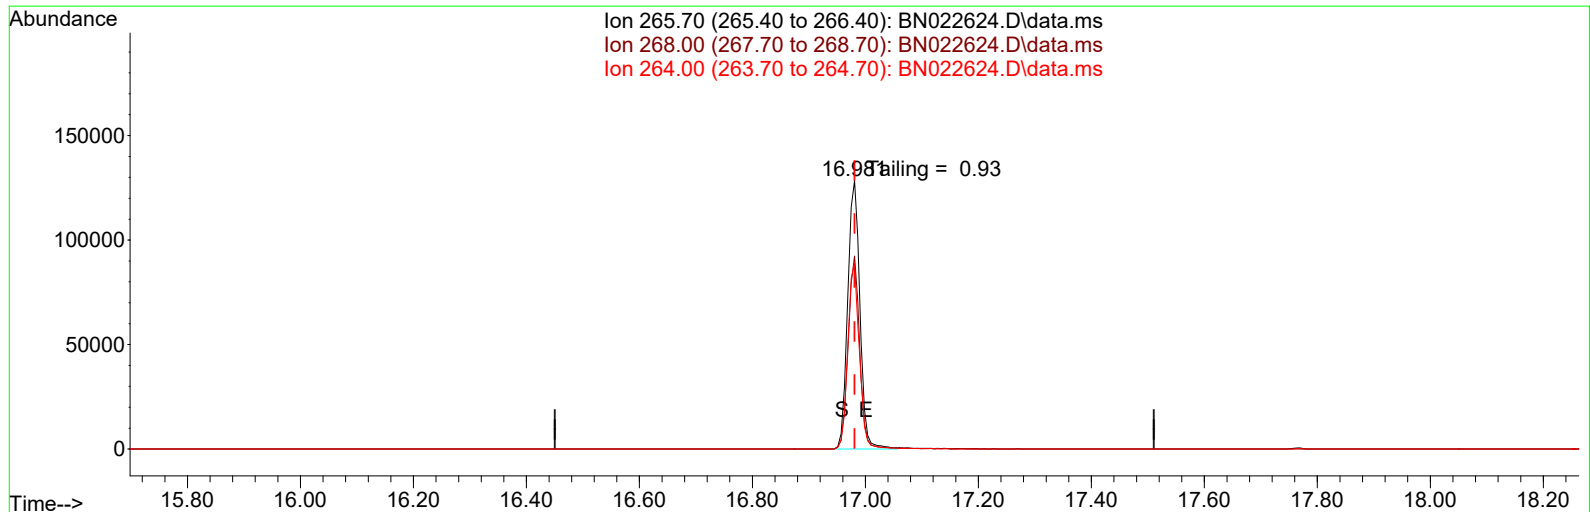

TIC: BN022624.D\data.ms

(70) Pentachlorophenol (C)

16.981min (0.000) 19417.00 ng




response 192608

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.89
264.00	61.60	69.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111322\
Data File : BN022624.D
Acq On : 12 Nov 2022 11:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 14 08:30:17 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 14 08:30:11 2022
Response via : Initial Calibration

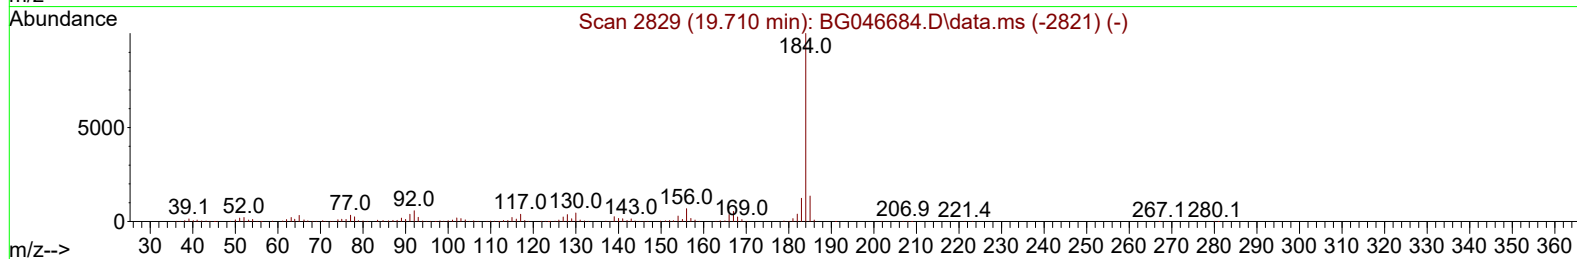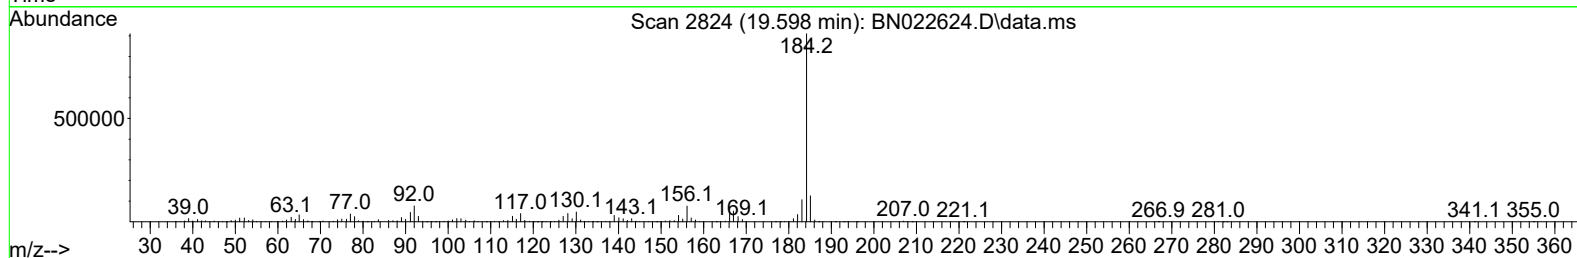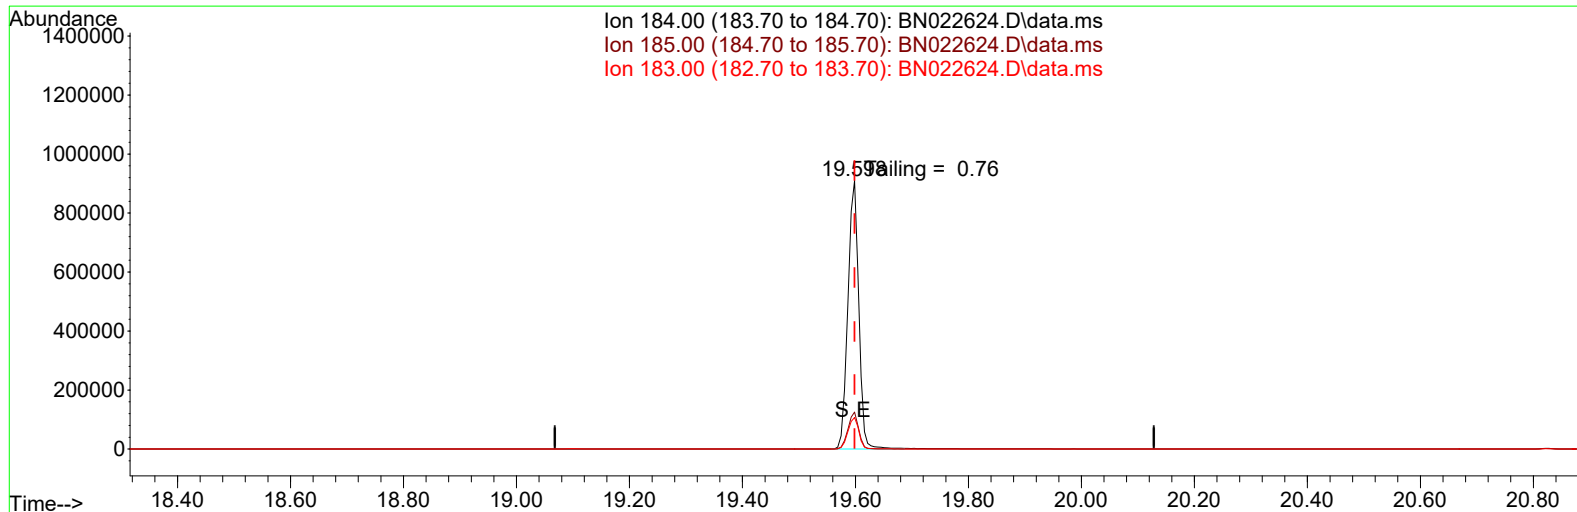

TIC: BN022624.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 1222595

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.77
183.00	13.20	11.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2022	BNA_N	<u>BN022624.D</u>
Compound Name	Response	Retention Time
DDT	576194	20.828
DDD	8494	20.433
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8494	584688	1.45

Instrument :
BNA_N
ClientSampleId :
DFTPP