
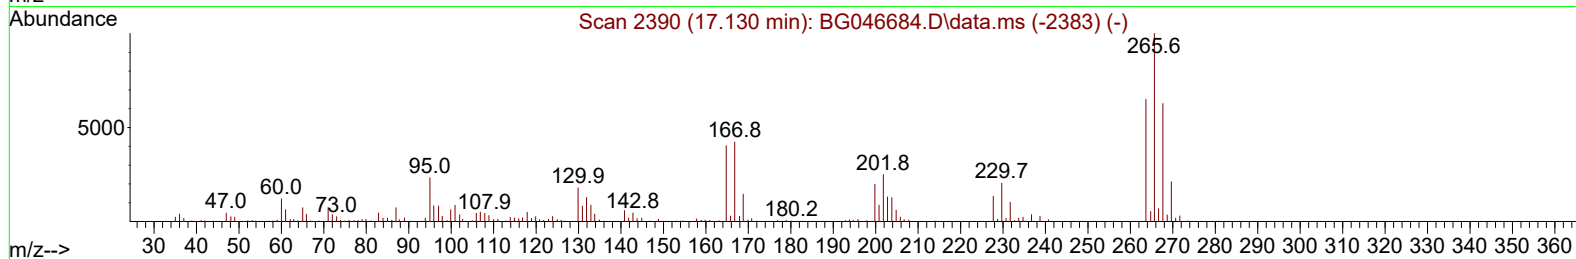
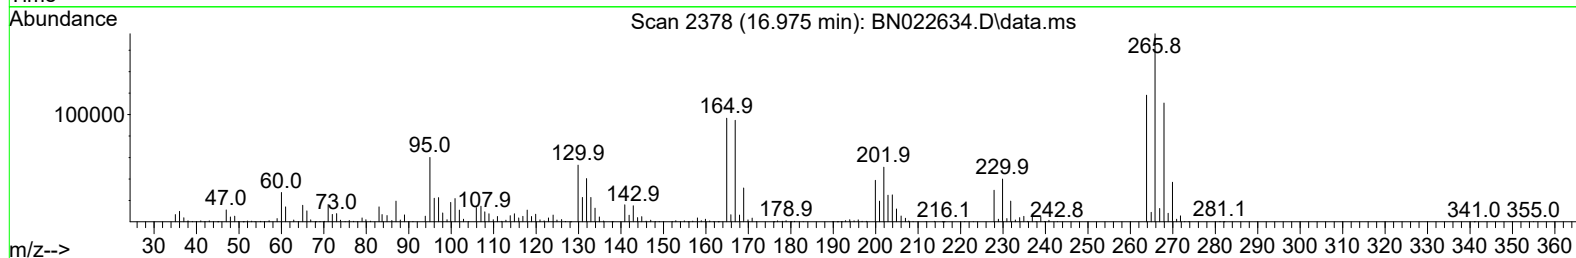


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111422\
Data File : BN022634.D
Acq On : 14 Nov 2022 09:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 05:30:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 15 05:30:26 2022
Response via : Initial Calibration

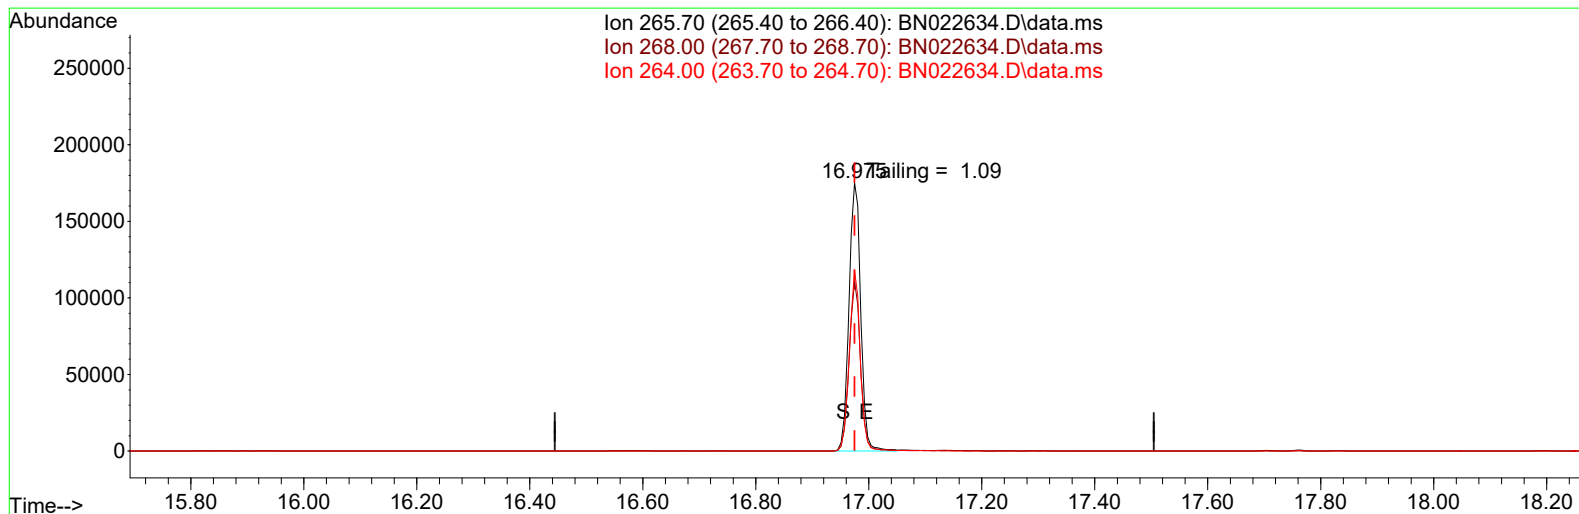

TIC: BN022634.D\data.ms

(70) Pentachlorophenol (C)




16.975min (0.000) 21196.66 ng

response 252846

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.23
264.00	61.60	67.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111422\
Data File : BN022634.D
Acq On : 14 Nov 2022 09:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 05:30:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 15 05:30:26 2022
Response via : Initial Calibration

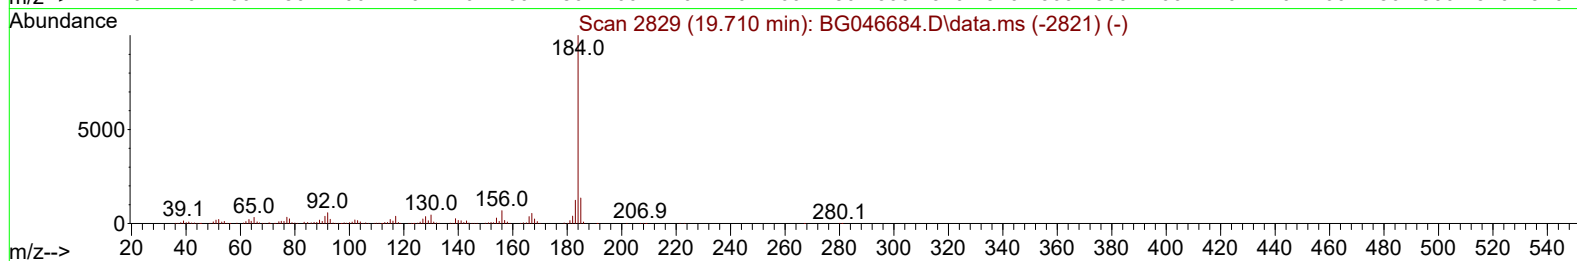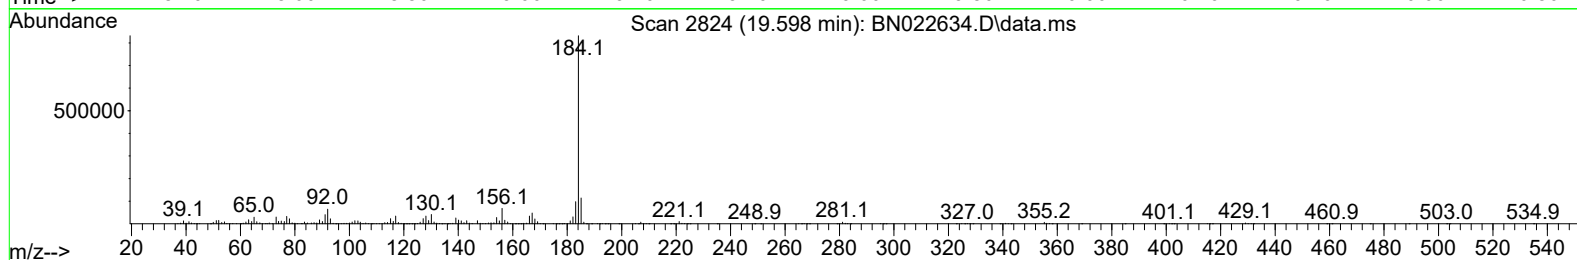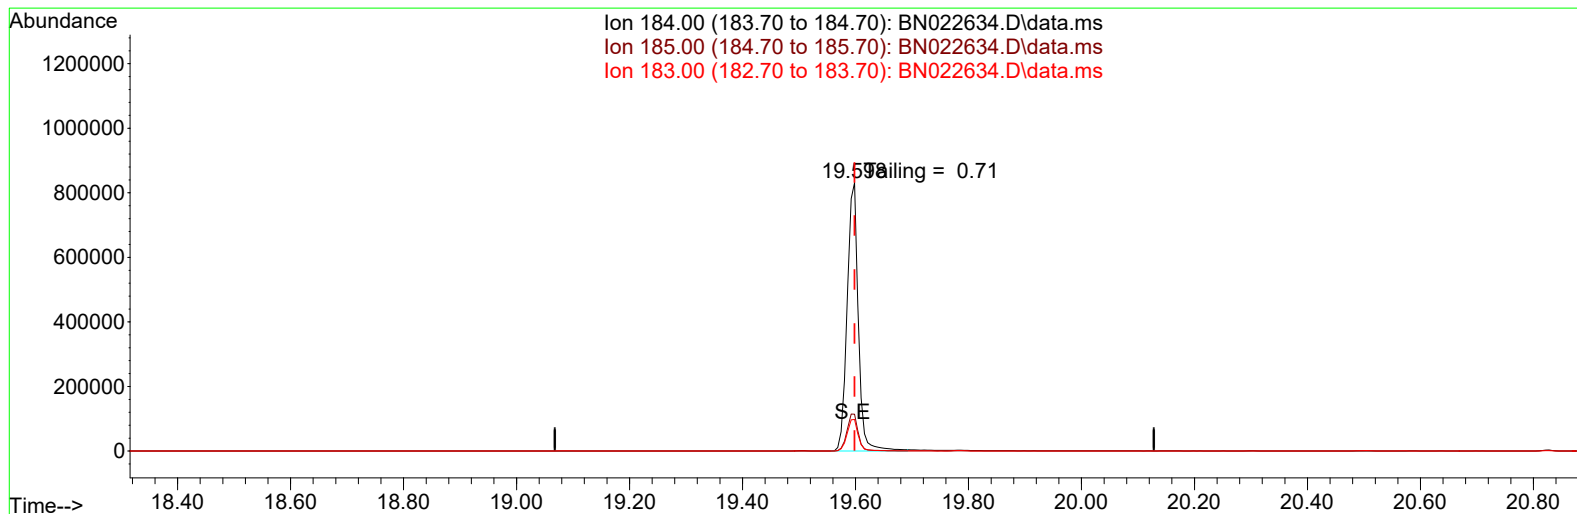

TIC: BN022634.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 1149737

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.79
0.00	0.00	0.00