
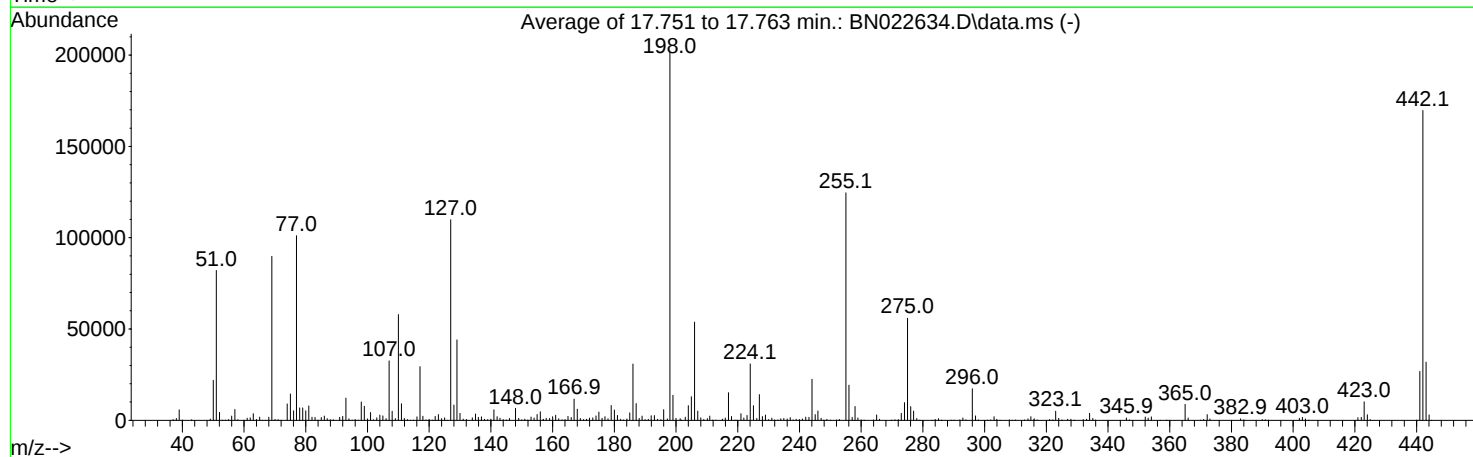


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111422\
 Data File : BN022634.D
 Acq On : 14 Nov 2022 09:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 15 00:38:02 2022

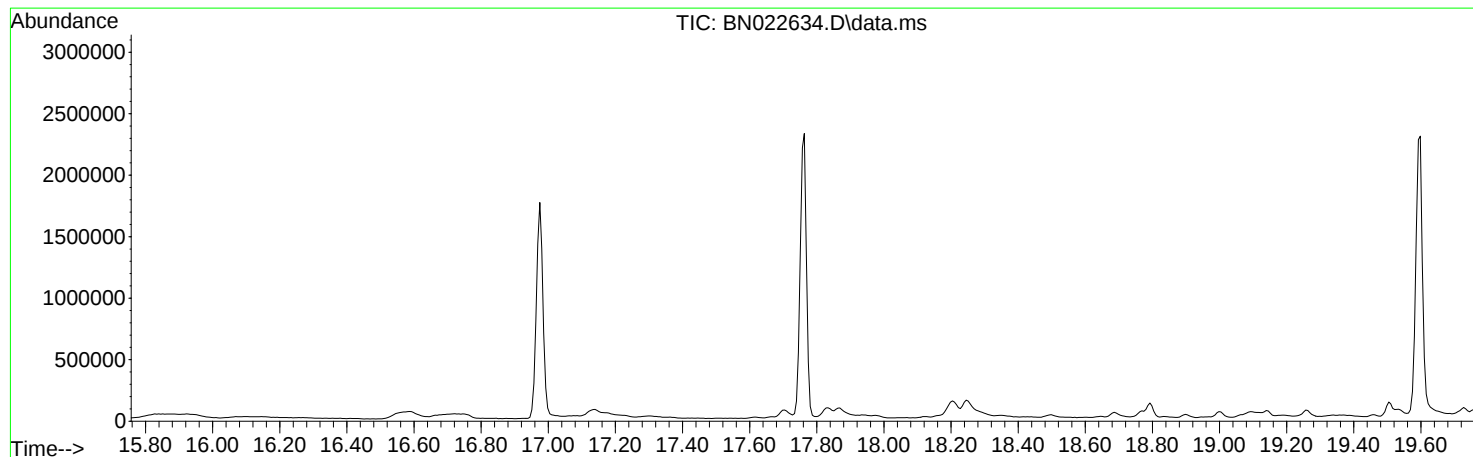




AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	82026	PASS
68	69	0.00	2	1.9	1682	PASS
69	198	0.00	100	44.6	89763	PASS
70	69	0.00	2	0.6	531	PASS
127	198	10	80	54.5	109850	PASS
197	198	0.00	2	0.4	740	PASS
198	198	100	100	100.0	201451	PASS
199	198	5	9	6.8	13723	PASS
275	198	10	60	27.7	55829	PASS
365	198	1	100	4.3	8761	PASS
441	198	0.01	100	13.3	26809	PASS
442	442	50	100	100.0	169645	PASS
443	442	15	24	18.8	31829	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111422\
 Data File : BN022634.D
 Acq On : 14 Nov 2022 09:21
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Nov 15 05:30:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 15 05:30:26 2022
 Response via : Initial Calibration

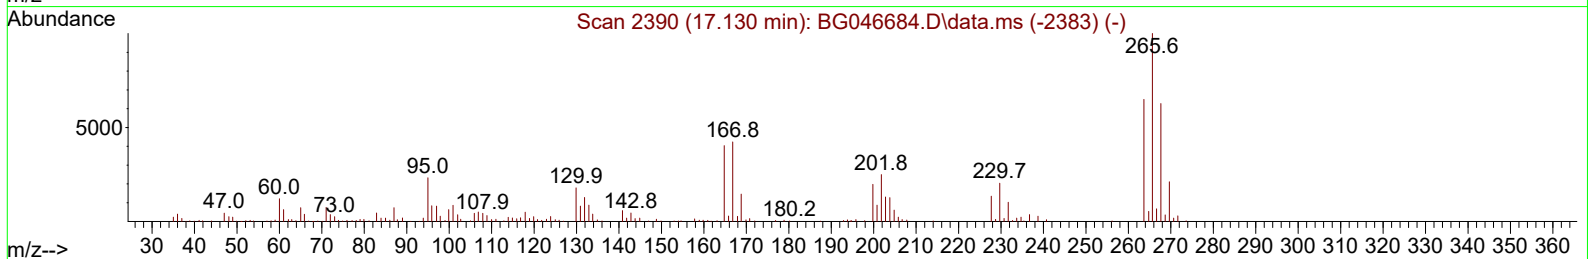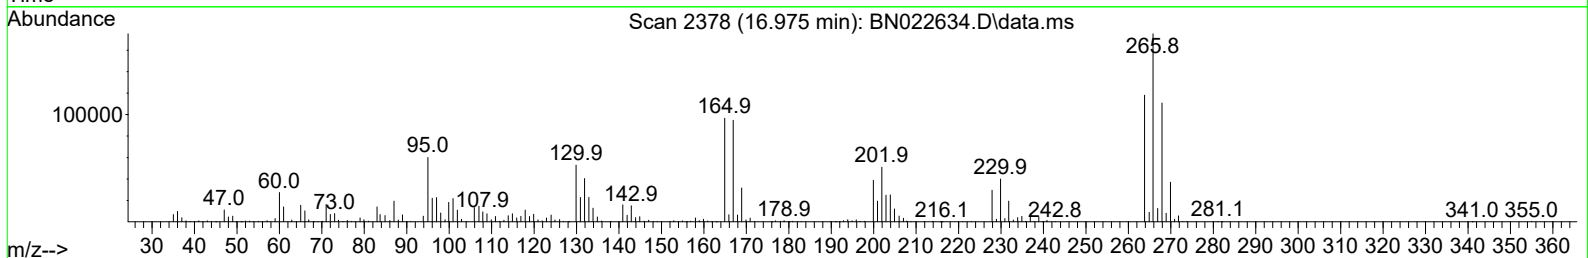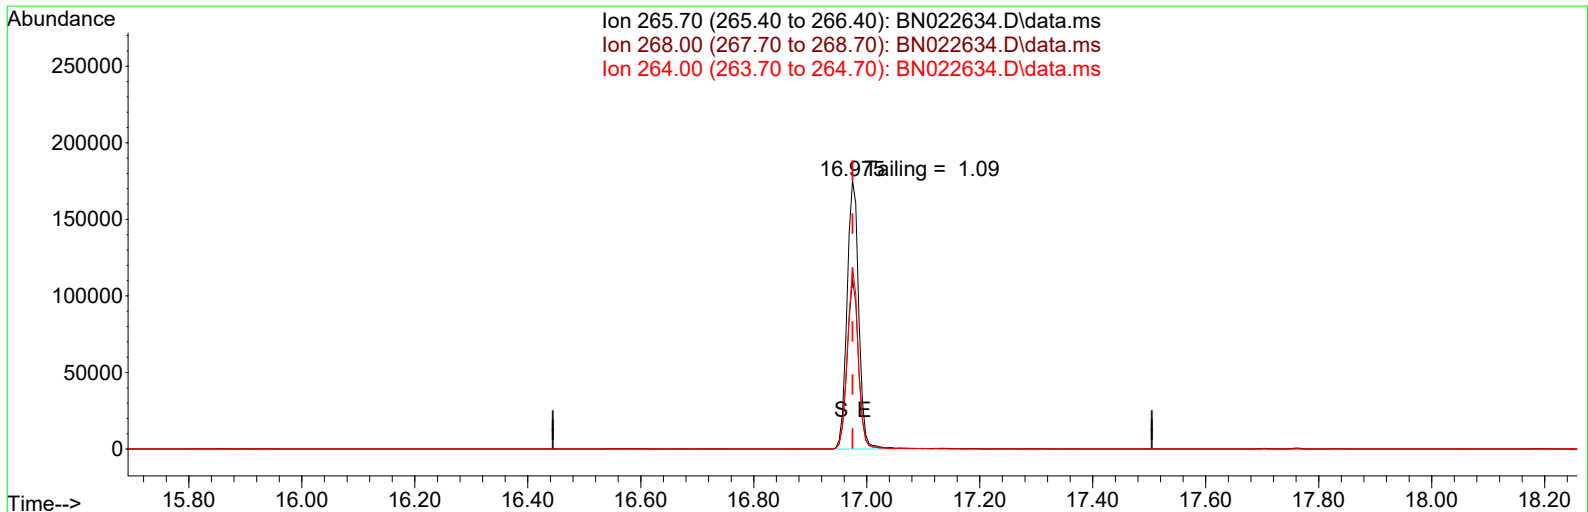

TIC: BN022634.D\data.ms

(70) Pentachlorophenol (C)

16.975min (0.000) 21196.66 ng




response 252846

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.23
264.00	61.60	67.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111422\
Data File : BN022634.D
Acq On : 14 Nov 2022 09:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 15 05:30:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 15 05:30:26 2022
Response via : Initial Calibration

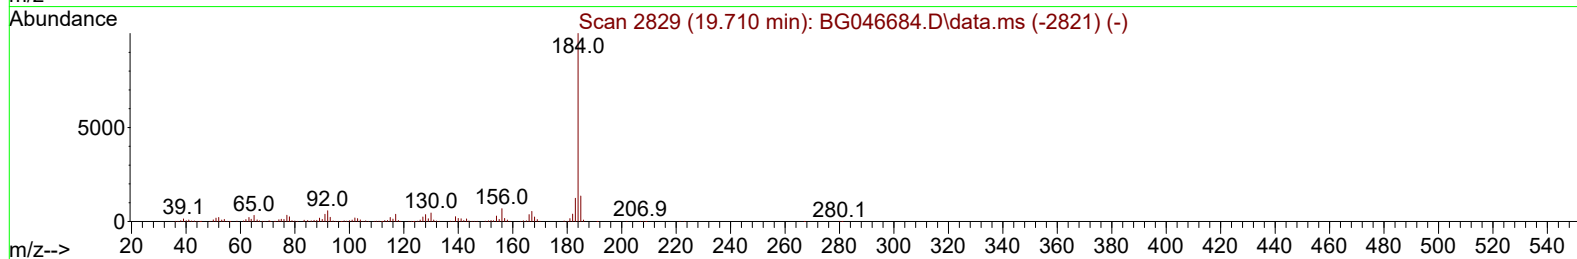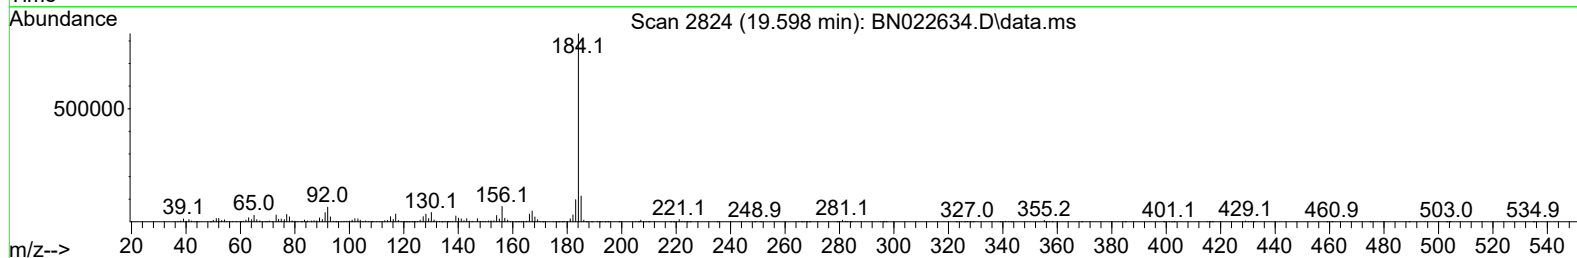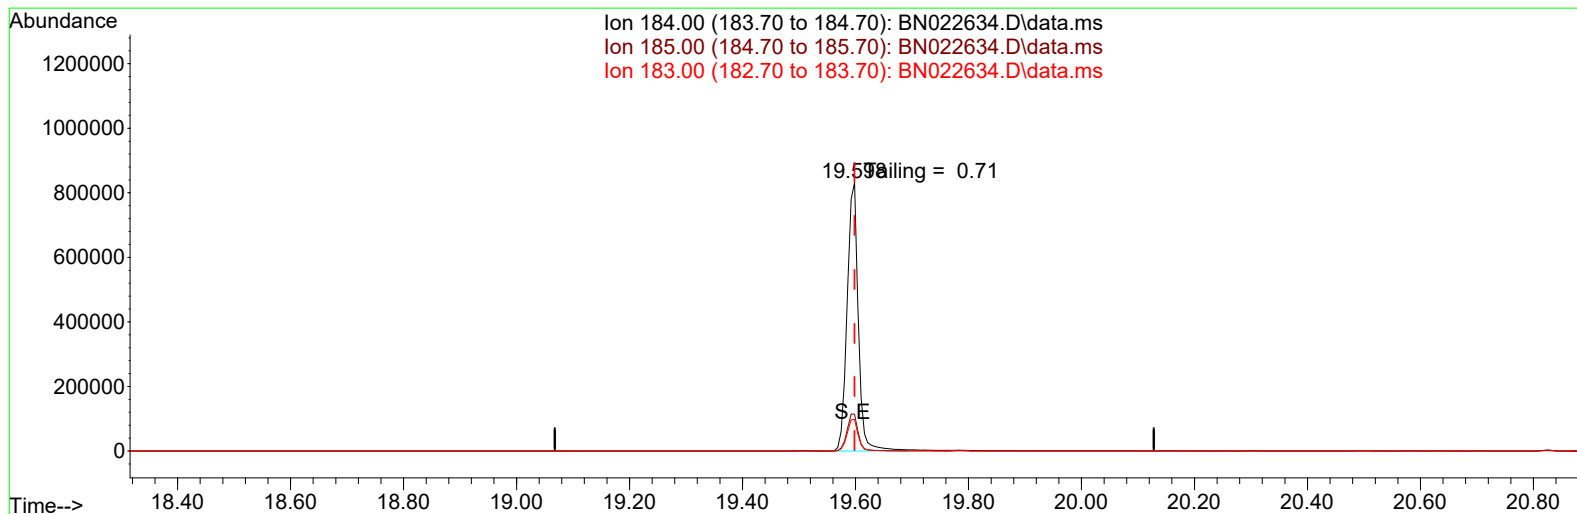

TIC: BN022634.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response 1149737

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.70
183.00	13.20	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/14/2022	BNA_N	<u>BN022634.D</u>
Compound Name	Response	Retention Time
DDT	672250	20.827
DDD	18573	20.386
DDE	708	19.869
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19281	691531	2.79

Instrument :
BNA_N
ClientSampleId :
DFTPP