
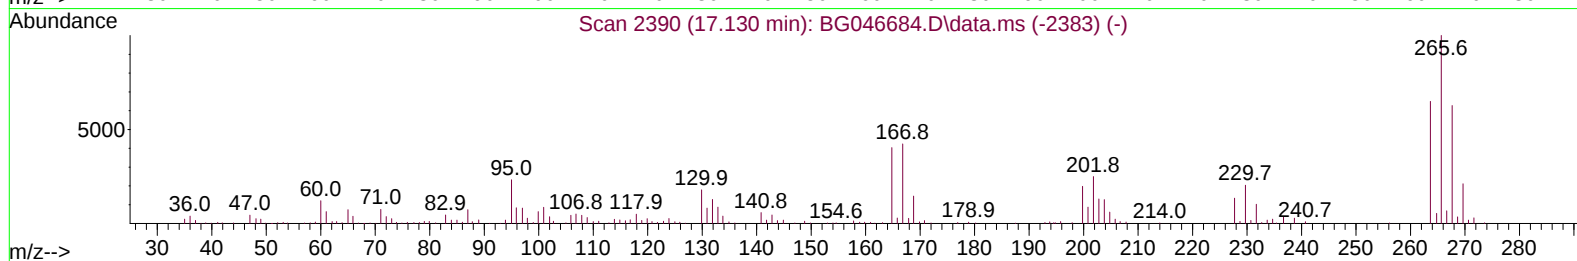
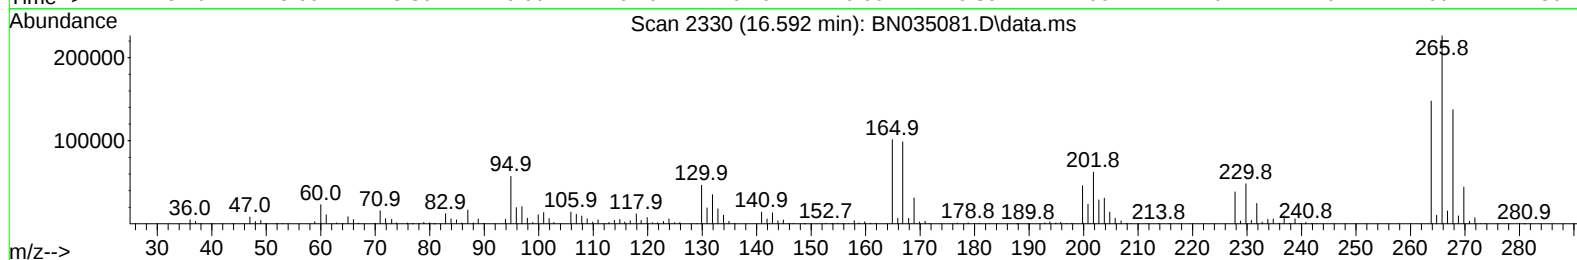


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111424\
Data File : BN035081.D
Acq On : 14 Nov 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 01:14:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 15 01:14:43 2024
Response via : Initial Calibration

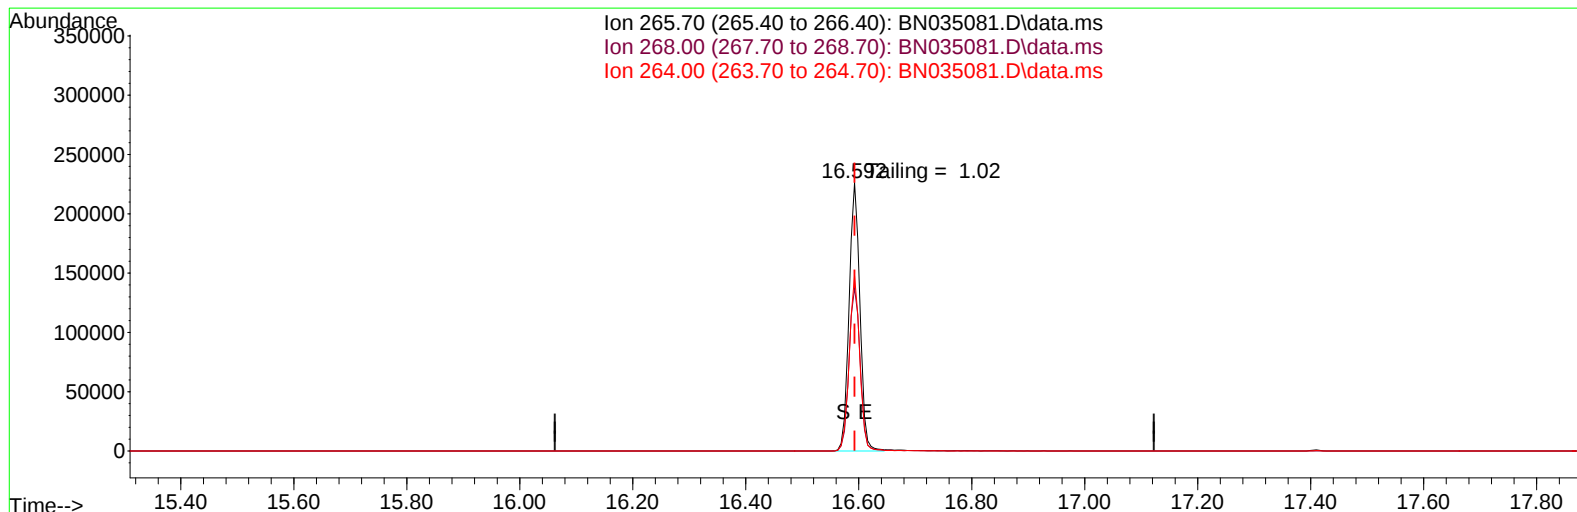

TIC: BN035081.D\data.ms

(70) Pentachlorophenol (C)




16.592min (0.000) 22635.68 ng

response 303230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.69
264.00	61.60	65.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111424\
Data File : BN035081.D
Acq On : 14 Nov 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 01:14:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 15 01:14:43 2024
Response via : Initial Calibration

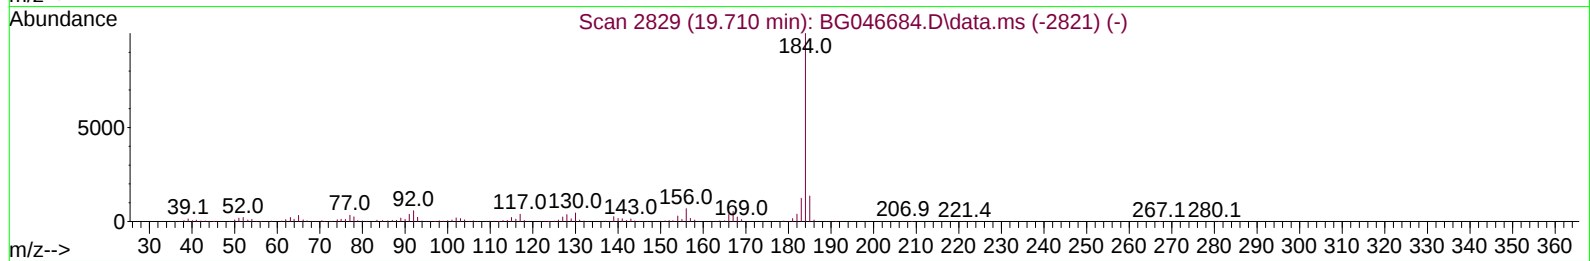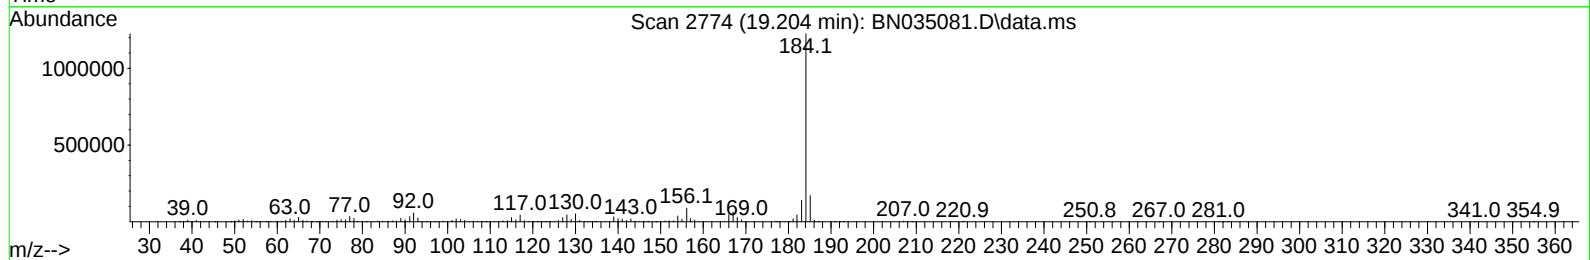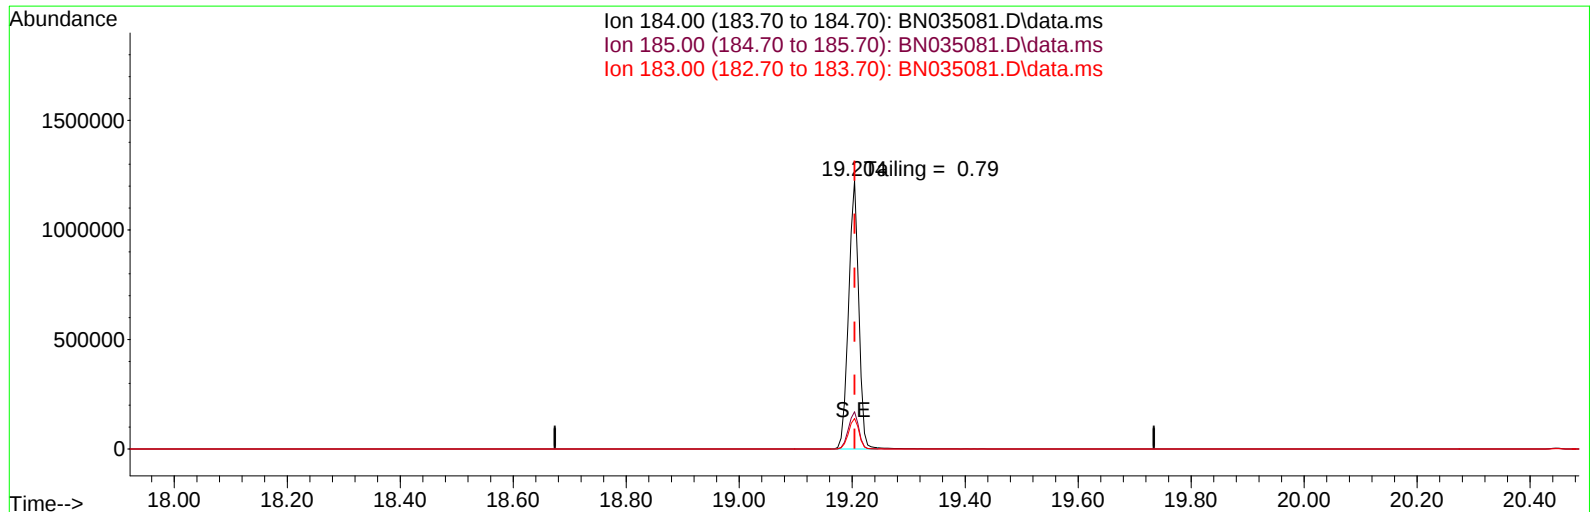

TIC: BN035081.D\data.ms

(77) Benzidine

19.204min (0.000) 0.00 ng

response 1534532

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	11.39
0.00	0.00	0.00