


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111424\
Data File : BN035081.D
Acq On : 14 Nov 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 17:18:14 2024

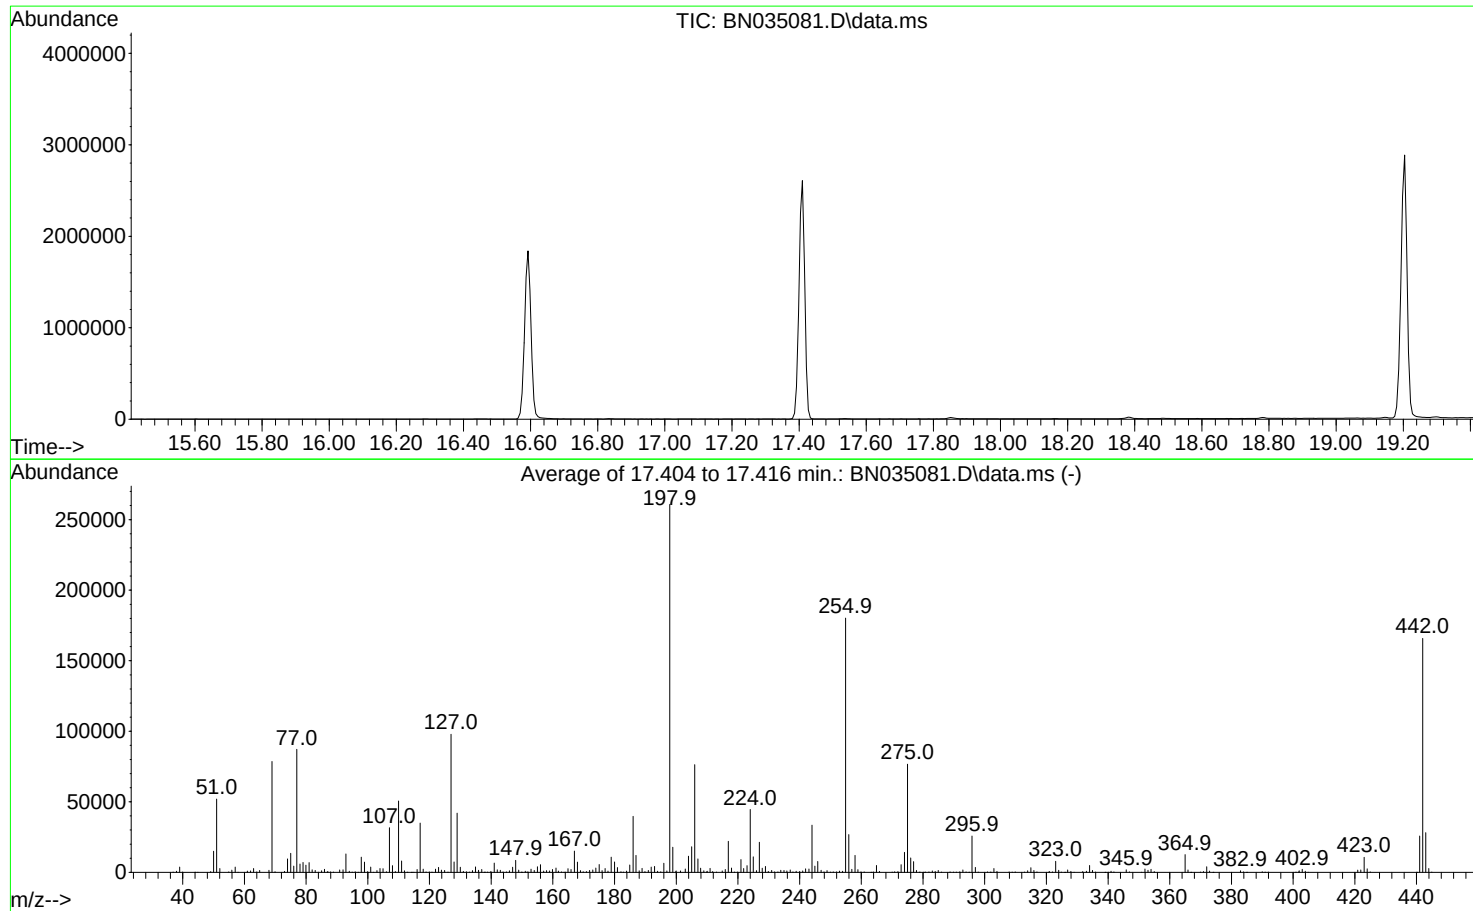




AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.9	51893	PASS
68	69	0.00	2	1.9	1465	PASS
69	198	0.00	100	30.1	78547	PASS
70	69	0.00	2	0.6	499	PASS
127	198	10	80	37.5	97883	PASS
197	198	0.00	2	0.4	1067	PASS
198	198	100	100	100.0	260736	PASS
199	198	5	9	6.8	17819	PASS
275	198	10	60	29.4	76672	PASS
365	198	1	100	4.8	12586	PASS
441	198	0.01	100	9.9	25771	PASS
442	442	50	100	100.0	165845	PASS
443	442	15	24	16.9	28101	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111424\
Data File : BN035081.D
Acq On : 14 Nov 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 15 01:14:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 15 01:14:43 2024
Response via : Initial Calibration

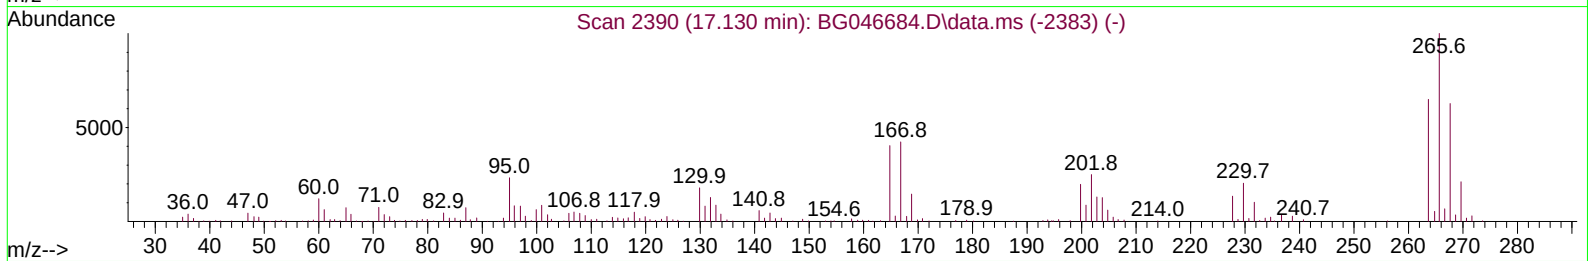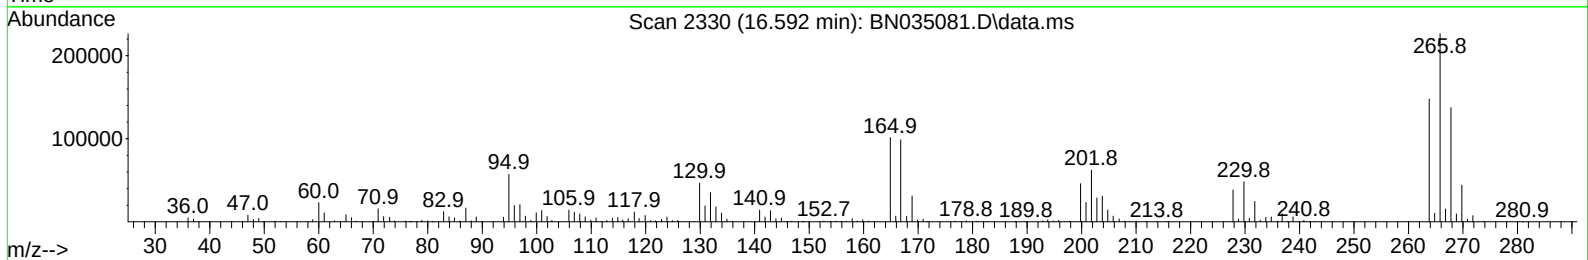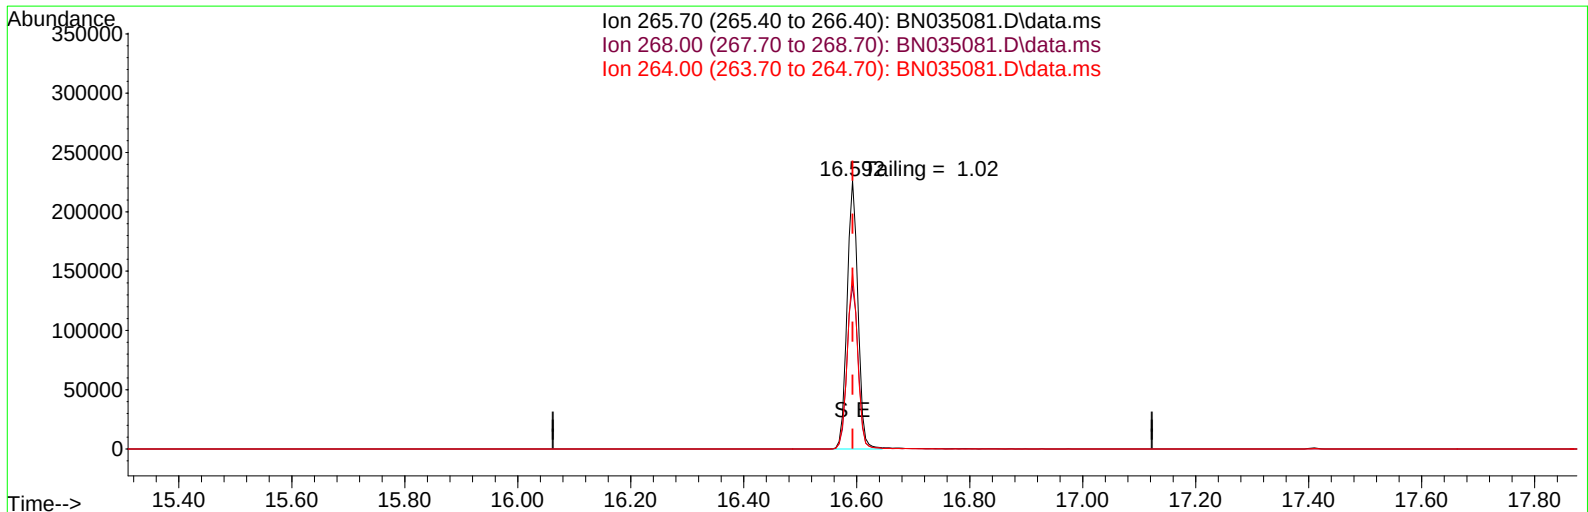

TIC: BN035081.D\data.ms

(70) Pentachlorophenol (C)

16.592min (0.000) 22635.68 ng




response 303230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	60.69
264.00	61.60	65.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111424\
Data File : BN035081.D
Acq On : 14 Nov 2024 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Nov 15 01:14:50 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 15 01:14:43 2024
Response via : Initial Calibration

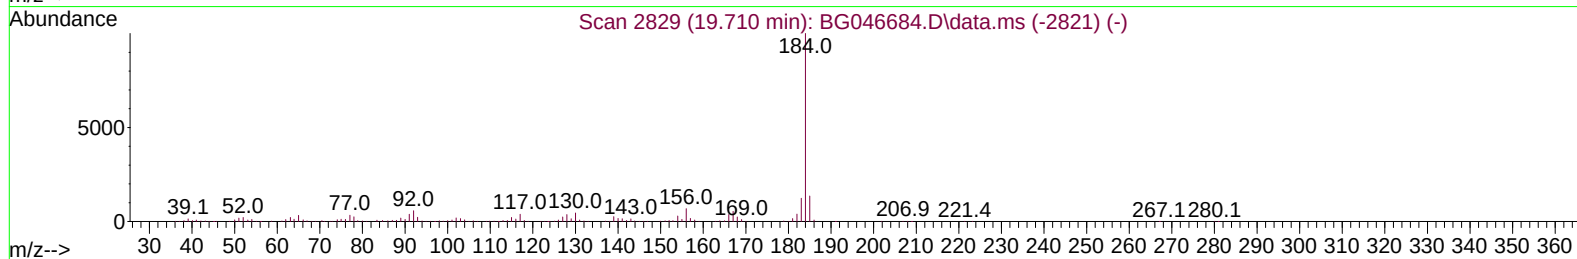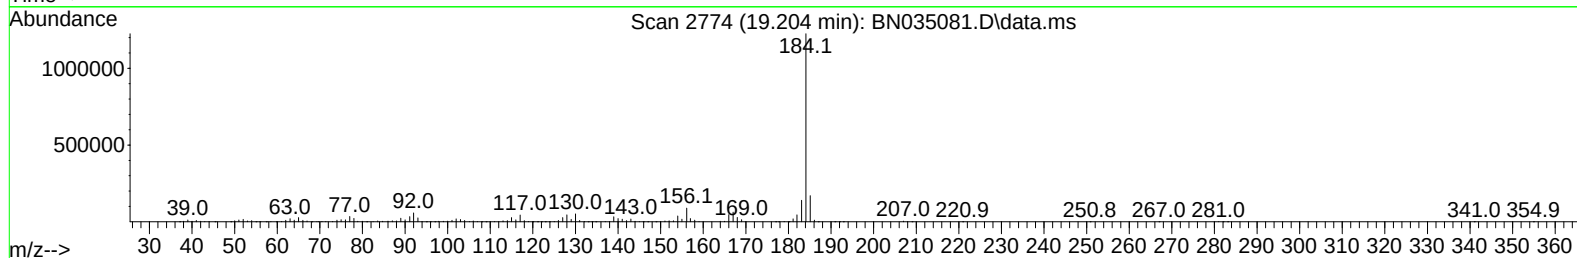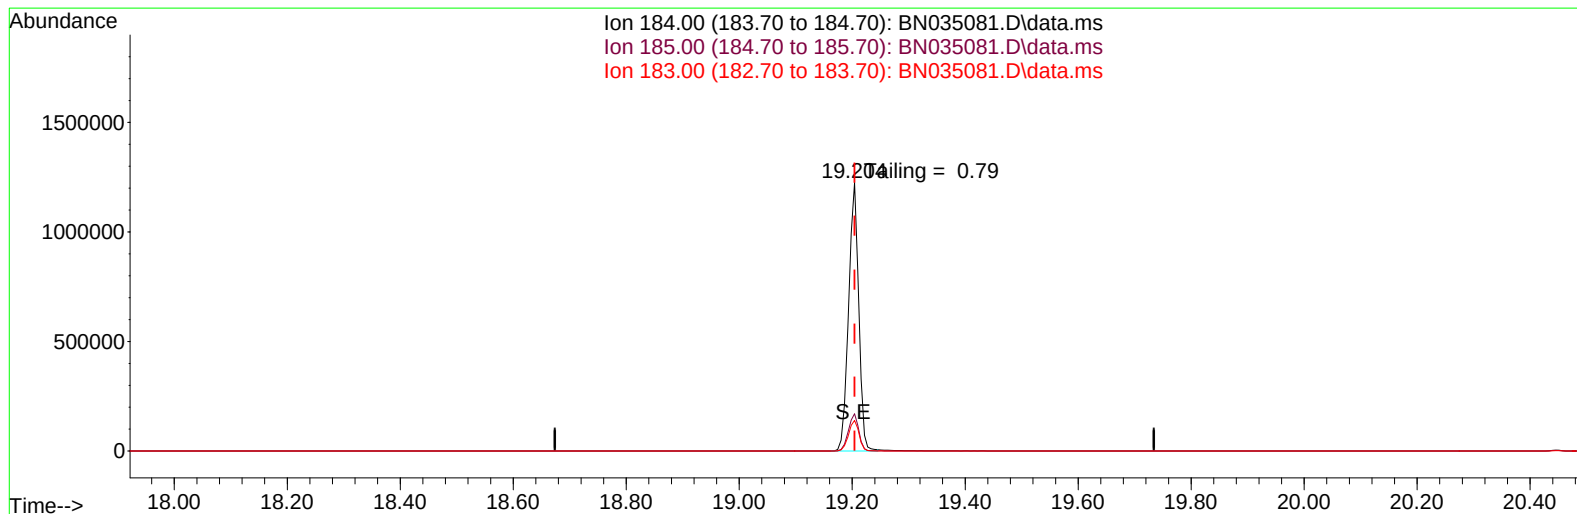

TIC: BN035081.D\data.ms

(77) Benzidine

19.204min (0.000) 0.00 ng

response 1534532

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/14/2024	BNA_N	<u>BN035081.D</u>
Compound Name	Response	Retention Time
DDT	954250	20.445
DDD	16295	20.004
DDE	363	19.458
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16658	970908	1.72

Instrument :
BNA_N
ClientSampleId :
DFTPP