

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022658.D
 Acq On : 15 Nov 2022 20:40
 Operator : CG/JU
 Sample : N5570-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBMW2

Quant Time: Nov 15 23:17:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	88315	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	395994	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	243680	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	484660	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	403838	20.000	ng/ul	0.00
88) Perylene-d12	23.962	264	355469	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.199	96	8315	3.214	ng/uL	0.00
4) Pyridine-d5	3.640	84	50063	6.844	ng/ul	0.01
7) Phenol-d5	7.052	99	40799	4.891	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	98155	19.627	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	100025	16.375	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	77186	11.721	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	60229	19.650	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	65792	19.237	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	120906	20.736	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	117668	13.249	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	412396	23.267	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	437835	22.419	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	14983	4.240	ng/ul	0.01
60) Fluorene-d10	15.557	176	334689	23.024	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	59809	19.415	ng/ul	0.00
73) Anthracene-d10	17.422	188	517281	24.375	ng/ul	0.00
81) Pyrene-d10	19.727	212	539026	25.756	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.798	264	418938	23.445	ng/ul	0.00
Target Compounds						
71) Pentachlorophenol	16.969	266	29676	8.372	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022658.D
Acq On : 15 Nov 2022 20:40
Operator : CG/JU
Sample : N5570-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBMW2

Quant Time: Nov 15 23:17:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

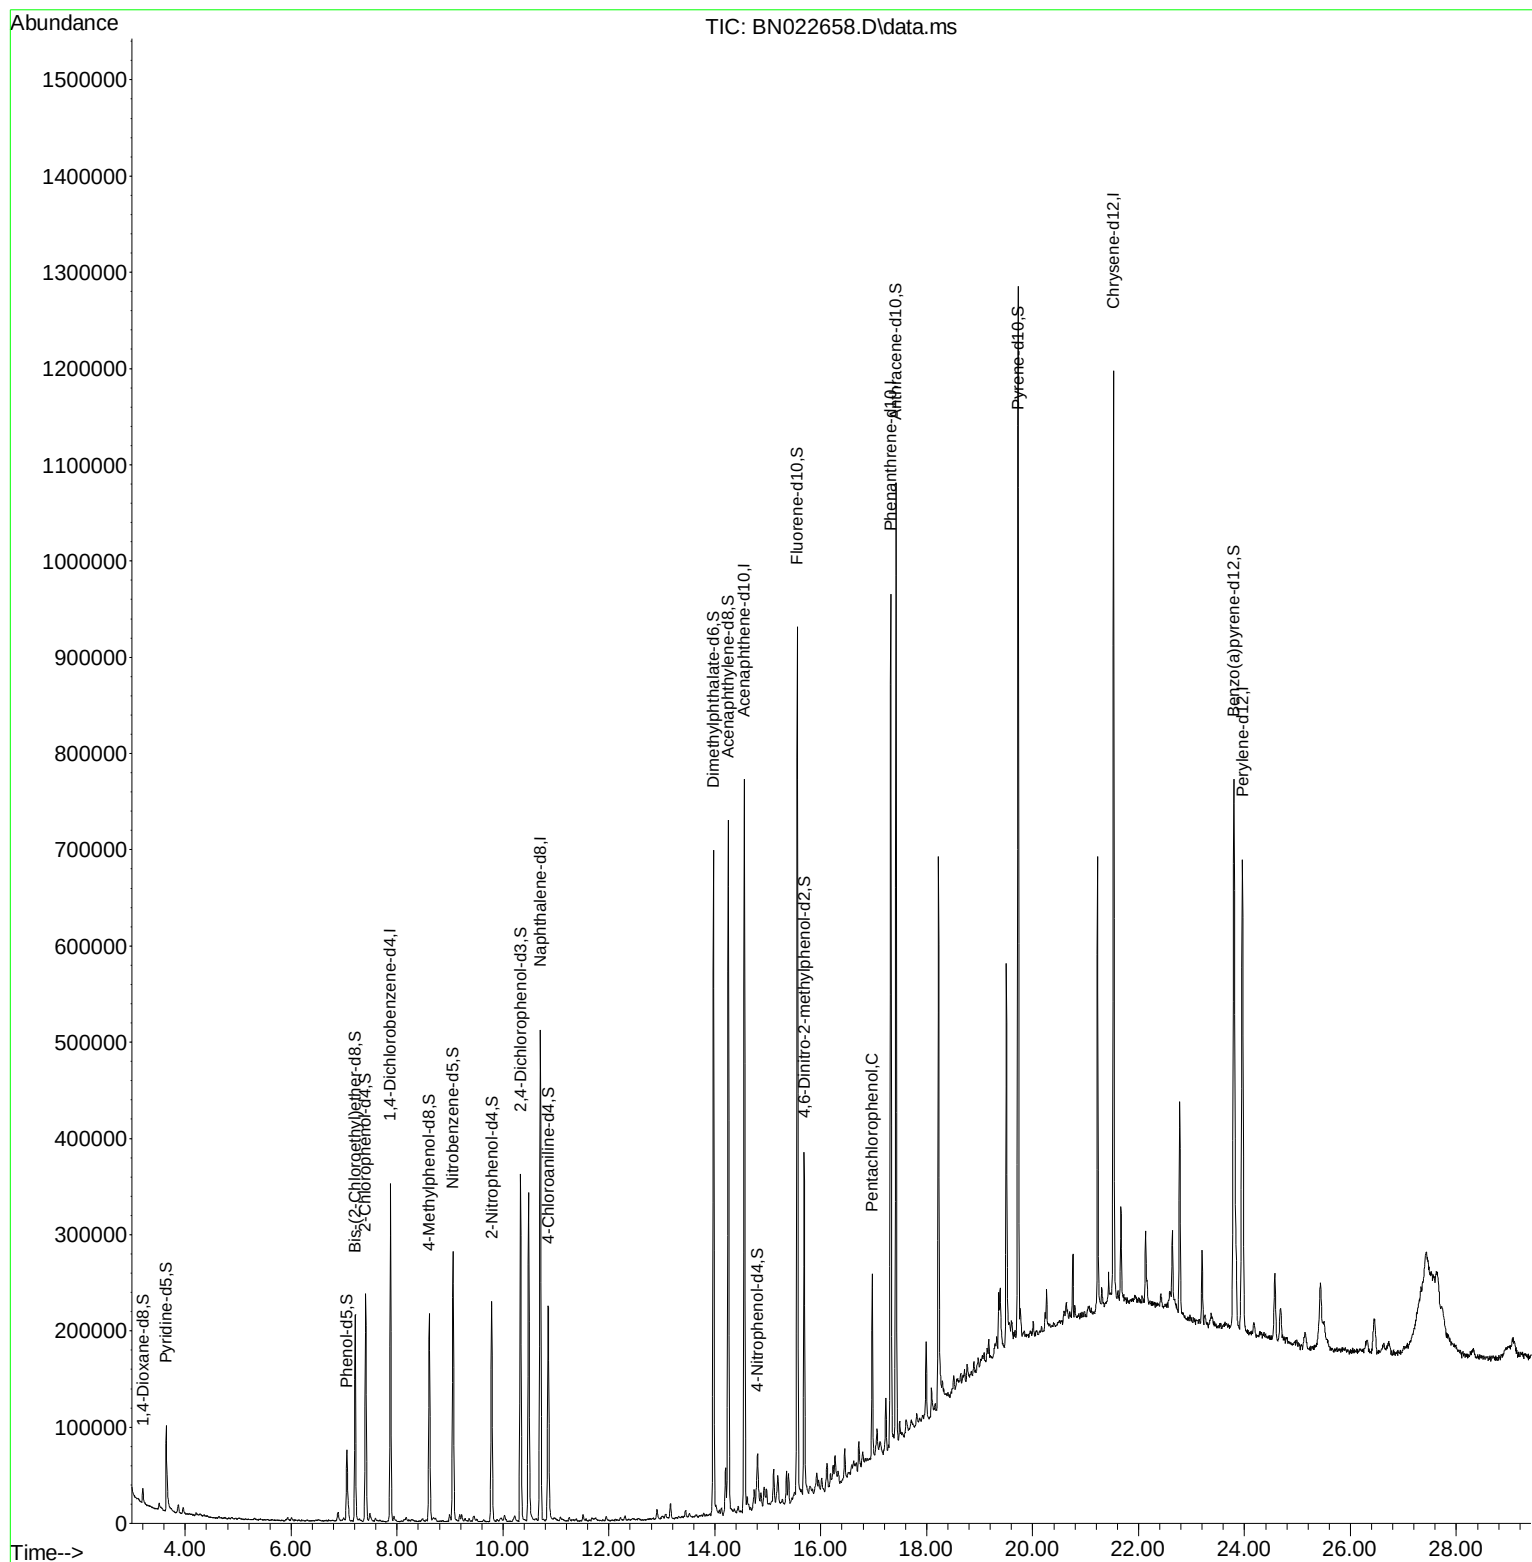



Abundance Scan 2377 (16.969 min): BN022645.D\data.ms (-2371) (-)

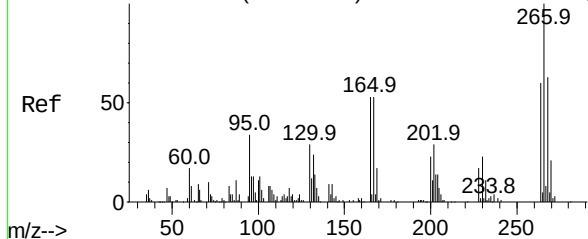

Pentachlorophenol
Concen: 8.372 ng/ul
RT: 16.969 min Scan# 1
Delta R.T. -0.000 min
Lab File: BN022658.D
Acq: 15 Nov 2022 20:40

Instrument :
BNA_N
ClientSampleId :
GBMW2

Tgt Ion:	266	Resp:	29676
Ion	Ratio	Lower	Upper
266	100		
264	67.7	47.8	71.8
268	63.2	50.2	75.2

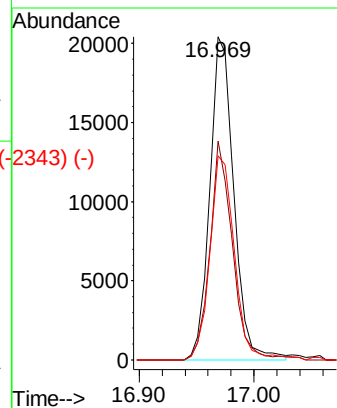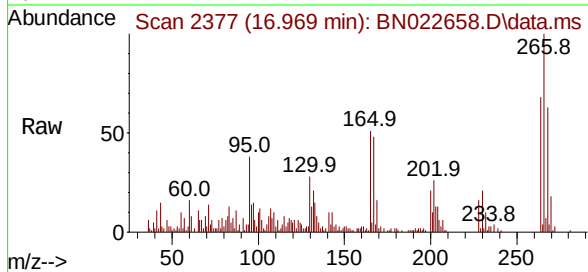

Abundance Scan 2377 (16.969 min): BN022658.D\data.ms (-2343) (-)

