

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022681.D
 Acq On : 16 Nov 2022 11:26
 Operator : CG/JU
 Sample : PB149090BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Nov 16 14:16:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	67004	20.000	ng/ul	0.00
20) Naphthalene-d8	10.698	136	303507	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	195358	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	397599	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	376979	20.000	ng/ul	0.00
88) Perylene-d12	23.962	264	366102	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	11759	5.992	ng/uL	0.00
4) Pyridine-d5	3.628	84	166681	30.032	ng/ul	0.00
7) Phenol-d5	7.046	99	200245	31.642	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	124128	32.714	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	151569	32.704	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	161207	32.267	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	77031	32.789	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	85014	32.432	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	142059	31.789	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	220497	32.393	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	479470	33.743	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	516416	32.984	ng/ul	0.00
54) 4-Nitrophenol-d4	14.787	143	83361	29.428	ng/ul	-0.01
60) Fluorene-d10	15.557	176	393170	33.737	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	59755	23.645	ng/ul	0.00
73) Anthracene-d10	17.422	188	611137	35.103	ng/ul	0.00
81) Pyrene-d10	19.727	212	657947	33.678	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.804	264	613604	33.342	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.604	70	4350	1.024	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022681.D
Acq On : 16 Nov 2022 11:26
Operator : CG/JU
Sample : PB149090BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Nov 16 14:16:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

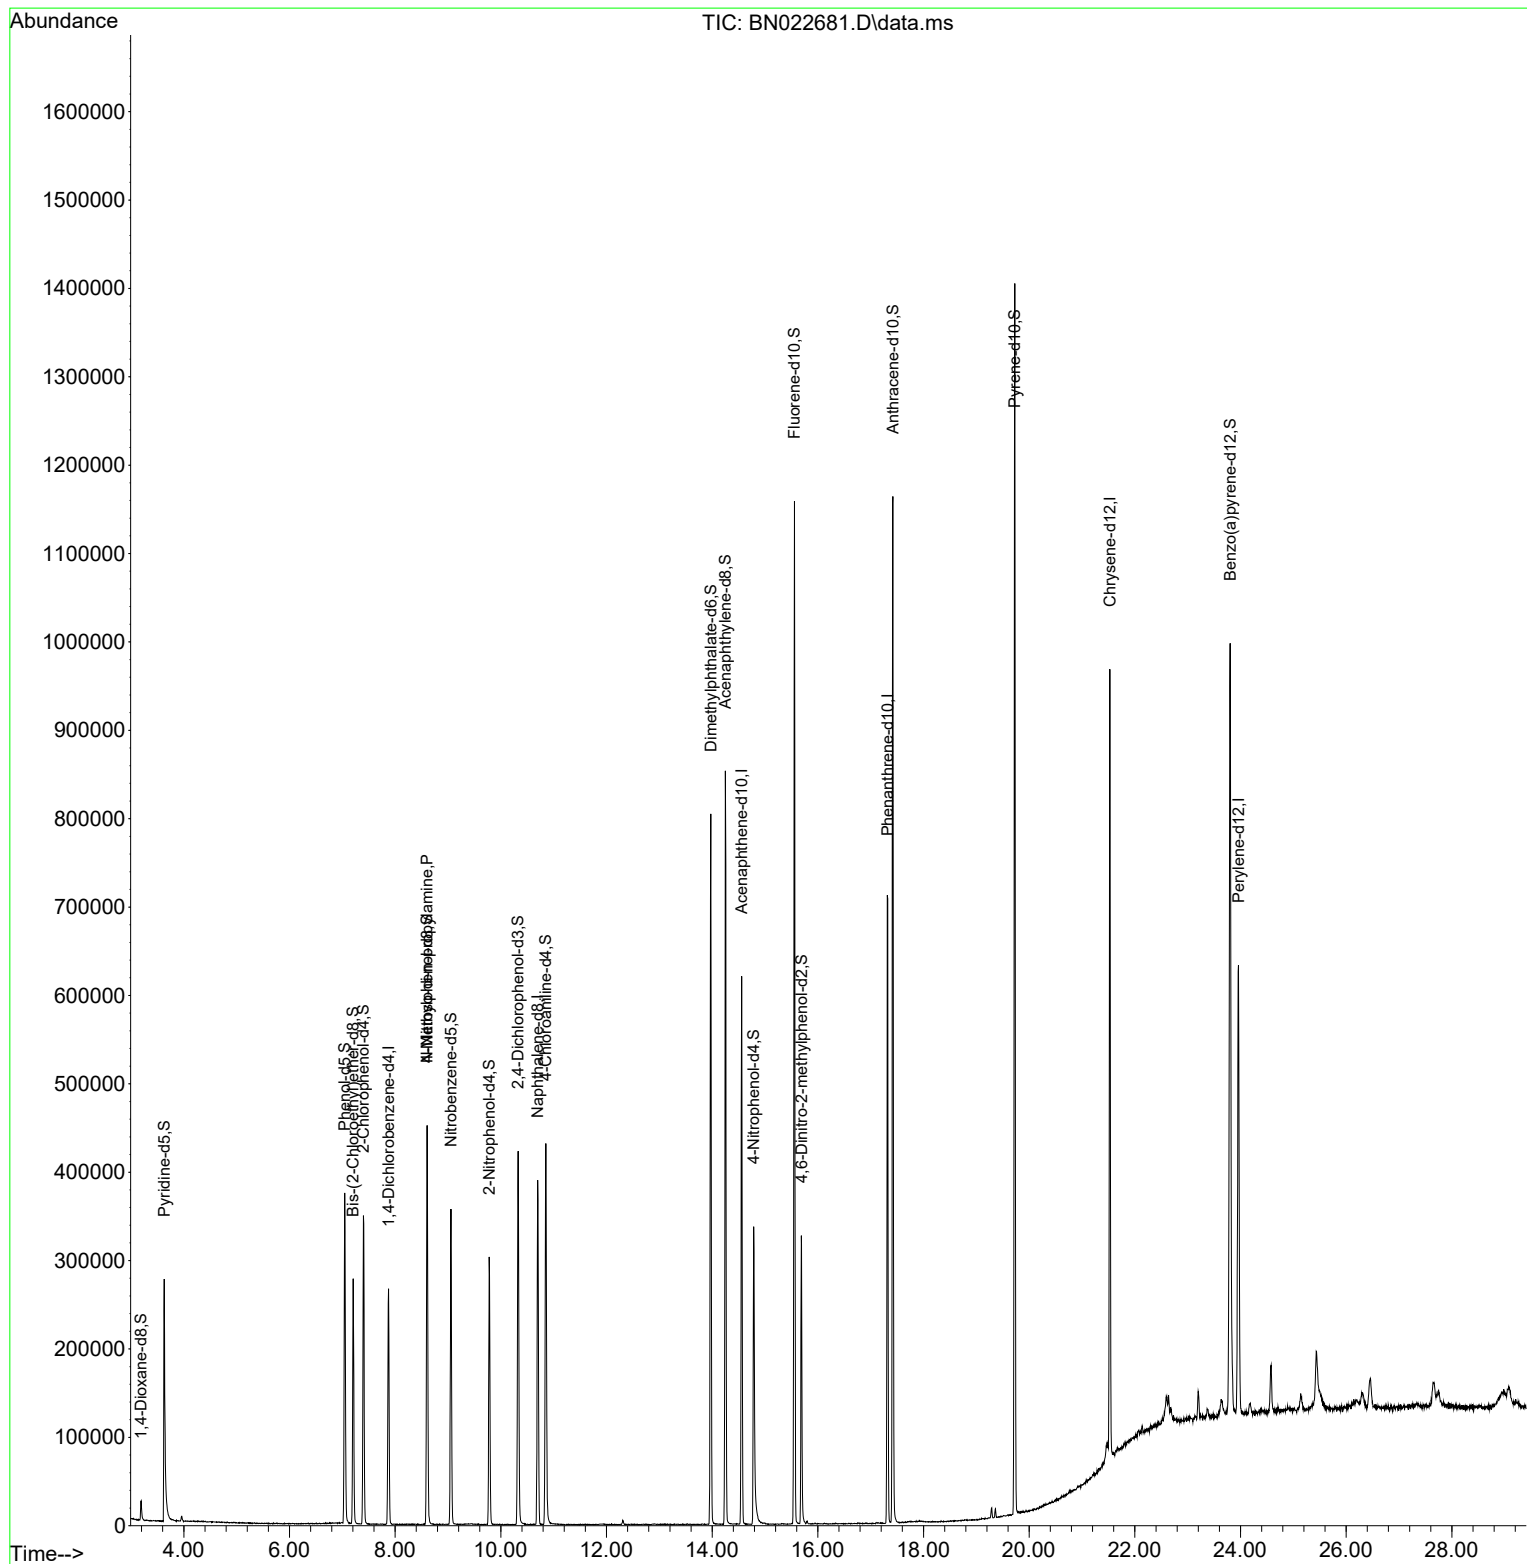

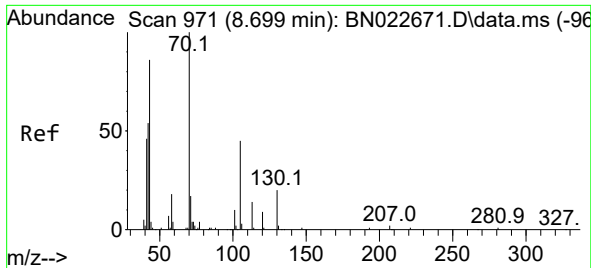

#17
 N-Nitroso-di-n-propylamine
 Concen: 1.024 ng/ul
 RT: 8.604 min Scan# 91
 Delta R.T. -0.100 min
 Lab File: BN022681.D
 Acq: 16 Nov 2022 11:26

Instrument :
 BNA_N
 ClientSampleId :

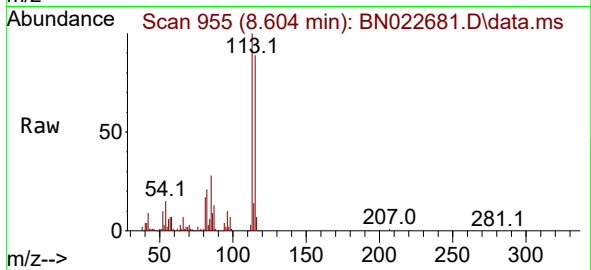

Tgt Ion:	70	Resp:	4350
Ion	Ratio	Lower	Upper
70	100		
42	342.3	43.4	65.2#
101	0.0	8.0	12.0#
130	0.0	16.2	24.4#

