




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022659.D
Acq On : 15 Nov 2022 21:17
Operator : CG/JU
Sample : N5570-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBMW5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 23:17:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
Supervised By :mohammad ahmed 11/16/2022

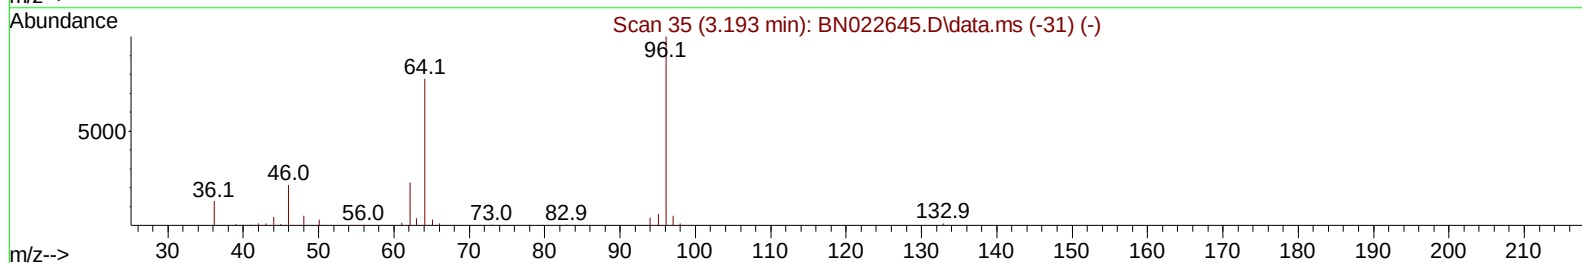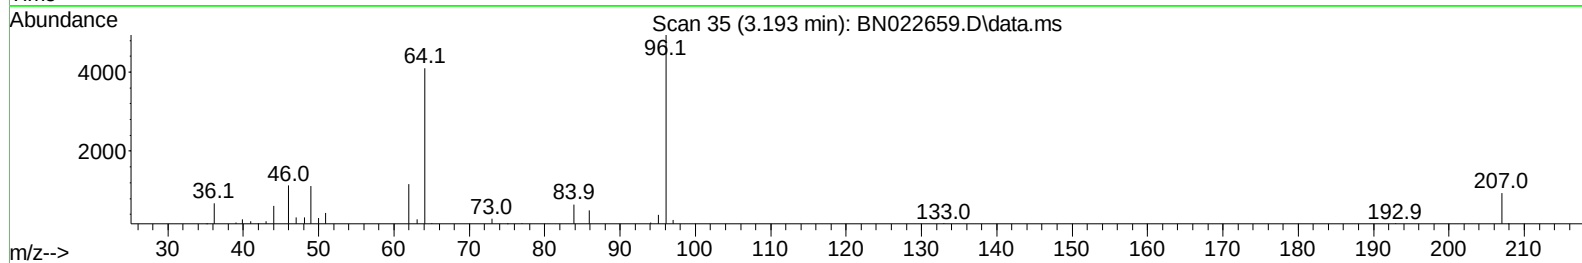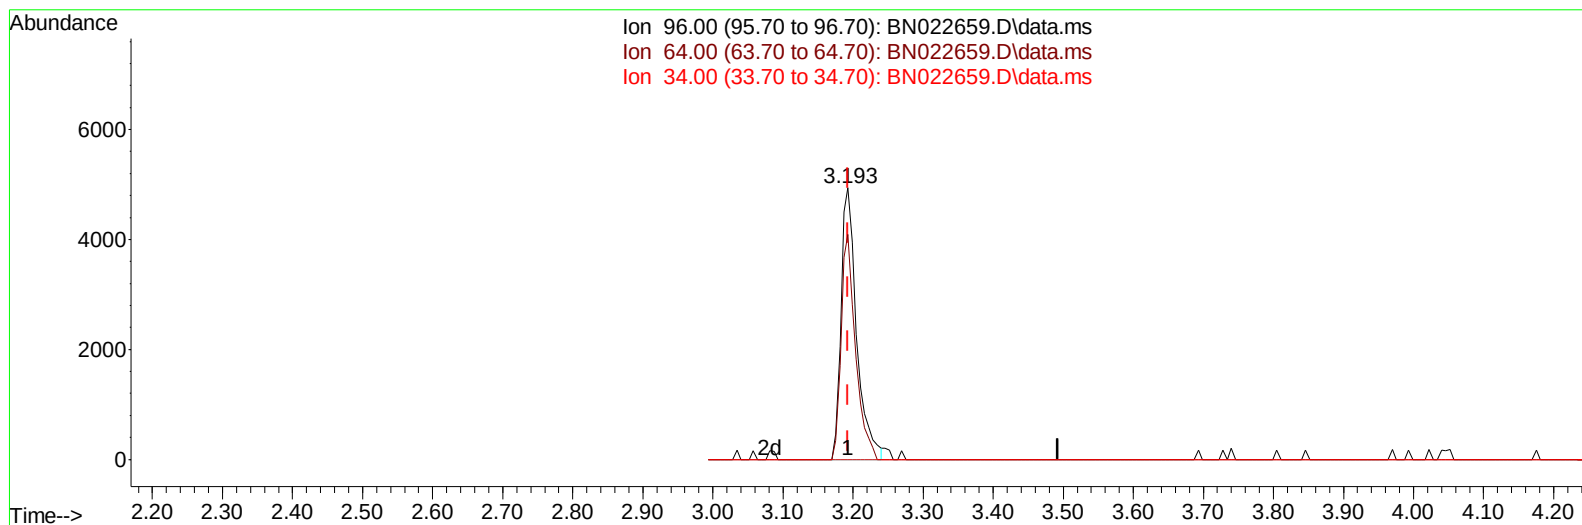

TIC: BN022659.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.193min (-0.000) 4.12 ng/uL

response 7661

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	82.95
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022659.D
 Acq On : 15 Nov 2022 21:17
 Operator : CG/JU
 Sample : N5570-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBMW5

Manual IntegrationsAPPROVED

Quant Time: Nov 15 23:17:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

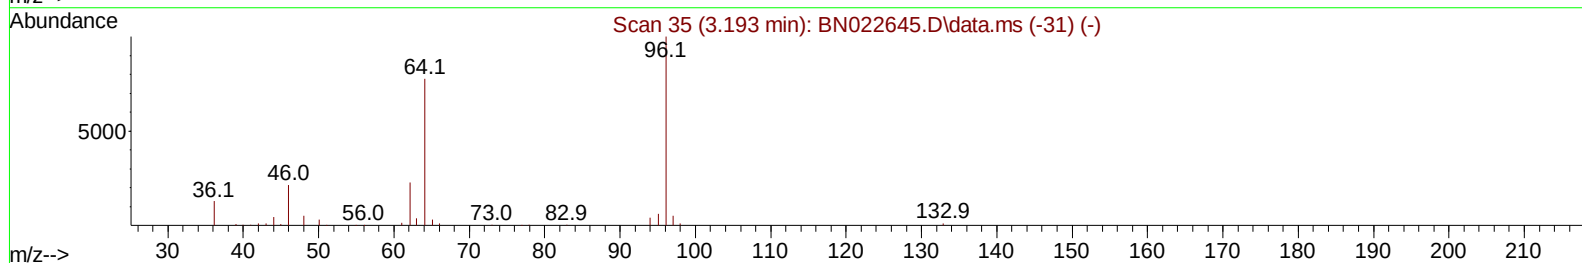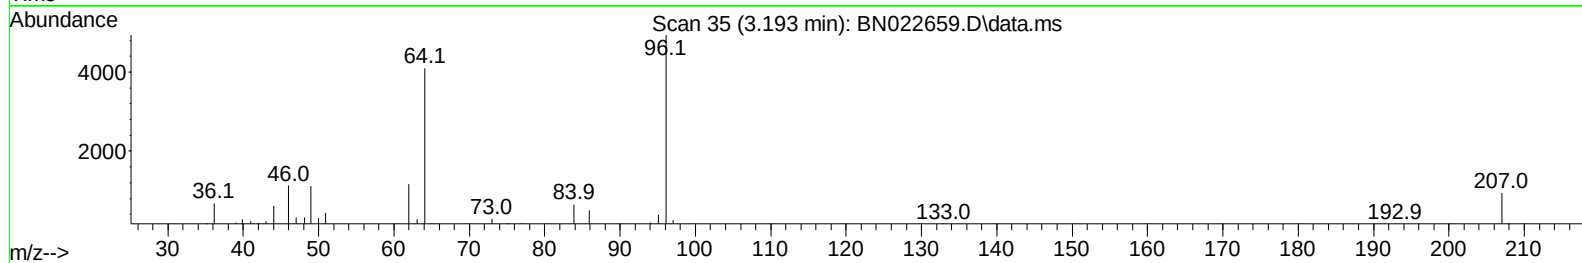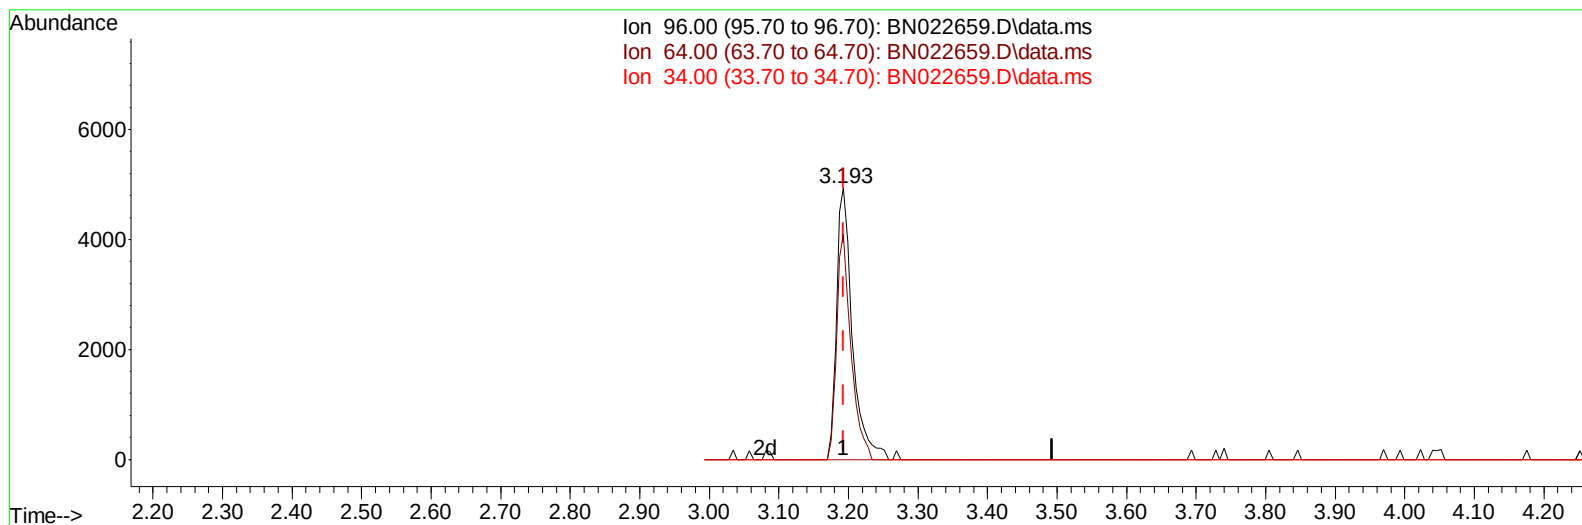

TIC: BN022659.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.193min (-0.000) 4.19 ng/uL m

response 7796

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	82.95
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022659.D
 Acq On : 15 Nov 2022 21:17
 Operator : CG/JU
 Sample : N5570-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBMW5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

Quant Time: Nov 15 23:17:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	63550	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	282662	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	190214	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	392818	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	367428	20.000	ng/ul	0.00
88) Perylene-d12	23.962	264	371749	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	7796m	4.188	ng/uL	0.00
4) Pyridine-d5	3.640	84	26105	4.959	ng/ul	0.01
7) Phenol-d5	7.052	99	37436	6.237	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	107960	29.999	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	100281	22.814	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	69508	14.669	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	67688	30.937	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	71203	29.166	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	115128	27.662	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	130968	20.659	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	452384	32.698	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	479061	31.425	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	14711	5.334	ng/ul	0.00
60) Fluorene-d10	15.557	176	378004	33.312	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	73866	29.584	ng/ul	0.00
73) Anthracene-d10	17.422	188	640321	37.227	ng/ul	0.00
81) Pyrene-d10	19.727	212	694006	36.447	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.804	264	669115	35.806	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022659.D
Acq On : 15 Nov 2022 21:17
Operator : CG/JU
Sample : N5570-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBMW5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/16/2022
Supervised By :mohammad ahmed 11/16/2022

Quant Time: Nov 15 23:17:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

