




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022662.D
 Acq On : 15 Nov 2022 23:07
 Operator : CG/JU
 Sample : N5570-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBMW3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:01:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

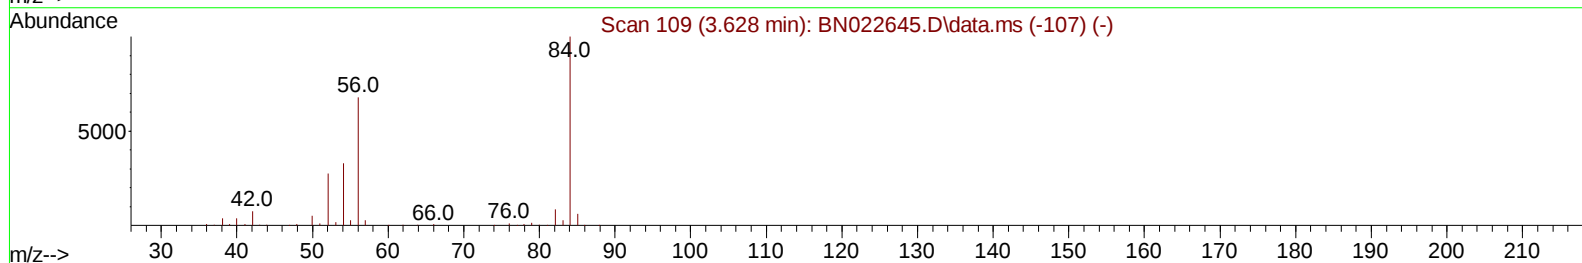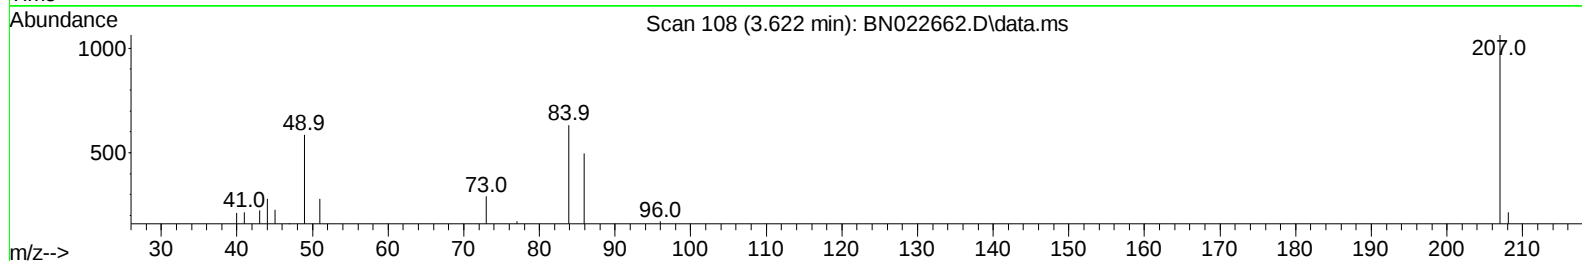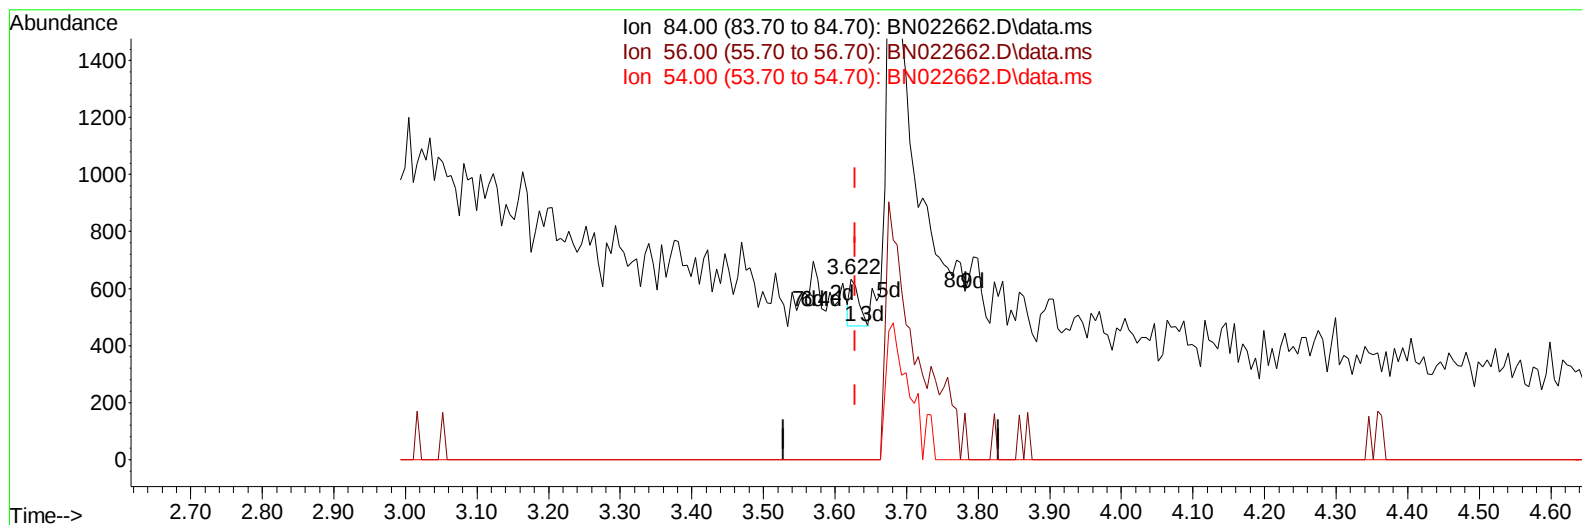

TIC: BN022662.D\data.ms

(4) Pyridine-d5 (S)

3.622min (-0.006) 0.03 ng/u1

response 147

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	0.00#
54.00	31.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022662.D
 Acq On : 15 Nov 2022 23:07
 Operator : CG/JU
 Sample : N5570-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBMW3

Manual IntegrationsAPPROVED

Quant Time: Nov 16 00:01:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

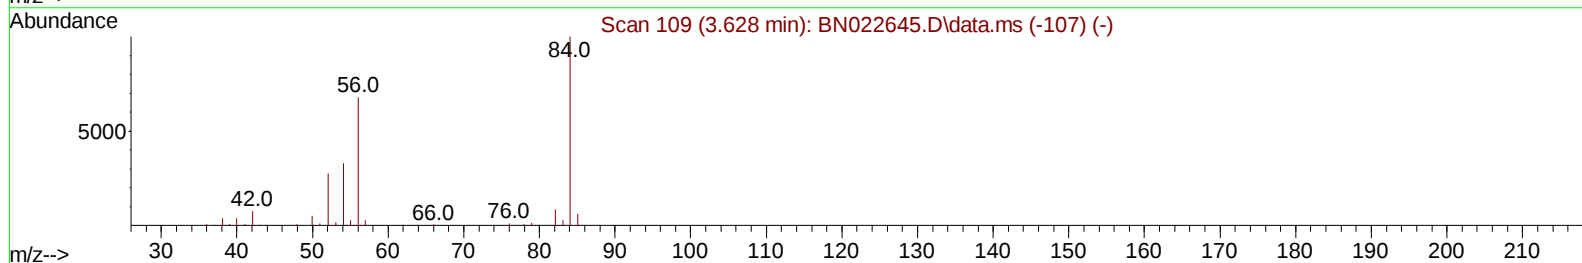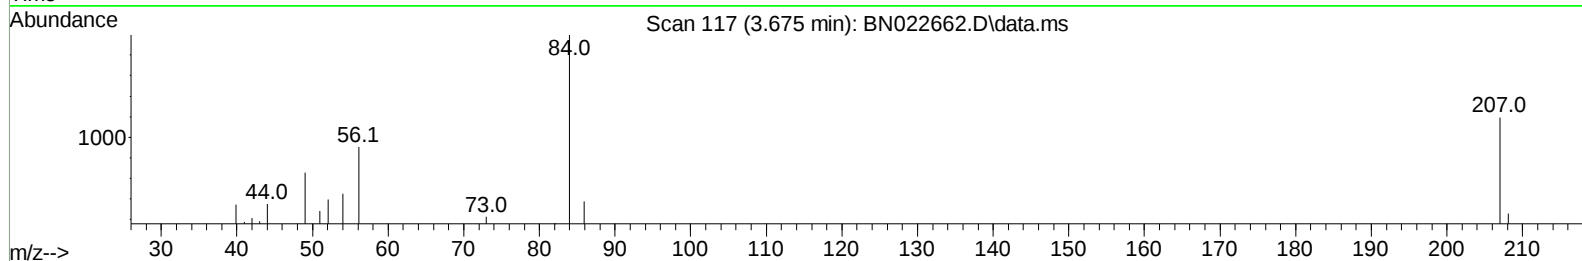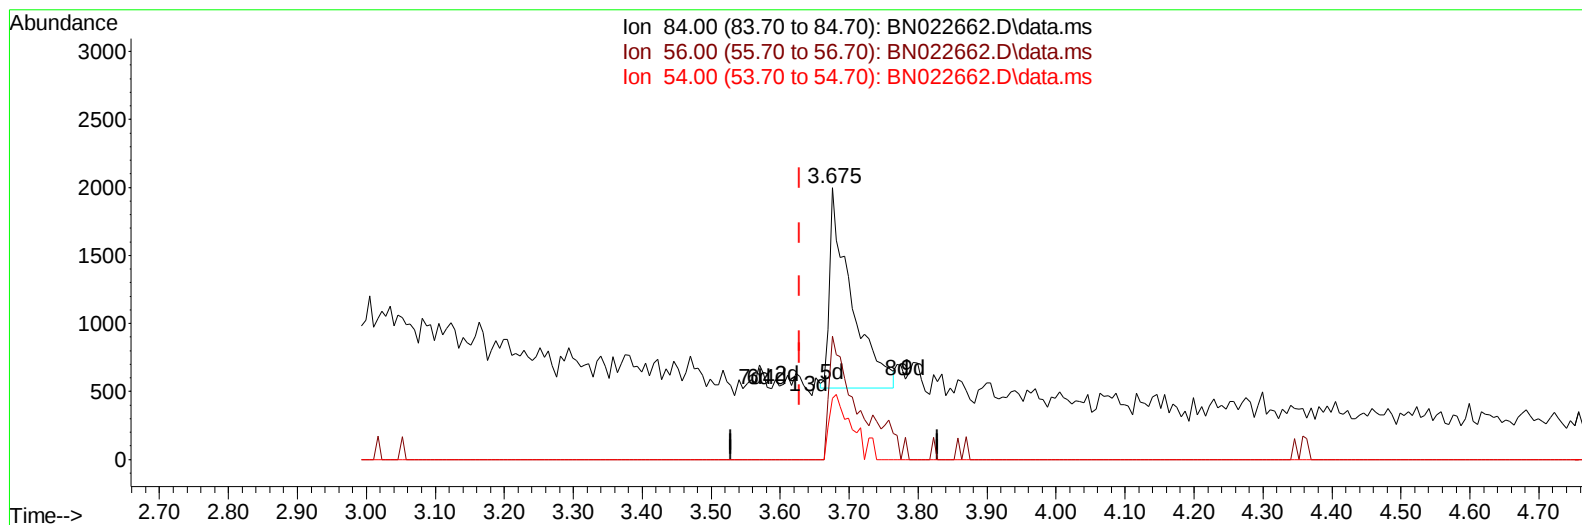

TIC: BN022662.D\data.ms

(4) Pyridine-d5 (S)

3.675min (+ 0.047) 0.55 ng/u1 m

response 3193

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	66.30	45.29#
54.00	31.90	22.60#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022662.D
 Acq On : 15 Nov 2022 23:07
 Operator : CG/JU
 Sample : N5570-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBMW3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

Quant Time: Nov 16 00:01:28 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	69685	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	304372	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	198739	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.316	188	416261	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	392936	20.000	ng/ul	0.00
88) Perylene-d12	23.957	264	362185	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	7258	3.556	ng/uL	0.00
4) Pyridine-d5	3.675	84	3193m	0.553	ng/ul	0.05
7) Phenol-d5	7.052	99	26271	3.992	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	59926	15.186	ng/ul	0.00
11) 2-Chlorophenol-d4	7.405	132	60125	12.474	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	44813	8.625	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	35874	15.227	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	36041	13.710	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165	63352	14.136	ng/ul	0.00
31) 4-Chloroaniline-d4	10.857	131	24170	3.541	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	240696	16.651	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	241619	15.170	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	10639	3.692	ng/ul	0.00
60) Fluorene-d10	15.557	176	203440	17.160	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	33126	12.520	ng/ul	0.00
73) Anthracene-d10	17.416	188	332894	18.264	ng/ul	0.00
81) Pyrene-d10	19.722	212	380502	18.686	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.798	264	337838	18.556	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.081	94	7508	1.095	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022662.D
Acq On : 15 Nov 2022 23:07
Operator : CG/JU
Sample : N5570-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBMW3

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/16/2022
Supervised By :mohammad ahmed 11/16/2022

Quant Time: Nov 16 00:01:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

