




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022669.D
 Acq On : 16 Nov 2022 03:23
 Operator : CG/JU
 Sample : N5577-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9840

Manual IntegrationsAPPROVED

Quant Time: Nov 16 04:05:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

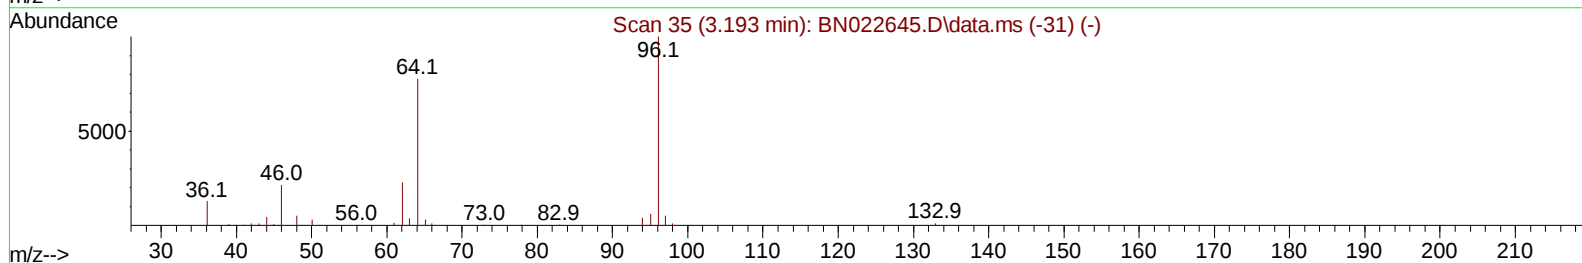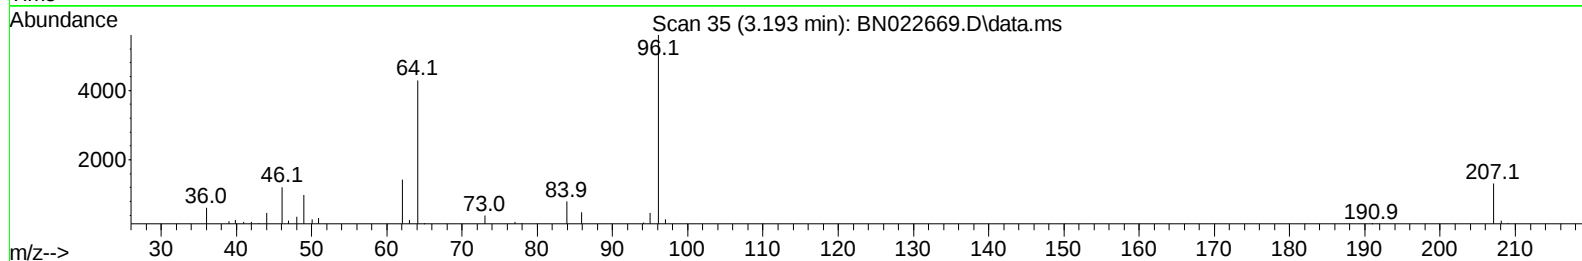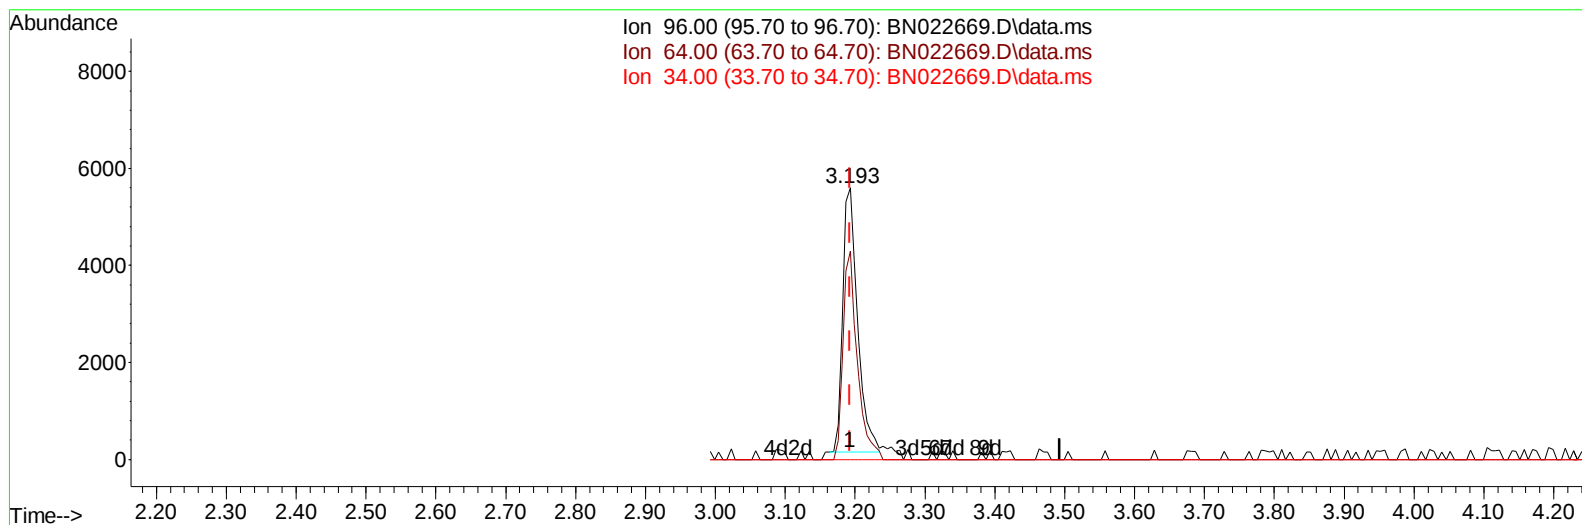

TIC: BN022669.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.193min (+ 0.000) 3.72 ng/uL

response 7963

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	76.76
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022669.D
 Acq On : 16 Nov 2022 03:23
 Operator : CG/JU
 Sample : N5577-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9840

Manual IntegrationsAPPROVED

Quant Time: Nov 16 04:05:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

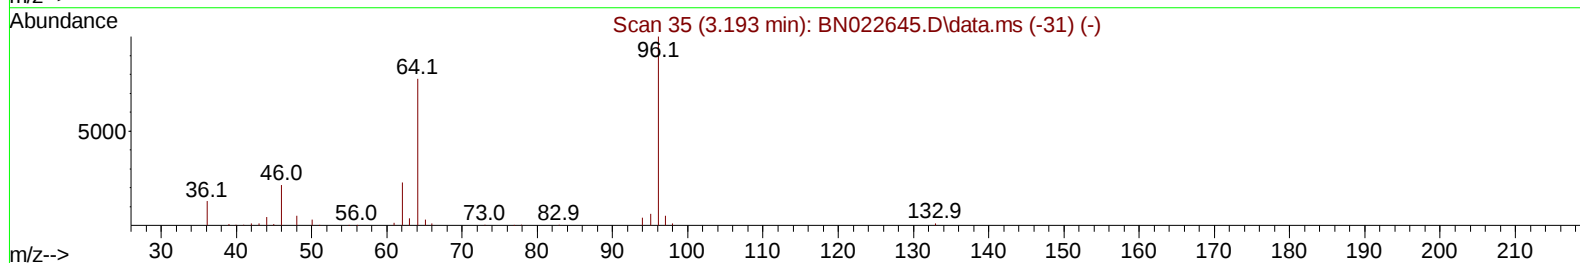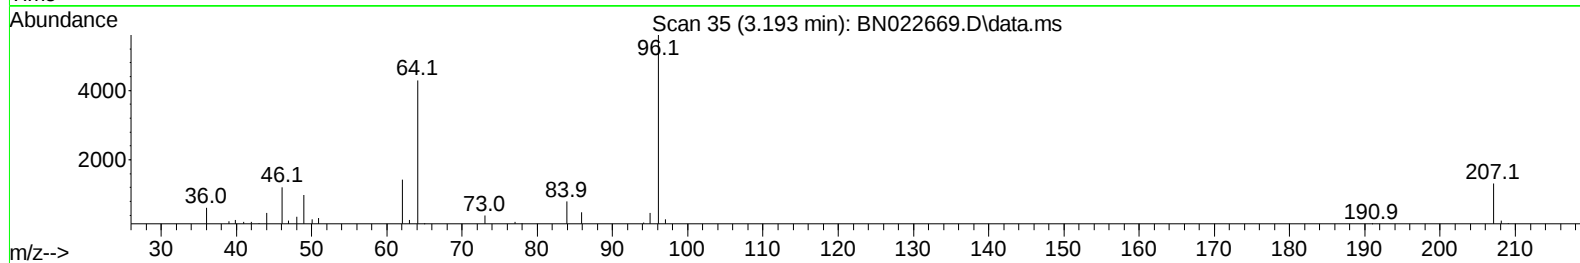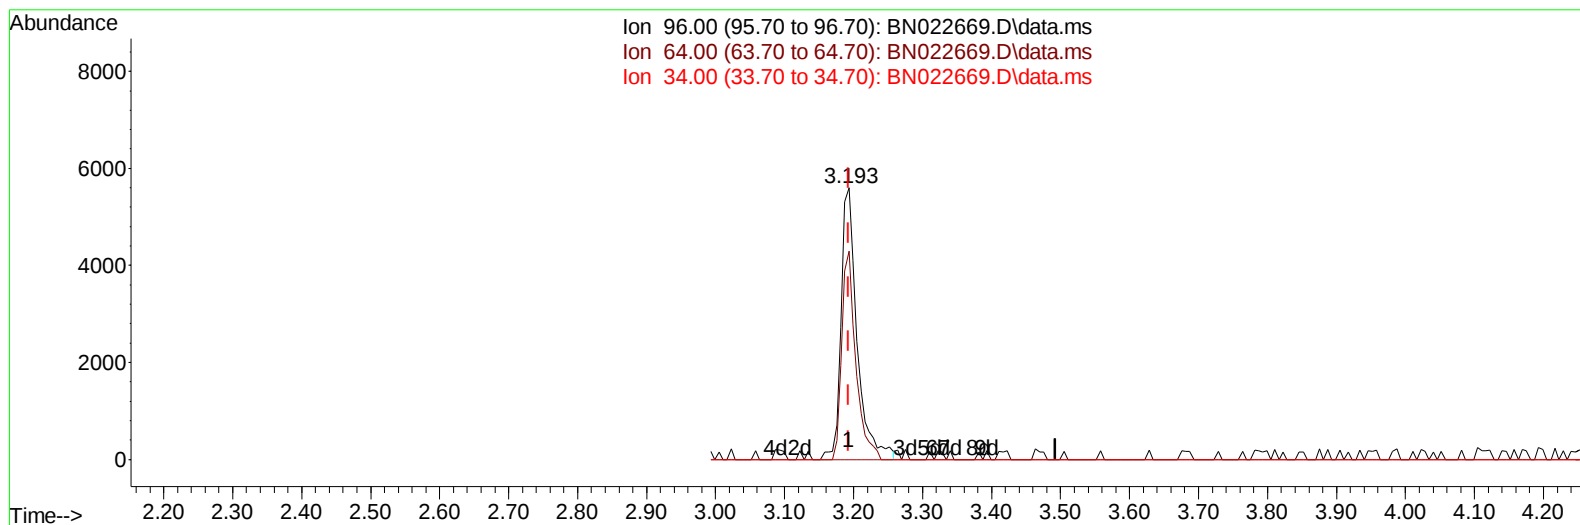

TIC: BN022669.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.193min (+ 0.000) 4.24 ng/uL m

response 9061

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	76.76
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022669.D
 Acq On : 16 Nov 2022 03:23
 Operator : CG/JU
 Sample : N5577-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9840

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

Quant Time: Nov 16 04:05:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	73026	20.000	ng/ul	0.00
20) Naphthalene-d8	10.699	136	321439	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	209462	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	434071	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	424211	20.000	ng/ul	0.00
88) Perylene-d12	23.963	264	398632	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	9061m	4.236	ng/uL	0.00
4) Pyridine-d5	3.658	84	8258	1.365	ng/ul	0.03
7) Phenol-d5	7.046	99	146341	21.218	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	93410	22.588	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	110244	21.826	ng/ul	0.00
15) 4-Methylphenol-d8	8.605	113	121552	22.323	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	55923	22.476	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	62634	22.561	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	103065	21.776	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	142339	19.744	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	368185	24.166	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	374610	22.316	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	54563	17.965	ng/ul	0.00
60) Fluorene-d10	15.557	176	304347	24.357	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	41439	15.019	ng/ul	0.00
73) Anthracene-d10	17.416	188	461061	24.257	ng/ul	0.00
81) Pyrene-d10	19.727	212	510322	23.213	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.798	264	476891	23.798	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022669.D
Acq On : 16 Nov 2022 03:23
Operator : CG/JU
Sample : N5577-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9840

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/16/2022
Supervised By :mohammad ahmed 11/16/2022

Quant Time: Nov 16 04:05:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

