




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022675.D
 Acq On : 16 Nov 2022 07:39
 Operator : CG/JU
 Sample : N5577-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9835

Manual IntegrationsAPPROVED

Quant Time: Nov 16 08:08:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

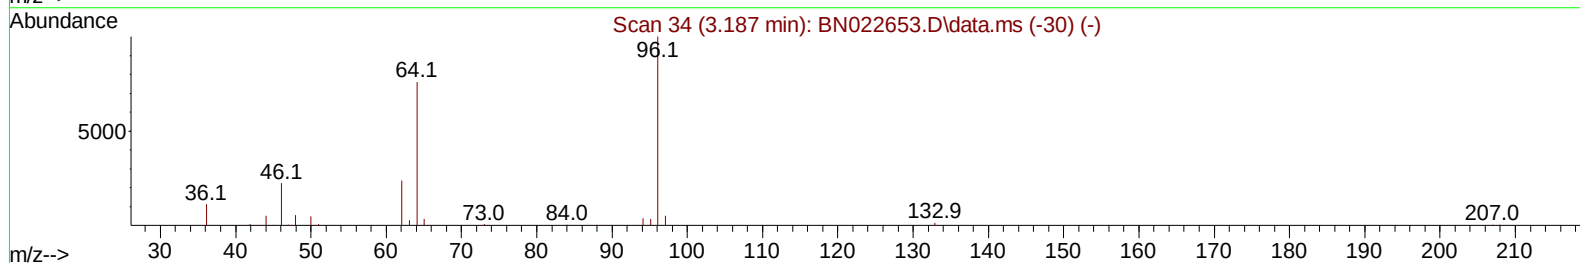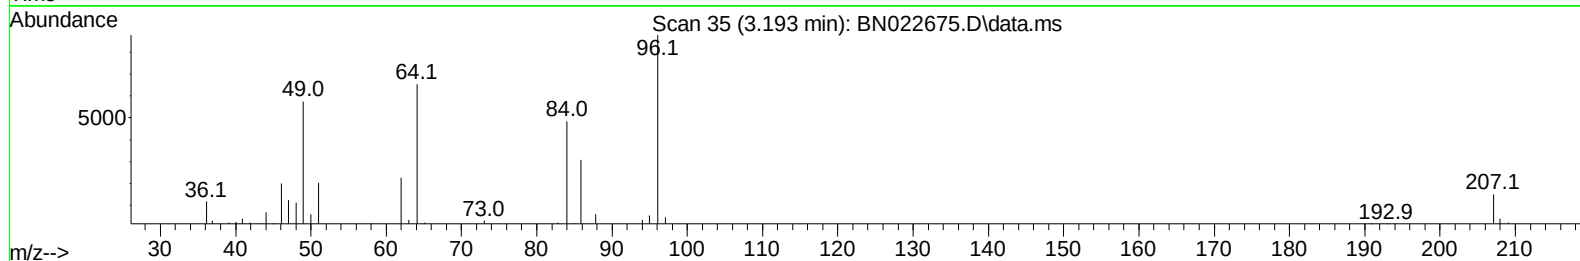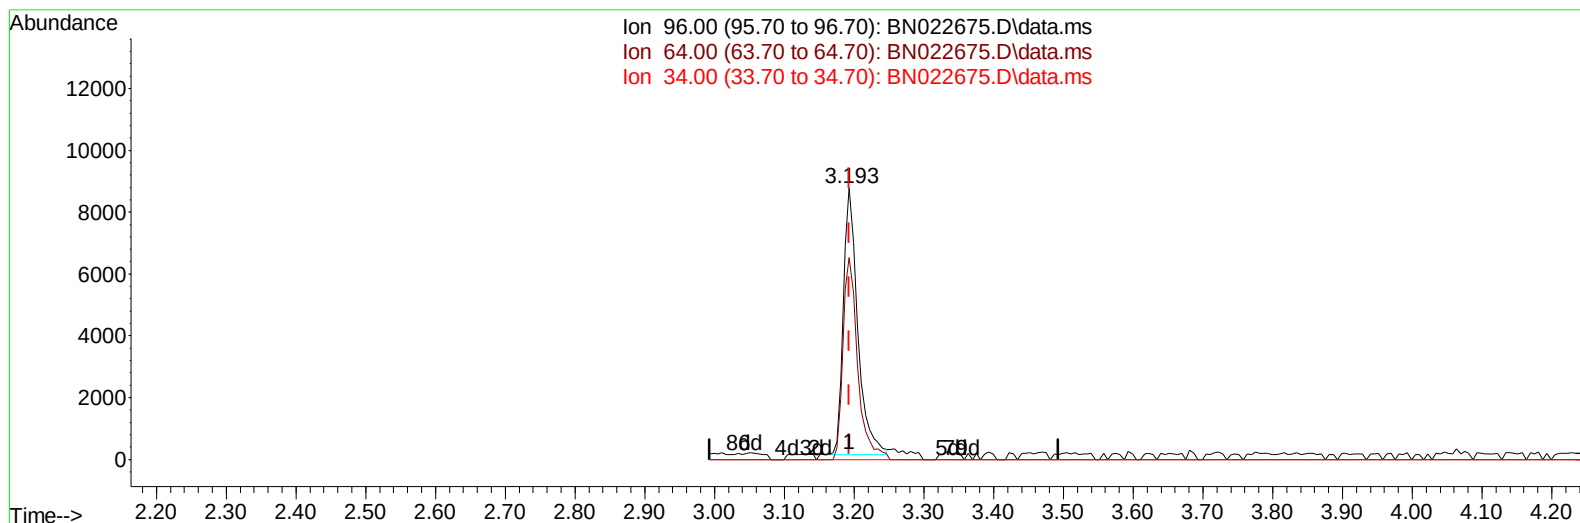

TIC: BN022675.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.193min (-0.000) 5.12 ng/uL

response 12314

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	74.46
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022675.D
 Acq On : 16 Nov 2022 07:39
 Operator : CG/JU
 Sample : N5577-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9835

Manual IntegrationsAPPROVED

Quant Time: Nov 16 08:08:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

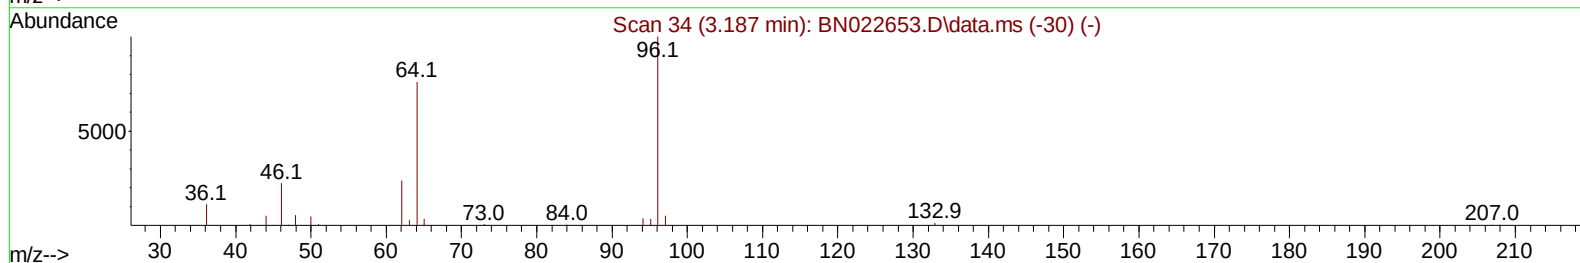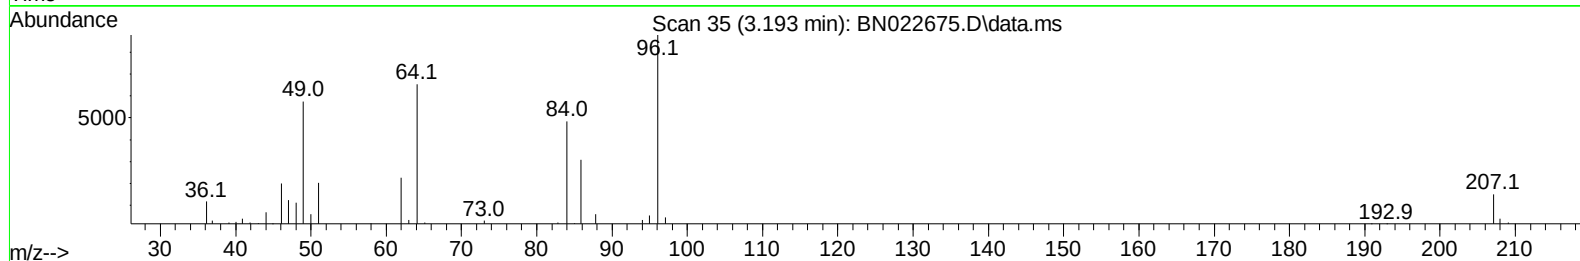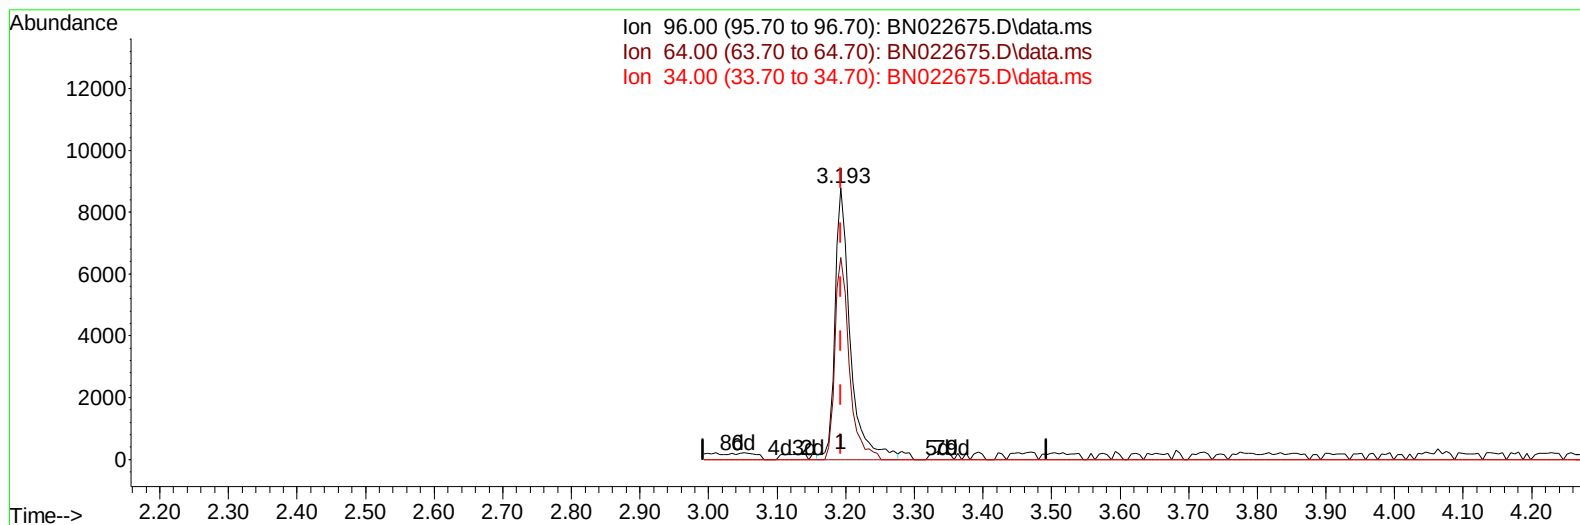

TIC: BN022675.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.193min (-0.000) 5.67 ng/uL m

response 13635

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	77.50	74.46
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022675.D
 Acq On : 16 Nov 2022 07:39
 Operator : CG/JU
 Sample : N5577-11
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9835

Manual IntegrationsAPPROVED

Quant Time: Nov 16 08:08:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 11/16/2022
 Supervised By :mohammad ahmed 11/16/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	82056	20.000	ng/ul	0.00
20) Naphthalene-d8	10.698	136	357293	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.557	164	230627	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.322	188	467182	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	438013	20.000	ng/ul	0.00
88) Perylene-d12	23.962	264	393384	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	13635m	5.673	ng/uL	0.00
4) Pyridine-d5	3.640	84	32342	4.758	ng/ul	0.01
7) Phenol-d5	7.046	99	220644	28.470	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.204	67	136762	29.432	ng/ul	0.00
11) 2-Chlorophenol-d4	7.399	132	168635	29.712	ng/ul	0.00
15) 4-Methylphenol-d8	8.604	113	174316	28.491	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128	85507	30.918	ng/ul	0.00
24) 2-Nitrophenol-d4	9.781	143	94219	30.532	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	156579	29.764	ng/ul	0.00
31) 4-Chloroaniline-d4	10.851	131	213429	26.634	ng/ul	0.00
46) Dimethylphthalate-d6	13.975	166	535451	31.920	ng/ul	0.00
49) Acenaphthylene-d8	14.251	160	564030	30.516	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	79227	23.692	ng/ul	0.00
60) Fluorene-d10	15.557	176	432959	31.469	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.686	200	55487	18.686	ng/ul	0.00
73) Anthracene-d10	17.422	188	682211	33.349	ng/ul	0.00
81) Pyrene-d10	19.727	212	743046	32.734	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.798	264	631321	31.925	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022675.D
Acq On : 16 Nov 2022 07:39
Operator : CG/JU
Sample : N5577-11
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9835

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 11/16/2022
Supervised By :mohammad ahmed 11/16/2022

Quant Time: Nov 16 08:08:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

