

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022657.D
 Acq On : 15 Nov 2022 20:04
 Operator : CG/JU
 Sample : N5570-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 GBMW1

Quant Time: Nov 15 23:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	92441	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	396494	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.563	164	244108	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	425688	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	308481	20.000	ng/ul	0.00
88) Perylene-d12	23.962	264	291303	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	9462	3.495	ng/uL	0.00
4) Pyridine-d5	3.658	84	18821	2.458	ng/ul	0.03
7) Phenol-d5	7.052	99	37906	4.342	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	92942	17.755	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	94540	14.786	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	68461	9.932	ng/ul	0.00
21) Nitrobenzene-d5	9.057	128				

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022657.D
Acq On : 15 Nov 2022 20:04
Operator : CG/JU
Sample : N5570-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
GBMW1

Quant Time: Nov 15 23:17:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration




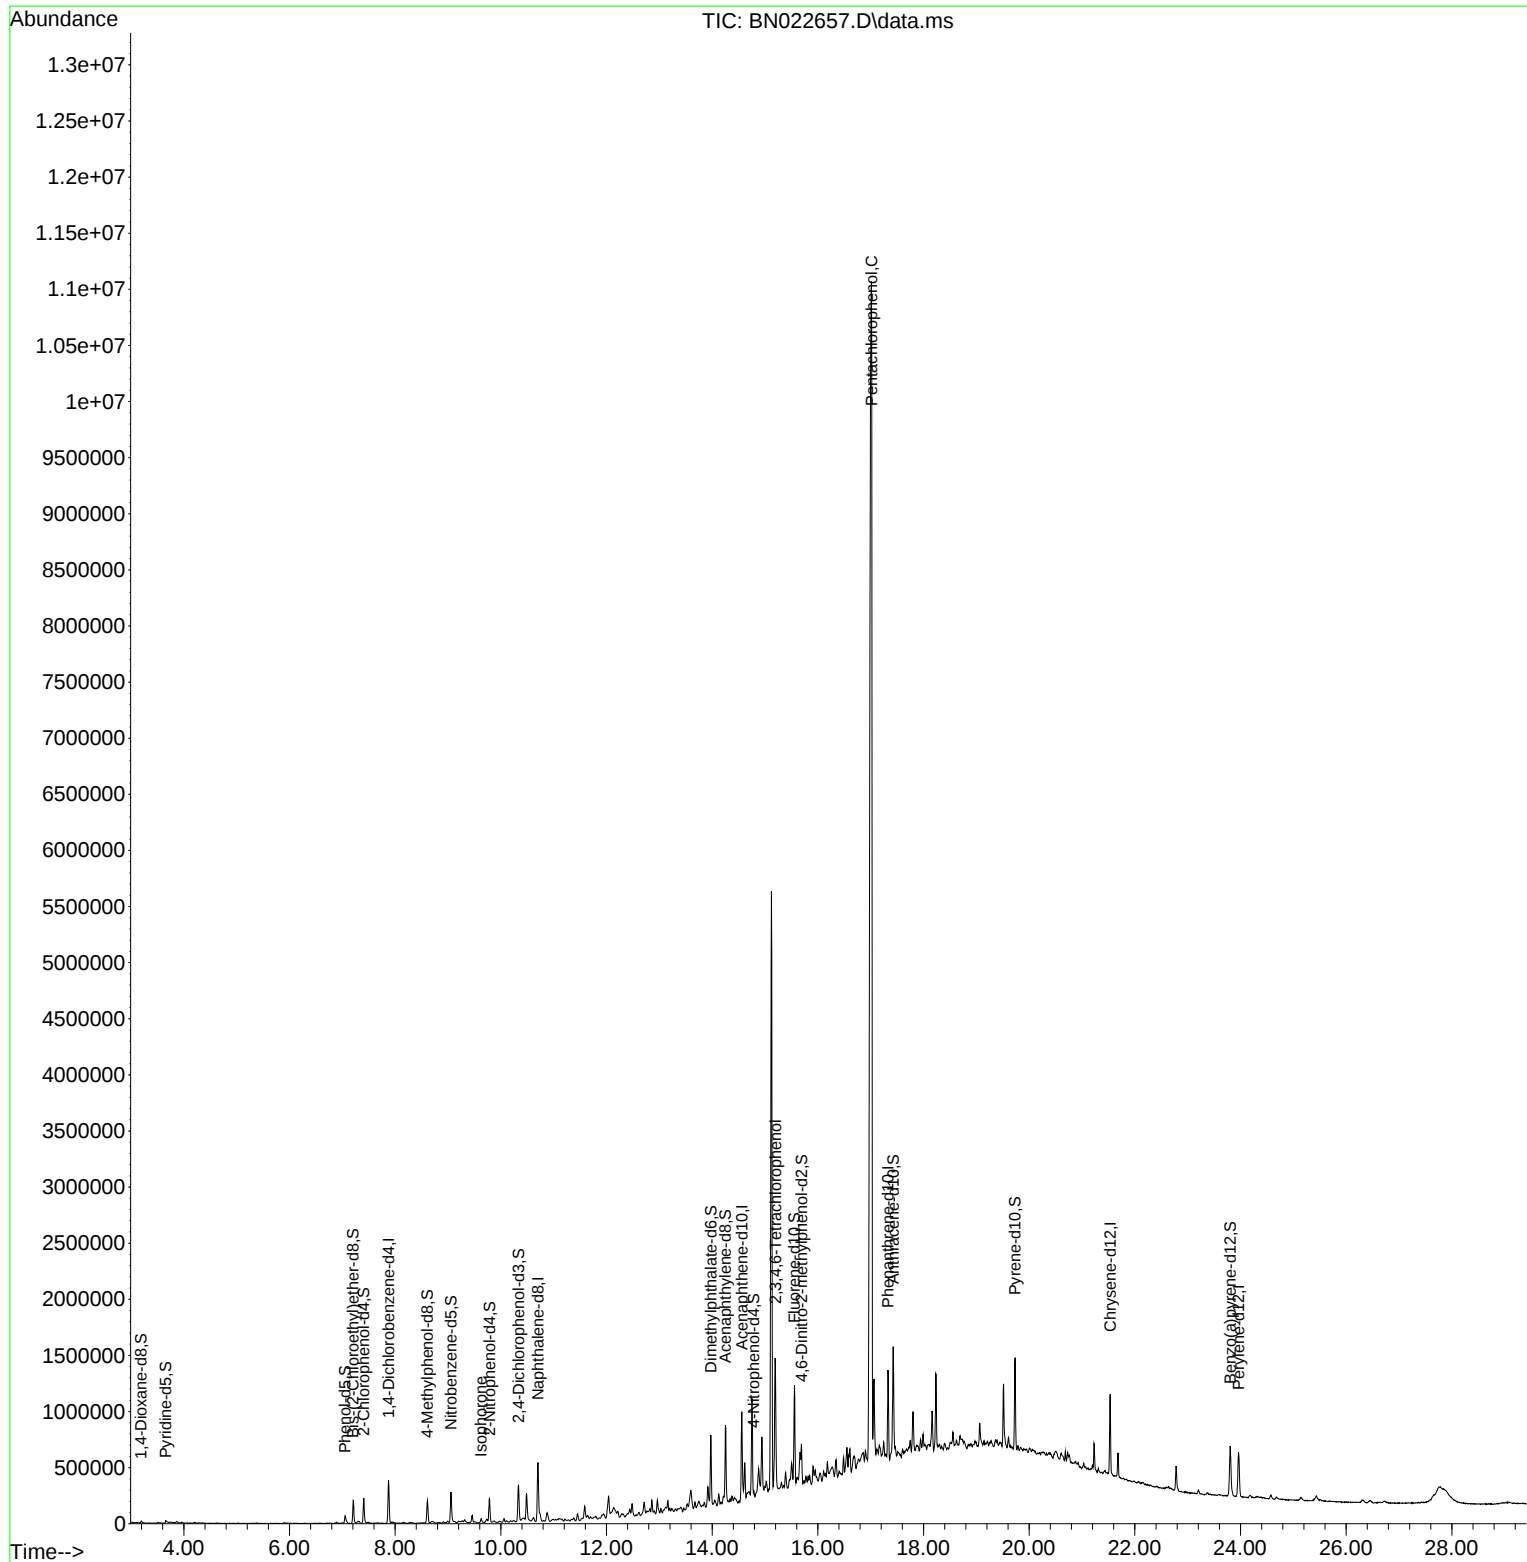


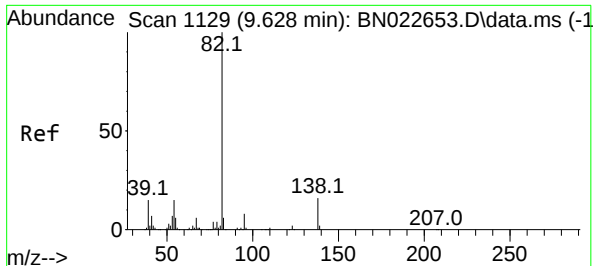

#23
Isophorone
Concen: 1.438 ng/ul
RT: 9.628 min Scan# 1129
Delta R.T. -0.006 min
Lab File: BN022657.D
Acq: 15 Nov 2022 20:04




Instrument :
BNA_N
ClientSampleId :
GBMW1


Tgt Ion: 82 Resp: 22869
Ion Ratio Lower Upper
82 100
95 10.8 6.3 9.5#
138 14.3 12.8 19.2

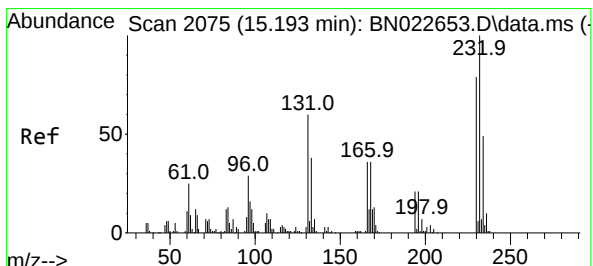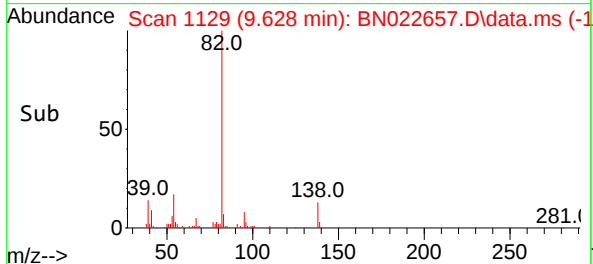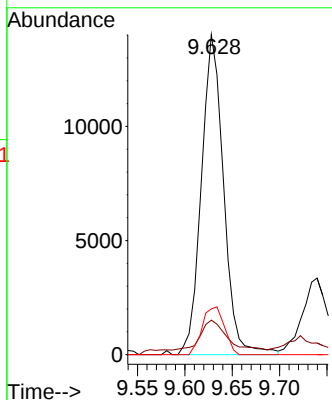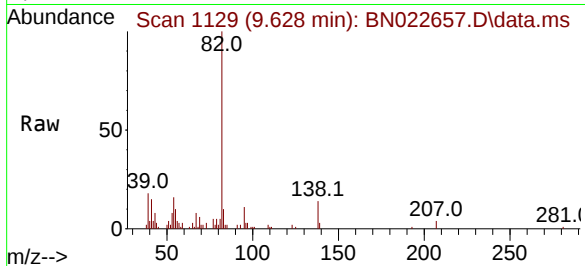

#58
2,3,4,6-Tetrachlorophenol
Concen: 29.680 ng/ul
RT: 15.198 min Scan# 2076
Delta R.T. 0.006 min
Lab File: BN022657.D
Acq: 15 Nov 2022 20:04

Tgt Ion: 232 Resp: 125227
Ion Ratio Lower Upper
232 100
131 60.2 47.4 71.0
130 4.9 2.6 3.8#
166 38.7 29.2 43.8

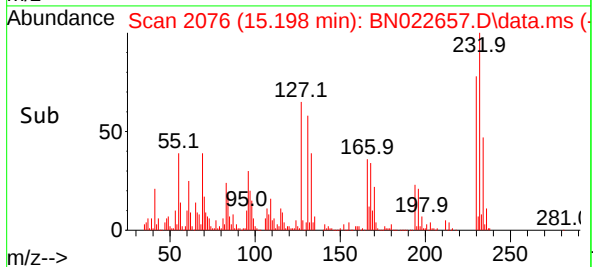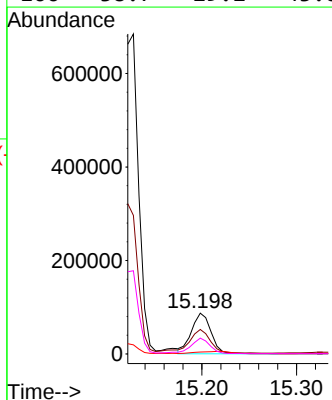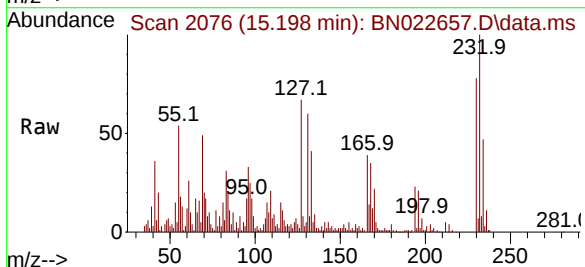

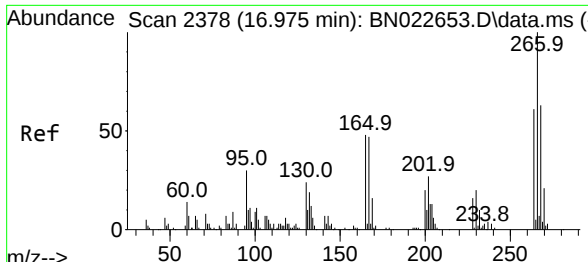

#71
 Pentachlorophenol
 Concen: 1410.695 ng/ul
 RT: 17.016 min Scan# 21
 Delta R.T. 0.047 min
 Lab File: BN022657.D
 Acq: 15 Nov 2022 20:04

Instrument :
 BNA_N
 ClientSampleId :
 GBMW1

Tgt Ion:266 Resp: 4392052
 Ion Ratio Lower Upper
 266 100
 264 58.4 47.8 71.8
 268 55.8 50.2 75.2

