

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022674.D
 Acq On : 16 Nov 2022 07:03
 Operator : CG/JU
 Sample : N5577-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C9831

Quant Time: Nov 16 08:04:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Nov 15 22:53:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	79232	20.000	ng/u1	0.00
20) Naphthalene-d8	10.699	136	350491	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.557	164	230572	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.322	188	478394	20.000	ng/u1	0.00
79) Chrysene-d12	21.527	240	441443	20.000	ng/u1	0.00
88) Perylene-d12	23.963	264	423344	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	8584	3.699	ng/uL	0.00
4) Pyridine-d5	3.640	84	37979	5.787	ng/u1	0.01
7) Phenol-d5	7.046	99	144620	19.326	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.205	67	95601	21.307	ng/u1	0.00
11) 2-Chlorophenol-d4	7.405	132	110055	20.082	ng/u1	0.00
15) 4-Methylphenol-d8	8.605	113	119660	20.255	ng/u1	0.00
21) Nitrobenzene-d5	9.057	128	57620	21.239	ng/u1	0.00
24) 2-Nitrophenol-d4	9.781	143	64516	21.313	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	105492	20.442	ng/u1	0.00
31) 4-Chloroaniline-d4	10.852	131	144644	18.401	ng/u1	0.00
46) Dimethylphthalate-d6	13.975	166	403506	24.060	ng/u1	0.00
49) Acenaphthylene-d8	14.251	160	396048	21.433	ng/u1	0.00
54) 4-Nitrophenol-d4	14.793	143	60804	18.187	ng/u1	0.00
60) Fluorene-d10	15.557	176	323532	23.521	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.687	200	44933	14.777	ng/u1	0.00
73) Anthracene-d10	17.416	188	492840	23.527	ng/u1	0.00
81) Pyrene-d10	19.728	212	528102	23.084	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.798	264	467162	21.952	ng/u1	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.016	77	4405	1.163	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022674.D
Acq On : 16 Nov 2022 07:03
Operator : CG/JU
Sample : N5577-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C9831

Quant Time: Nov 16 08:04:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Nov 15 22:53:43 2022
Response via : Initial Calibration

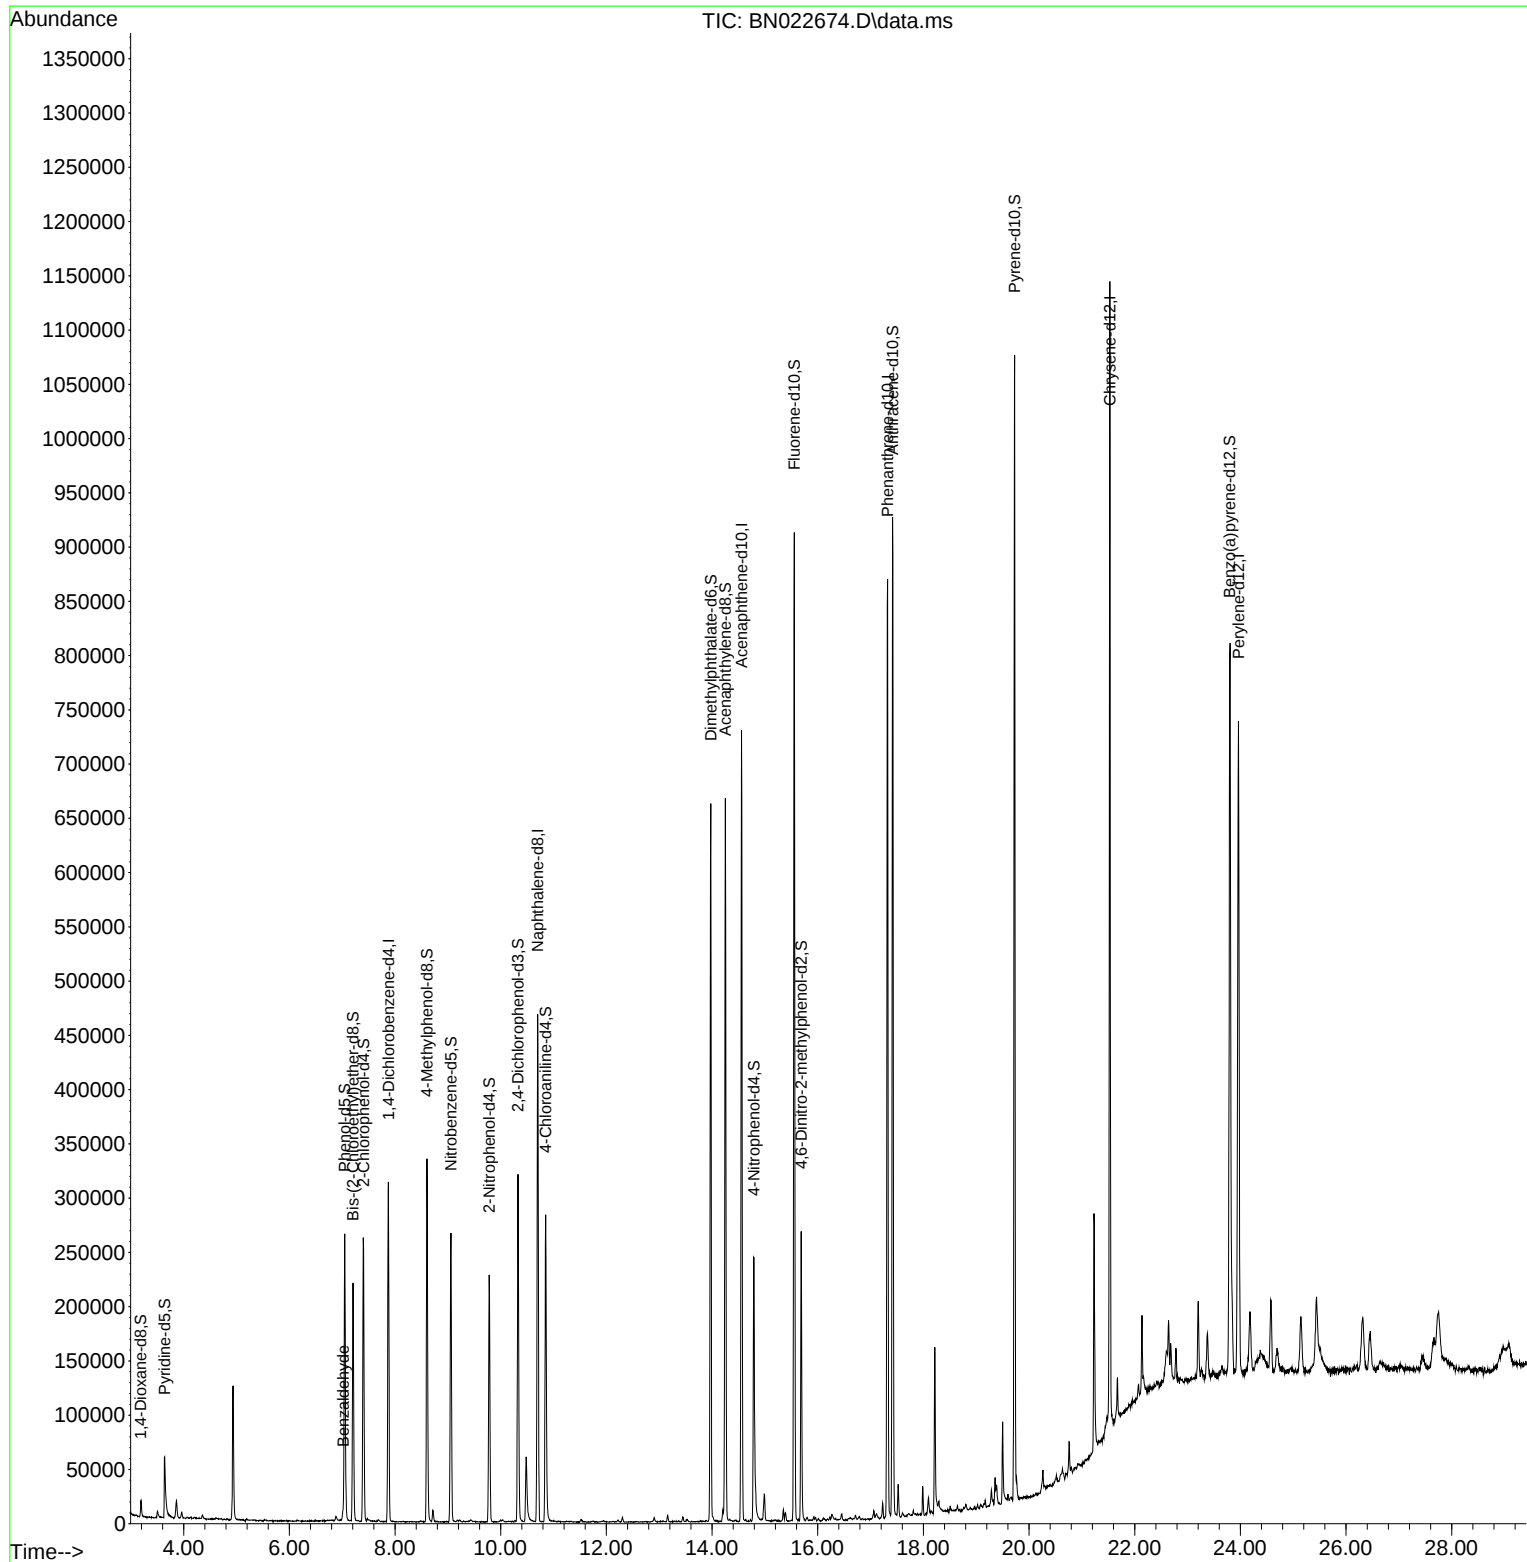

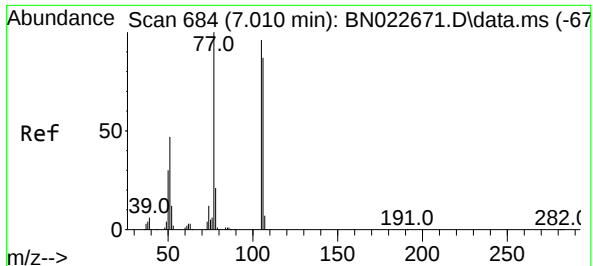

#6
Benzaldehyde
Concen: 1.163 ng/ul
RT: 7.016 min Scan# 685
Delta R.T. 0.006 min
Lab File: BN022674.D
Acq: 16 Nov 2022 07:03

Instrument :
BNA_N
ClientSampleId :
C9831

Tgt Ion: 77 Resp: 4405
Ion Ratio Lower Upper
77 100
105 96.3 75.2 112.8
106 87.1 69.0 103.6

