

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022650.D
 Acq On : 15 Nov 2022 14:43
 Operator : CG/JU
 Sample : PB149003BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK003

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	45	rVB	21659	33175	1.63%	0.158%
2	3.628	106	109	132	rBV	238302	399008	19.63%	1.900%
3	3.958	161	165	172	rVB	4768	7323	0.36%	0.035%
4	7.052	684	691	710	rVB	326510	518873	25.53%	2.471%
5	7.205	711	717	729	rVB	244745	393962	19.38%	1.876%
6	7.405	744	751	765	rBV	319212	509897	25.08%	2.428%
7	7.875	824	831	842	rVB	264318	418946	20.61%	1.995%
8	8.611	949	956	967	rBV	385930	631833	31.08%	3.009%
9	9.058	1023	1032	1045	rBV	313667	508106	25.00%	2.420%
10	9.787	1148	1156	1168	rBV	264237	437355	21.52%	2.083%
11	10.334	1241	1249	1265	rBV	358730	626436	30.82%	2.983%
12	10.705	1302	1312	1319	rBV	367125	623179	30.66%	2.968%
13	10.852	1330	1337	1354	rBV	318094	566785	27.88%	2.699%
14	12.310	1578	1585	1591	rBV3	4185	7791	0.38%	0.037%
15	13.975	1861	1868	1880	rBV	757947	1039916	51.16%	4.952%
16	14.251	1907	1915	1928	rBV	767505	1157267	56.93%	5.511%
17	14.557	1961	1967	1976	rBV	587531	879588	43.27%	4.189%
18	14.793	2001	2007	2024	rBV	343544	564298	27.76%	2.687%
19	15.010	2042	2044	2050	rVB2	1880	2578	0.13%	0.012%
20	15.557	2131	2137	2144	rVV	1066926	1464579	72.05%	6.975%
21	15.687	2153	2159	2173	rVV	394711	557602	27.43%	2.655%
22	15.804	2173	2179	2181	rBV2	2540	3868	0.19%	0.018%
23	17.322	2430	2437	2443	rBV	736655	1070203	52.65%	5.097%
24	17.422	2447	2454	2466	rVV	1135043	1655403	81.44%	7.883%
25	17.698	2497	2501	2502	rBV3	2799	3005	0.15%	0.014%
26	17.939	2539	2542	2552	rVB6	6884	16285	0.80%	0.078%
27	18.216	2585	2589	2594	rBV3	9450	13743	0.68%	0.065%
28	18.292	2598	2602	2608	rBV	6406	8916	0.44%	0.042%
29	19.286	2767	2771	2775	rVB4	12409	17139	0.84%	0.082%
30	19.357	2779	2783	2787	rBV	12130	15954	0.78%	0.076%
31	19.504	2805	2808	2813	rBV6	6205	9416	0.46%	0.045%
32	19.728	2840	2846	2856	rBV	1372243	1875909	92.29%	8.933%
33	21.527	3147	3152	3164	rVB	980257	1245832	61.29%	5.933%
34	22.598	3328	3334	3344	rVB4	151523	431760	21.24%	2.056%
35	23.804	3532	3539	3550	rVB2	1013868	2032709	100.00%	9.680%
36	23.963	3559	3566	3582	rVB2	612912	1249974	61.49%	5.953%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022650.D
Acq On : 15 Nov 2022 14:43
Operator : CG/JU
Sample : PB149003BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK003

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION


Sum of corrected areas: 20998613

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022650.D
Acq On : 15 Nov 2022 14:43
Operator : CG/JU
Sample : PB149003BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

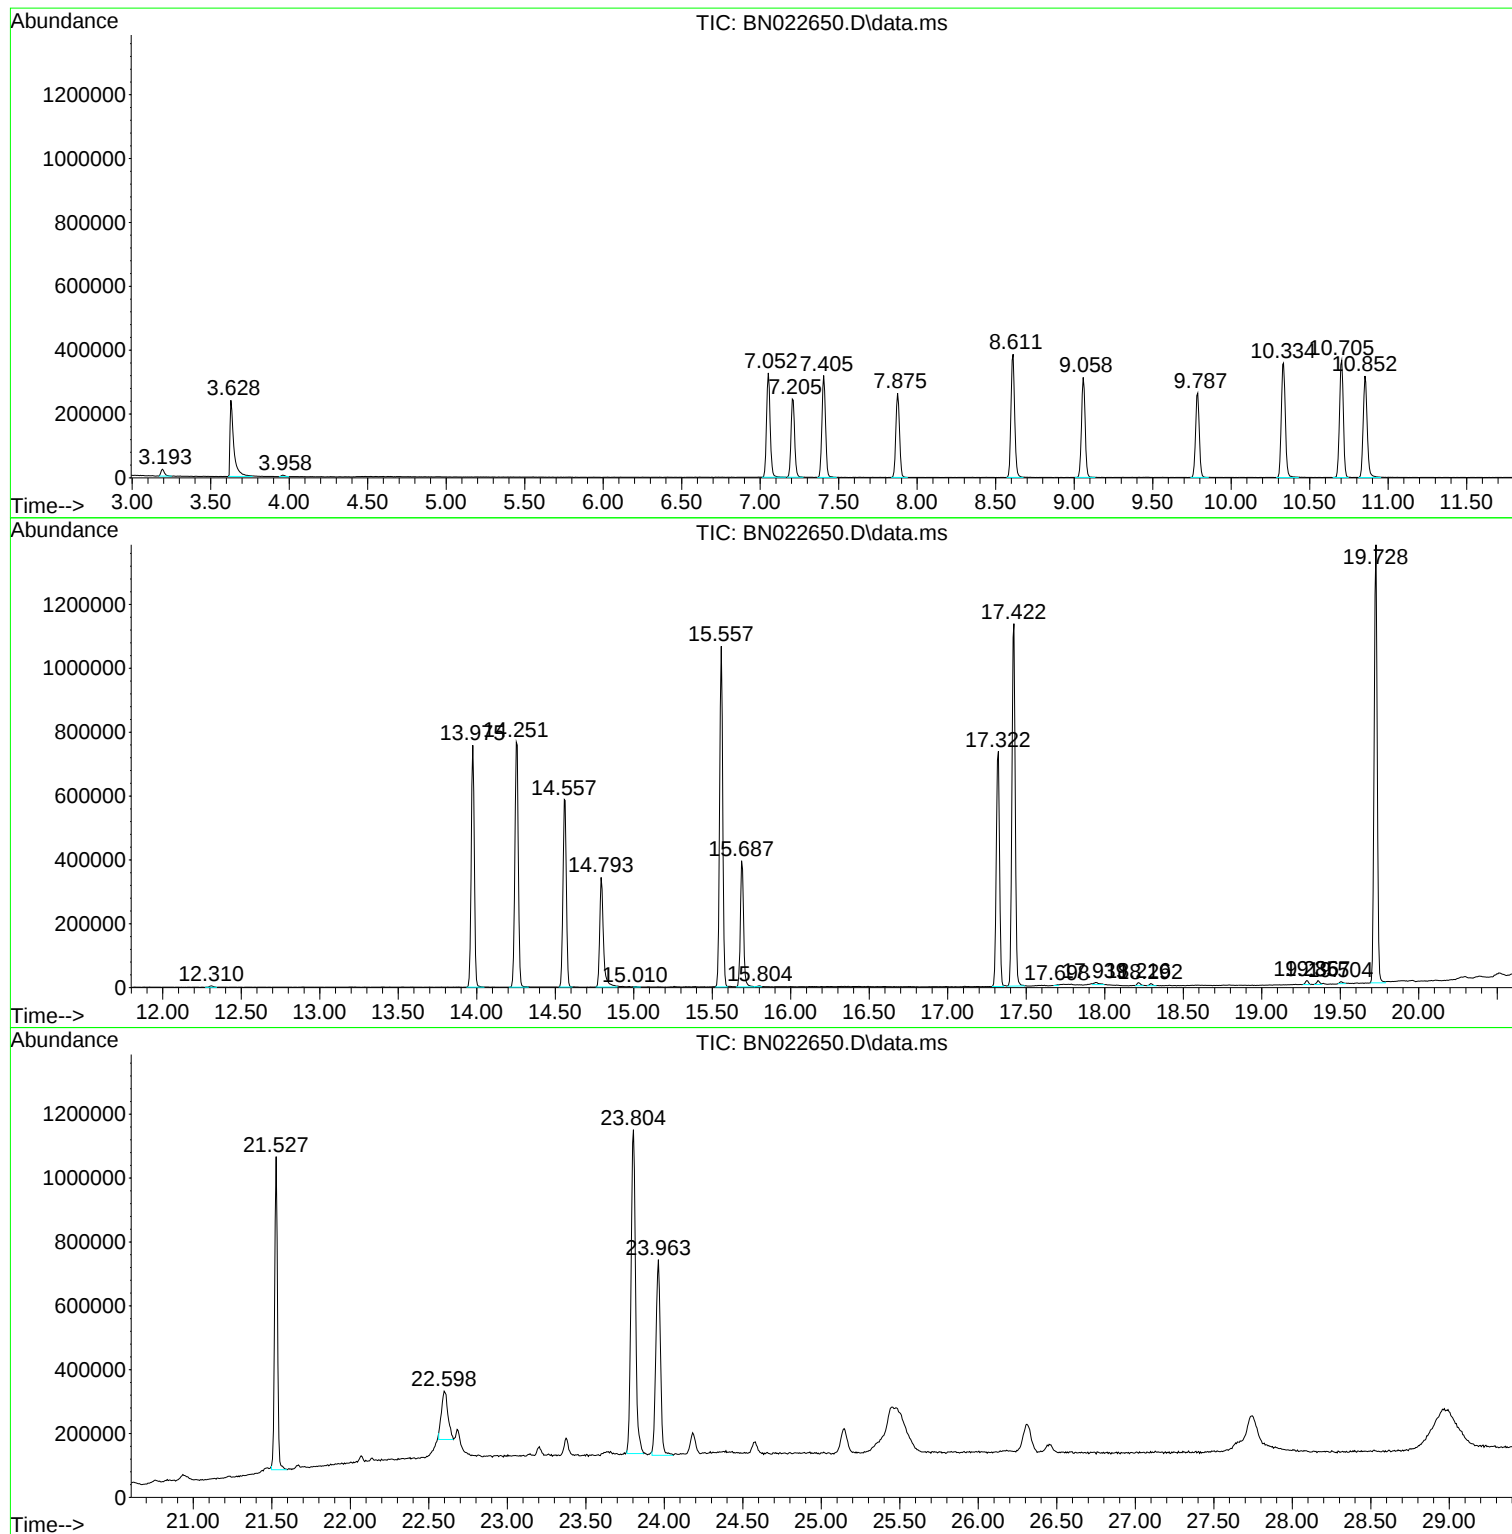

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022650.D
Acq On : 15 Nov 2022 14:43
Operator : CG/JU
Sample : PB149003BL
Misc :
ALS Vial : 9 Sample Multiplier: 1










Instrument :
BNA_N
ClientSampleId :
SBLK003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclononasiloxane, octadeca... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
22.598	6.93 ng/ul	431760	Chrysene-d12		21.528	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Cyclononasiloxane, octadecamethyl-		666	C18H54O9Si9	000556-71-8	58
2	2-Amino-2-oxo-acetic acid, N-[3,...		221	C12H15NO3	024451-17-0	38
3	1,1,1,3,3,5,5,7,7,9,9,11,11,13,1...		606	C18H54O7Si8	000556-69-4	38
4	Hexasiloxane, tetradecamethyl-		458	C14H42O5Si6	000107-52-8	27
5	3-Isopropoxy-1,1,1,7,7,7-hexamet...		576	C18H52O7Si7	071579-69-6	27

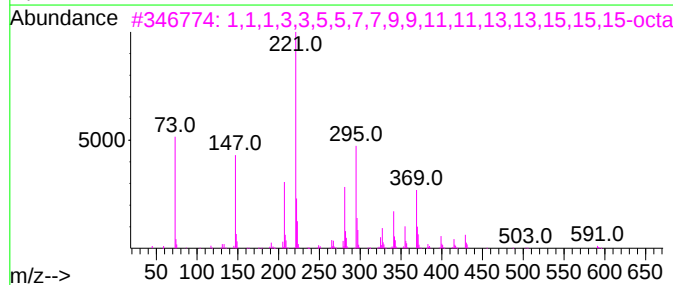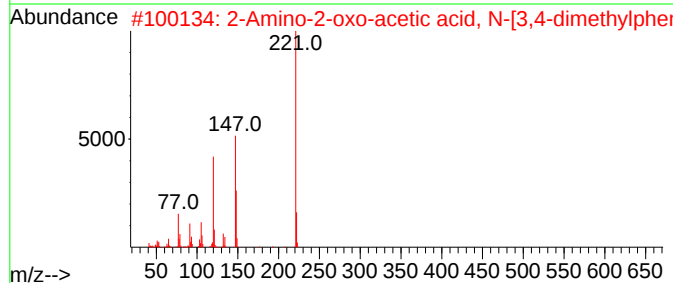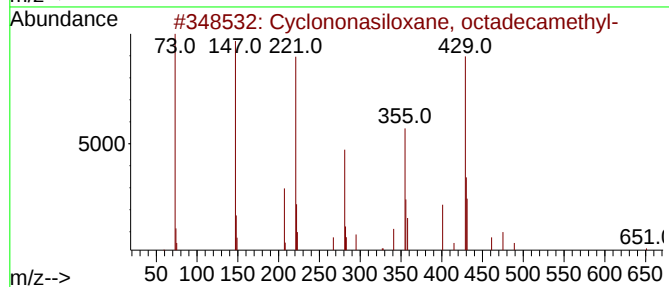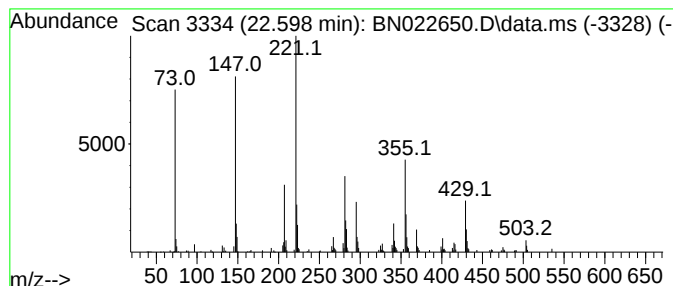

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022650.D
Acq On : 15 Nov 2022 14:43
Operator : CG/JU
Sample : PB149003BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK003

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclononasilo...	22.598	6.9	ng/u1	431760	5	21.528	1245830	20.0