

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
 Data File : BN022655.D
 Acq On : 15 Nov 2022 18:50
 Operator : CG/JU
 Sample : PB149004BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK004

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
 Title : SVOA CALIBRATION

Signal : TIC: BN022655.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	47	rVB	23880	40114	1.91%	0.189%
2	3.628	106	109	131	rBV	242562	407876	19.38%	1.921%
3	3.958	161	165	169	rBV	5497	7920	0.38%	0.037%
4	7.052	684	691	705	rBV	324689	518122	24.62%	2.440%
5	7.205	711	717	729	rVB	248321	397422	18.89%	1.871%
6	7.405	744	751	764	rBV	321604	517336	24.59%	2.436%
7	7.875	825	831	841	rBV	254134	397699	18.90%	1.873%
8	8.611	949	956	971	rBV	379266	628927	29.89%	2.962%
9	9.058	1023	1032	1047	rBV	309955	514130	24.43%	2.421%
10	9.787	1149	1156	1169	rVB	259808	432395	20.55%	2.036%
11	10.328	1242	1248	1270	rBV	348324	617641	29.35%	2.908%
12	10.705	1304	1312	1323	rBV	349963	577008	27.42%	2.717%
13	10.852	1330	1337	1353	rBV	309651	555619	26.41%	2.616%
14	12.310	1579	1585	1593	rBV3	4201	7398	0.35%	0.035%
15	13.975	1861	1868	1880	rBV	760137	1029395	48.92%	4.847%
16	14.251	1909	1915	1923	rBV	762942	1116318	53.05%	5.257%
17	14.563	1961	1968	1975	rBV	532851	806324	38.32%	3.797%
18	14.793	2001	2007	2026	rBV	349599	559376	26.58%	2.634%
19	15.557	2131	2137	2147	rVB	1012235	1420904	67.53%	6.691%
20	15.687	2153	2159	2174	rVB	383880	547819	26.04%	2.580%
21	15.798	2174	2178	2184	rBV4	3012	3996	0.19%	0.019%
22	17.104	2397	2400	2404	rBV3	1662	2879	0.14%	0.014%
23	17.322	2430	2437	2443	rBV	711996	1005654	47.79%	4.736%
24	17.422	2447	2454	2471	rVB	1124797	1646122	78.23%	7.751%
25	17.716	2501	2504	2505	rBV3	3239	3082	0.15%	0.015%
26	18.216	2586	2589	2598	rVB5	9699	16974	0.81%	0.080%
27	18.292	2598	2602	2606	rBV5	2135	3309	0.16%	0.016%
28	19.286	2767	2771	2776	rBV	11097	15354	0.73%	0.072%
29	19.357	2779	2783	2788	rBV	10878	16086	0.76%	0.076%
30	19.504	2804	2808	2815	rBV7	6351	10637	0.51%	0.050%
31	19.728	2840	2846	2854	rBV	1381064	1862088	88.50%	8.768%
32	21.527	3147	3152	3164	rVB	914366	1175415	55.86%	5.535%
33	22.598	3326	3334	3345	rBV3	345414	1077895	51.23%	5.076%
34	23.804	3531	3539	3552	rVB2	1045032	2104138	100.00%	9.908%
35	23.957	3559	3565	3576	rVB2	579905	1193065	56.70%	5.618%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022655.D
Acq On : 15 Nov 2022 18:50
Operator : CG/JU
Sample : PB149004BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK004

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Title : SVOA CALIBRATION




Sum of corrected areas: 21236437

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022655.D
Acq On : 15 Nov 2022 18:50
Operator : CG/JU
Sample : PB149004BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

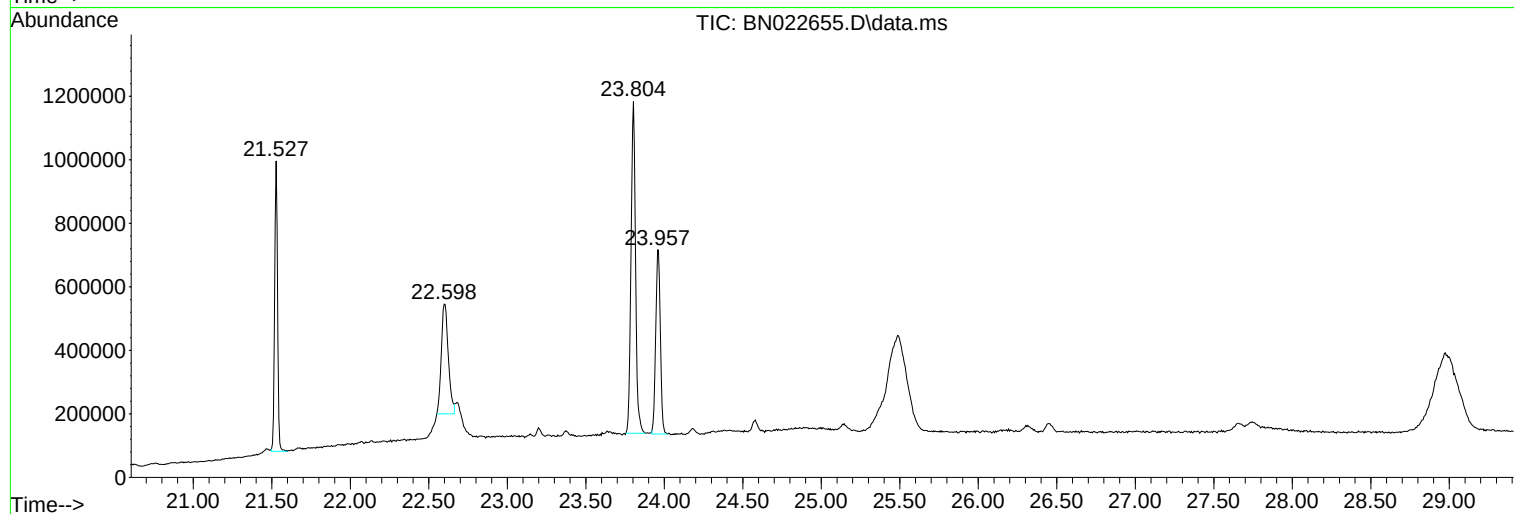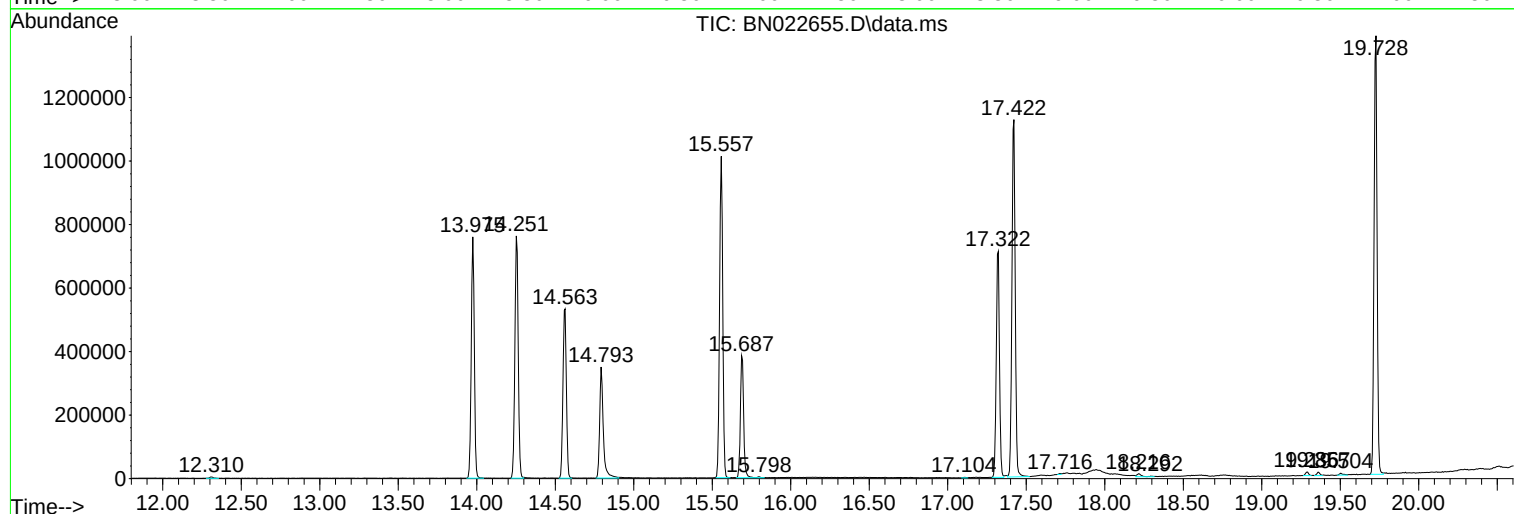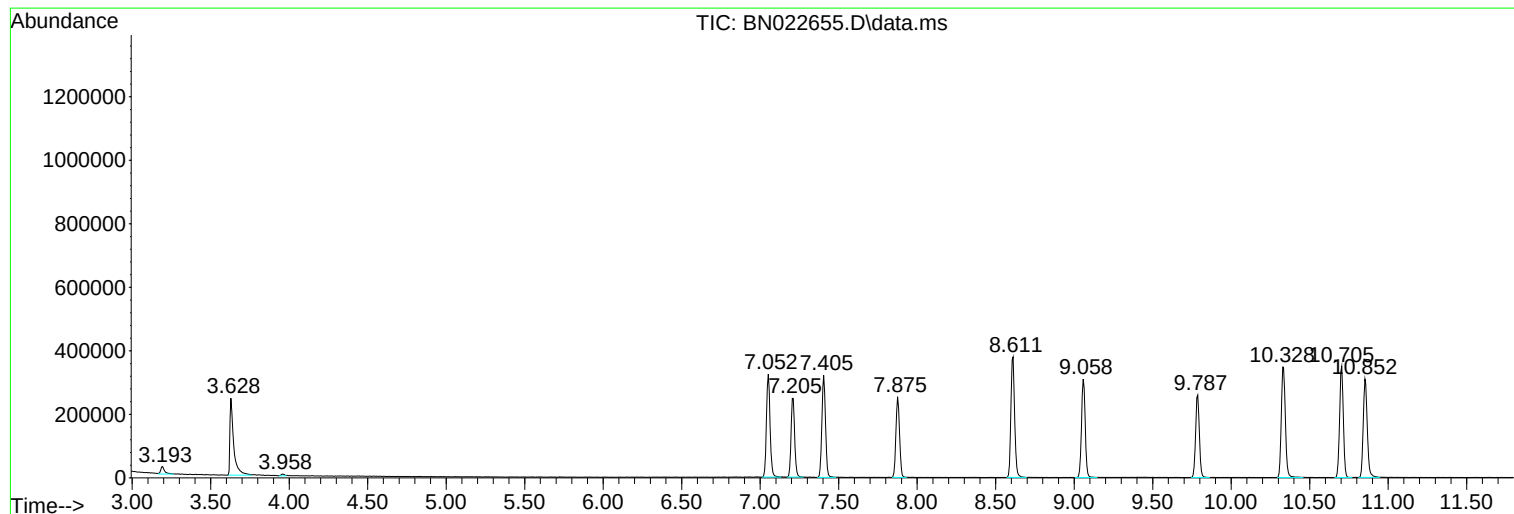

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022655.D
Acq On : 15 Nov 2022 18:50
Operator : CG/JU
Sample : PB149004BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK004










Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclononasiloxane, octadeca... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
22.598	18.34 ng/ul	1077900	Chrysene-d12	21.528

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclononasiloxane, octadecamethyl-	666	C18H54O9Si9	000556-71-8	86
2			Hexasiloxane, tetradecamethyl-	458	C14H42O5Si6	000107-52-8	62
3			Heptasiloxane, hexadecamethyl-	532	C16H48O6Si7	000541-01-5	38
4			Mercaptoacetic acid, 2TMS deriva...	236	C8H20O2SSi2	006398-62-5	37
5			2-Amino-2-oxo-acetic acid, N-[3,...	221	C12H15NO3	024451-17-0	37

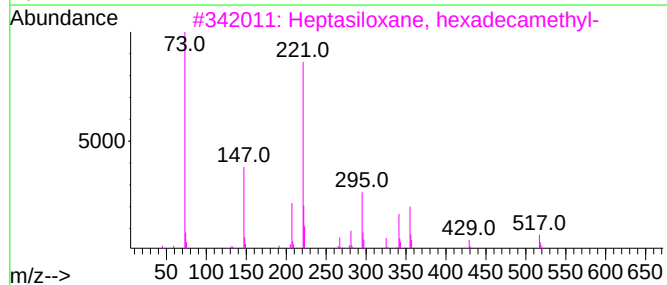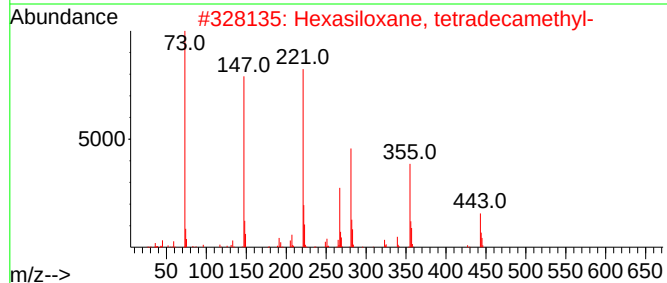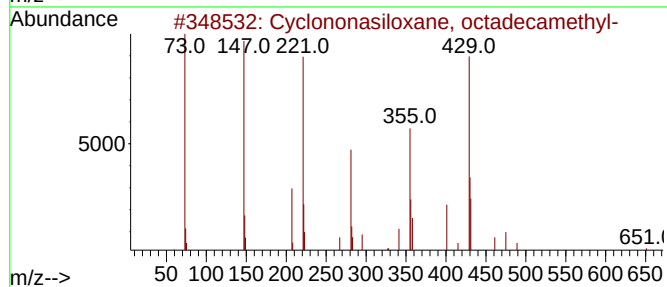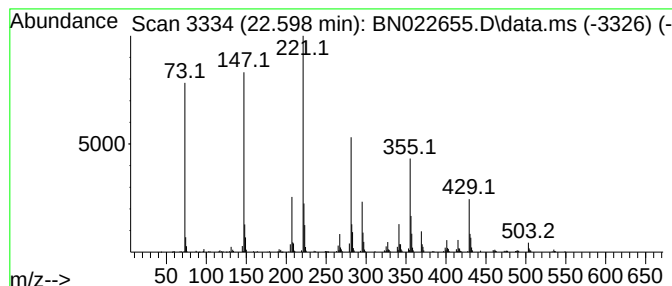

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN111522\
Data File : BN022655.D
Acq On : 15 Nov 2022 18:50
Operator : CG/JU
Sample : PB149004BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK004

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN111522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclononasilo...	22.598	18.3	ng/ul	1077900	5	21.528	1175420	20.0